
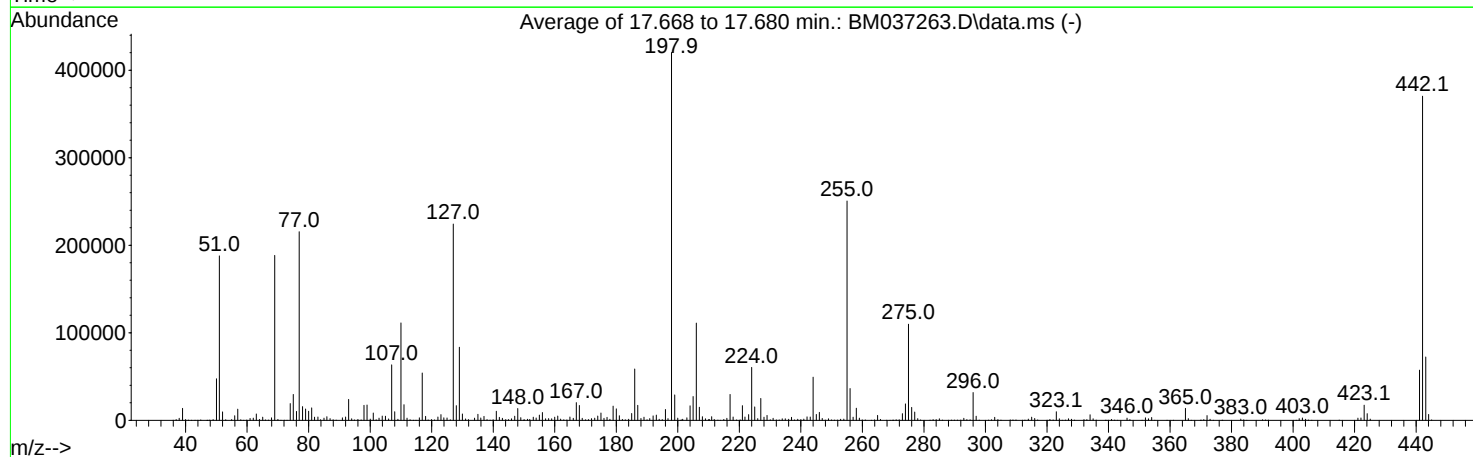


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102922\
 Data File : BM037263.D
 Acq On : 29 Oct 2022 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 31 01:34:15 2022

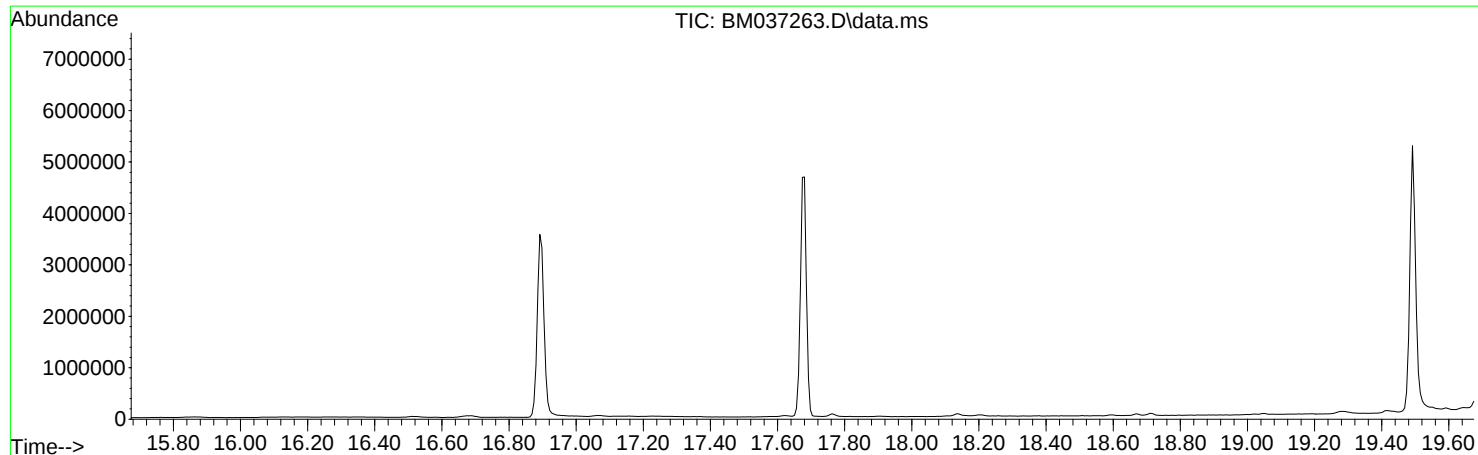




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	187879	PASS
68	69	0.00	2	1.5	2818	PASS
69	198	0.00	100	44.8	188391	PASS
70	69	0.00	2	0.5	1014	PASS
127	198	10	80	53.3	224171	PASS
197	198	0.00	2	0.4	1855	PASS
198	198	100	100	100.0	420331	PASS
199	198	5	9	6.9	28899	PASS
275	198	10	60	26.1	109856	PASS
365	198	1	100	3.2	13624	PASS
441	198	0.01	100	13.6	57232	PASS
442	442	50	100	100.0	370283	PASS
443	442	15	24	19.5	72245	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102922\
 Data File : BM037263.D
 Acq On : 29 Oct 2022 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Oct 31 04:41:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 31 01:34:15 2022
 Response via : Initial Calibration

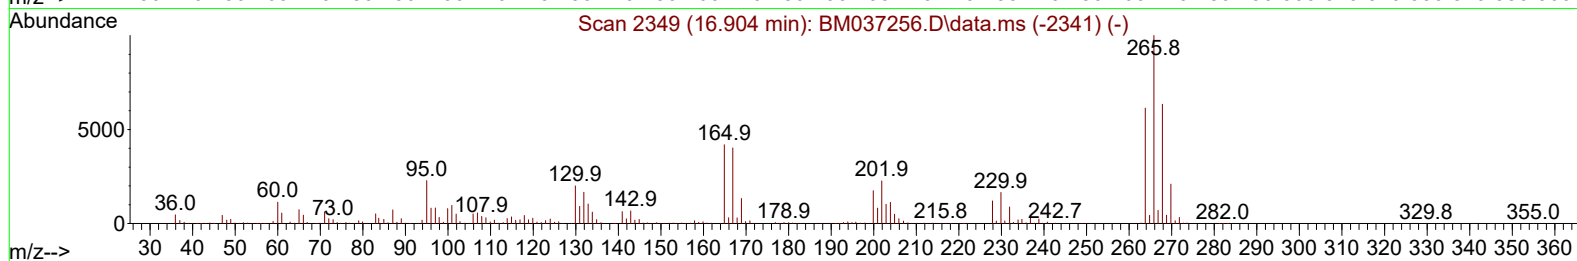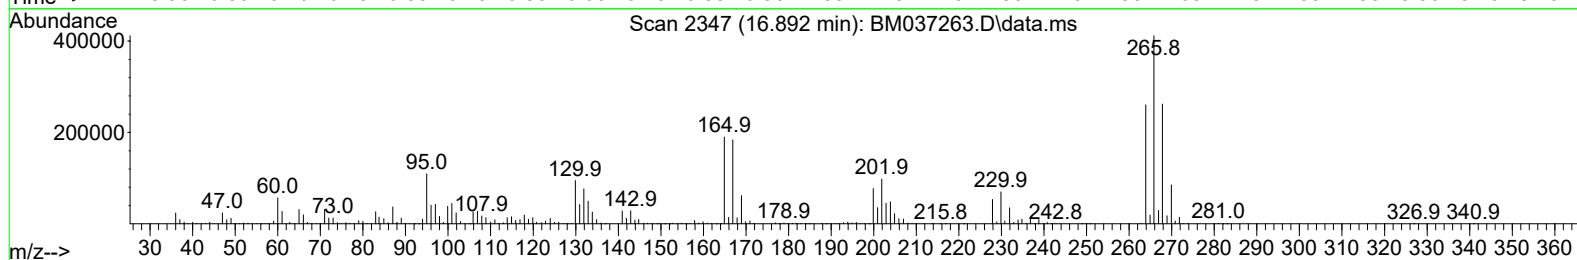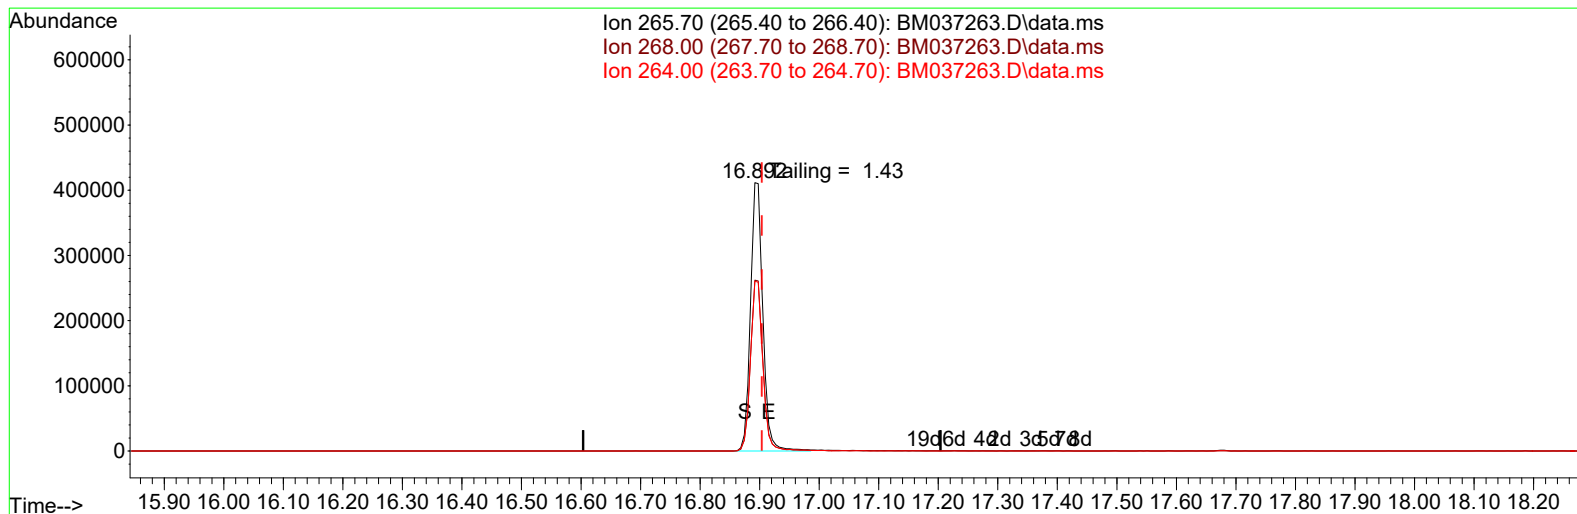

TIC: BM037263.D\data.ms

(70) Pentachlorophenol (C)

16.892min (-0.012) 24281.23 ng m




response 604997

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	63.69
264.00	61.40	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102922\
 Data File : BM037263.D
 Acq On : 29 Oct 2022 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Oct 31 04:41:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 31 01:34:15 2022
 Response via : Initial Calibration

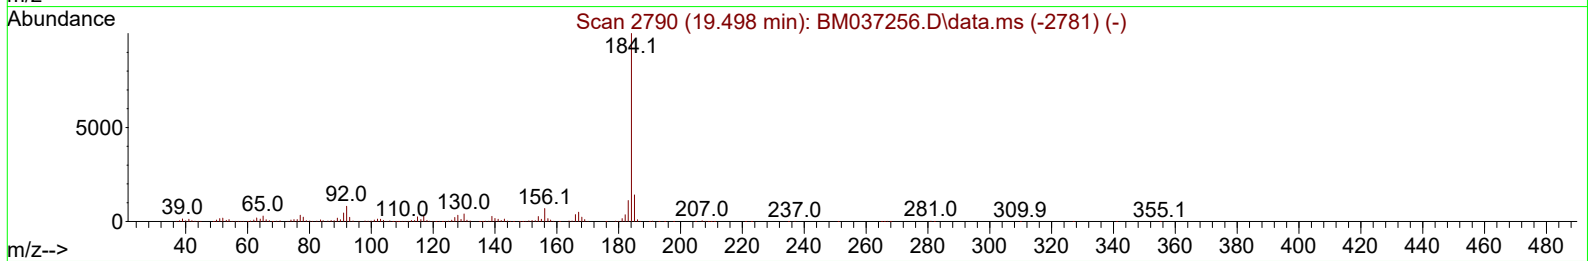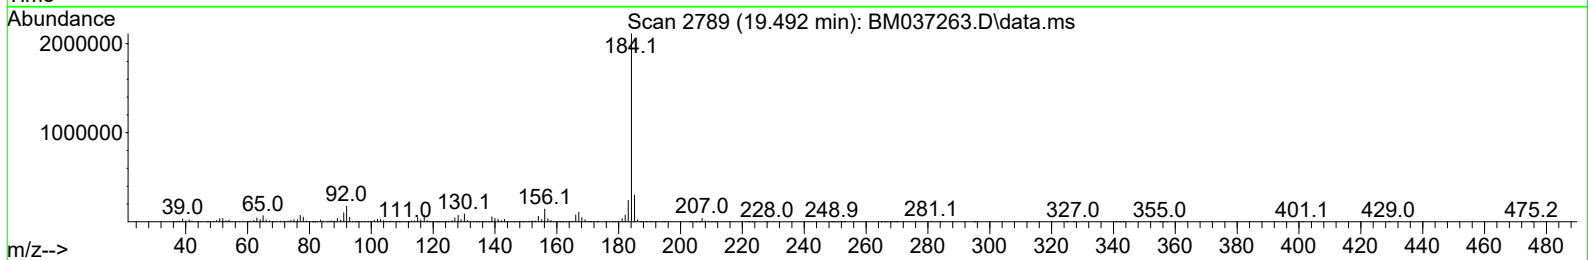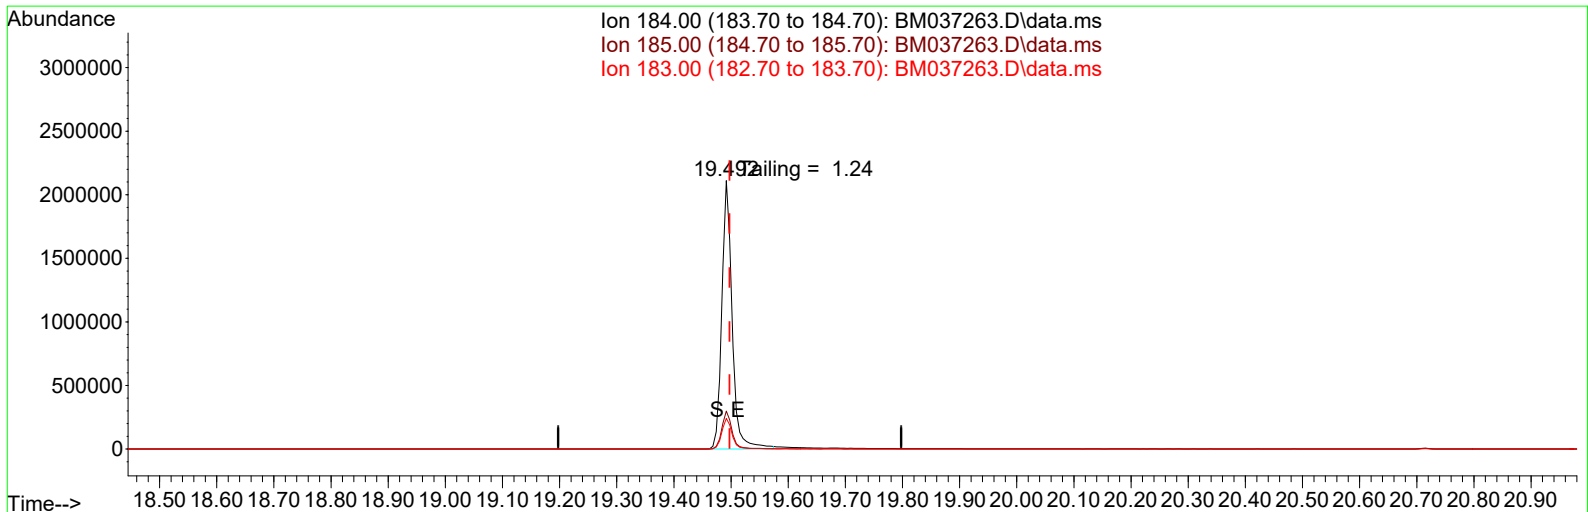

TIC: BM037263.D\data.ms

(77) Benzidine

19.492min (-0.006) 3332708.65 ng m

response 2782937

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.13
183.00	11.20	11.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/29/2022	BNA_M	<u>BM037263.D</u>
Compound Name	Response	Retention Time
DDT	1432869	20.715
DDD	24773	20.28
DDE	1942	19.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26715	1459584	1.83

Instrument :
BNA_M
ClientSampleId :
DFTPP