

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
 Data File : BM037315.D
 Acq On : 02 Nov 2022 14:26
 Operator : CG/JU
 Sample : N5301-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBWQ4

Quant Time: Nov 02 22:53:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 02 03:33:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	304893	20.000	ng/u1	0.00
20) Naphthalene-d8	10.657	136	1346799	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.492	164	842335	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.233	188	1641299	20.000	ng/u1	0.00
79) Chrysene-d12	21.403	240	1254014	20.000	ng/u1	0.00
88) Perylene-d12	23.750	264	1198361	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	30912	4.469	ng/uL	0.00
4) Pyridine-d5	3.699	84	213751	10.353	ng/u1	0.00
7) Phenol-d5	7.028	99	189853	7.155	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.193	67	523797	32.169	ng/u1	0.00
11) 2-Chlorophenol-d4	7.387	132	518185	25.560	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	352412	16.265	ng/u1	0.00
21) Nitrobenzene-d5	9.022	128	333608	33.160	ng/u1	0.00
24) 2-Nitrophenol-d4	9.745	143	337266	30.776	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	577021	28.560	ng/u1	0.00
31) 4-Chloroaniline-d4	10.804	131	833403	26.993	ng/u1	0.00
46) Dimethylphthalate-d6	13.910	166	2030080	34.857	ng/u1	0.00
49) Acenaphthylene-d8	14.186	160	2411228	34.437	ng/u1	0.00
54) 4-Nitrophenol-d4	14.710	143	57517	4.941	ng/u1	0.00
60) Fluorene-d10	15.480	176	1887250	36.337	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.610	200	284875	27.403	ng/u1	0.00
73) Anthracene-d10	17.327	188	2885876	38.178	ng/u1	0.00
81) Pyrene-d10	19.621	212	2935481	44.796	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.597	264	2334616	37.847	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.310	88	11413	1.571	ng/uL	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037315.D
Acq On : 02 Nov 2022 14:26
Operator : CG/JU
Sample : N5301-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBWQ4


Quant Time: Nov 02 22:53:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 02 03:33:37 2022
Response via : Initial Calibration

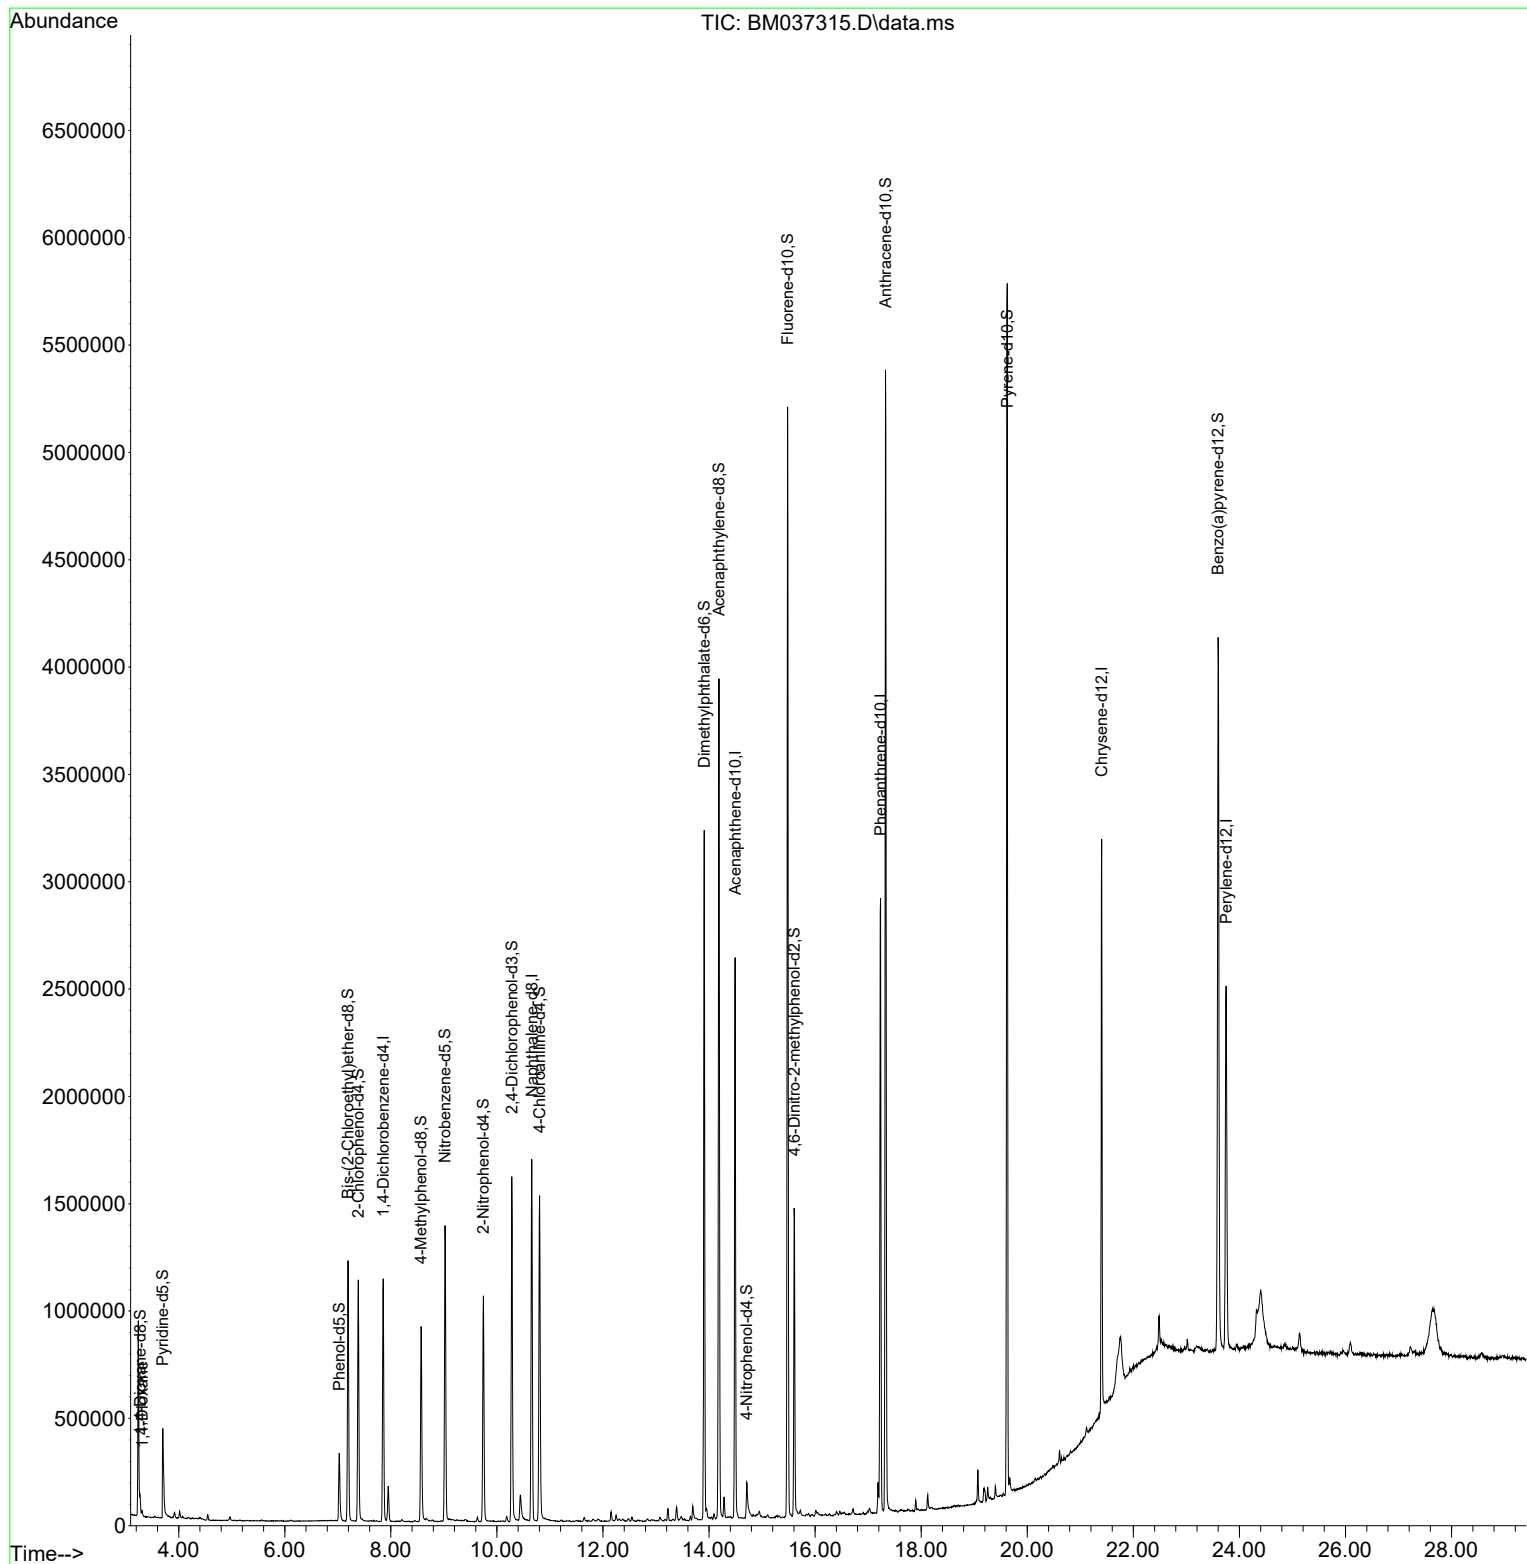

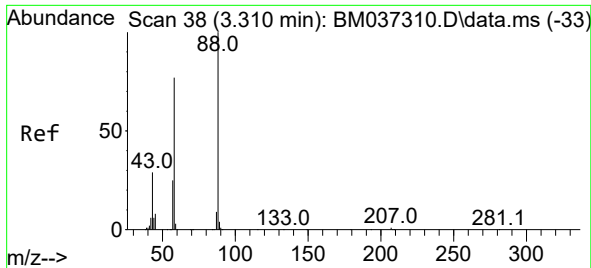

1,4-Dioxane
 Concen: 1.571 ng/uL
 RT: 3.310 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BM037315.D
 Acq: 02 Nov 2022 14:26

Instrument :
 BNA_M
 ClientSampleId :
 DBWQ4

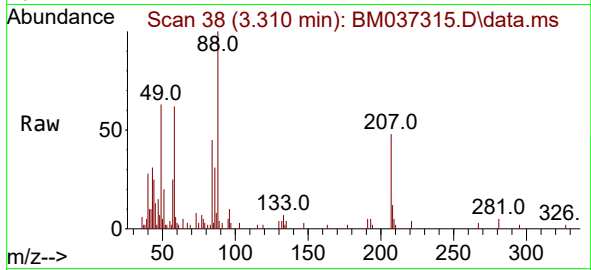

Tgt Ion:	88	Resp:	11413
Ion	Ratio	Lower	Upper
88	100		
43	31.2	23.4	35.0
58	62.0	59.4	89.0

