

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
 Data File : BM037327.D
 Acq On : 02 Nov 2022 21:41
 Operator : CG/JU
 Sample : N5301-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBWN4

Quant Time: Nov 02 22:55:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 02 03:33:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	370899	20.000	ng/ul	0.00
20) Naphthalene-d8	10.657	136	1642300	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.492	164	1072784	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.227	188	2169740	20.000	ng/ul	0.00
79) Chrysene-d12	21.403	240	1617996	20.000	ng/ul	0.00
88) Perylene-d12	23.750	264	1457903	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	30295	3.601	ng/uL	0.00
4) Pyridine-d5	3.704	84	254112	10.117	ng/ul	0.00
7) Phenol-d5	7.028	99	168261	5.213	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.192	67	443274	22.379	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	423690	17.180	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	302083	11.461	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	284208	23.167	ng/ul	0.00
24) 2-Nitrophenol-d4	9.745	143	269794	20.190	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	490905	19.926	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	745198	19.793	ng/ul	0.00
46) Dimethylphthalate-d6	13.910	166	1753716	23.643	ng/ul	0.00
49) Acenaphthylene-d8	14.186	160	2114346	23.710	ng/ul	0.00
54) 4-Nitrophenol-d4	14.710	143	54340	3.665	ng/ul	0.00
60) Fluorene-d10	15.480	176	1640856	24.807	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.604	200	234503	17.064	ng/ul	0.00
73) Anthracene-d10	17.327	188	2505806	25.076	ng/ul	0.00
81) Pyrene-d10	19.615	212	2345388	27.740	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.597	264	1865292	24.855	ng/ul	0.00
Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.634	70	242048	11.528	ng/ul#	34
18) 4-Methylphenol	8.639	108	2641103	92.534	ng/ul	89
83) Butylbenzylphthalate	20.533	149	50766	1.193	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037327.D
Acq On : 02 Nov 2022 21:41
Operator : CG/JU
Sample : N5301-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBWN4

Quant Time: Nov 02 22:55:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 02 03:33:37 2022
Response via : Initial Calibration




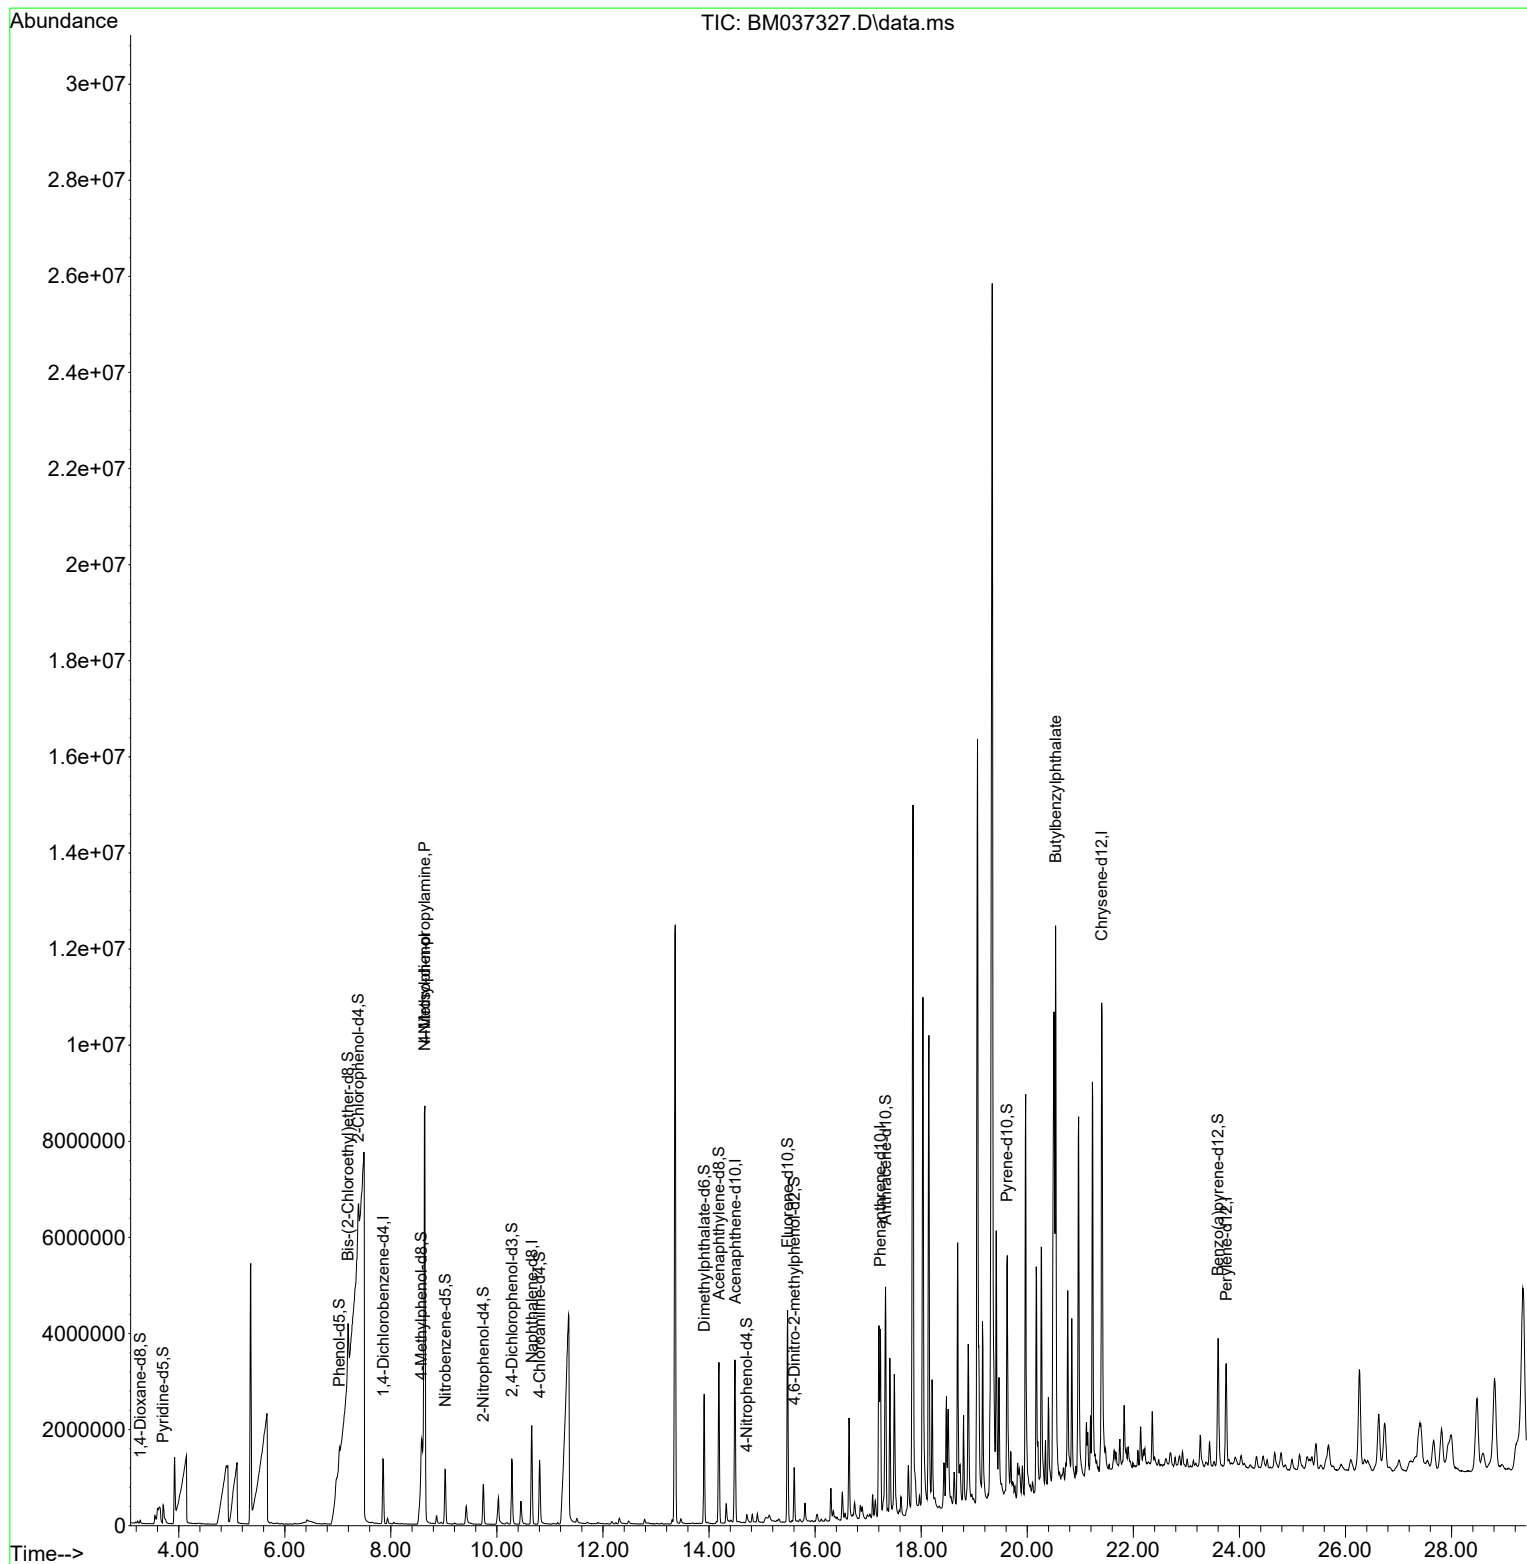


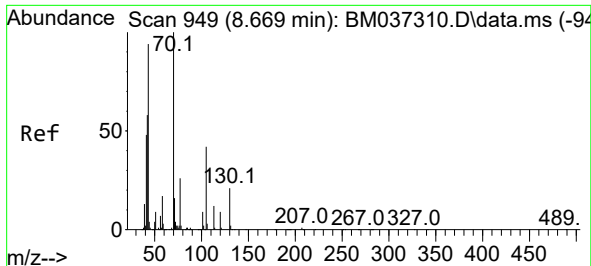

#17
N-Nitroso-di-n-propylamine
Concen: 11.528 ng/ul
RT: 8.634 min Scan# 949
Delta R.T. -0.041 min
Lab File: BM037327.D
Acq: 02 Nov 2022 21:41




Instrument :
BNA_M
ClientSampleId :
DBWN4


Tgt Ion: 70 Resp: 242048
Ion Ratio Lower Upper
70 100
42 107.2 46.8 70.2#
101 54.4 8.2 12.2#
130 0.8 17.7 26.5#

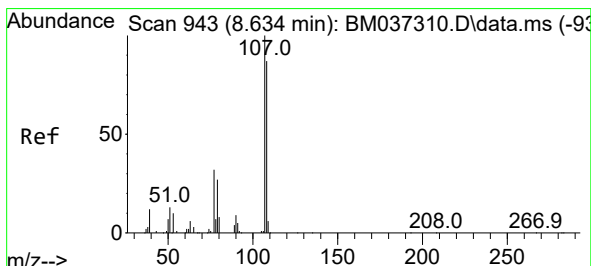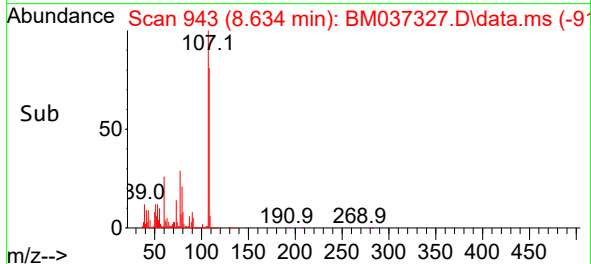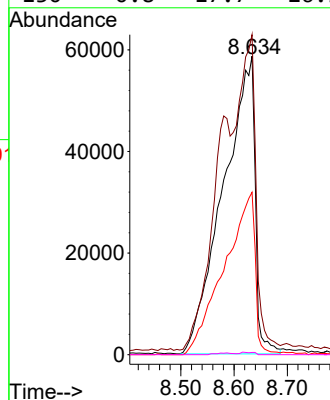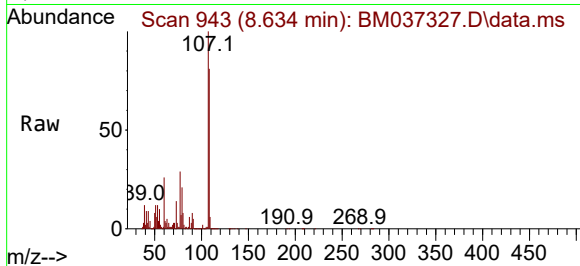

#18
4-Methylphenol
Concen: 92.534 ng/ul
RT: 8.639 min Scan# 944
Delta R.T. -0.000 min
Lab File: BM037327.D
Acq: 02 Nov 2022 21:41

Tgt Ion: 108 Resp: 2641103
Ion Ratio Lower Upper
108 100
107 123.3 89.3 133.9

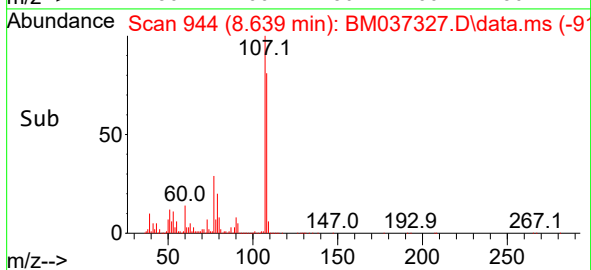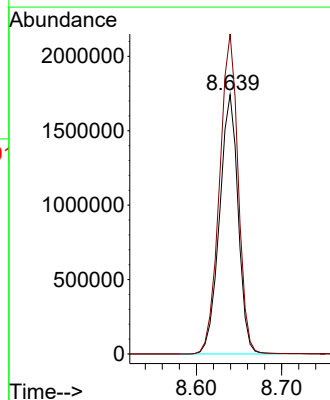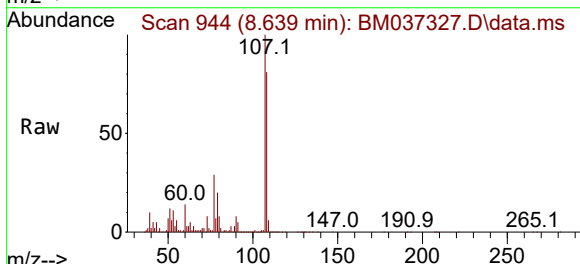

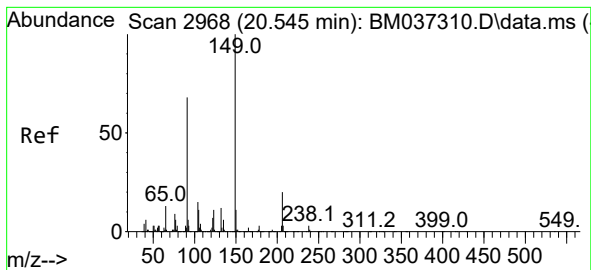

#83
 Butylbenzylphthalate
 Concen: 1.193 ng/ul
 RT: 20.533 min Scan# 2966
 Delta R.T. -0.012 min
 Lab File: BM037327.D
 Acq: 02 Nov 2022 21:41

Instrument :
 BNA_M
 ClientSampleId :
 DBWN4

Tgt Ion:149 Resp: 50766
 Ion Ratio Lower Upper
 149 100
 91 36.0 54.2 81.4#
 206 6.3 16.1 24.1#

