

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
 Data File : BM037311.D
 Acq On : 02 Nov 2022 10:47
 Operator : CG/JU
 Sample : PB148668BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK668

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037311.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	44	rVB	92430	126183	1.67%	0.161%
2	3.693	101	103	126	rBV	1017542	1584981	20.97%	2.022%
3	4.016	155	158	165	rVB	20778	28250	0.37%	0.036%
4	7.028	663	670	684	rBV	1172093	1899164	25.13%	2.423%
5	7.192	691	698	712	rVB	1069426	1625483	21.51%	2.074%
6	7.387	724	731	741	rBV	1251826	1947872	25.77%	2.485%
7	7.851	804	810	823	rBV	1115170	1776334	23.50%	2.266%
8	8.569	924	932	948	rBV	1474437	2414096	31.94%	3.080%
9	9.022	1001	1009	1021	rBV	1191520	1915460	25.34%	2.444%
10	9.745	1124	1132	1141	rBV	933919	1537824	20.35%	1.962%
11	10.281	1216	1223	1238	rBV	1423926	2375042	31.42%	3.030%
12	10.657	1279	1287	1297	rBV	1662914	2679088	35.44%	3.418%
13	10.804	1304	1312	1328	rBV	1450989	2580726	34.14%	3.292%
14	12.251	1553	1558	1568	rBV2	16382	39299	0.52%	0.050%
15	12.839	1655	1658	1665	rVB8	5014	10853	0.14%	0.014%
16	13.910	1831	1840	1850	rBV	2726591	3787803	50.11%	4.832%
17	14.186	1880	1887	1904	rBV	3216398	4731565	62.60%	6.036%
18	14.486	1931	1938	1948	rBV	2548873	3747018	49.57%	4.780%
19	14.704	1969	1975	1989	rBV	961940	1659014	21.95%	2.116%
20	15.263	2065	2070	2074	rBV7	6224	11751	0.16%	0.015%
21	15.480	2096	2107	2122	rBV	4508333	6171835	81.65%	7.874%
22	15.610	2122	2129	2143	rVV	1151566	1711146	22.64%	2.183%
23	15.715	2144	2147	2154	rVB2	23178	41365	0.55%	0.053%
24	16.662	2303	2308	2309	rBV5	4670	7843	0.10%	0.010%
25	17.015	2364	2368	2373	rVV3	7384	12608	0.17%	0.016%
26	17.233	2398	2405	2414	rBV	3031911	4340886	57.43%	5.538%
27	17.327	2415	2421	2439	rVV	4915563	6700996	88.65%	8.549%
28	19.180	2733	2736	2741	rBV2	47354	64731	0.86%	0.083%
29	19.251	2745	2748	2754	rVV	37937	57364	0.76%	0.073%
30	19.615	2804	2810	2821	rBV	5819749	7558542	100.00%	9.643%
31	21.403	3109	3114	3127	rBV	3537504	4599943	60.86%	5.868%
32	23.597	3481	3487	3503	rVB2	3362452	6581032	87.07%	8.396%
33	23.750	3507	3513	3526	rVB2	2144746	4058857	53.70%	5.178%




Sum of corrected areas: 78384954

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037311.D
Acq On : 02 Nov 2022 10:47
Operator : CG/JU
Sample : PB148668BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK668

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM11022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

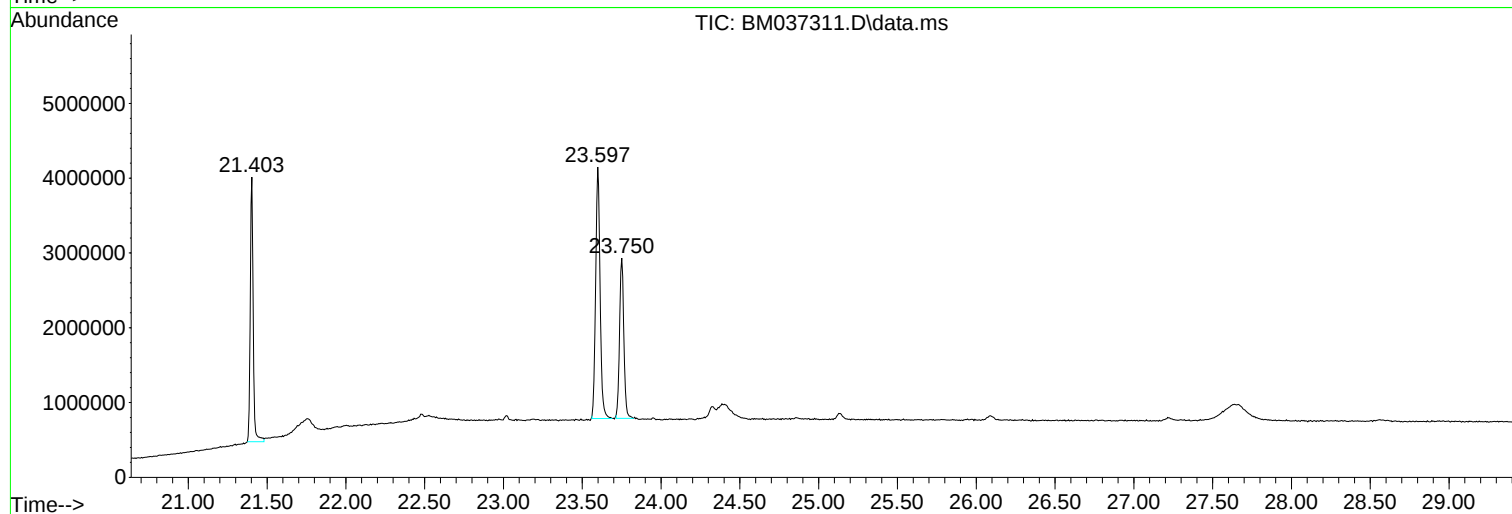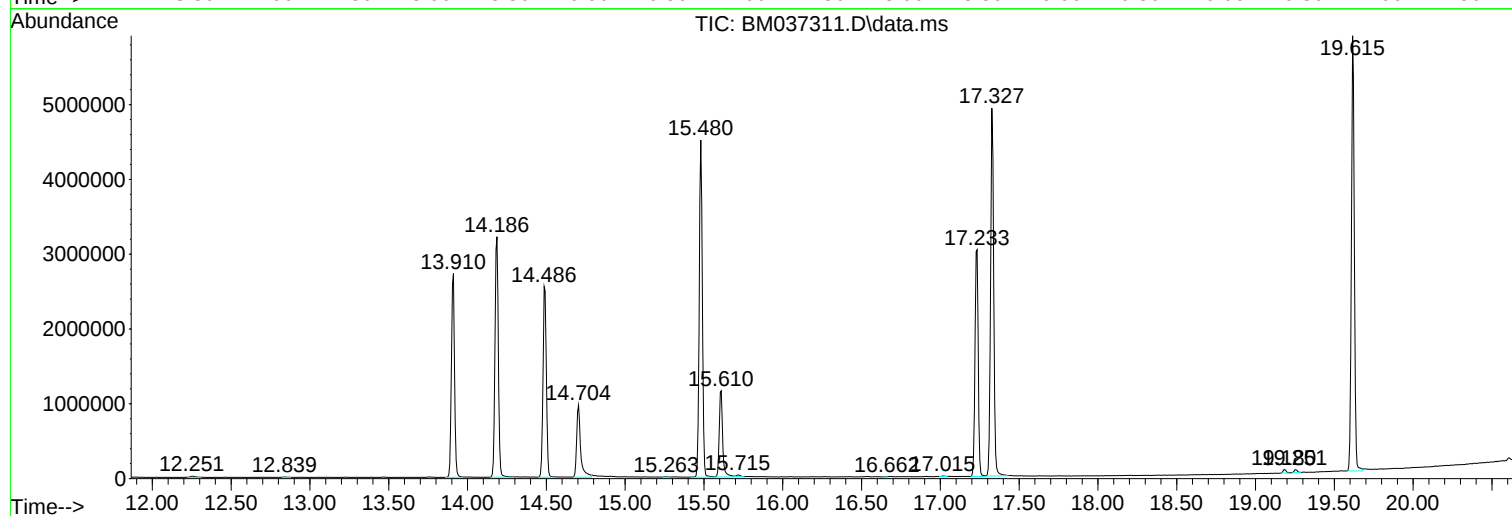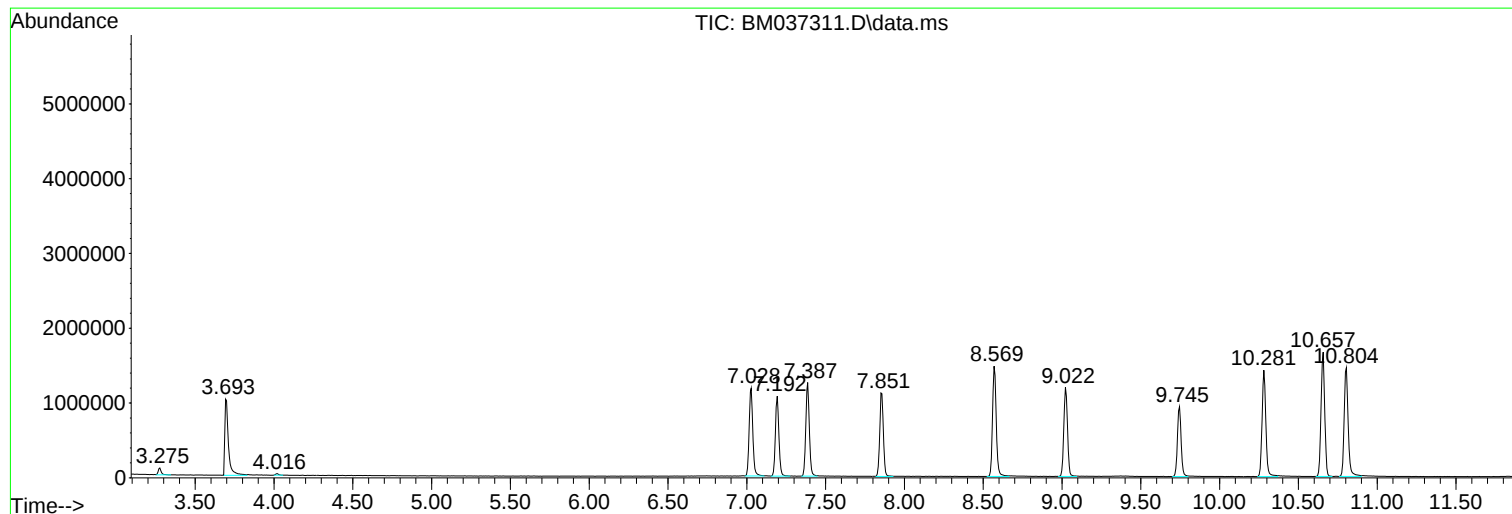

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037311.D
Acq On : 02 Nov 2022 10:47
Operator : CG/JU
Sample : PB148668BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK668

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037311.D
Acq On : 02 Nov 2022 10:47
Operator : CG/JU
Sample : PB148668BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK668

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc