

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
 Data File : BM037320.D
 Acq On : 02 Nov 2022 17:29
 Operator : CG/JU
 Sample : PB148669BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK669

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	38	rVB	100685	122920	1.45%	0.138%
2	3.698	100	104	121	rBV	1179844	1775047	20.96%	1.995%
3	4.016	155	158	163	rVB	25949	34267	0.40%	0.039%
4	7.028	664	670	684	rBV	1382241	2165303	25.56%	2.433%
5	7.192	691	698	715	rVB	1212638	1855185	21.90%	2.085%
6	7.386	724	731	741	rBV	1434382	2235660	26.39%	2.512%
7	7.857	803	811	822	rBV	1310789	2048001	24.18%	2.301%
8	8.575	924	933	952	rBV	1678434	2794684	32.99%	3.140%
9	9.027	1002	1010	1018	rBV	1335928	2169417	25.61%	2.438%
10	9.745	1123	1132	1143	rBV	1114803	1790317	21.14%	2.012%
11	10.280	1216	1223	1238	rBV	1627252	2768682	32.69%	3.111%
12	10.657	1279	1287	1298	rBV	1899332	3107753	36.69%	3.492%
13	10.804	1305	1312	1325	rBV	1704242	2940072	34.71%	3.304%
14	11.898	1493	1498	1506	rVB10	5123	11929	0.14%	0.013%
15	12.251	1552	1558	1567	rBV2	21003	43199	0.51%	0.049%
16	12.839	1652	1658	1660	rBV7	5241	8842	0.10%	0.010%
17	13.468	1760	1765	1770	rBV5	5768	10564	0.12%	0.012%
18	13.757	1808	1814	1818	rBV7	5143	8801	0.10%	0.010%
19	13.910	1833	1840	1851	rBV	3170982	4306727	50.85%	4.840%
20	14.186	1877	1887	1902	rBV	3826372	5394644	63.69%	6.062%
21	14.492	1931	1939	1953	rBV	3088062	4398535	51.93%	4.943%
22	14.704	1968	1975	1995	rBV	1159301	1999615	23.61%	2.247%
23	14.898	2006	2008	2017	rVB8	8991	18971	0.22%	0.021%
24	15.480	2098	2107	2121	rBV	5054076	7023845	82.92%	7.893%
25	15.609	2123	2129	2143	rVV	1491175	2042436	24.11%	2.295%
26	15.721	2144	2148	2153	rVB	23610	39166	0.46%	0.044%
27	16.686	2309	2312	2318	rBV8	5297	8725	0.10%	0.010%
28	17.021	2364	2369	2374	rBV4	7635	13683	0.16%	0.015%
29	17.233	2398	2405	2412	rBV	3578528	5047548	59.59%	5.672%
30	17.327	2415	2421	2444	rVB	5394529	7576156	89.45%	8.513%
31	19.186	2733	2737	2743	rBV	56010	76913	0.91%	0.086%
32	19.256	2745	2749	2756	rBV3	50391	77641	0.92%	0.087%
33	19.621	2805	2811	2821	rBV	6533733	8470183	100.00%	9.518%
34	21.403	3109	3114	3123	rBV	4291476	5087022	60.06%	5.716%
35	23.603	3481	3488	3502	rVB	3593513	7099328	83.82%	7.978%
36	23.750	3507	3513	3524	rVB2	2318751	4418935	52.17%	4.966%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037320.D
Acq On : 02 Nov 2022 17:29
Operator : CG/JU
Sample : PB148669BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK669

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Title : SVOA CALIBRATION




Sum of corrected areas: 88990716

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037320.D
Acq On : 02 Nov 2022 17:29
Operator : CG/JU
Sample : PB148669BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK669

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

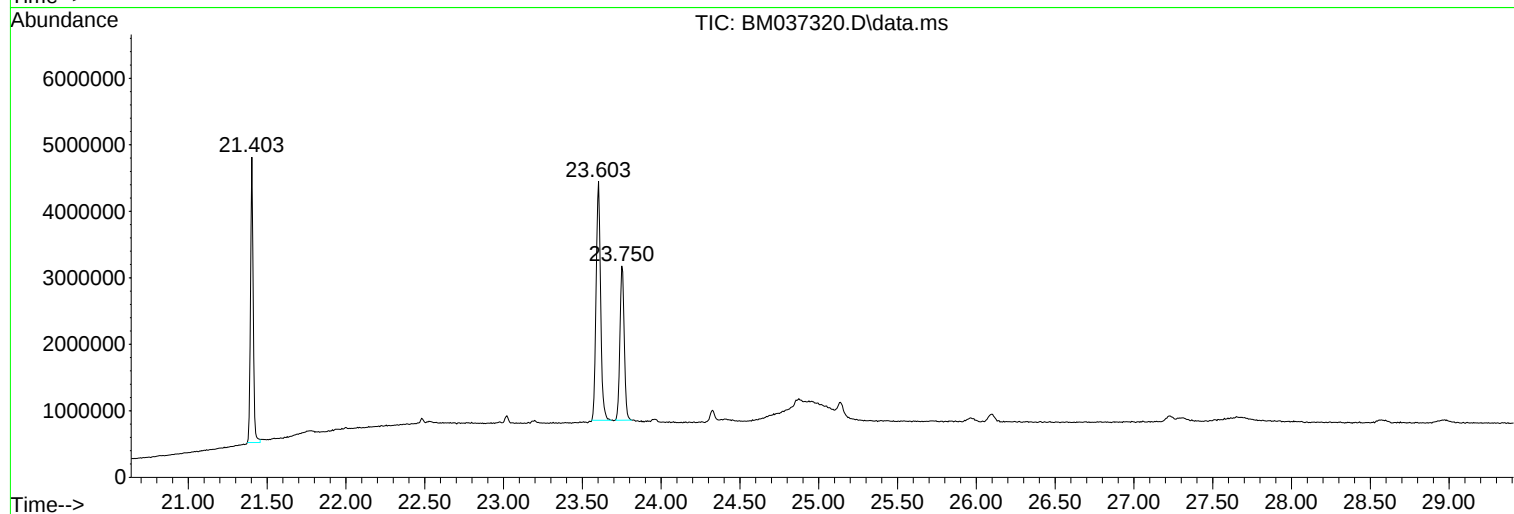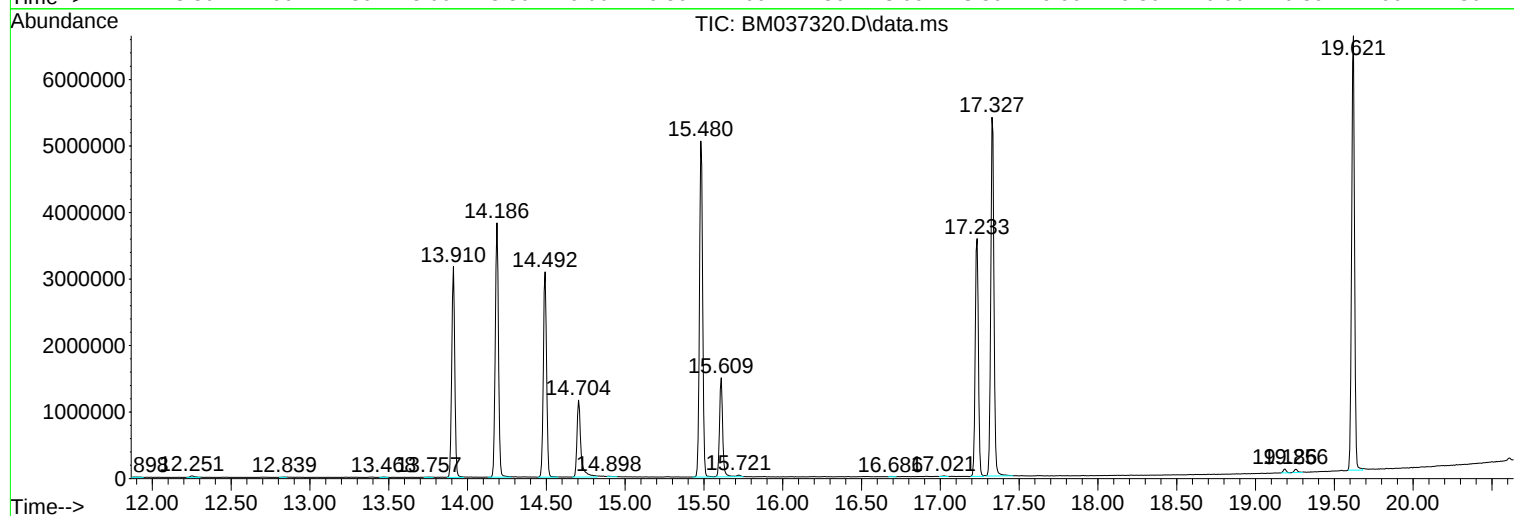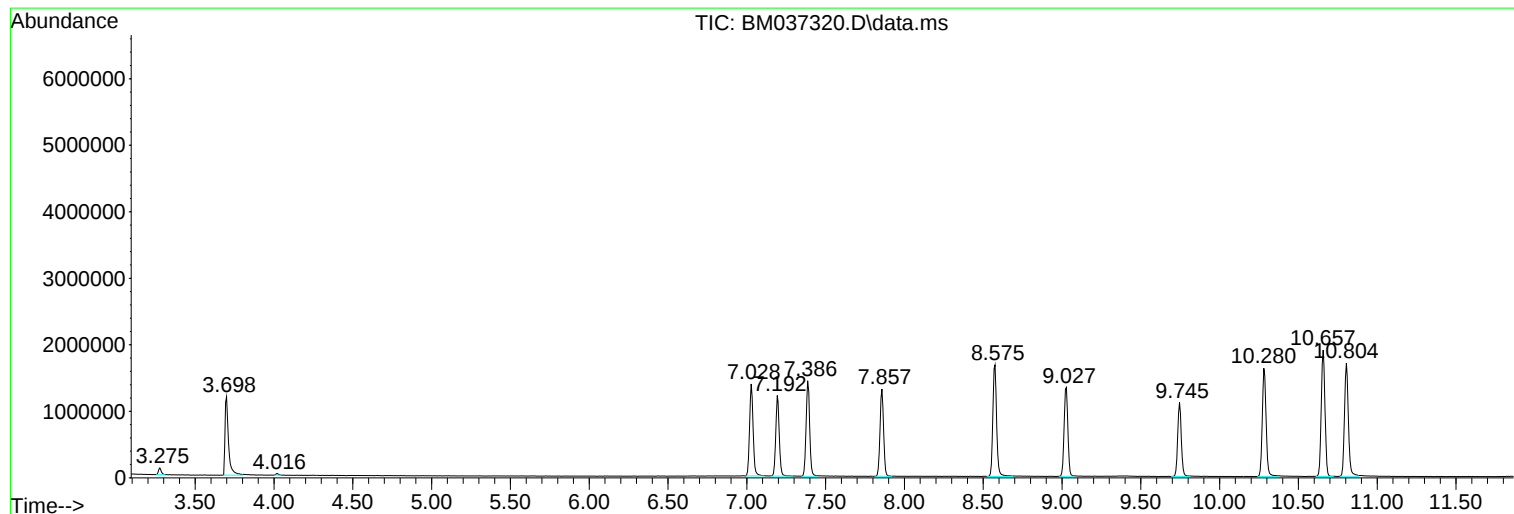

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037320.D
Acq On : 02 Nov 2022 17:29
Operator : CG/JU
Sample : PB148669BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK669

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037320.D
Acq On : 02 Nov 2022 17:29
Operator : CG/JU
Sample : PB148669BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK669

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc