

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
 Data File : BM037321.D
 Acq On : 02 Nov 2022 18:05
 Operator : CG/JU
 Sample : PB148670BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK670

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	39	rVB	108848	142413	1.64%	0.164%
2	3.705	102	105	120	rBV	299246	483206	5.55%	0.557%
3	4.016	155	158	168	rVB	26226	42993	0.49%	0.050%
4	7.028	663	670	684	rBV	1451837	2301307	26.42%	2.653%
5	7.193	691	698	708	rBV	1265154	1920700	22.05%	2.214%
6	7.387	724	731	742	rBV	1499072	2365113	27.16%	2.727%
7	7.857	803	811	823	rBV	1198935	1865156	21.42%	2.150%
8	8.575	925	933	953	rBV	1794275	2924836	33.58%	3.372%
9	9.028	1002	1010	1021	rBV	1395495	2295845	26.36%	2.647%
10	9.745	1125	1132	1143	rBV	1127894	1858495	21.34%	2.143%
11	10.281	1216	1223	1243	rBV	1673715	2882261	33.10%	3.323%
12	10.657	1278	1287	1298	rBV	1764226	2827714	32.47%	3.260%
13	10.810	1306	1313	1325	rBV	161965	349435	4.01%	0.403%
14	11.898	1497	1498	1506	rVB6	7483	10021	0.12%	0.012%
15	12.251	1551	1558	1565	rBV2	23928	53278	0.61%	0.061%
16	12.839	1654	1658	1663	rBV8	4187	8756	0.10%	0.010%
17	13.463	1760	1764	1769	rVB5	5283	9133	0.10%	0.011%
18	13.763	1808	1815	1820	rBV9	4684	10315	0.12%	0.012%
19	13.910	1832	1840	1852	rBV	3258139	4388147	50.39%	5.059%
20	14.186	1880	1887	1904	rBV	3890725	5562474	63.87%	6.413%
21	14.492	1932	1939	1951	rBV	2721580	3924091	45.06%	4.524%
22	14.704	1968	1975	1998	rBV	1332749	2167816	24.89%	2.499%
23	14.898	2006	2008	2020	rVB	9065	20758	0.24%	0.024%
24	15.263	2067	2070	2074	rBV4	5774	9091	0.10%	0.010%
25	15.480	2095	2107	2121	rBV	5355575	7201150	82.69%	8.302%
26	15.610	2123	2129	2144	rVV	1546392	2144626	24.63%	2.472%
27	15.721	2144	2148	2153	rVB	24235	39968	0.46%	0.046%
28	17.015	2365	2368	2371	rBV5	8309	11383	0.13%	0.013%
29	17.233	2398	2405	2415	rBV	3244514	4523311	51.94%	5.215%
30	17.327	2415	2421	2436	rVV	5332329	7719028	88.63%	8.899%
31	19.186	2733	2737	2744	rBV	55559	77443	0.89%	0.089%
32	19.256	2745	2749	2755	rBV	55062	75806	0.87%	0.087%
33	19.621	2805	2811	2818	rBV	6777537	8708915	100.00%	10.040%
34	21.403	3109	3114	3123	rBV	3805391	4887754	56.12%	5.635%
35	23.603	3481	3488	3500	rBV2	4126338	8263222	94.88%	9.526%
36	23.756	3507	3514	3527	rVB2	2336761	4666585	53.58%	5.380%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037321.D
Acq On : 02 Nov 2022 18:05
Operator : CG/JU
Sample : PB148670BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK670

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Title : SVOA CALIBRATION




Sum of corrected areas: 86742545

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037321.D
Acq On : 02 Nov 2022 18:05
Operator : CG/JU
Sample : PB148670BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK670

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

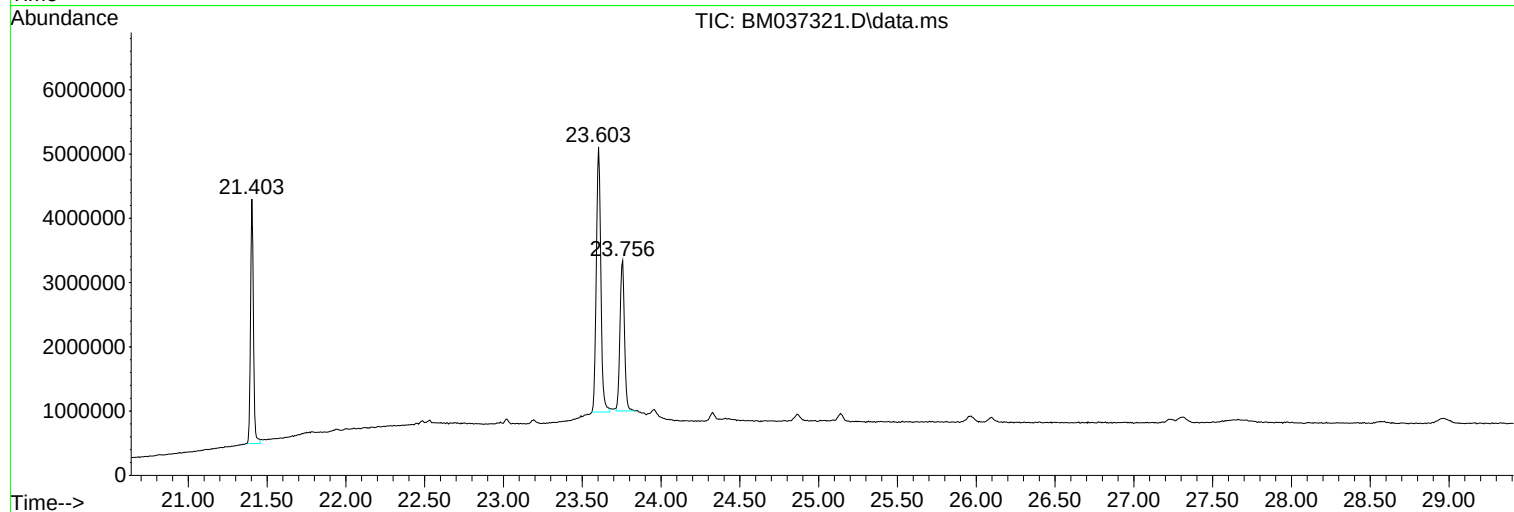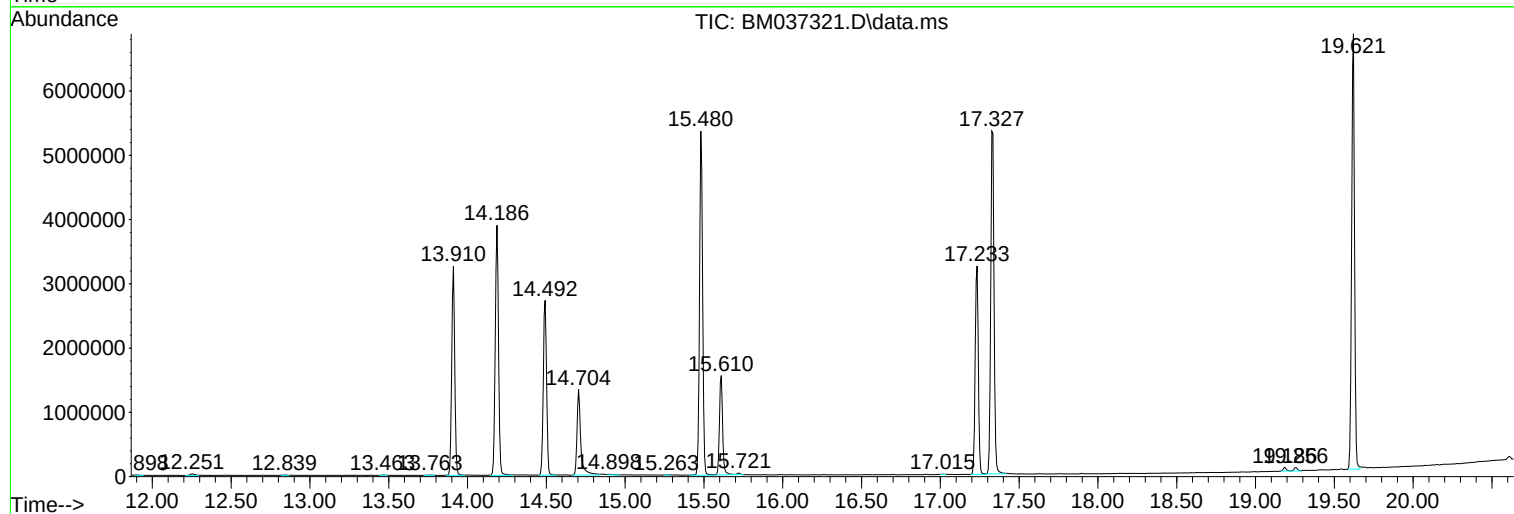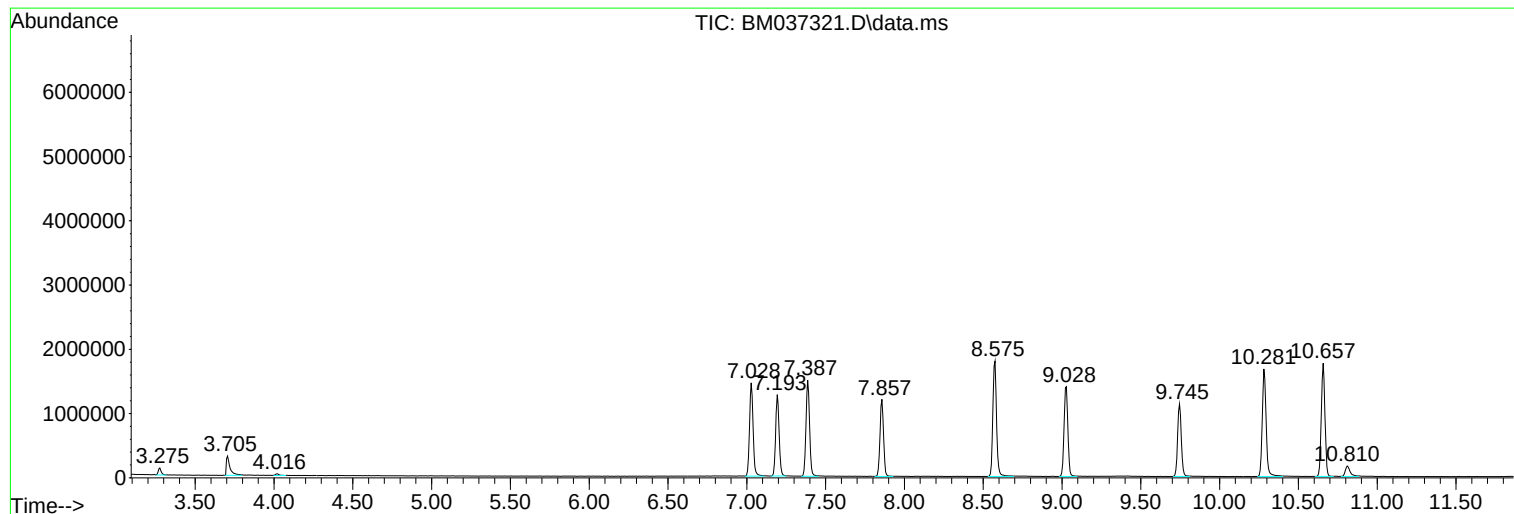

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037321.D
Acq On : 02 Nov 2022 18:05
Operator : CG/JU
Sample : PB148670BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK670

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037321.D
Acq On : 02 Nov 2022 18:05
Operator : CG/JU
Sample : PB148670BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK670

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc