

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
 Data File : BM037323.D
 Acq On : 02 Nov 2022 19:17
 Operator : CG/JU
 Sample : N5301-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBXA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	21	26	45	rVB	1189881	1849817	20.06%	2.156%
2	3.704	102	105	121	rBV	318208	504053	5.47%	0.588%
3	3.922	137	142	149	rVB	29992	46742	0.51%	0.054%
4	4.022	154	159	166	rVB	31769	47496	0.52%	0.055%
5	4.551	244	249	258	rVB5	16947	31088	0.34%	0.036%
6	4.969	315	320	326	rVB	17355	28413	0.31%	0.033%
7	7.028	664	670	690	rVB	316326	532152	5.77%	0.620%
8	7.192	691	698	708	rBV	1215387	1858839	20.16%	2.167%
9	7.387	724	731	741	rBV	1112153	1742872	18.90%	2.031%
10	7.457	741	743	750	rVB7	8152	12190	0.13%	0.014%
11	7.857	803	811	821	rBV	1218692	1924528	20.87%	2.243%
12	7.951	821	827	836	rVB3	30054	60487	0.66%	0.071%
13	8.204	867	870	877	rVB7	5217	9916	0.11%	0.012%
14	8.575	926	933	954	rBV	896141	1501719	16.28%	1.750%
15	9.028	1001	1010	1019	rBV	1345539	2227231	24.15%	2.596%
16	9.098	1019	1022	1029	rVB4	12287	22402	0.24%	0.026%
17	9.745	1124	1132	1142	rBV	1048547	1713738	18.58%	1.998%
18	10.281	1216	1223	1240	rBV	1600776	2673101	28.99%	3.116%
19	10.445	1247	1251	1269	rBV	39623	108306	1.17%	0.126%
20	10.657	1278	1287	1296	rBV	1807144	2927453	31.75%	3.412%
21	10.804	1304	1312	1329	rBV	1469197	2573824	27.91%	3.000%
22	11.827	1480	1486	1490	rBV9	4518	9245	0.10%	0.011%
23	12.192	1544	1548	1552	rBV7	7852	12418	0.13%	0.014%
24	12.245	1552	1557	1564	rVB3	25133	45571	0.49%	0.053%
25	12.851	1655	1660	1662	rBV6	7097	10458	0.11%	0.012%
26	13.069	1692	1697	1707	rVB7	13944	29420	0.32%	0.034%
27	13.222	1719	1723	1729	rBV7	8026	11508	0.12%	0.013%
28	13.292	1729	1735	1743	rVV7	4988	12247	0.13%	0.014%
29	13.380	1743	1750	1757	rVV4	13898	28928	0.31%	0.034%
30	13.463	1760	1764	1770	rVB6	8327	17316	0.19%	0.020%
31	13.910	1831	1840	1852	rBV	3448207	4530352	49.13%	5.281%
32	14.186	1879	1887	1898	rBV	3930408	5559696	60.29%	6.480%
33	14.492	1932	1939	1946	rBV	2970717	4143614	44.93%	4.830%
34	14.716	1971	1977	1994	rBV	178489	417410	4.53%	0.487%
35	15.280	2068	2073	2076	rBV	40889	58801	0.64%	0.069%
36	15.315	2076	2079	2085	rVB2	19687	28850	0.31%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
 Data File : BM037323.D
 Acq On : 02 Nov 2022 19:17
 Operator : CG/JU
 Sample : N5301-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBXA6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	15.480	2098	2107	2121	rBV	5358484	7322211	79.40%	8.535%
38	15.604	2123	2128	2142	rVV	1583312	2192077	23.77%	2.555%
39	15.721	2143	2148	2156	rVB	27608	56866	0.62%	0.066%
40	16.262	2237	2240	2244	rVB6	8002	11482	0.12%	0.013%
41	17.227	2398	2404	2411	rVB	3408496	4756864	51.58%	5.545%
42	17.327	2415	2421	2435	rBV	5836479	7934565	86.04%	9.248%
43	17.898	2514	2518	2524	rBV2	33151	43287	0.47%	0.050%
44	18.121	2552	2556	2564	rBV3	61544	97127	1.05%	0.113%
45	19.068	2714	2717	2721	rVB3	41490	37999	0.41%	0.044%
46	19.180	2733	2736	2742	rVB	61534	91325	0.99%	0.106%
47	19.251	2744	2748	2753	rBV	67140	106706	1.16%	0.124%
48	19.398	2770	2773	2778	rBV2	63415	83677	0.91%	0.098%
49	19.615	2804	2810	2816	rBV	7320804	9221548	100.00%	10.748%
50	21.403	3109	3114	3122	rBV	3834056	4862927	52.73%	5.668%
51	23.597	3480	3487	3502	rVB	4155475	7440467	80.69%	8.672%
52	23.750	3507	3513	3524	rVB2	2135901	4222511	45.79%	4.922%




Sum of corrected areas: 85793840

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037323.D
Acq On : 02 Nov 2022 19:17
Operator : CG/JU
Sample : N5301-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBXA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

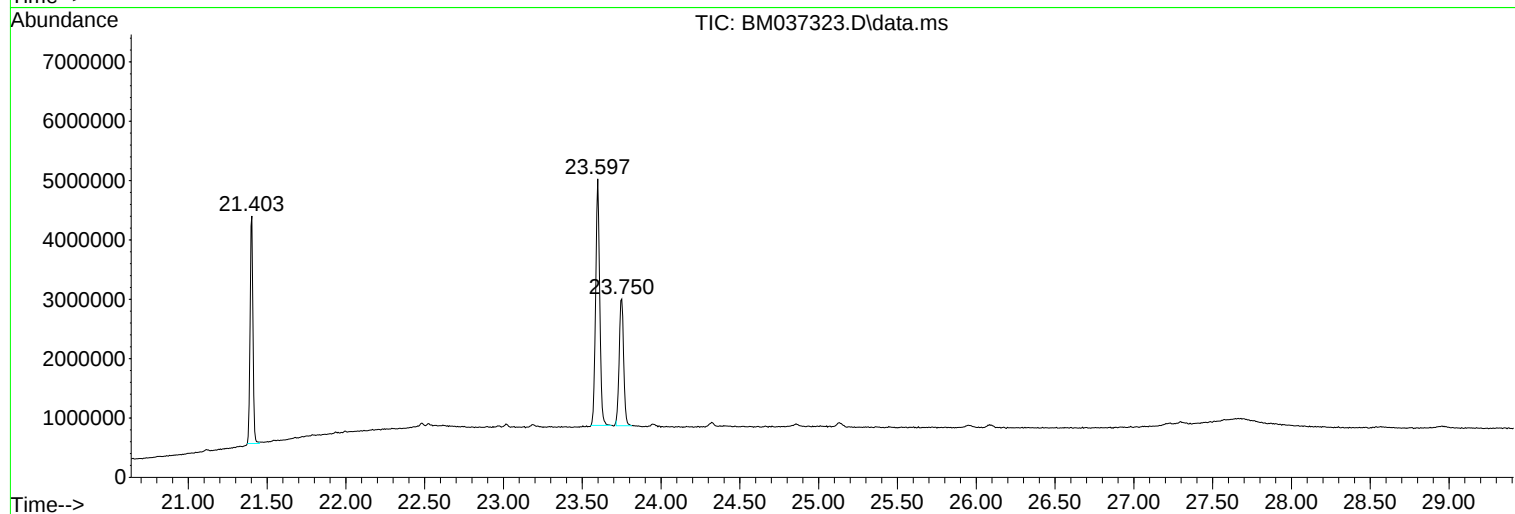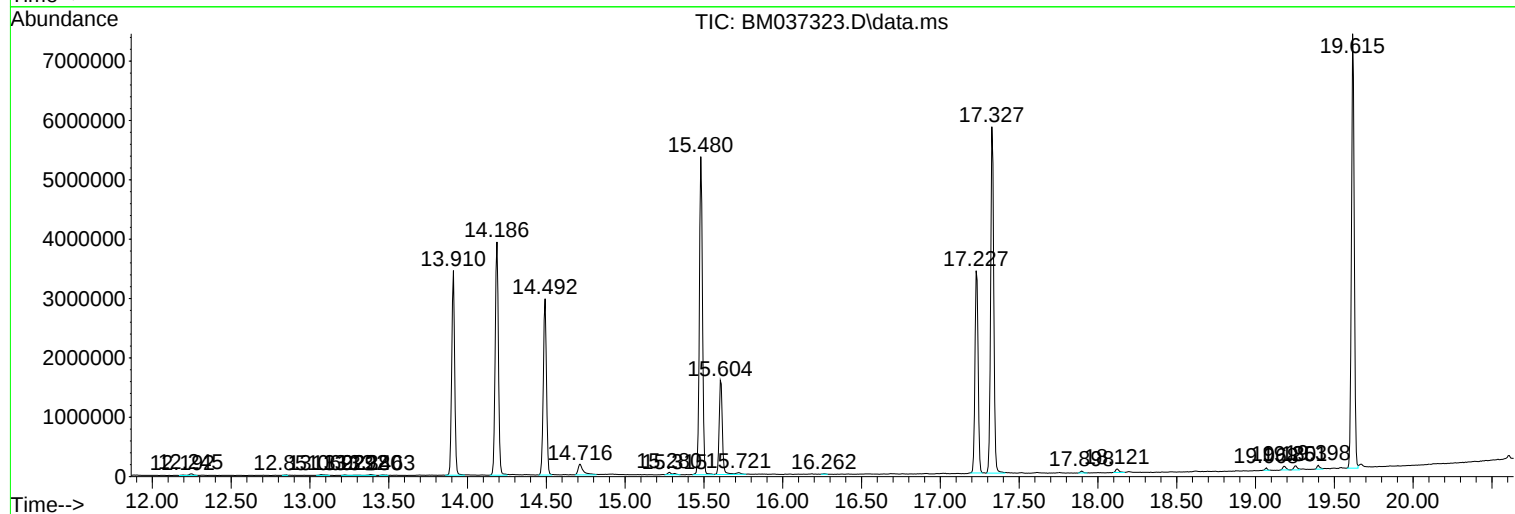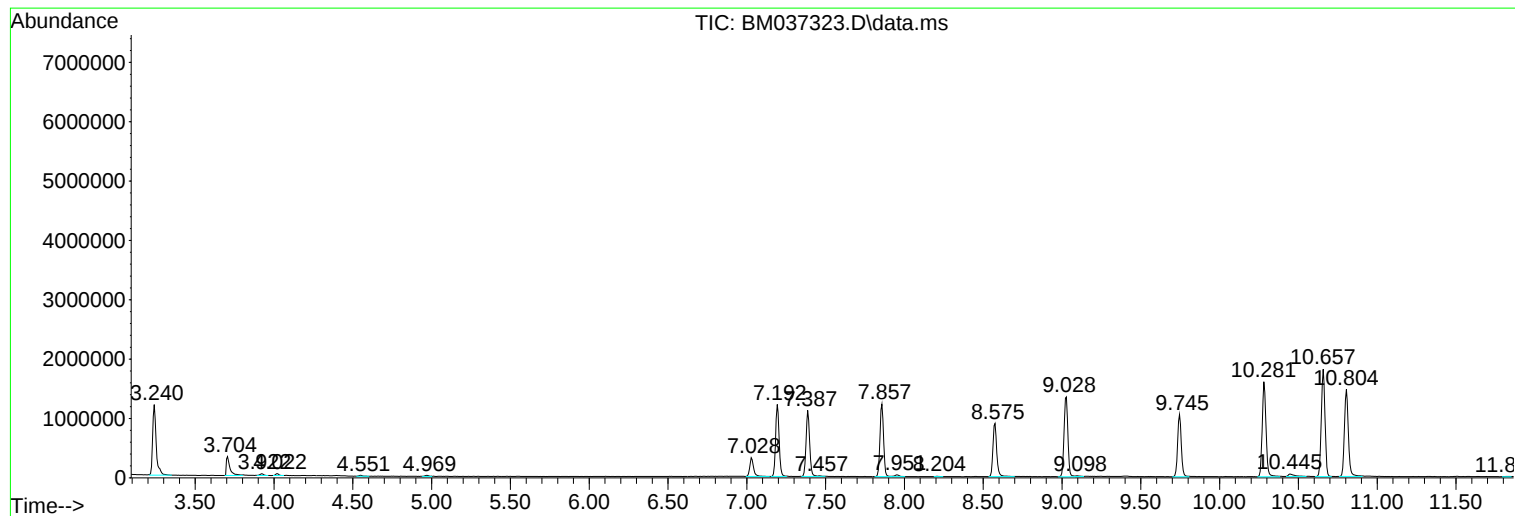

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037323.D
Acq On : 02 Nov 2022 19:17
Operator : CG/JU
Sample : N5301-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBXA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037323.D
Acq On : 02 Nov 2022 19:17
Operator : CG/JU
Sample : N5301-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBXA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc