

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
 Data File : BM037325.D
 Acq On : 02 Nov 2022 20:29
 Operator : CG/JU
 Sample : N5301-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBXB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	20	26	44	rVB	6327984	9257596	26.74%	6.446%
2	3.699	102	104	120	rBV	418201	668203	1.93%	0.465%
3	3.922	137	142	148	rVB	28603	44879	0.13%	0.031%
4	4.016	154	158	164	rBV	35116	51293	0.15%	0.036%
5	4.551	242	249	263	rBV	23567505	34618898	100.00%	24.104%
6	7.028	664	670	685	rBV	364720	609657	1.76%	0.424%
7	7.192	692	698	712	rVB	1371479	2098065	6.06%	1.461%
8	7.387	724	731	741	rBV	1279662	2001825	5.78%	1.394%
9	7.857	803	811	820	rBV	1236594	1954134	5.64%	1.361%
10	7.951	820	827	835	rVB2	52163	104996	0.30%	0.073%
11	8.569	925	932	946	rBV	1039276	1750657	5.06%	1.219%
12	9.022	1002	1009	1018	rBV	1557468	2516089	7.27%	1.752%
13	9.745	1124	1132	1145	rBV	1178961	1947163	5.62%	1.356%
14	10.280	1215	1223	1240	rBV	1827268	3073716	8.88%	2.140%
15	10.439	1244	1250	1261	rBV	270402	534463	1.54%	0.372%
16	10.657	1279	1287	1299	rVB	1810063	2971218	8.58%	2.069%
17	10.804	1303	1312	1327	rBV	1654108	2881266	8.32%	2.006%
18	12.245	1549	1557	1563	rBV2	28274	51611	0.15%	0.036%
19	13.386	1745	1751	1758	rVB2	57968	100365	0.29%	0.070%
20	13.910	1831	1840	1853	rBV	3924474	5395751	15.59%	3.757%
21	14.186	1876	1887	1899	rBV	4579922	6564453	18.96%	4.571%
22	14.492	1932	1939	1951	rVB	2912316	4144018	11.97%	2.885%
23	14.710	1970	1976	1993	rBV	268205	585237	1.69%	0.407%
24	15.480	2097	2107	2116	rBV	6283409	8612007	24.88%	5.996%
25	15.604	2122	2128	2137	rBV	1948263	2631303	7.60%	1.832%
26	15.721	2144	2148	2153	rVB2	25850	41731	0.12%	0.029%
27	17.186	2393	2397	2399	rBV	61546	80176	0.23%	0.056%
28	17.227	2399	2404	2414	rVB	3541961	4826791	13.94%	3.361%
29	17.327	2415	2421	2431	rBV	6961222	9653467	27.88%	6.721%
30	17.898	2514	2518	2522	rBV	110688	131982	0.38%	0.092%
31	18.121	2551	2556	2566	rBV	154723	248090	0.72%	0.173%
32	19.068	2713	2717	2722	rBV	213677	237365	0.69%	0.165%
33	19.180	2732	2736	2744	rBV2	86469	171468	0.50%	0.119%
34	19.250	2745	2748	2752	rBV	84080	104217	0.30%	0.073%
35	19.398	2769	2773	2783	rBV	155454	265228	0.77%	0.185%
36	19.615	2804	2810	2816	rBV	9093076	11543232	33.34%	8.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037325.D
Acq On : 02 Nov 2022 20:29
Operator : CG/JU
Sample : N5301-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBXB4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Title : SVOA CALIBRATION

37	19.668	2816	2819	2828	rVB	370801	515938	1.49%	0.359%
38	21.397	3109	3113	3121	rBV	4217347	5307803	15.33%	3.696%
39	23.597	3480	3487	3503	rVB2	5366840	10531079	30.42%	7.333%
40	23.750	3506	3513	3521	rVB2	2520593	4794144	13.85%	3.338%




Sum of corrected areas: 143621574

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037325.D
Acq On : 02 Nov 2022 20:29
Operator : CG/JU
Sample : N5301-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBXB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

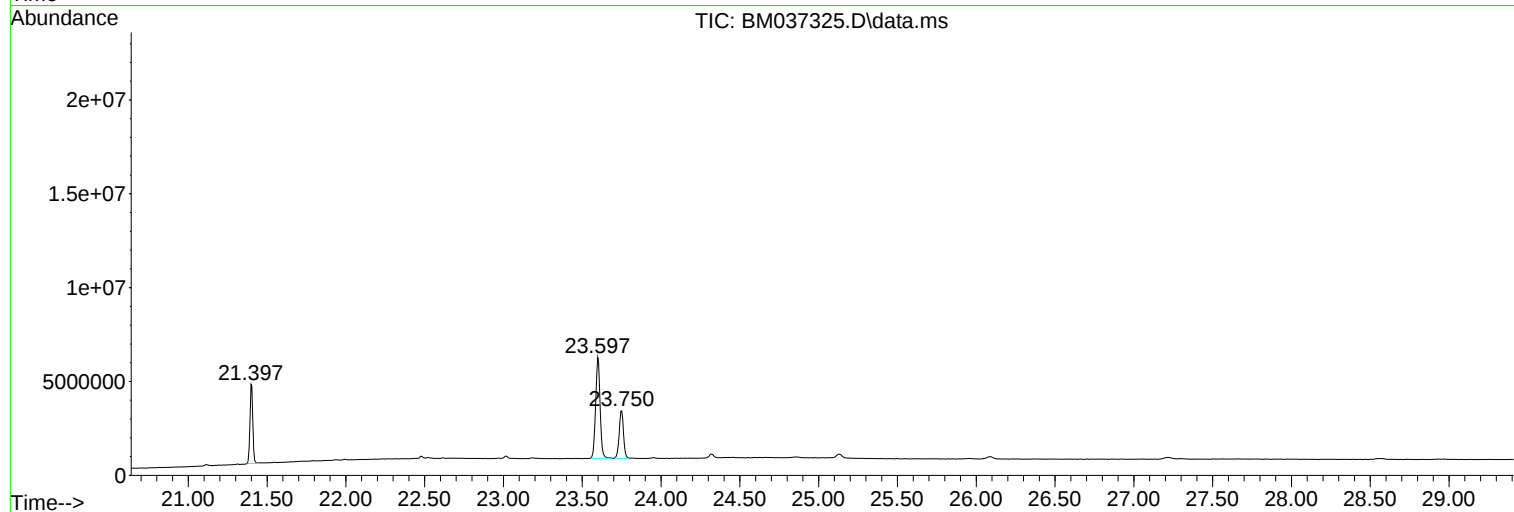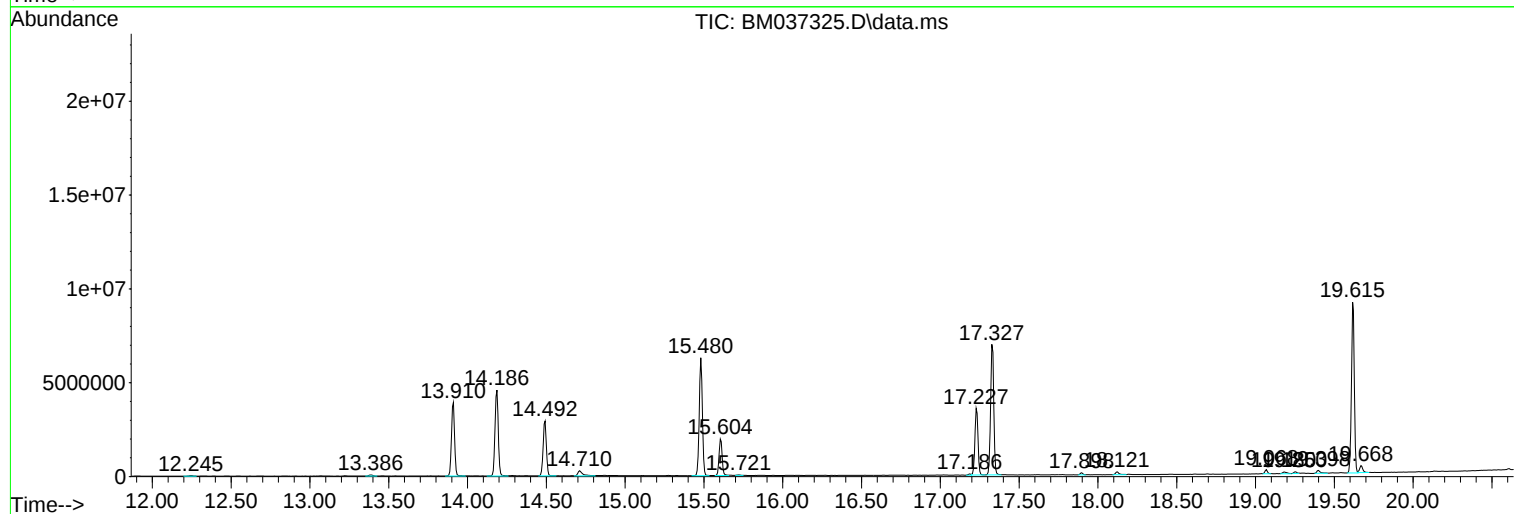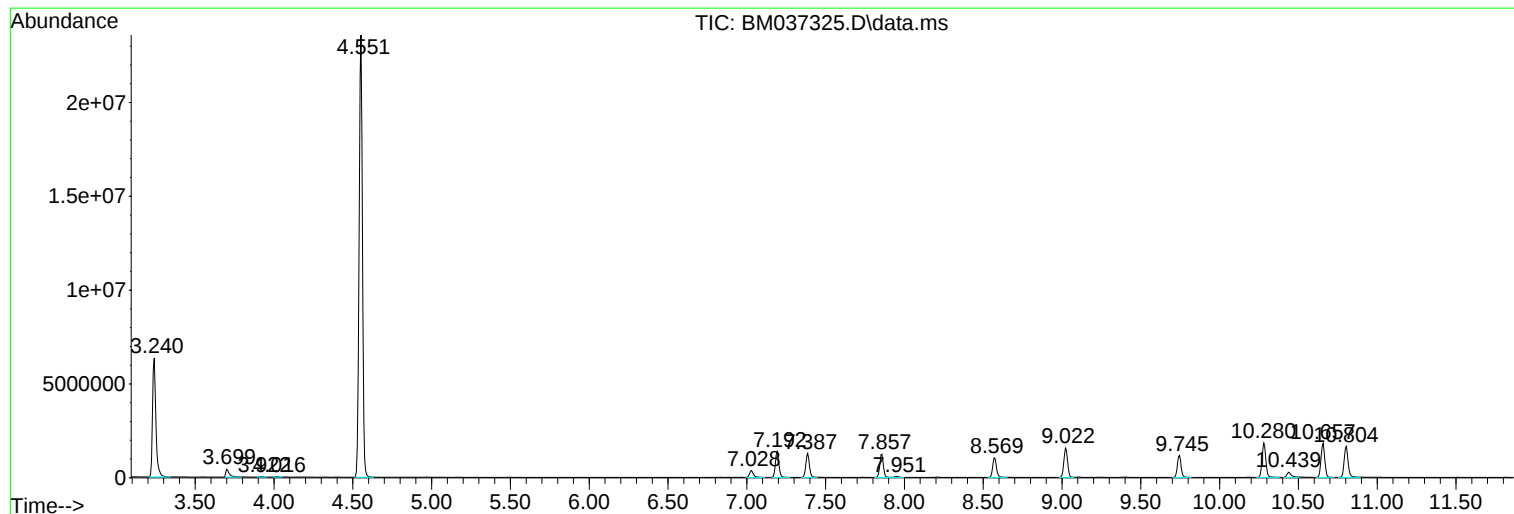

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037325.D
Acq On : 02 Nov 2022 20:29
Operator : CG/JU
Sample : N5301-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBXB4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.439	3.60 ng/ul	534463	Naphthalene-d8	10.657

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	86
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	86
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	78

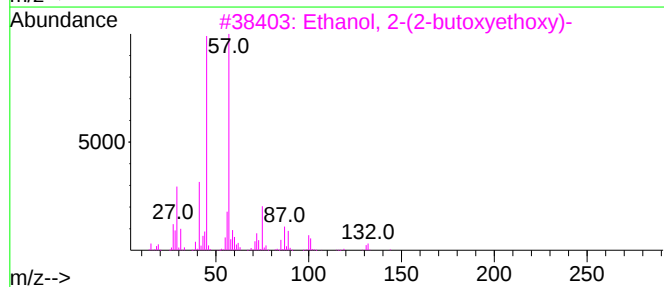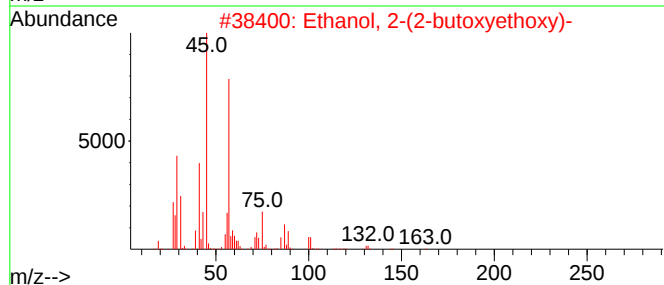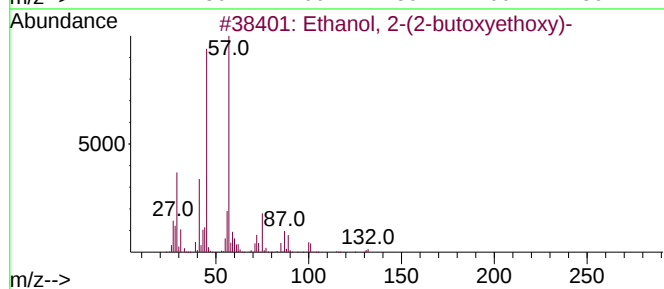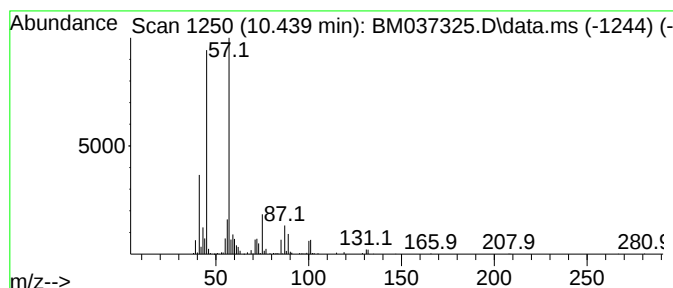

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037325.D
Acq On : 02 Nov 2022 20:29
Operator : CG/JU
Sample : N5301-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBXB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.439	3.6	ng/u1	534463	2	10.657	2971220	20.0