

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
 Data File : BM037332.D
 Acq On : 03 Nov 2022 00:38
 Operator : CG/JU
 Sample : N5321-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBWW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037332.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	20	26	49	rVB	6579404	9876333	73.84%	8.929%
2	3.699	102	104	119	rBV	453285	717227	5.36%	0.648%
3	3.922	138	142	147	rVB2	27569	44448	0.33%	0.040%
4	4.016	155	158	163	rVB	28502	35364	0.26%	0.032%
5	4.546	242	248	263	rBV	9214907	13375592	100.00%	12.093%
6	6.281	538	543	546	rBV4	10197	15469	0.12%	0.014%
7	7.028	664	670	677	rBV	331274	553685	4.14%	0.501%
8	7.093	677	681	688	rVB	85703	141782	1.06%	0.128%
9	7.192	691	698	710	rBV	1360315	2118438	15.84%	1.915%
10	7.387	722	731	741	rBV	1273636	2007854	15.01%	1.815%
11	7.851	797	810	819	rBV	1176841	1843141	13.78%	1.666%
12	7.951	819	827	834	rVB5	60406	120292	0.90%	0.109%
13	8.569	926	932	944	rBV	751889	1272154	9.51%	1.150%
14	9.022	1002	1009	1017	rBV	1620837	2569031	19.21%	2.323%
15	9.086	1017	1020	1027	rVB7	15043	33818	0.25%	0.031%
16	9.245	1042	1047	1054	rVB6	9112	17908	0.13%	0.016%
17	9.404	1064	1074	1080	rVB	29398	59198	0.44%	0.054%
18	9.739	1123	1131	1143	rBV	1263283	2100720	15.71%	1.899%
19	10.281	1214	1223	1236	rBV	1860565	3122074	23.34%	2.823%
20	10.651	1278	1286	1296	rBV	1689892	2803409	20.96%	2.535%
21	10.804	1305	1312	1332	rBV	802948	1498149	11.20%	1.354%
22	11.480	1419	1427	1429	rBV8	13198	30558	0.23%	0.028%
23	11.639	1448	1454	1460	rBV9	12387	24615	0.18%	0.022%
24	11.898	1491	1498	1507	rVB2	18682	41357	0.31%	0.037%
25	12.245	1550	1557	1564	rBV	32802	57197	0.43%	0.052%
26	12.469	1588	1595	1602	rBV10	11055	32063	0.24%	0.029%
27	12.845	1653	1659	1662	rBV7	8592	14230	0.11%	0.013%
28	13.092	1698	1701	1709	rVB9	8617	17631	0.13%	0.016%
29	13.222	1719	1723	1728	rBV8	14595	21866	0.16%	0.020%
30	13.304	1734	1737	1745	rVV7	17517	32152	0.24%	0.029%
31	13.392	1746	1752	1757	rVV9	13881	34121	0.26%	0.031%
32	13.457	1760	1763	1770	rVV7	12122	24468	0.18%	0.022%
33	13.698	1800	1804	1809	rBV5	16440	30899	0.23%	0.028%
34	13.910	1832	1840	1846	rBV	3910720	5409037	40.44%	4.890%
35	14.180	1876	1886	1899	rBV	4781625	6847019	51.19%	6.190%
36	14.280	1900	1903	1908	rVB6	16686	23656	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
 Data File : BM037332.D
 Acq On : 03 Nov 2022 00:38
 Operator : CG/JU
 Sample : N5321-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBWW1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	14.486	1931	1938	1945	rBV	2782937	3967392	29.66%	3.587%
38	14.710	1970	1976	1989	rBV	208122	468286	3.50%	0.423%
39	15.233	2059	2065	2069	rBV	35179	57077	0.43%	0.052%
40	15.315	2075	2079	2084	rVB2	24097	38917	0.29%	0.035%
41	15.480	2100	2107	2113	rBV	6099459	8614357	64.40%	7.788%
42	15.527	2113	2115	2122	rVB5	34902	49542	0.37%	0.045%
43	15.604	2122	2128	2142	rBV	1957599	2586696	19.34%	2.339%
44	15.715	2143	2147	2152	rVB2	31081	45070	0.34%	0.041%
45	15.845	2165	2169	2171	rBV5	10355	13463	0.10%	0.012%
46	16.004	2192	2196	2202	rBV3	28466	46140	0.34%	0.042%
47	16.457	2268	2273	2278	rBV	72451	102370	0.77%	0.093%
48	16.515	2279	2283	2289	rVB	25109	40203	0.30%	0.036%
49	16.768	2323	2326	2332	rVB3	13789	21132	0.16%	0.019%
50	17.039	2367	2372	2379	rVB	165857	229840	1.72%	0.208%
51	17.186	2393	2397	2398	rBV	41285	46572	0.35%	0.042%
52	17.227	2398	2404	2414	rVB	3206762	4360888	32.60%	3.943%
53	17.327	2414	2421	2432	rBV	5972008	8246179	61.65%	7.455%
54	17.592	2462	2466	2475	rBV4	27806	68133	0.51%	0.062%
55	18.121	2551	2556	2564	rBV	192101	326765	2.44%	0.295%
56	19.180	2732	2736	2740	rBV2	80201	103035	0.77%	0.093%
57	19.251	2744	2748	2751	rBV	97548	138912	1.04%	0.126%
58	19.398	2769	2773	2783	rBV2	163000	269292	2.01%	0.243%
59	19.615	2804	2810	2817	rBV	7145972	9011770	67.37%	8.148%
60	21.397	3108	3113	3119	rBV	3219293	3834555	28.67%	3.467%
61	23.591	3480	3486	3498	rVB2	3851296	7511799	56.16%	6.791%
62	23.744	3506	3512	3522	rVB2	1732355	3440745	25.72%	3.111%




Sum of corrected areas: 110606085

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037332.D
Acq On : 03 Nov 2022 00:38
Operator : CG/JU
Sample : N5321-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBWW1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

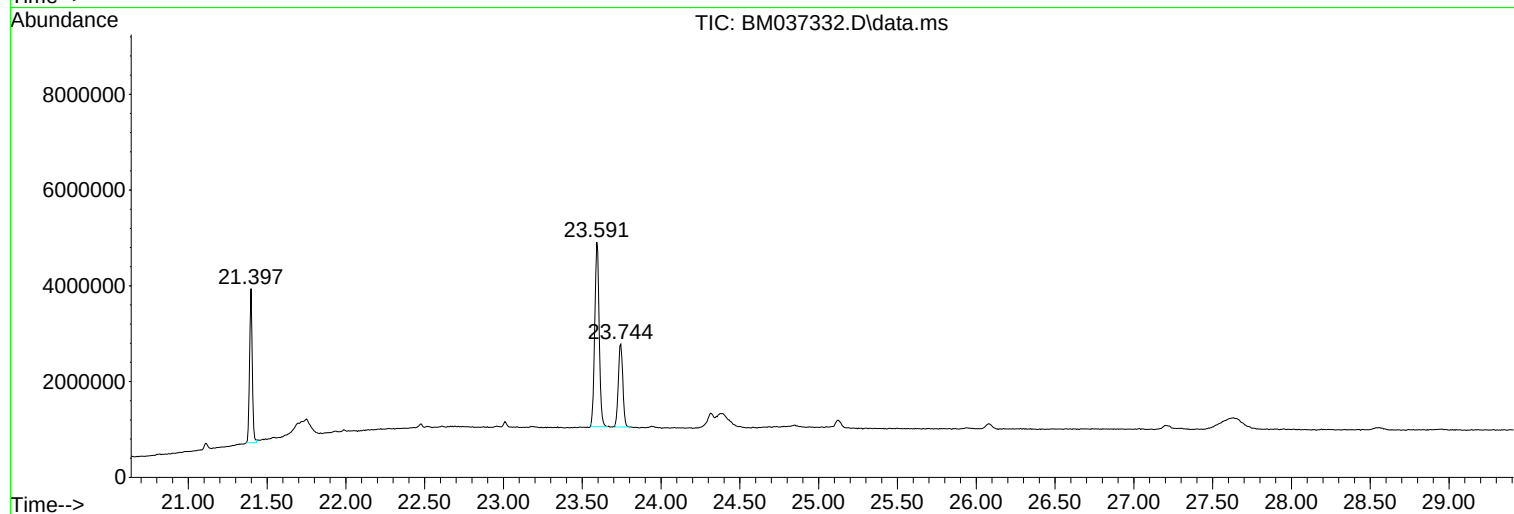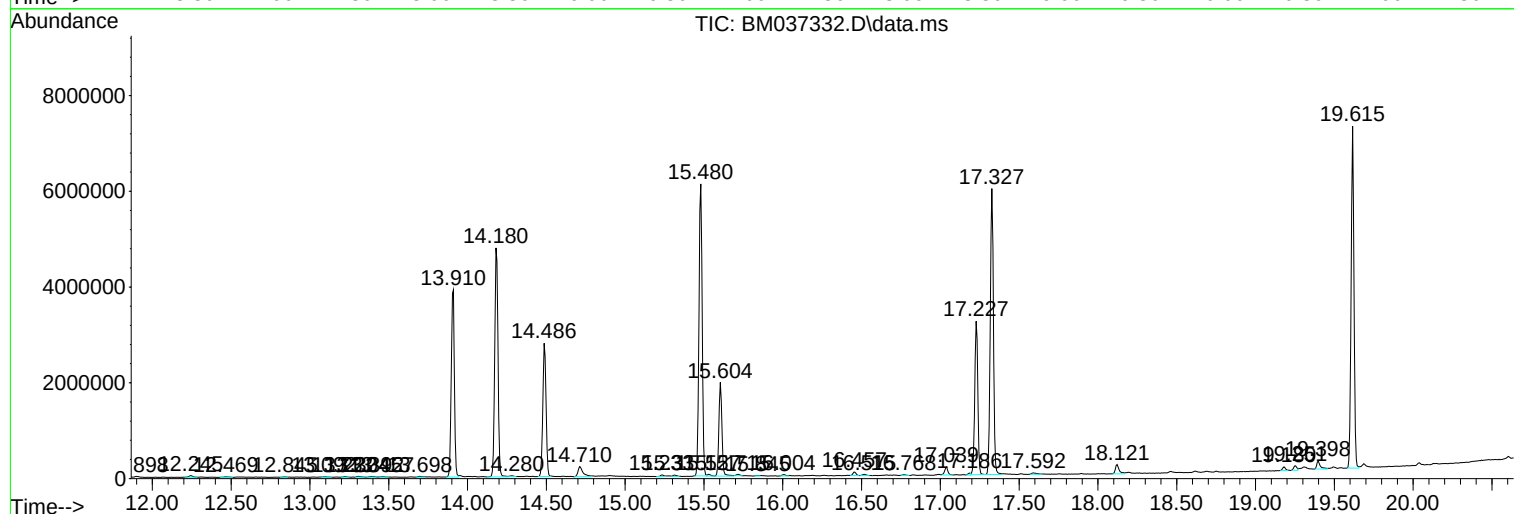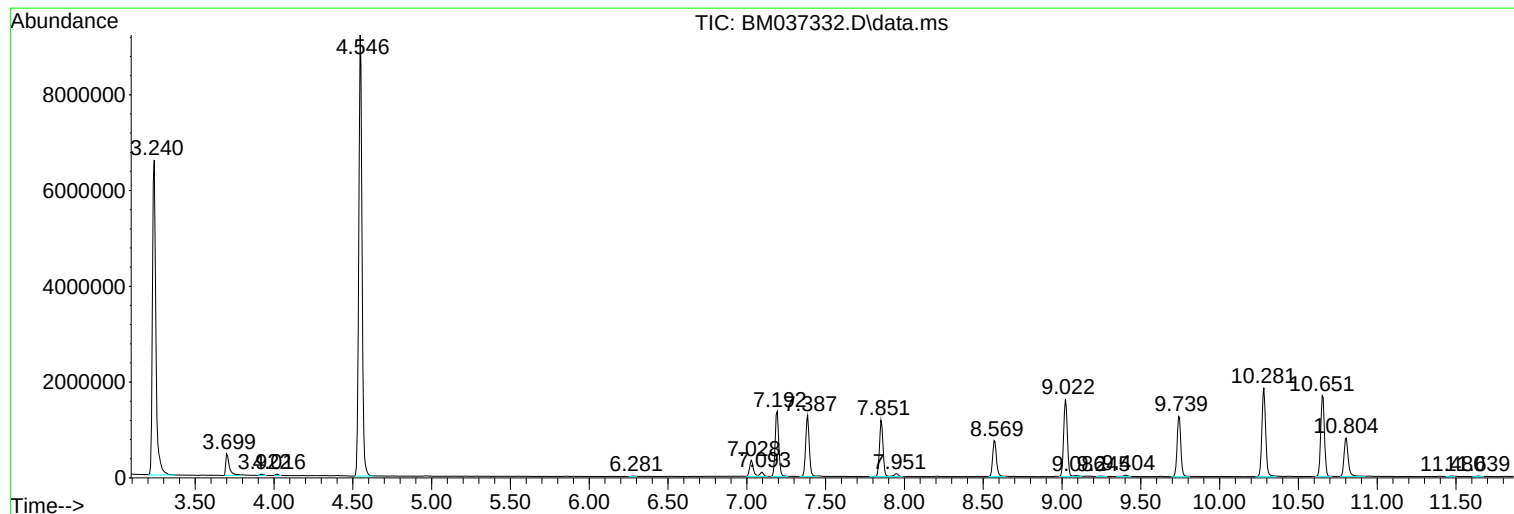

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037332.D
Acq On : 03 Nov 2022 00:38
Operator : CG/JU
Sample : N5321-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBWW1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037332.D
Acq On : 03 Nov 2022 00:38
Operator : CG/JU
Sample : N5321-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBWW1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc