

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
 Data File : BM037333.D
 Acq On : 03 Nov 2022 01:14
 Operator : CG/JU
 Sample : N5321-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBWW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037333.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	20	26	43	rVB	5175533	7683560	50.55%	6.936%
2	3.699	101	104	122	rBV	454437	711178	4.68%	0.642%
3	3.922	137	142	147	rVB	24336	36661	0.24%	0.033%
4	4.016	155	158	164	rVB	30451	41338	0.27%	0.037%
5	4.546	242	248	263	rBV	10606690	15199233	100.00%	13.721%
6	4.969	315	320	326	rVB5	9678	16632	0.11%	0.015%
7	5.216	356	362	367	rBV6	19420	30723	0.20%	0.028%
8	7.028	664	670	678	rBV	284213	484481	3.19%	0.437%
9	7.093	678	681	688	rVB	72695	116980	0.77%	0.106%
10	7.193	691	698	709	rBV	1183601	1847462	12.15%	1.668%
11	7.387	724	731	742	rBV	1093767	1727638	11.37%	1.560%
12	7.851	803	810	819	rBV	1402662	2181195	14.35%	1.969%
13	7.957	822	828	836	rVB	14336	34393	0.23%	0.031%
14	8.569	924	932	943	rBV	818370	1353833	8.91%	1.222%
15	9.022	1002	1009	1018	rBV	1412025	2234007	14.70%	2.017%
16	9.404	1065	1074	1081	rVB2	17849	42469	0.28%	0.038%
17	9.740	1123	1131	1143	rBV	1056096	1770873	11.65%	1.599%
18	10.281	1215	1223	1238	rBV	1667930	2858206	18.80%	2.580%
19	10.651	1278	1286	1295	rBV	1962172	3290107	21.65%	2.970%
20	10.804	1303	1312	1333	rBV	1160377	2124840	13.98%	1.918%
21	10.951	1333	1337	1342	rVB6	10742	19525	0.13%	0.018%
22	11.898	1490	1498	1504	rBV8	8320	18255	0.12%	0.016%
23	12.245	1549	1557	1562	rBV	28645	51123	0.34%	0.046%
24	13.110	1697	1704	1710	rVB7	6538	17154	0.11%	0.015%
25	13.316	1734	1739	1745	rVB6	16970	36876	0.24%	0.033%
26	13.386	1745	1751	1757	rVB7	11396	16409	0.11%	0.015%
27	13.910	1831	1840	1854	rBV	3529603	4929476	32.43%	4.450%
28	14.180	1876	1886	1899	rBV	4126853	6094284	40.10%	5.501%
29	14.486	1931	1938	1947	rBV	3126392	4496944	29.59%	4.059%
30	14.710	1970	1976	1990	rBV	181084	416531	2.74%	0.376%
31	14.904	2005	2009	2010	rBV3	14325	15260	0.10%	0.014%
32	15.322	2078	2080	2089	rVB3	16835	24516	0.16%	0.022%
33	15.480	2100	2107	2114	rBV	5787362	7805610	51.36%	7.046%
34	15.604	2122	2128	2140	rBV	1781041	2340671	15.40%	2.113%
35	15.716	2143	2147	2154	rVB4	31524	55315	0.36%	0.050%
36	16.004	2192	2196	2201	rBV2	18851	28013	0.18%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
 Data File : BM037333.D
 Acq On : 03 Nov 2022 01:14
 Operator : CG/JU
 Sample : N5321-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBWW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	16.457	2268	2273	2278	rBV	150498	205414	1.35%	0.185%
38	16.516	2279	2283	2287	rVV	42564	57904	0.38%	0.052%
39	17.227	2398	2404	2412	rBV	3850175	4968994	32.69%	4.486%
40	17.327	2415	2421	2432	rVV	6136339	8407909	55.32%	7.590%
41	18.121	2551	2556	2566	rBV	276286	451193	2.97%	0.407%
42	19.180	2733	2736	2741	rVB	71595	94678	0.62%	0.085%
43	19.251	2745	2748	2752	rBV	85722	106381	0.70%	0.096%
44	19.398	2769	2773	2782	rBV	246767	373195	2.46%	0.337%
45	19.615	2804	2810	2818	rBV	7487573	9369460	61.64%	8.458%
46	21.109	3061	3064	3070	rBV	253303	373096	2.45%	0.337%
47	21.398	3108	3113	3118	rBV	3840188	4688305	30.85%	4.232%
48	23.592	3480	3486	3499	rVB2	3779571	7470430	49.15%	6.744%
49	23.745	3506	3512	3521	rVB2	2166933	4058378	26.70%	3.664%




Sum of corrected areas: 110777108

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037333.D
Acq On : 03 Nov 2022 01:14
Operator : CG/JU
Sample : N5321-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBWW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

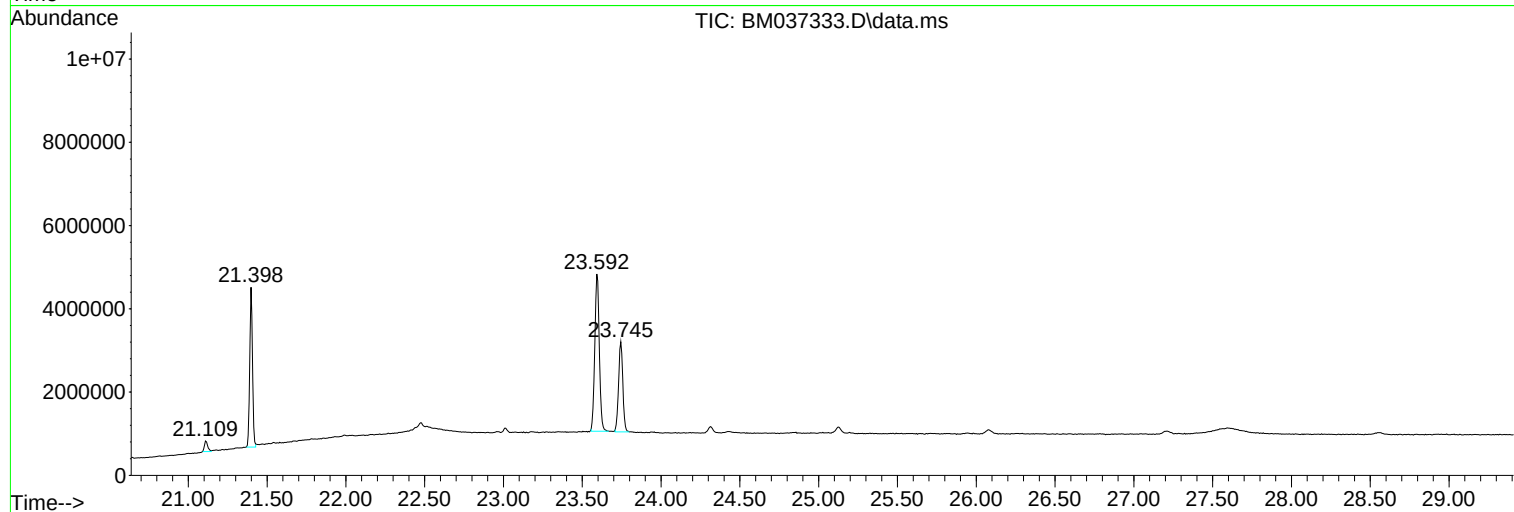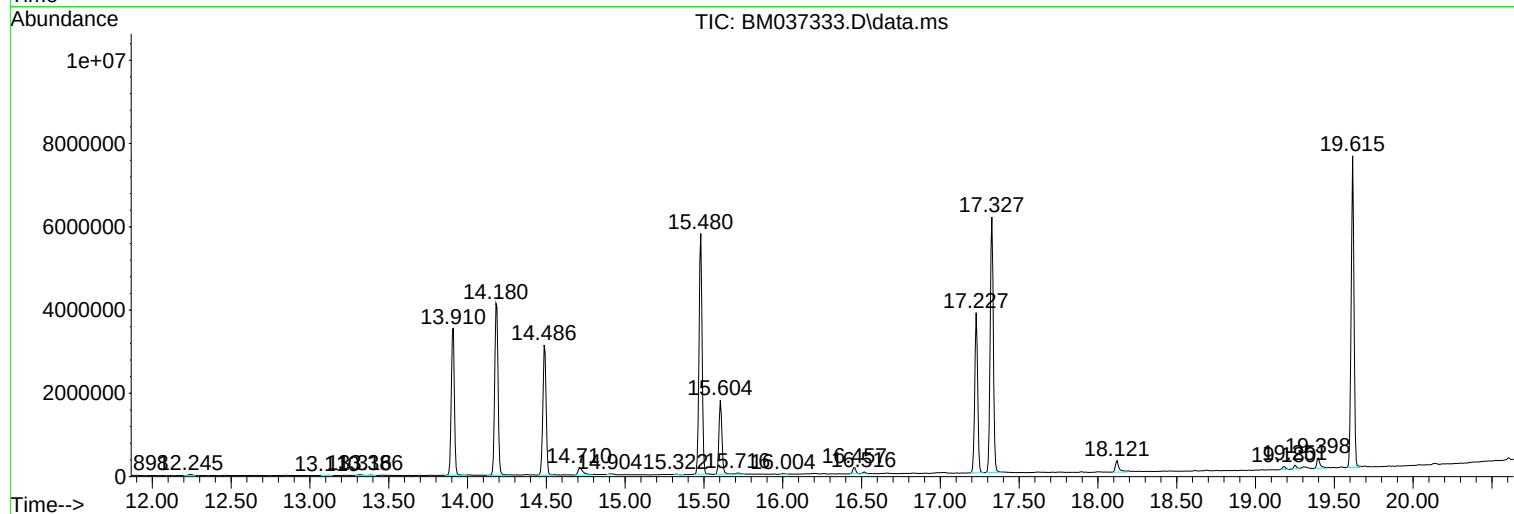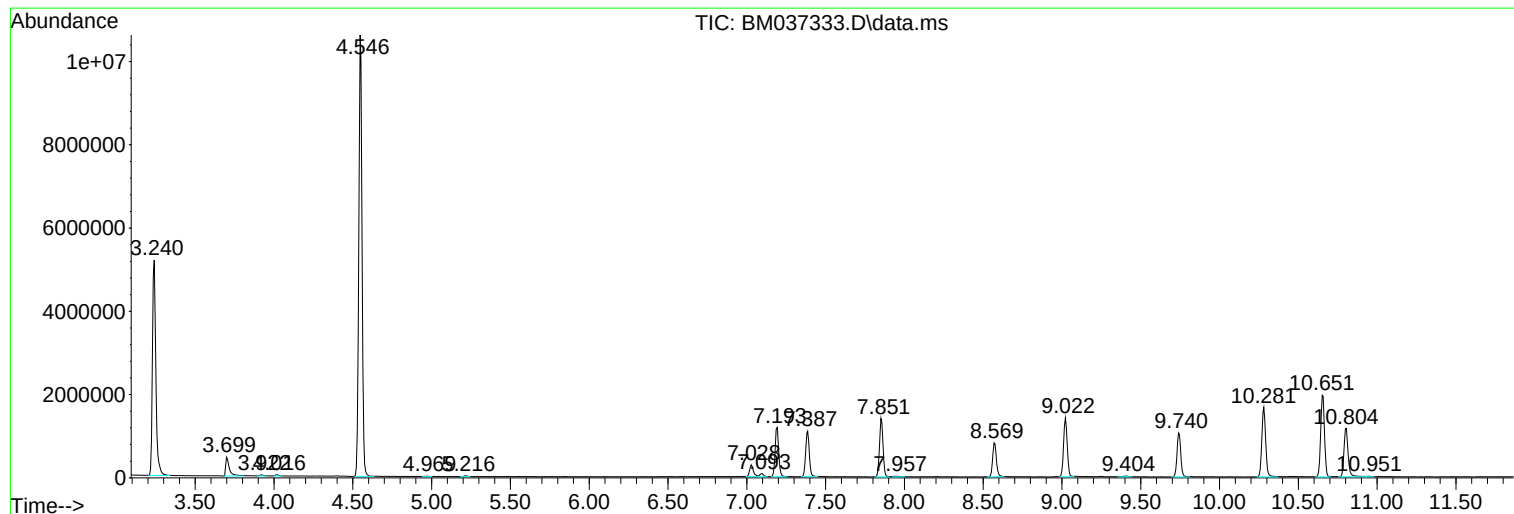

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037333.D
Acq On : 03 Nov 2022 01:14
Operator : CG/JU
Sample : N5321-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBWW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110222\
Data File : BM037333.D
Acq On : 03 Nov 2022 01:14
Operator : CG/JU
Sample : N5321-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBWW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
