

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111020\
 Data File : BM027774.D
 Acq On : 10 Nov 2020 17:40
 Operator : JU/CG
 Sample : PB132888BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK88

Quant Time: Nov 11 01:21:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 15:45:47 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.39	152	549	0.40	ng/ul	0.00
2) Naphthalene-d8	11.22	136	2006	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.00	164	1563	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.81	240	2992	0.40	ng/ul	0.00
20) Perylene-d12	24.25	264	2720	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.78	152	1146	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	2967	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.06	202	497	0.037	ng/ul#	1
23) Benzo(a)pyrene	24.09	252	1053	0.096	ng/ul#	28


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111020\
Data File : BM027774.D
Acq On : 10 Nov 2020 17:40
Operator : JU/CG
Sample : PB132888BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK88

Quant Time: Nov 11 01:21:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 15:45:47 2020
Response via : Initial Calibration

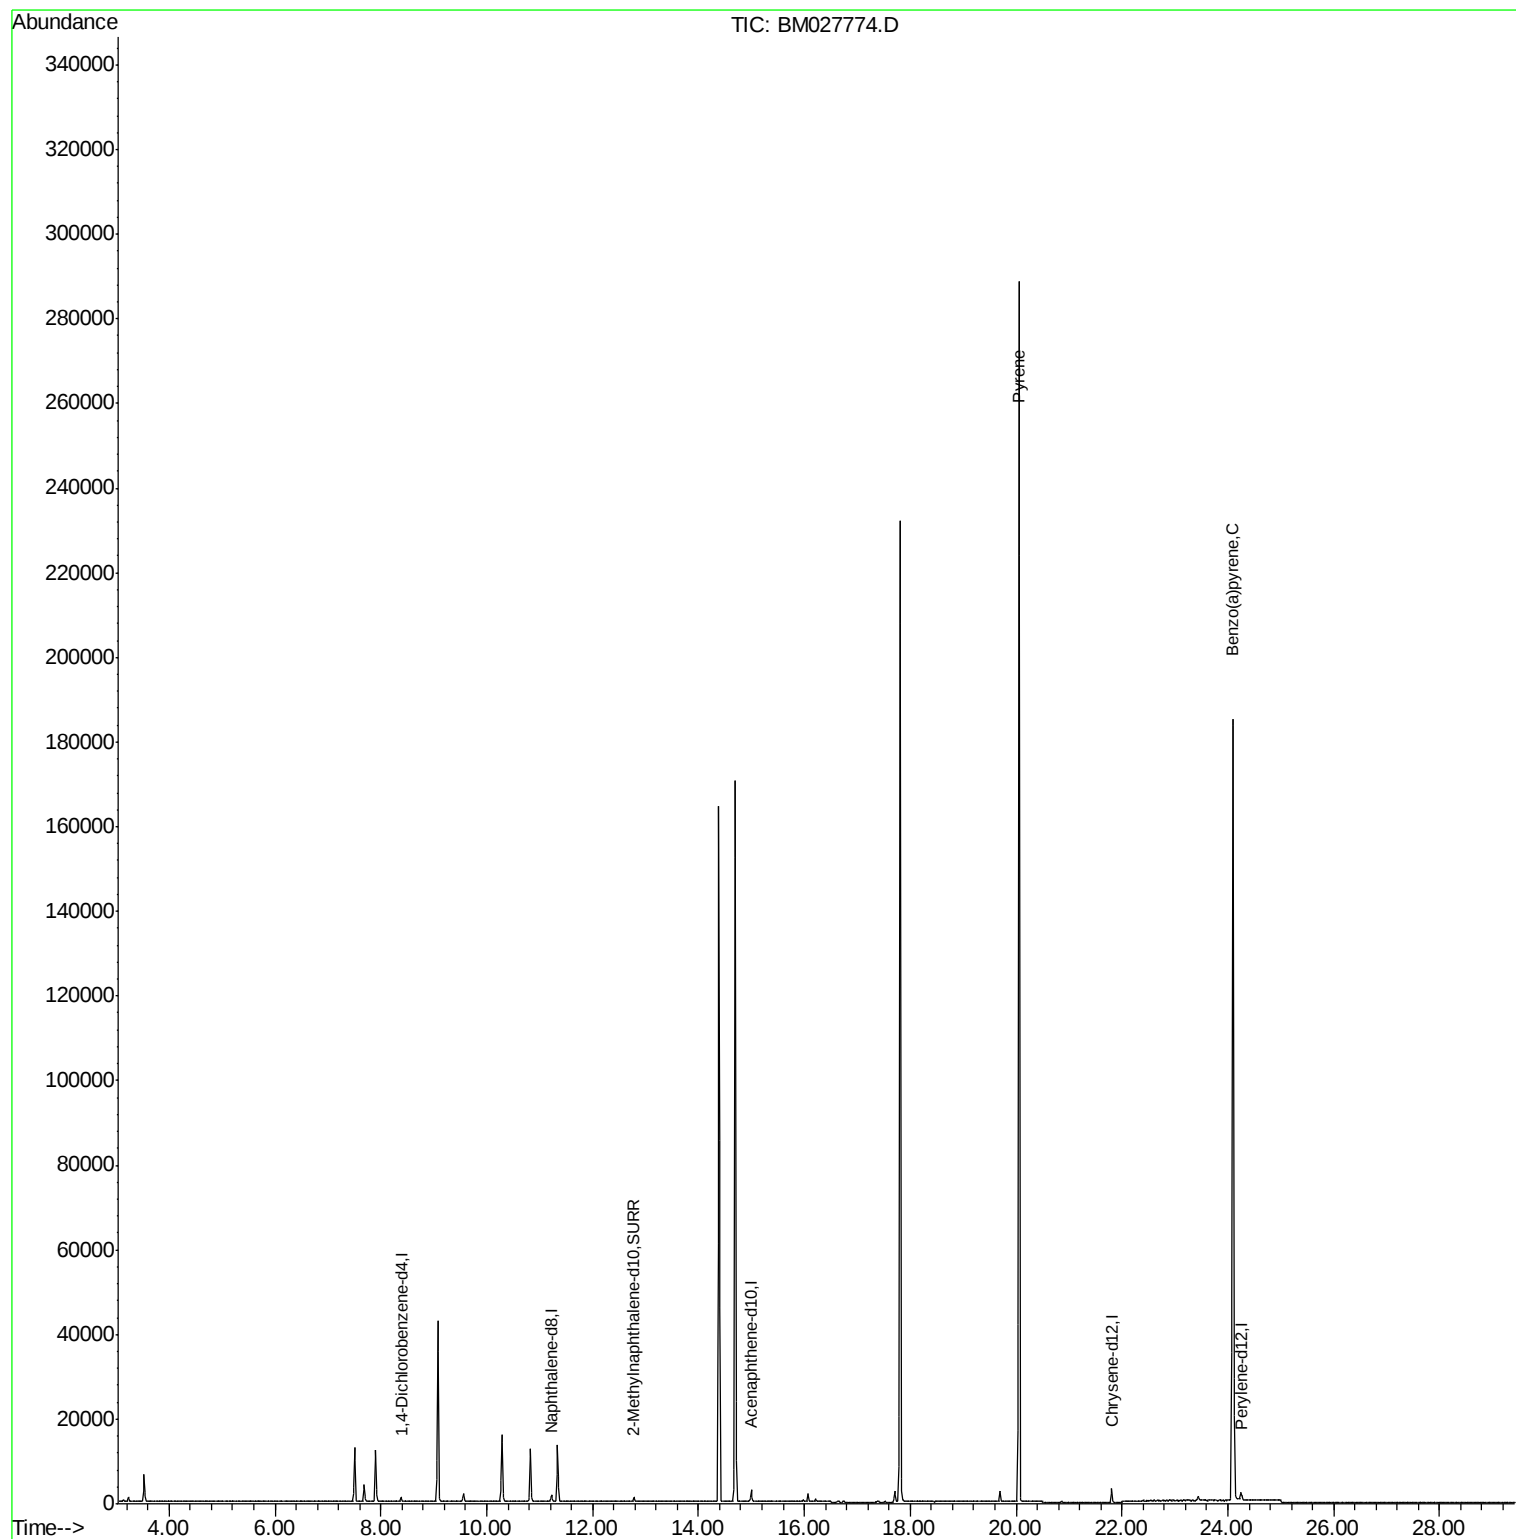

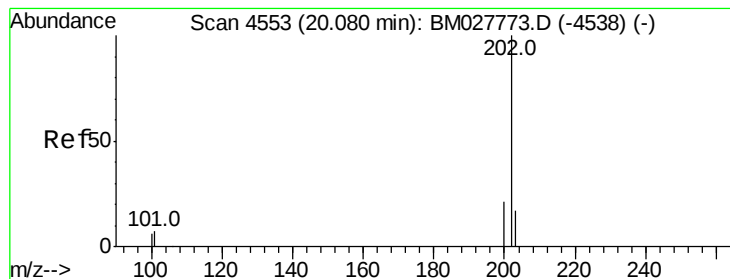

#17

Pvrene

Concen: 0.037 ng/ul

RT: 20.06 min Scan# 4547

Delta R.T. -0.02 min

Lab File: BM027774.D

Acq: 10 Nov 2020 17:40

Instrument :

BNA_M

ClientSampleId :

SBLK88


Tot Ion:202 Resp: 497

Ion Ratio Lower Upper

202 100

101 236.3 6.4 9.6#




100 1691.6 5.8 8.6#

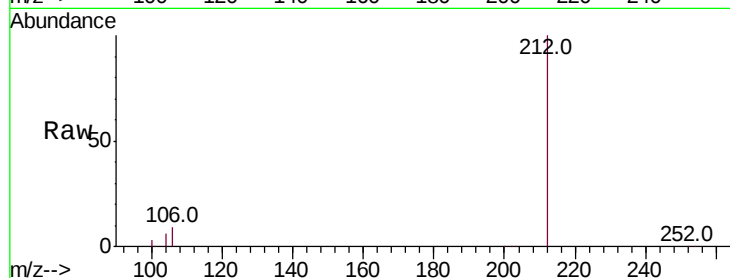

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

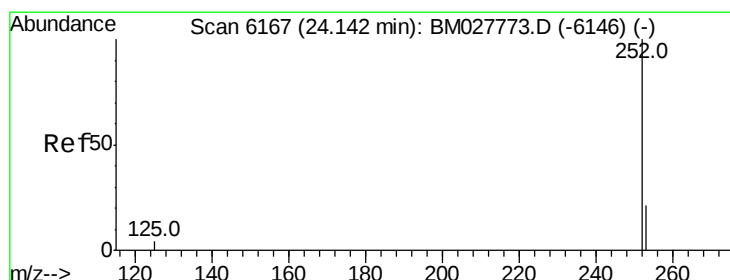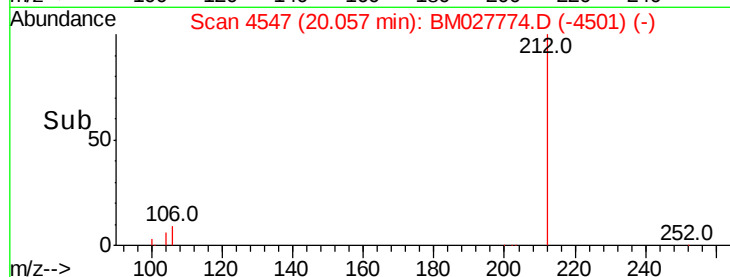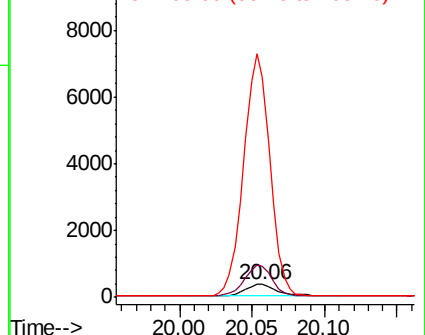

#23

Benzo(a)pyrene

Concen: 0.096 ng/ul

RT: 24.09 min Scan# 6147

Delta R.T. -0.05 min

Lab File: BM027774.D

Acq: 10 Nov 2020 17:40


Tgt Ion:252 Resp: 1053

Ion Ratio Lower Upper

252 100

253 47.9 21.0 31.6#

125 66.1 7.8 11.8#

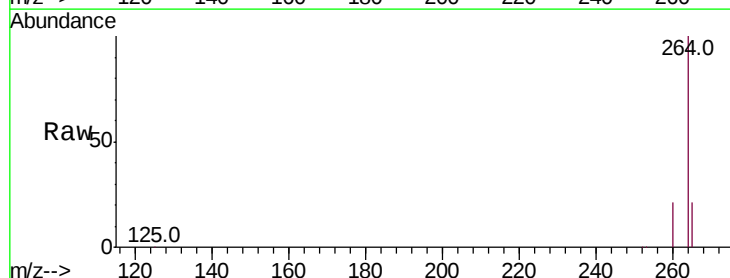

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

