




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111020\
 Data File : BM027778.D
 Acq On : 10 Nov 2020 20:06
 Operator : JU/CG
 Sample : L4661-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R02

Manual Integrations
 APPROVED

mohammad
 11/11/2020 10:33:20 AM

Quant Time: Nov 11 01:21:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 11 01:20:37 2020
 Response via : Initial Calibration

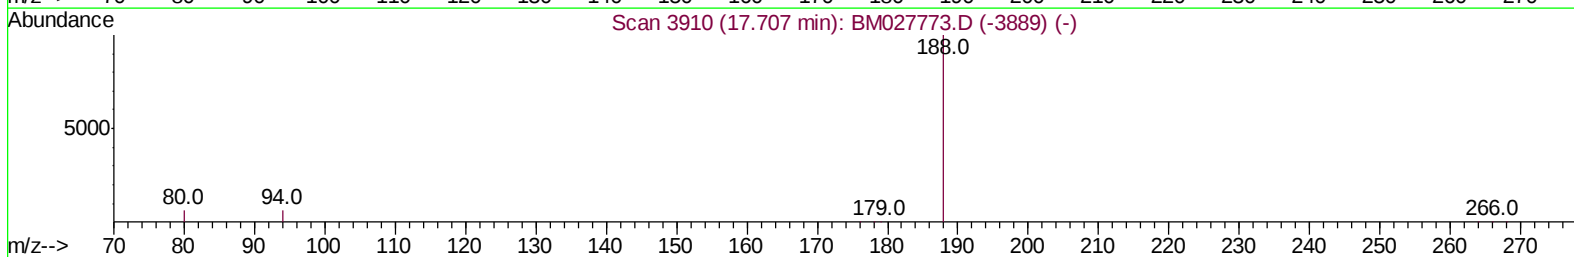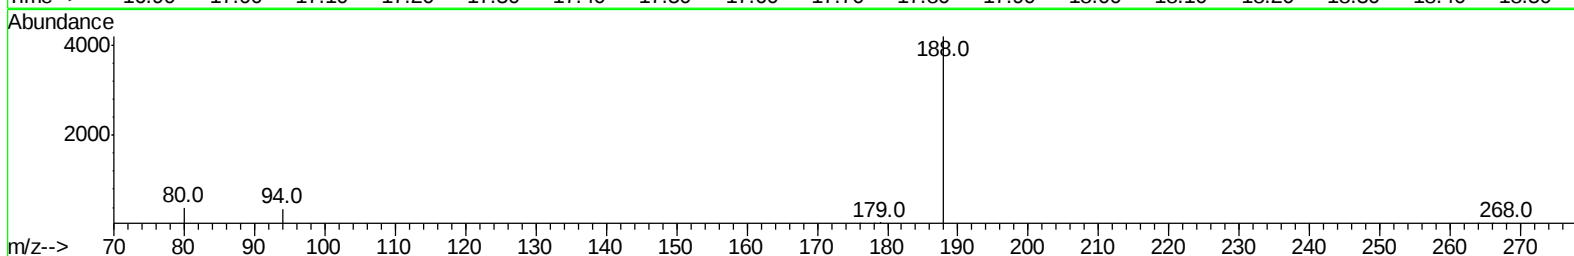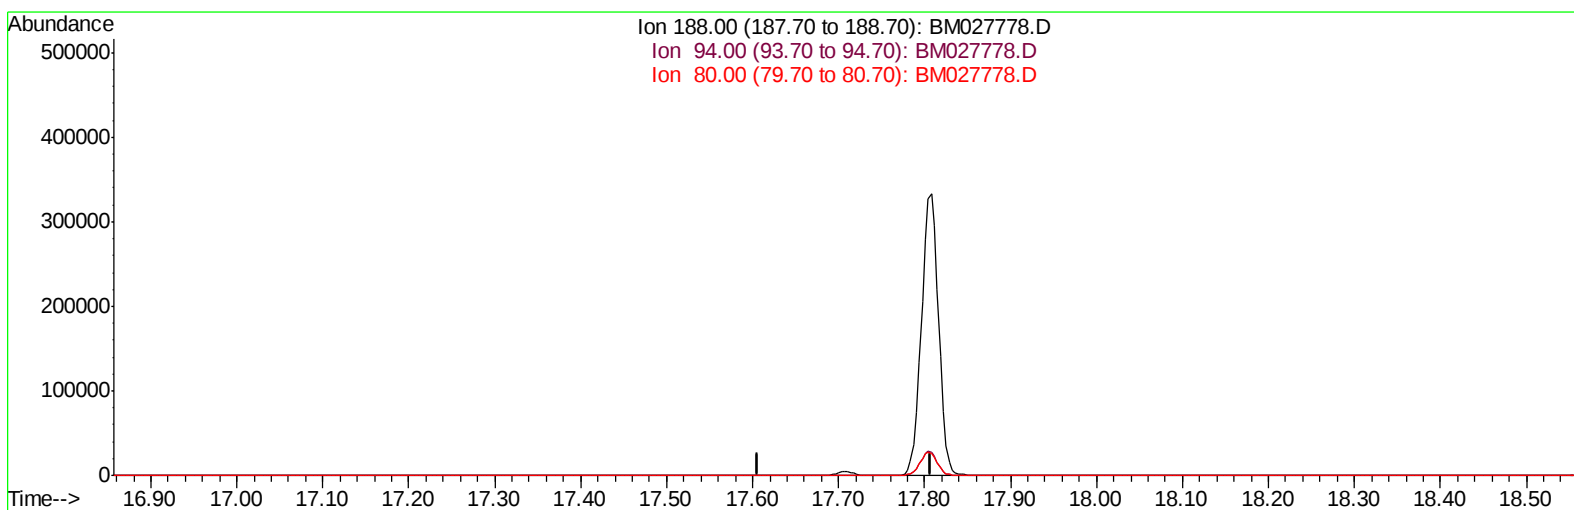

TIC: BM027778.D

(10) Phenanthrene-d10 (I)

17.707min (-17.707) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	9.00	0.00#
80.00	9.60	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111020\
 Data File : BM027778.D
 Acq On : 10 Nov 2020 20:06
 Operator : JU/CG
 Sample : L4661-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R02

Manual Integrations
 APPROVED

mohammad
 11/11/2020 10:33:20 AM

Quant Time: Nov 11 01:21:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 11 01:20:37 2020
 Response via : Initial Calibration

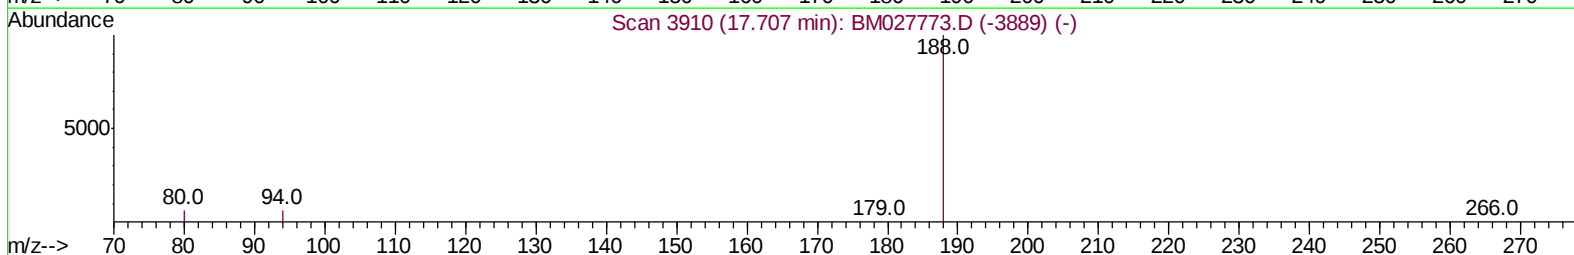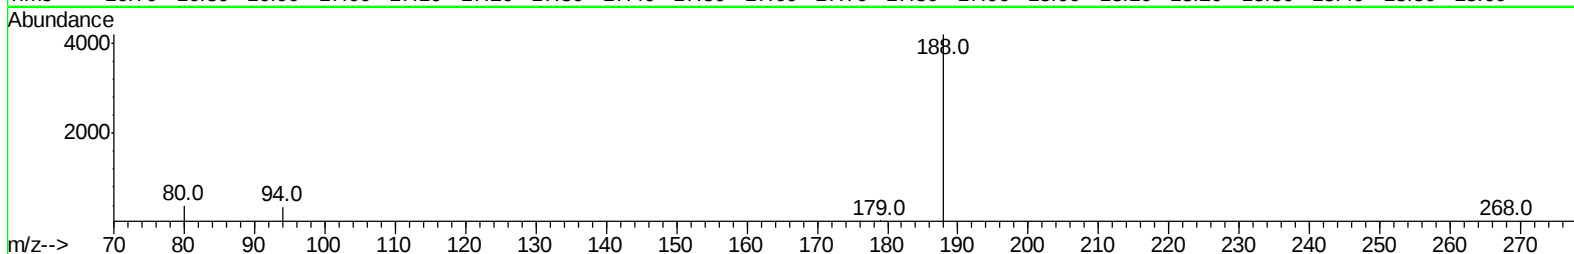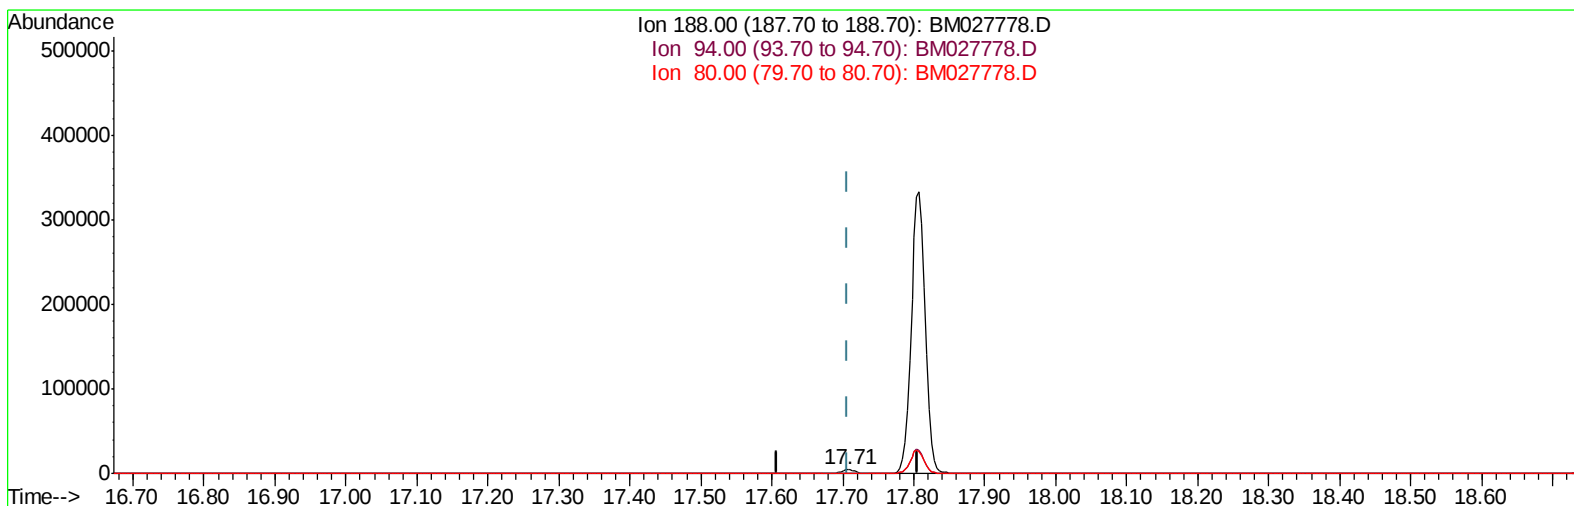

TIC: BM027778.D

(10) Phenanthrene-d10 (I)

17.707min (+0.000) 0.40ng/ul m

response 5730

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	8.63
80.00	9.60	9.61
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111020\
 Data File : BM027778.D
 Acq On : 10 Nov 2020 20:06
 Operator : JU/CG
 Sample : L4661-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R02

Manual Integrations
 APPROVED

mohammad
 11/11/2020 10:33:20 AM

Quant Time: Nov 11 01:33:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 11 01:20:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.39	152	1161	0.40	ng/ul	0.00
2) Naphthalene-d8	11.22	136	4468	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.99	164	2876	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	5730m	0.40	ng/ul	0.00
16) Chrysene-d12	21.81	240	4644	0.40	ng/ul	0.00
20) Perylene-d12	24.25	264	3975	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.79	152	2096	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	5393	0.32	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111020\
Data File : BM027778.D
Acq On : 10 Nov 2020 20:06
Operator : JU/CG
Sample : L4661-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F4R02

Manual Integrations
APPROVED

mohammad
11/11/2020 10:33:20 AM

Quant Time: Nov 11 01:33:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 11 01:20:37 2020
Response via : Initial Calibration

