




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111020\
 Data File : BM027780.D
 Acq On : 10 Nov 2020 21:19
 Operator : JU/CG
 Sample : L4661-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R01

Manual Integrations
 APPROVED

mohammad
 11/11/2020 10:33:25 AM

Quant Time: Nov 11 01:21:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 11 01:20:37 2020
 Response via : Initial Calibration

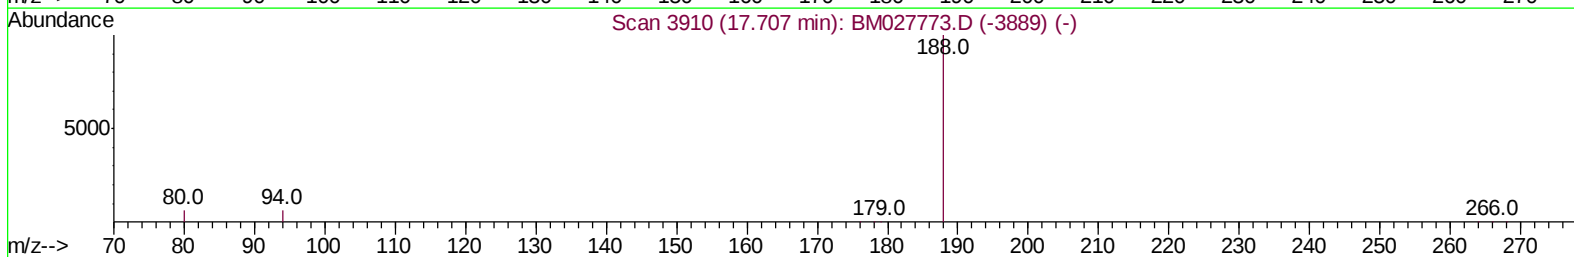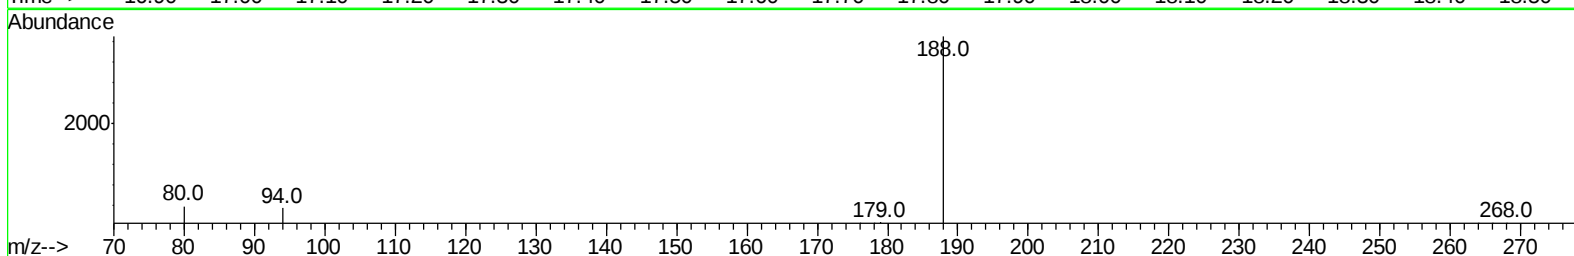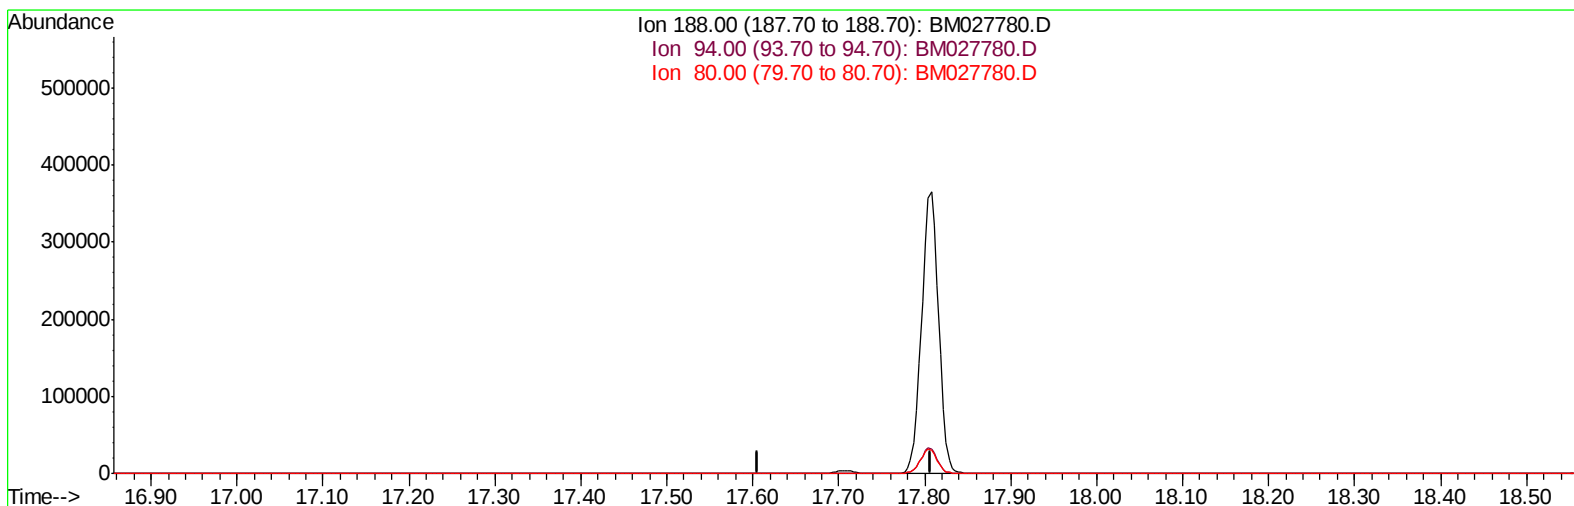

TIC: BM027780.D

(10) Phenanthrene-d10 (I)

17.707min (-17.707) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	9.00	0.00#
80.00	9.60	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111020\
Data File : BM027780.D
Acq On : 10 Nov 2020 21:19
Operator : JU/CG
Sample : L4661-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F4R01

Manual Integrations
APPROVED

mohammad
11/11/2020 10:33:25 AM

Quant Time: Nov 11 01:21:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 11 01:20:37 2020
Response via : Initial Calibration

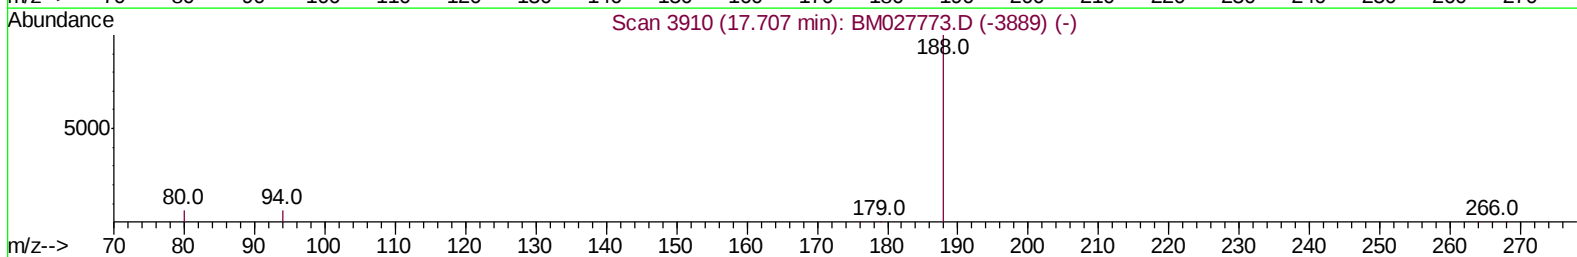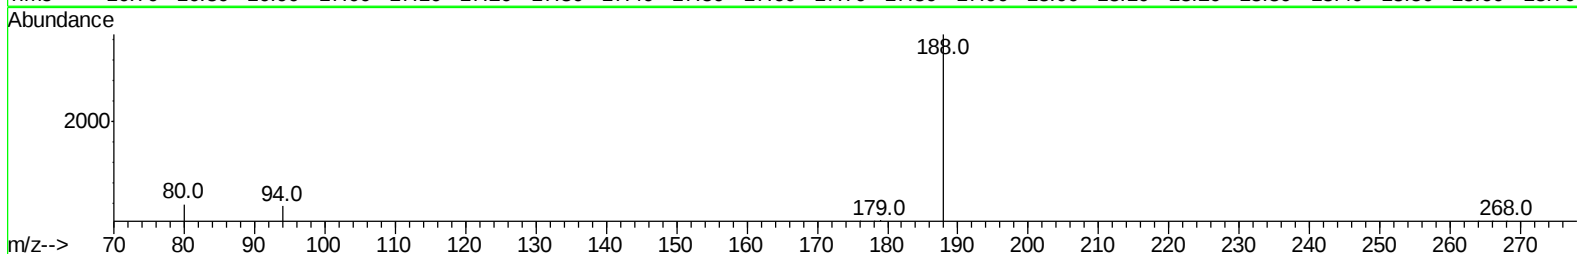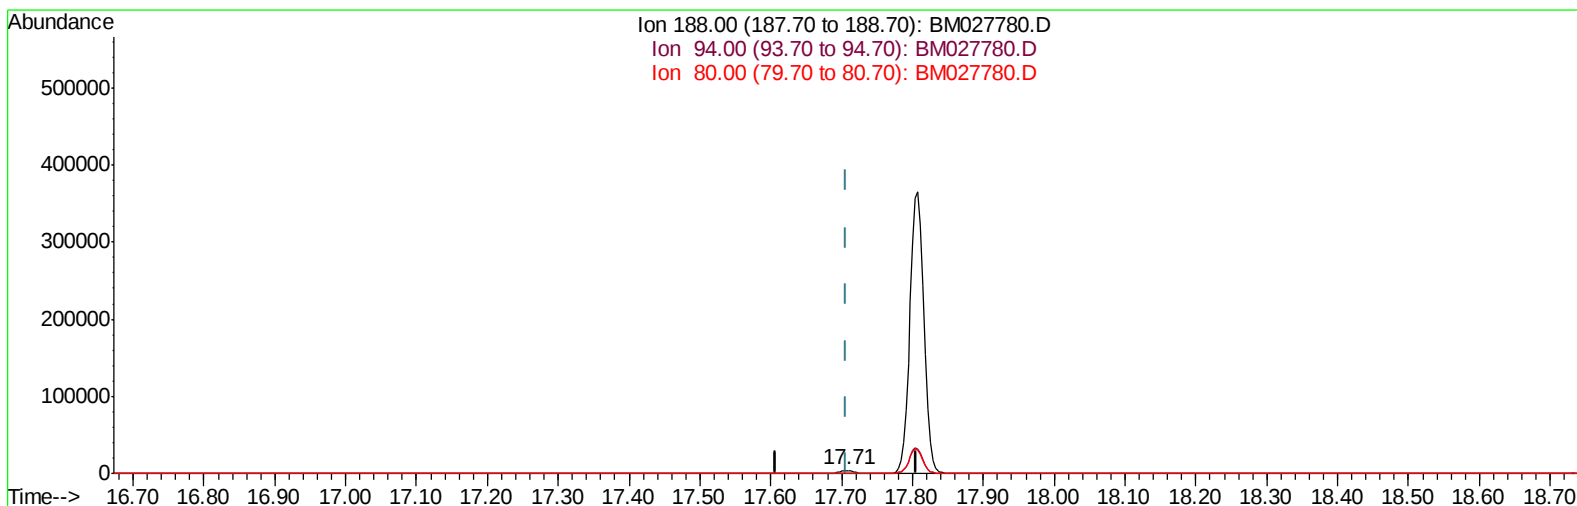

TIC: BM027780.D

(10) Phenanthrene-d10 (I)

17.707min (-0.000) 0.40ng/ul m

response 5053

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	9.34
80.00	9.60	10.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM111120\
 Data File : BM027784.D
 Acq On : 11 Nov 2020 10:47
 Operator : JU/CG
 Sample : PB132888BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R01

Manual Integrations
 APPROVED

mohammad
 11/11/2020 10:33:25 AM

Quant Time: Nov 11 11:33:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 11 11:32:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	586	0.40	ng/ul	0.00
2) Naphthalene-d8	11.22	136	2244	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.99	164	1741	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.81	240	2973	0.40	ng/ul	0.00
20) Perylene-d12	24.25	264	2634	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.78	152	1553	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	3720	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.05	202	577	0.044	ng/ul#	1
23) Benzo(a)pyrene	24.09	252	1254	0.118	ng/ul#	42

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM111120\
Data File : BM027784.D
Acq On : 11 Nov 2020 10:47
Operator : JU/CG
Sample : PB132888BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F4R01

Quant Time: Nov 11 11:33:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 11 11:32:20 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
11/11/2020 10:33:25 AM

