
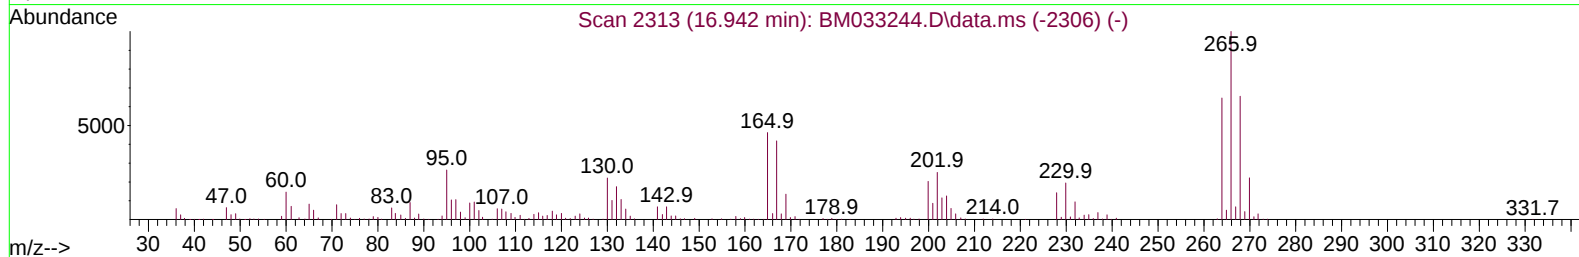
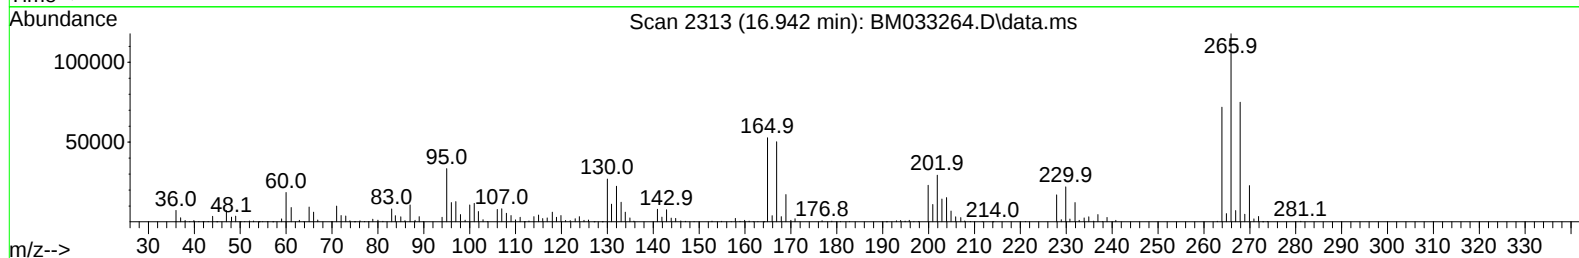


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112621\
Data File : BM033264.D
Acq On : 26 Nov 2021 14:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 17:24:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 24 15:16:33 2021
Response via : Initial Calibration

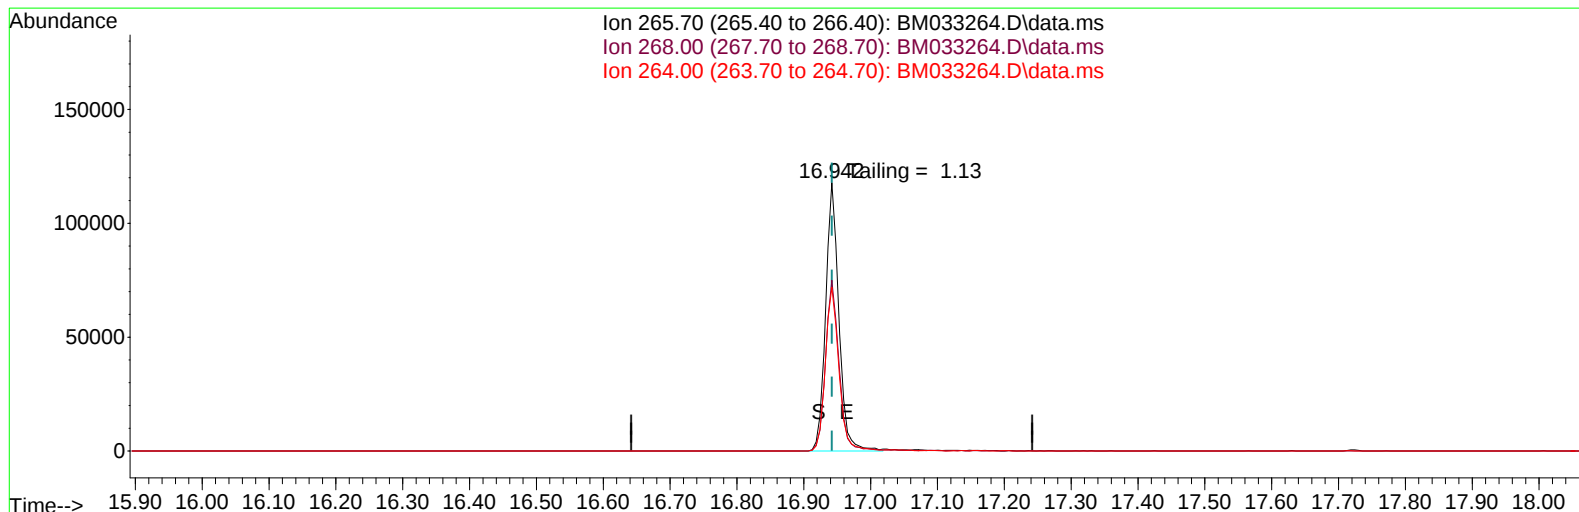

TIC: BM033264.D\data.ms

(70) Pentachlorophenol (C)




16.942min (-0.000) 0.00 ng

response 163860

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.61
264.00	65.10	60.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112621\
 Data File : BM033264.D
 Acq On : 26 Nov 2021 14:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 17:24:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 24 15:16:33 2021
 Response via : Initial Calibration

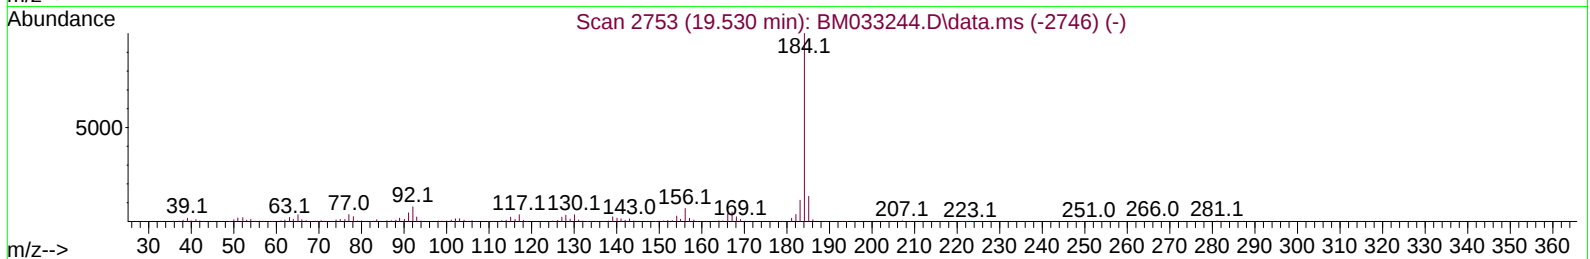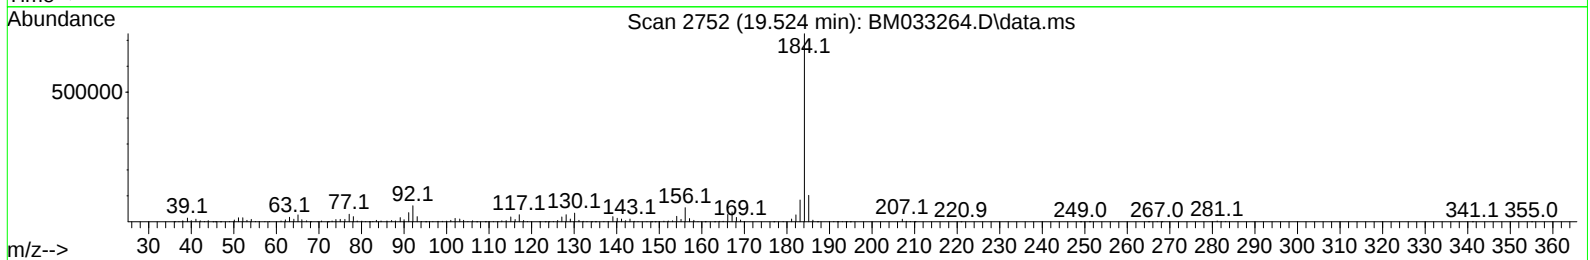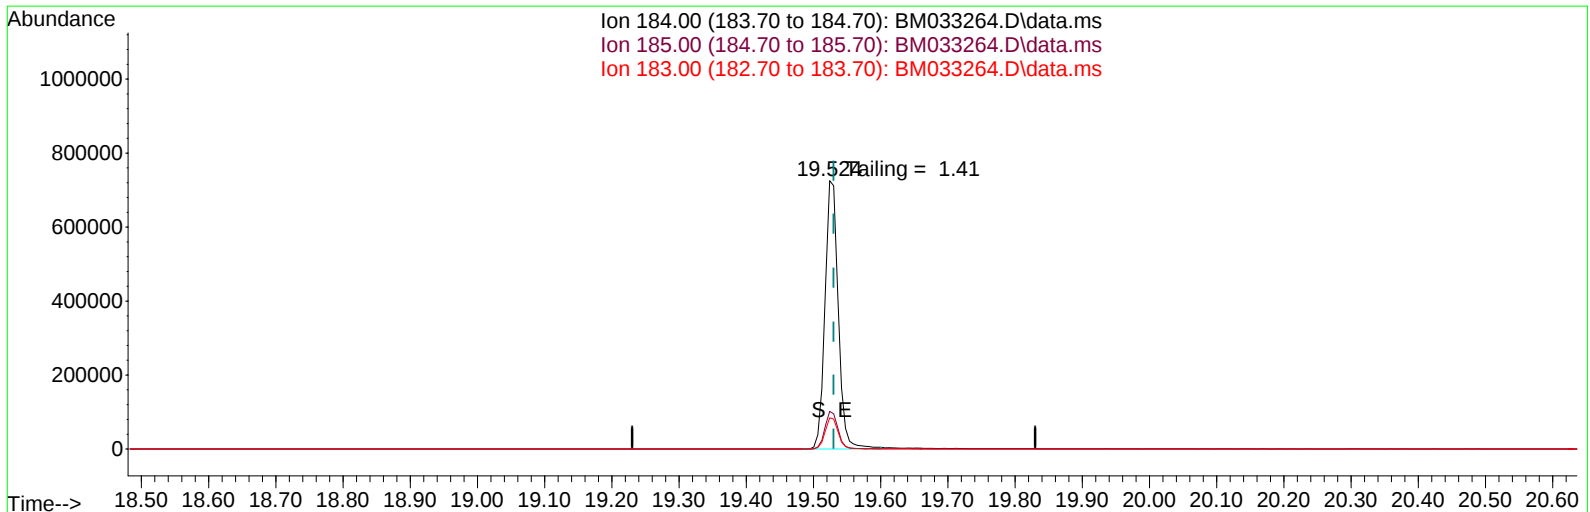

TIC: BM033264.D\data.ms

(77) Benzidine**19.524min (-0.006) 1461210.05 ng****response 1002159**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.03
183.00	11.20	11.62
0.00	0.00	0.00