
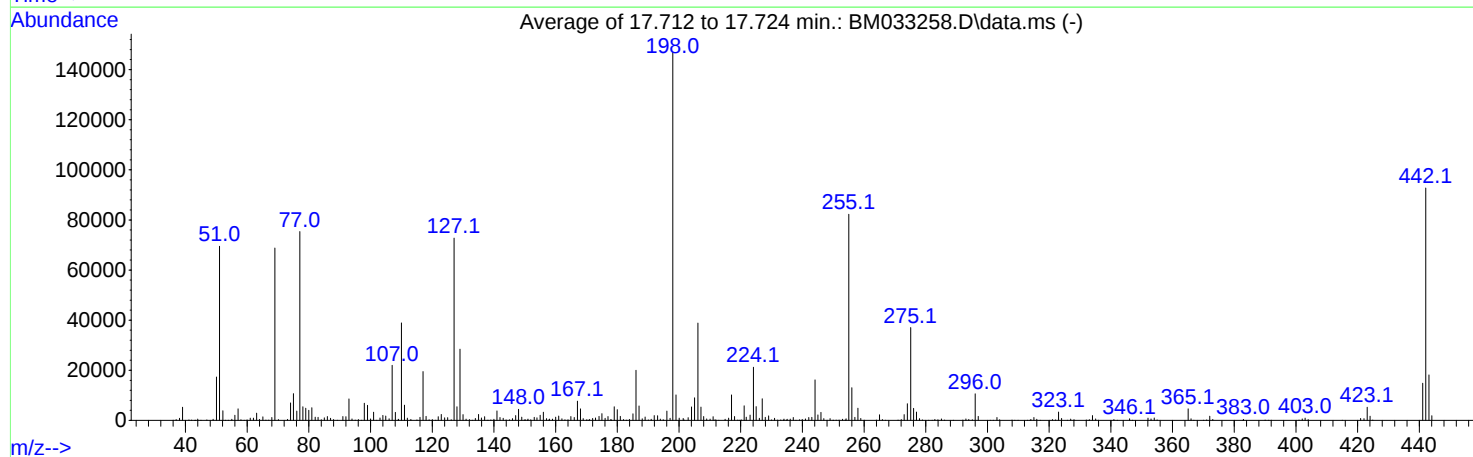


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112621\
 Data File : BM033258.D
 Acq On : 26 Nov 2021 10:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 24 15:16:33 2021

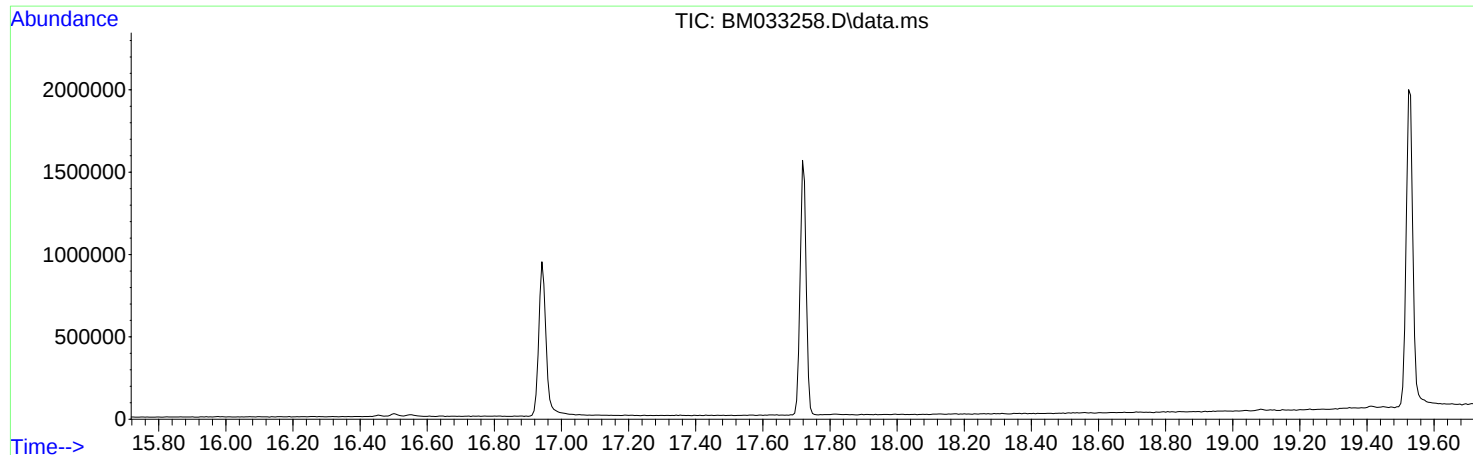




AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2438

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.3	69481	PASS
68	69	0.00	2	1.7	1183	PASS
69	198	0.00	100	46.8	68779	PASS
70	69	0.00	2	0.5	352	PASS
127	198	10	80	49.5	72739	PASS
197	198	0.00	2	0.6	808	PASS
198	198	100	100	100.0	146848	PASS
199	198	5	9	6.9	10169	PASS
275	198	10	60	25.2	37040	PASS
365	198	1	100	3.1	4609	PASS
441	198	0.01	100	10.1	14816	PASS
442	442	50	100	100.0	92755	PASS
443	442	15	24	19.6	18138	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112621\
Data File : BM033258.D
Acq On : 26 Nov 2021 10:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 26 11:59:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 24 15:16:33 2021
Response via : Initial Calibration

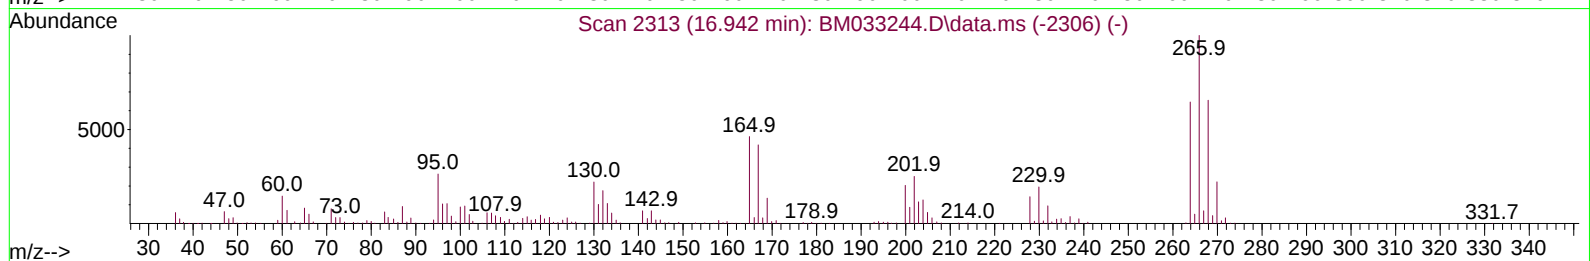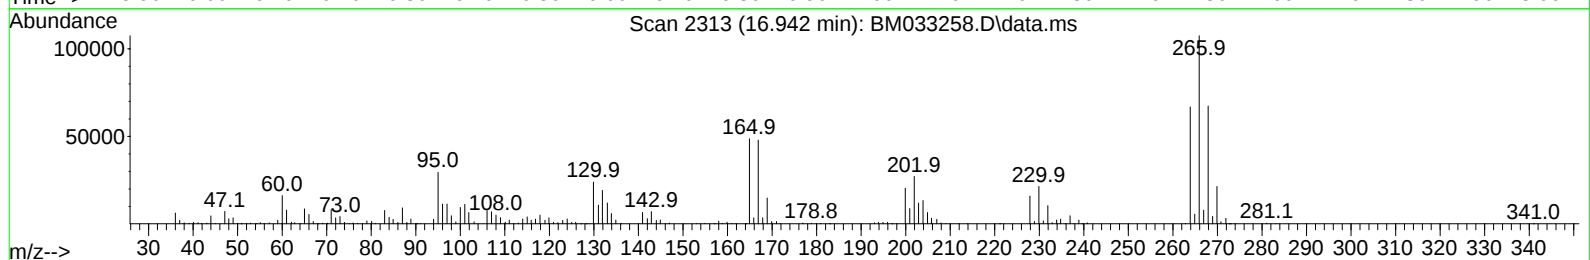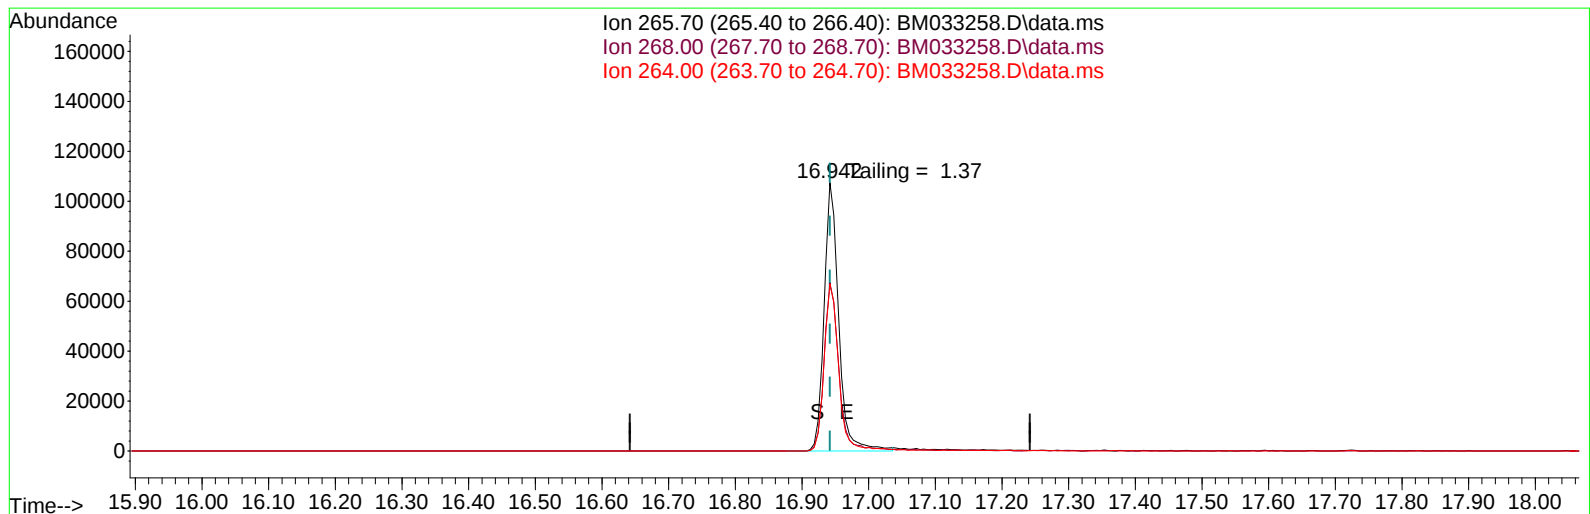

TIC: BM033258.D\data.ms

(70) Pentachlorophenol (C)

16.942min (-0.000) 0.00 ng




response 165164

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.69
264.00	65.10	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112621\
 Data File : BM033258.D
 Acq On : 26 Nov 2021 10:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Nov 26 11:59:36 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 24 15:16:33 2021
 Response via : Initial Calibration

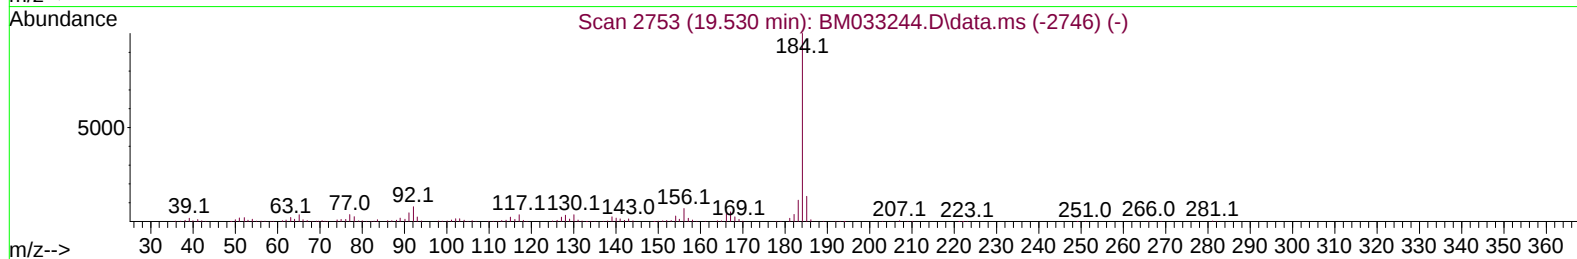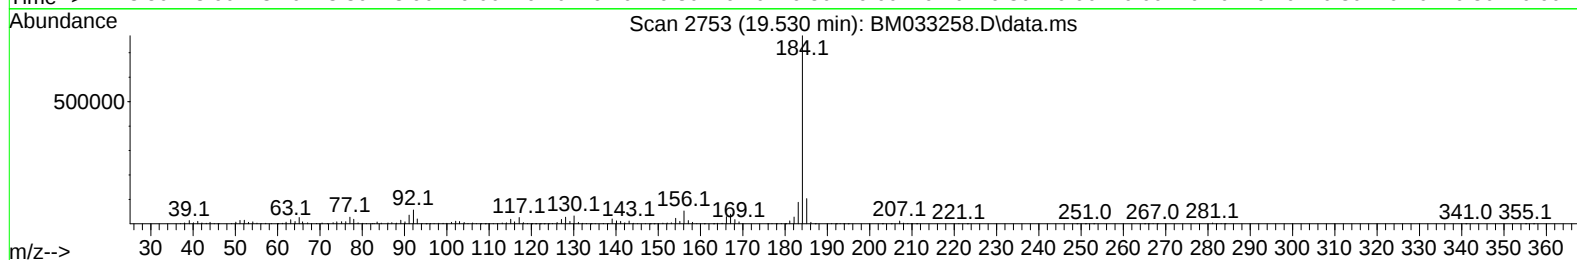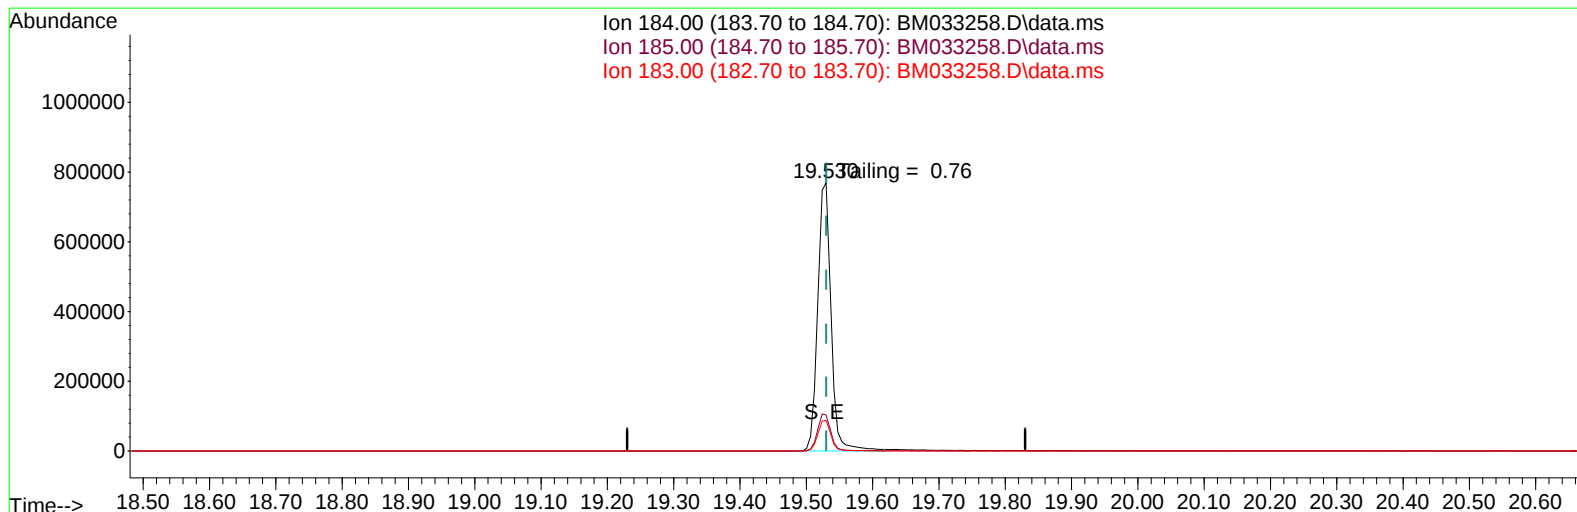

TIC: BM033258.D\data.ms

(77) Benzidine**19.530min (-0.000) 493991.81 ng****response 1083050**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	13.43
183.00	11.20	11.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/26/2021	BNA_M	<u>BM033258.D</u>
Compound Name	Response	Retention Time
DDT	468405	20.74
DDD	32692	20.31
DDE	8896	19.8
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
41588	509993	8.15

Instrument :
BNA_M
ClientSampleId :
DFTPP