
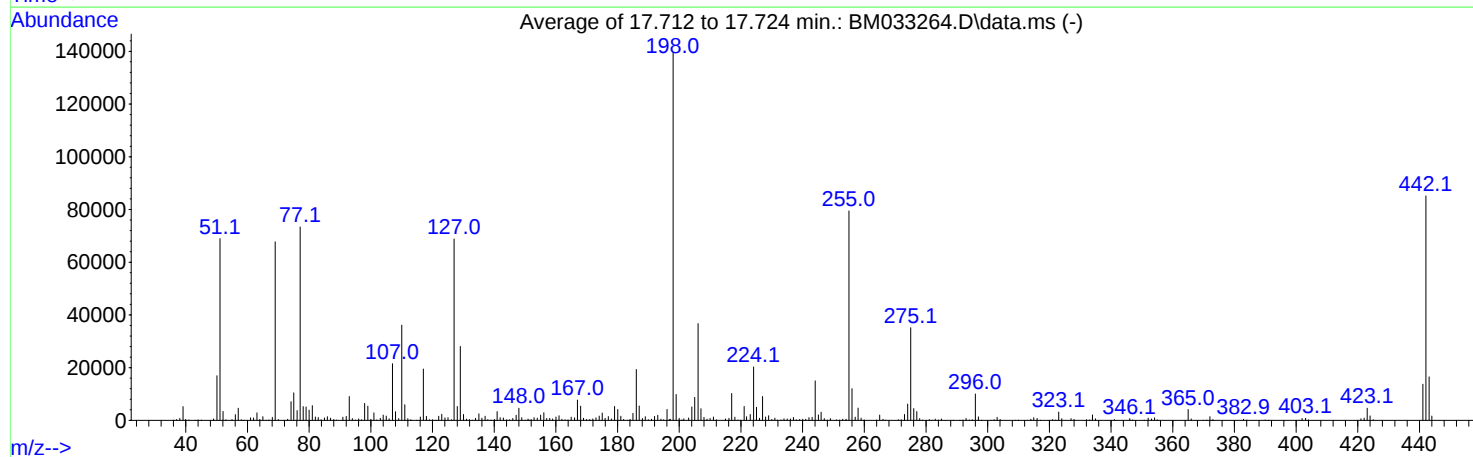


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112621\
 Data File : BM033264.D
 Acq On : 26 Nov 2021 14:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 24 15:16:33 2021

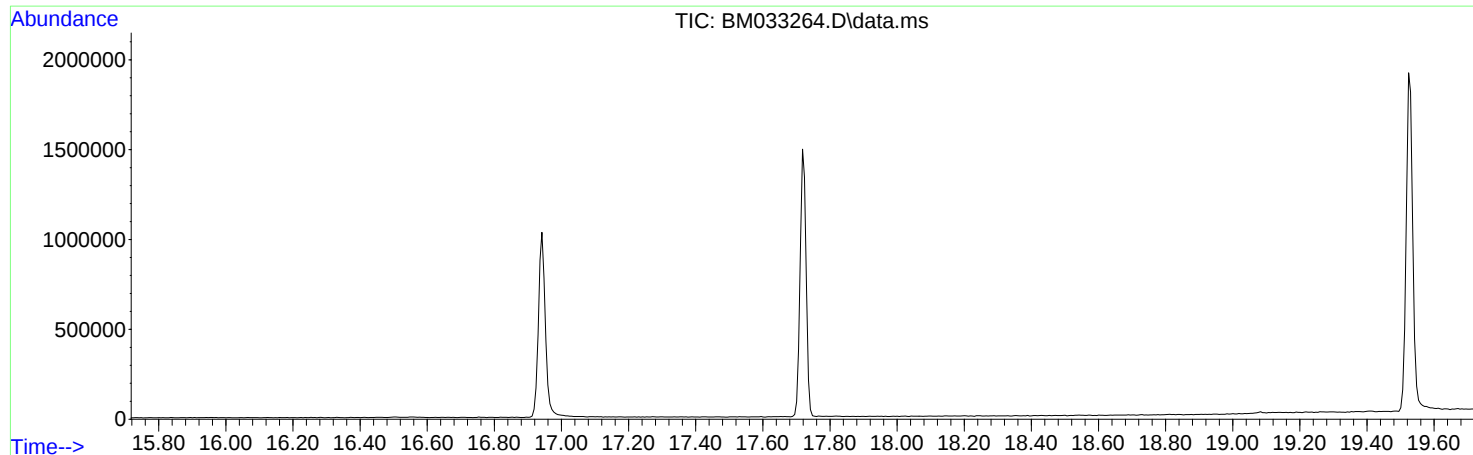




AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2438

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.4	68987	PASS
68	69	0.00	2	1.7	1162	PASS
69	198	0.00	100	48.6	67771	PASS
70	69	0.00	2	0.5	324	PASS
127	198	10	80	49.3	68819	PASS
197	198	0.00	2	0.3	431	PASS
198	198	100	100	100.0	139552	PASS
199	198	5	9	7.1	9856	PASS
275	198	10	60	25.2	35179	PASS
365	198	1	100	2.9	4107	PASS
441	198	0.01	100	9.8	13743	PASS
442	442	50	100	100.0	85179	PASS
443	442	15	24	19.4	16497	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112621\
Data File : BM033264.D
Acq On : 26 Nov 2021 14:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 26 17:24:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 24 15:16:33 2021
Response via : Initial Calibration

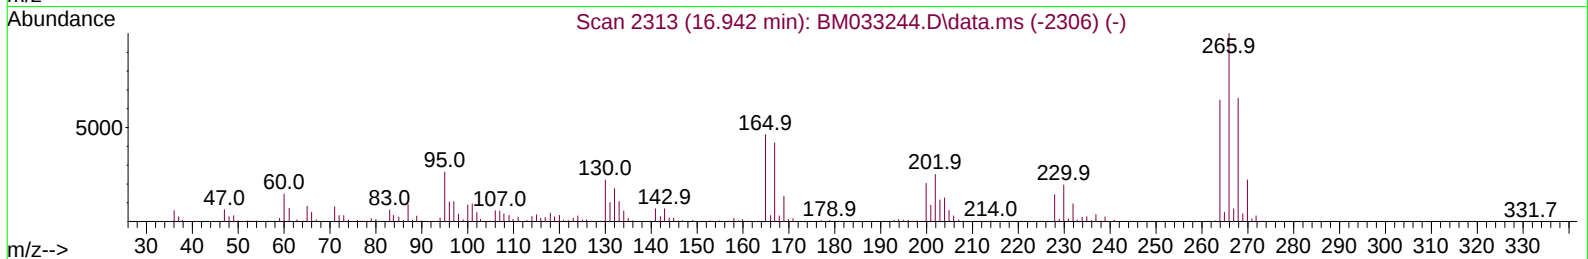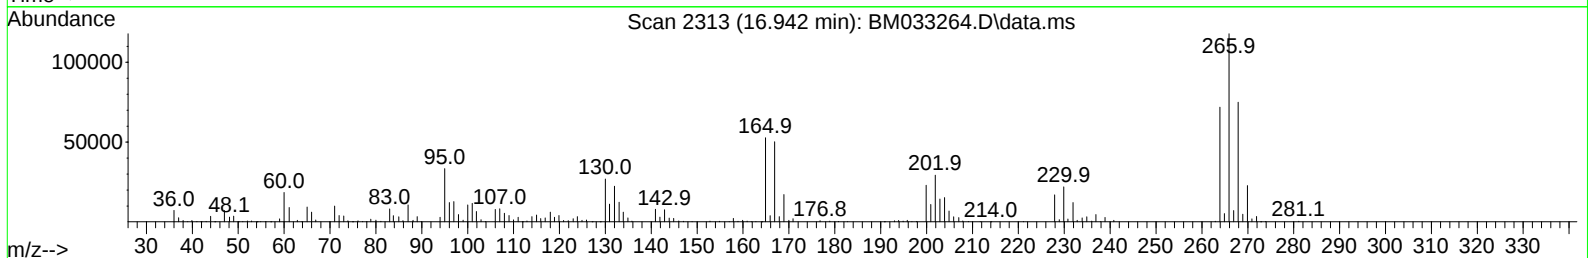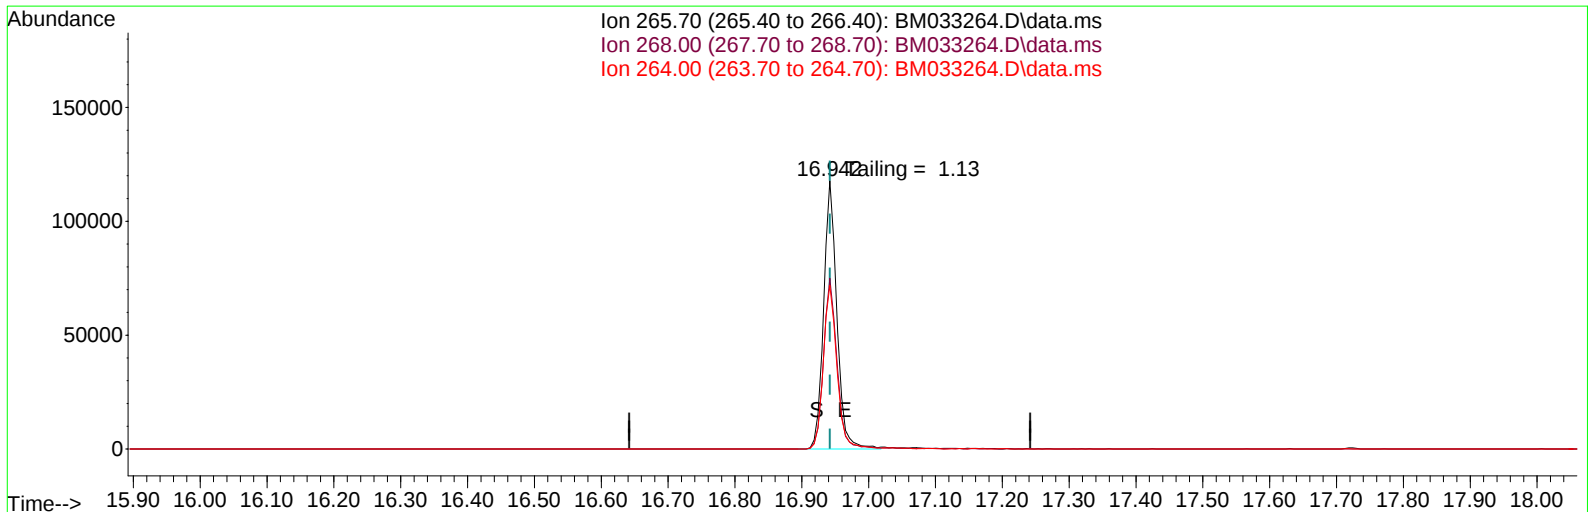

TIC: BM033264.D\data.ms

(70) Pentachlorophenol (C)

16.942min (-0.000) 0.00 ng




response 163860

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.61
264.00	65.10	60.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112621\
Data File : BM033264.D
Acq On : 26 Nov 2021 14:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 26 17:24:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 24 15:16:33 2021
Response via : Initial Calibration

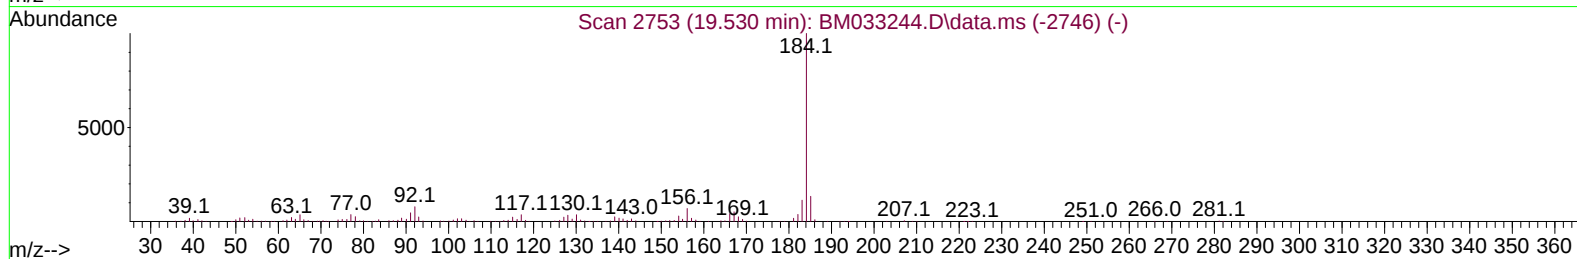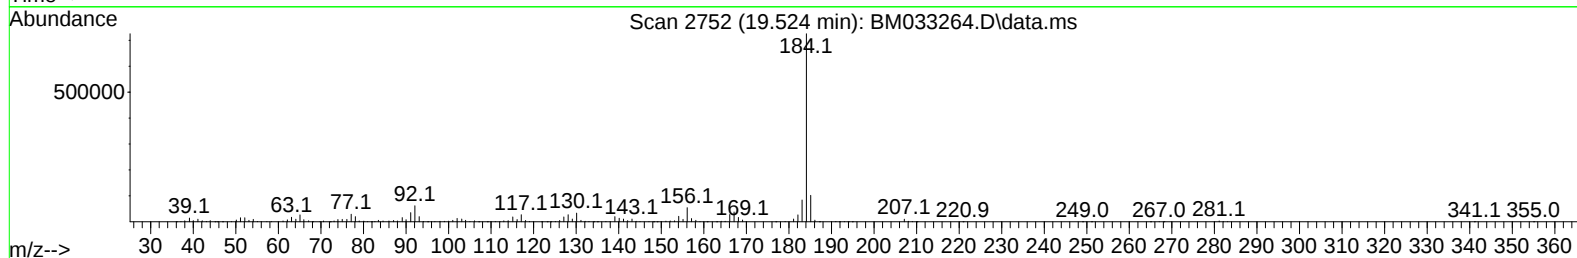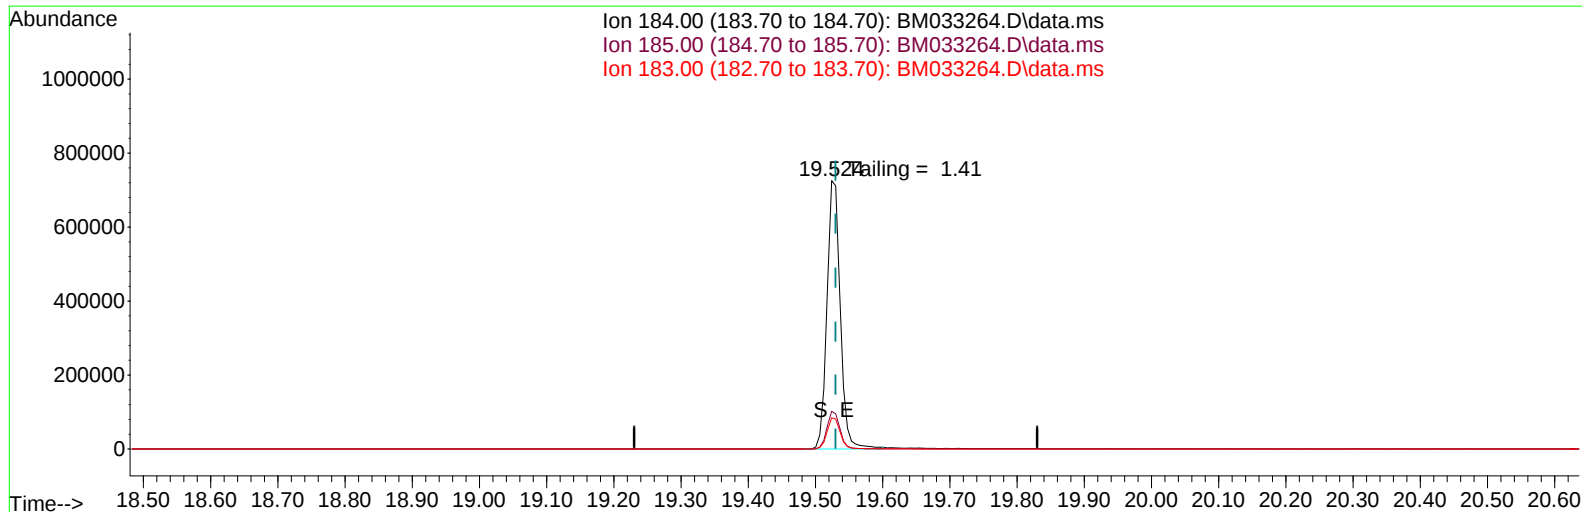

TIC: BM033264.D\data.ms

(77) Benzidine

19.524min (-0.006) 1461210.05 ng

response 1002159

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.03
183.00	11.20	11.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/26/2021	BNA_M	<u>BM033264.D</u>
Compound Name	Response	Retention Time
DDT	439028	20.74
DDD	24358	20.31
DDE	7823	19.8
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32181	471209	6.83

Instrument :
BNA_M
ClientSampleId :
DFTPP