

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120522\
 Data File : BM037844.D
 Acq On : 05 Dec 2022 15:03
 Operator : CG/JU
 Sample : N5738-11DL 20X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBNJ0DL

Quant Time: Dec 05 23:25:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 02 01:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	285624	20.000	ng/ul	0.00
20) Naphthalene-d8	10.910	136	1227343	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.722	164	745152	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	1617272	20.000	ng/ul	0.00
79) Chrysene-d12	21.627	240	1211967	20.000	ng/ul	0.00
88) Perylene-d12	24.115	264	1068689	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	532	0.087	ng/uL	0.00
4) Pyridine-d5	3.858	84	652	0.033	ng/ul	-0.01
7) Phenol-d5	7.246	99	20700	0.804	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	12619	0.841	ng/ul	0.00
11) 2-Chlorophenol-d4	7.616	132	16026	0.824	ng/ul	0.00
15) 4-Methylphenol-d8	8.798	113	16071	0.785	ng/ul	0.00
21) Nitrobenzene-d5	9.263	128	8518	0.874	ng/ul	0.00
24) 2-Nitrophenol-d4	9.992	143	7723	0.766	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.528	165	15046	0.804	ng/ul	0.00
31) 4-Chloroaniline-d4	11.051	131	6219	0.217	ng/ul	0.00
46) Dimethylphthalate-d6	14.128	166	52358	1.023	ng/ul	0.00
49) Acenaphthylene-d8	14.416	160	58074	0.933	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	6048	0.569	ng/ul	0.00
60) Fluorene-d10	15.704	176	50062	1.078	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	4613	0.541	ng/ul	0.00
73) Anthracene-d10	17.557	188	85521	1.150	ng/ul	0.00
81) Pyrene-d10	19.839	212	90495	1.441	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.945	264	55962	1.045	ng/ul	-0.01
Target Compounds						
71) Pentachlorophenol	17.110	266	422105	35.412	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120522\
Data File : BM037844.D
Acq On : 05 Dec 2022 15:03
Operator : CG/JU
Sample : N5738-11DL 20X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBNJ0DL

Quant Time: Dec 05 23:25:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 02 01:14:59 2022
Response via : Initial Calibration

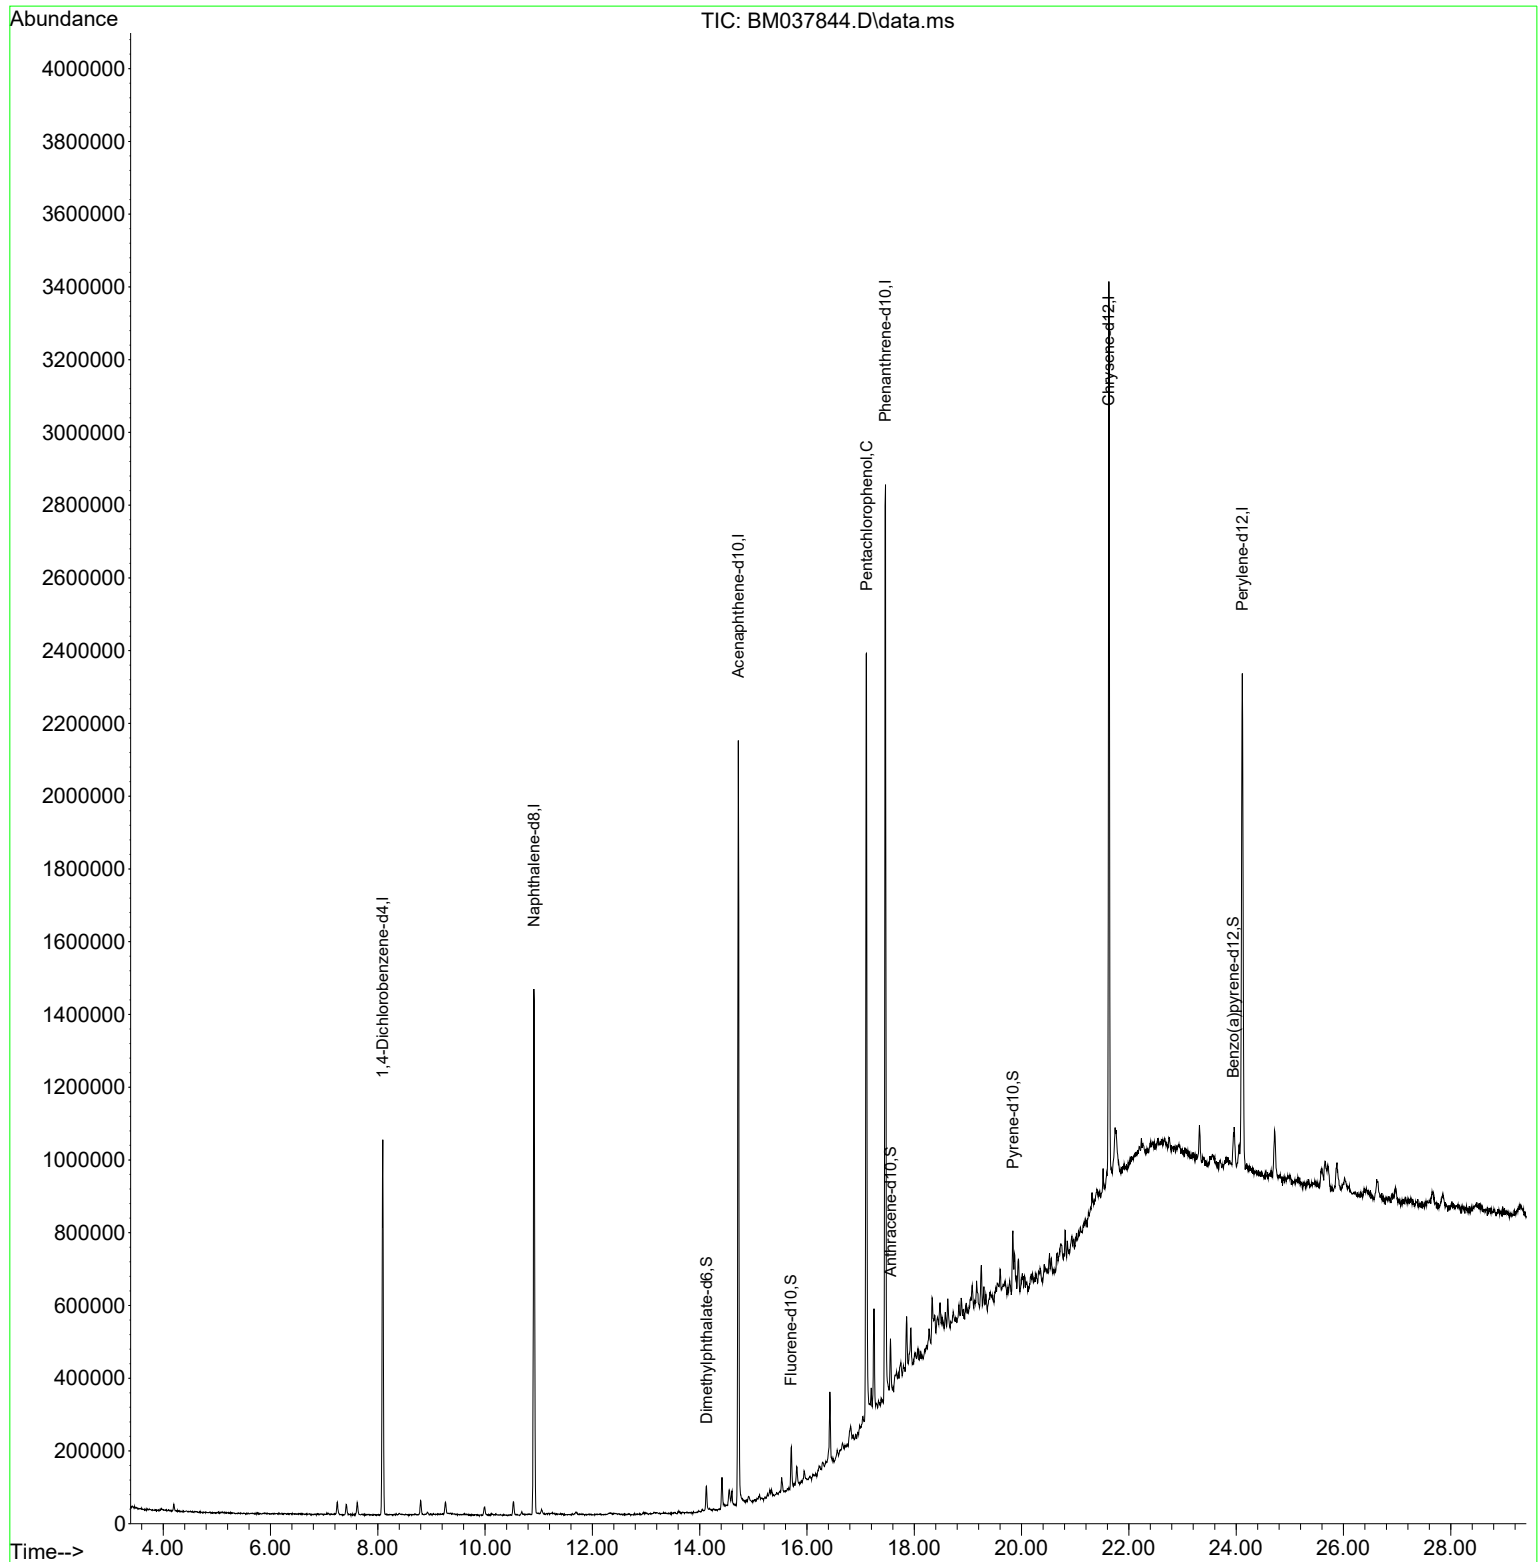

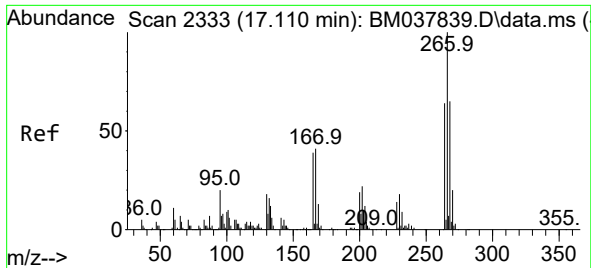

#71
 Pentachlorophenol
 Concen: 35.412 ng/ul
 RT: 17.110 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BM037844.D
 Acq: 05 Dec 2022 15:03

Instrument :
 BNA_M
 ClientSampleId :
 GBNJ0DL

Tgt Ion:266 Resp: 422105
 Ion Ratio Lower Upper
 266 100
 264 63.2 50.3 75.5
 268 62.8 52.2 78.2

