

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033363.D
 Acq On : 09 Dec 2021 18:00
 Operator : CG/JU
 Sample : PB141247BS
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS247

Quant Time: Dec 10 01:15:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 09 13:25:37 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 12/10/2021
 Supervised By :mohammad ahmed 12/15/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.913	152	44658	20.000	ng/u1	0.00
20) Naphthalene-d8	10.707	136	182854	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.536	164	125334	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.271	188	285990	20.000	ng/u1	0.00
79) Chrysene-d12	21.436	240	296355	20.000	ng/u1	0.00
88) Perylene-d12	23.759	264	281485	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.366	96	5485m	4.615	ng/uL	0.00
4) Pyridine-d5	3.784	84	85675	24.865	ng/u1	0.00
7) Phenol-d5	7.078	99	115977	27.426	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.243	67	76578	27.661	ng/u1	0.00
11) 2-Chlorophenol-d4	7.443	132	85337	28.823	ng/u1	0.00
15) 4-Methylphenol-d8	8.619	113	90149	27.236	ng/u1	0.00
21) Nitrobenzene-d5	9.072	128	44053	29.691	ng/u1	0.00
24) 2-Nitrophenol-d4	9.789	143	47165	30.984	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.331	165	90399	31.424	ng/u1	0.00
31) 4-Chloroaniline-d4	10.848	131	127793	29.962	ng/u1	0.00
46) Dimethylphthalate-d6	13.942	166	293960	31.390	ng/u1	0.00
49) Acenaphthylene-d8	14.230	160	357003	30.752	ng/u1	0.00
54) 4-Nitrophenol-d4	14.748	143	53605	31.527	ng/u1	0.00
60) Fluorene-d10	15.524	176	259678	31.001	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.642	200	46239	26.788	ng/u1	0.00
73) Anthracene-d10	17.371	188	422924	29.923	ng/u1	0.00
81) Pyrene-d10	19.659	212	513115	30.979	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.612	264	475073	31.137	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.402	88	12346	9.334	ng/uL	94
5) Pyridine	3.802	79	84309	23.758	ng/u1	98
6) Benzaldehyde	7.054	77	80105m	34.001	ng/u1	
8) Phenol	7.107	94	114574	26.304	ng/u1	93
10) Bis(2-Chloroethyl)ether	7.337	93	85367	26.051	ng/u1	99
12) 2-Chlorophenol	7.478	128	84107	27.471	ng/u1	97
13) 2-Methylphenol	8.354	108	81620	25.846	ng/u1	96
14) 2,2'-oxybis(1-Chloropr...	8.431	45	148687m	26.297	ng/u1	
16) Acetophenone	8.737	105	144182	26.296	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.713	70	82623	27.568	ng/u1	97
18) 4-Methylphenol	8.684	108	90311	26.138	ng/u1	95
19) Hexachloroethane	8.984	117	41350	26.733	ng/u1#	90
22) Nitrobenzene	9.113	77	123106	28.340	ng/u1	99
23) Isophorone	9.636	82	213682	28.727	ng/u1	98
25) 2-Nitrophenol	9.825	139	47231	29.267	ng/u1	97
26) 2,4-Dimethylphenol	9.878	107	104712	26.760	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.113	93	117702	28.136	ng/u1	98
29) 2,4-Dichlorophenol	10.354	162	83170	28.560	ng/u1	96
30) Naphthalene	10.754	128	283084	27.781	ng/u1	99
32) 4-Chloroaniline	10.872	127	108203	25.241	ng/u1	97
33) Hexachlorobutadiene	11.031	225	58772	27.571	ng/u1	96
34) Caprolactam	11.654	113	29584m	30.124	ng/u1	
35) 4-Chloro-3-methylphenol	11.989	107	103910	30.398	ng/u1	94
36) 2-Methylnaphthalene	12.360	142	196355	28.415	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033363.D
 Acq On : 09 Dec 2021 18:00
 Operator : CG/JU
 Sample : PB141247BS
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS247

Quant Time: Dec 10 01:15:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 09 13:25:37 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/10/2021
 Supervised By :mohammad ahmed 12/15/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.577	142	206715	28.784	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.725	216	107085	28.358	ng/ul	99
40) Hexachlorocyclopentadiene	12.701	237	76096	30.875	ng/ul	97
41) 2,4,6-Trichlorophenol	12.972	196	68272	30.714	ng/ul	98
42) 2,4,5-Trichlorophenol	13.048	196	74422	30.905	ng/ul	91
43) 1,1'-Biphenyl	13.372	154	277902	28.983	ng/ul	97
44) 2-Chloronaphthalene	13.413	162	211354	28.650	ng/ul	98
45) 2-Nitroaniline	13.624	65	83074	31.576	ng/ul	97
47) Dimethylphthalate	13.989	163	272739	29.332	ng/ul	100
48) 2,6-Dinitrotoluene	14.113	165	56239	31.289	ng/ul	92
50) Acenaphthylene	14.260	152	358380	29.650	ng/ul	100
51) 3-Nitroaniline	14.448	138	54227	30.650	ng/ul	99
52) Acenaphthene	14.595	153	235770	29.391	ng/ul	96
53) 2,4-Dinitrophenol	14.654	184	28412	26.898	ng/ul	93
55) 4-Nitrophenol	14.760	109	57104	31.073	ng/ul	94
56) Dibenzofuran	14.930	168	340878	29.303	ng/ul	100
57) 2,4-Dinitrotoluene	14.901	165	84346	31.944	ng/ul	90
58) 2,3,4,6-Tetrachlorophenol	15.160	232	65011	31.758	ng/ul	97
59) Diethylphthalate	15.348	149	294915	30.560	ng/ul	99
61) Fluorene	15.583	166	285059	29.803	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.571	204	142668	29.901	ng/ul	97
63) 4-Nitroaniline	15.607	138	65592	36.103	ng/ul	96
66) 4,6-Dinitro-2-methylph...	15.660	198	42637	24.797	ng/ul	96
67) N-Nitrosodiphenylamine	15.789	169	240844	28.642	ng/ul	99
68) 4-Bromophenyl-phenylether	16.465	248	81445	28.274	ng/ul	96
69) Hexachlorobenzene	16.577	284	95461	28.763	ng/ul	98
70) Atrazine	16.736	200	93834	28.123	ng/ul	99
71) Pentachlorophenol	16.924	266	61297	32.936	ng/ul	94
72) Phenanthrene	17.318	178	471015	28.549	ng/ul	98
74) Anthracene	17.407	178	478815	28.625	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.336	216	109639	26.581	ng/uL	95
76) Pentachlorobenzene	14.848	250	108363	26.604	ng/uL	96
77) Carbazole	17.677	167	431820	28.562	ng/ul	99
78) Di-n-butylphthalate	18.230	149	520042	30.656	ng/ul	99
80) Fluoranthene	19.324	202	570166	29.204	ng/ul	98
82) Pyrene	19.689	202	598825	29.299	ng/ul	98
83) Butylbenzylphthalate	20.571	149	245609	31.371	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.353	252	163525	24.277	ng/ul	96
85) Benzo(a)anthracene	21.418	228	563756	28.953	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.342	149	352559	31.332	ng/ul	100
87) Chrysene	21.471	228	556909	29.101	ng/ul	98
89) Di-n-octyl phthalate	22.242	149	609285	29.522	ng/ul	100
90) Benzo(b)fluoranthene	23.053	252	568666	29.486	ng/ul	99
91) Benzo(k)fluoranthene	23.100	252	540114	30.247	ng/ul	98
93) Benzo(a)pyrene	23.659	252	551932	29.826	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.135	276	576380	28.640	ng/ul	97
95) Dibenzo(a,h)anthracene	26.147	278	505744	28.890	ng/ul	97
96) Benzo(g,h,i)perylene	26.865	276	496910	28.949	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033363.D
 Acq On : 09 Dec 2021 18:00
 Operator : CG/JU
 Sample : PB141247BS
 Misc :
 ALS Vial : 16 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 SLCS247

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 12/10/2021
 Supervised By :mohammad ahmed 12/15/2021

Quant Time: Dec 10 01:15:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 09 13:25:37 2021
 Response via : Initial Calibration

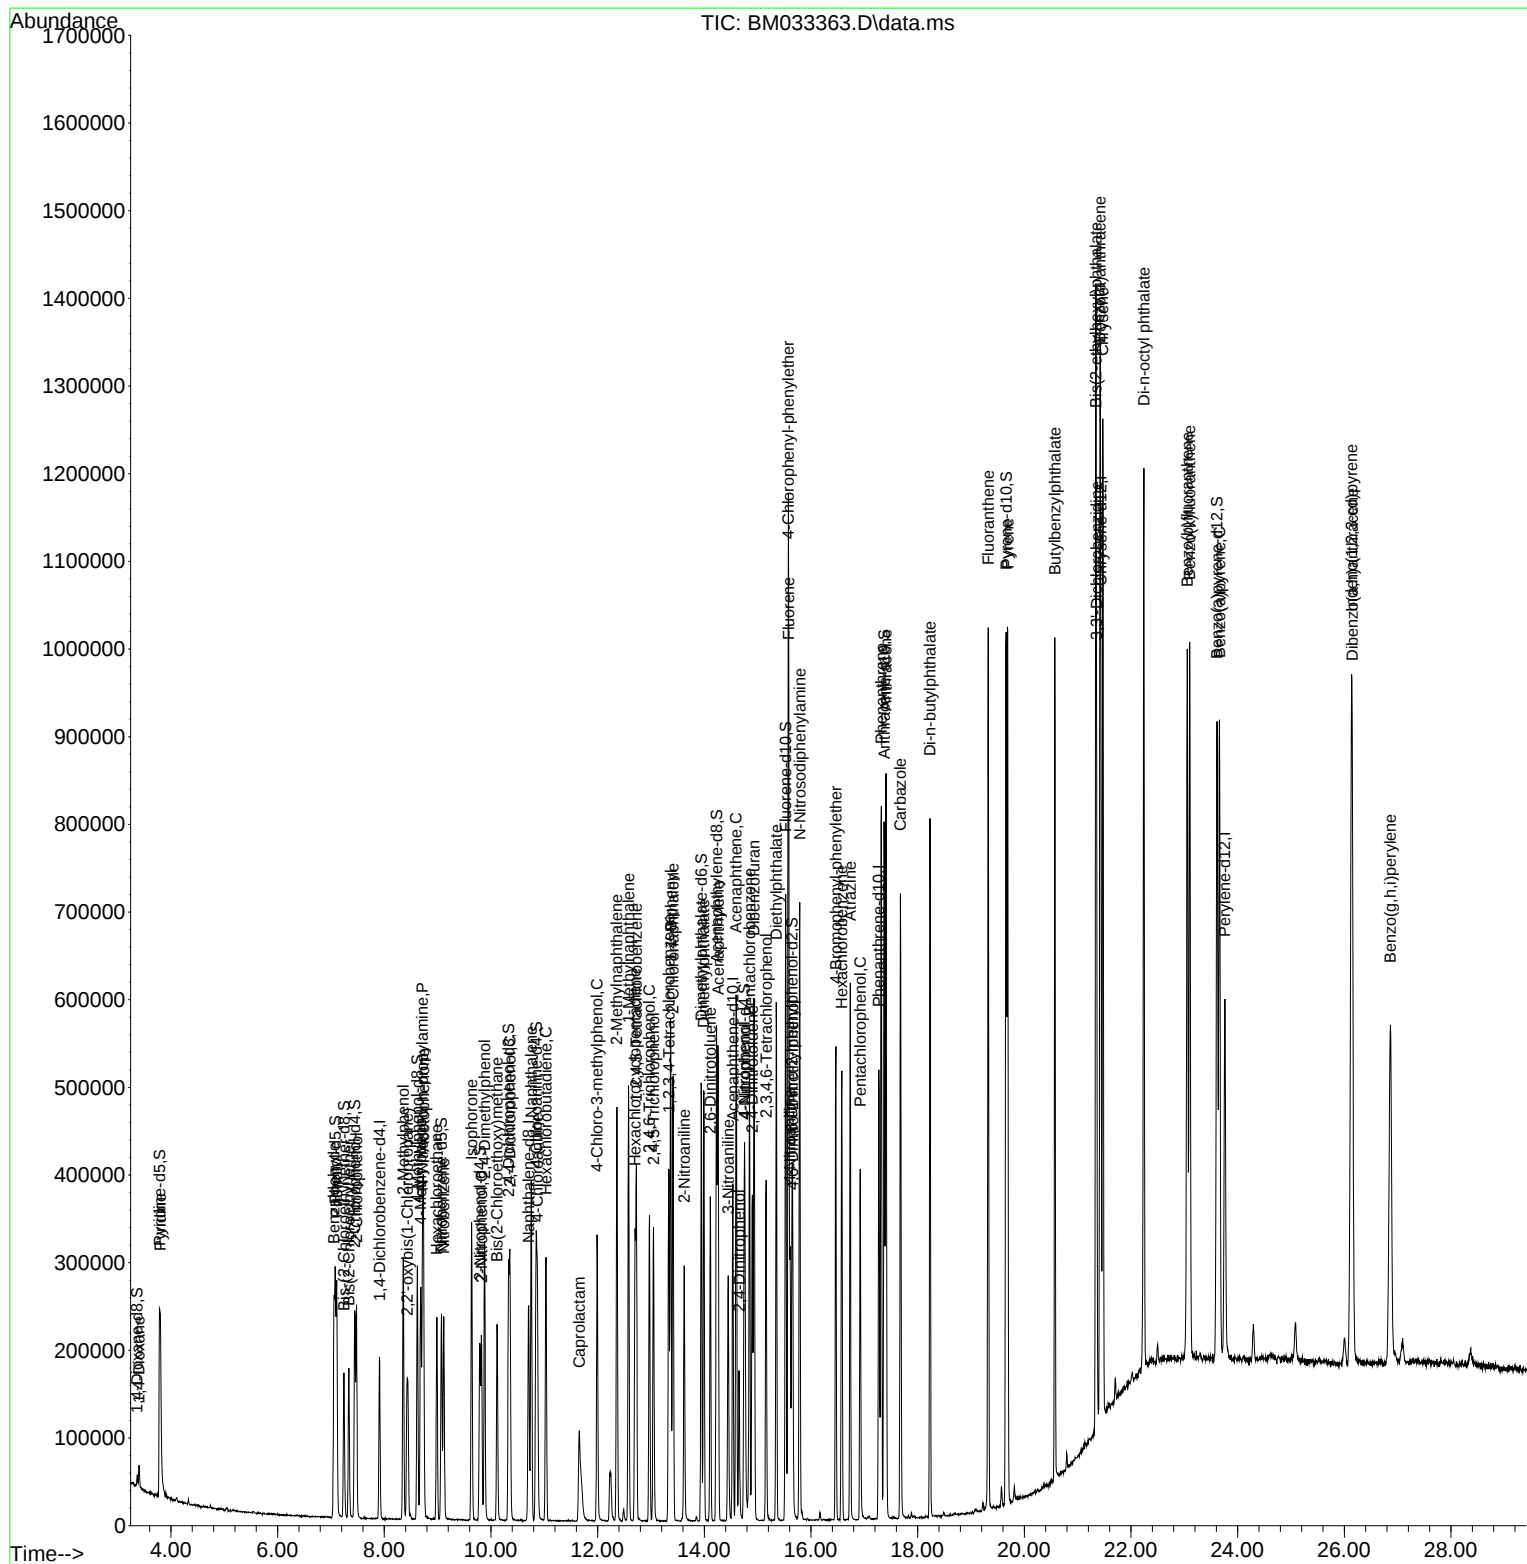







#2
1,4-Dioxane
Concen: 9.334 ng/uL
RT: 3.402 min Scan# 21
Delta R.T. 0.001 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Instrument :
BNA_M
ClientSampleId :
SLCS247

Tgt Ion: 88 Resp: 12340
Ion Ratio Lower Upper
88 100
43 46.8 36.2 54.4
58 78.7 68.5 102.7




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#5
Pyridine
Concen: 23.758 ng/uL
RT: 3.802 min Scan# 96
Delta R.T. -0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Tgt Ion: 79 Resp: 84309
Ion Ratio Lower Upper
79 100
52 97.2 78.1 117.1
51 48.4 36.0 54.0









#6
Benzaldehyde
Concen: 34.001 ng/ul m
RT: 7.054 min Scan# 649
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Instrument :
BNA_M
ClientSampleId :
SLCS247

Tgt Ion: 77 Resp: 8010
Ion Ratio Lower Upper
77 100
105 84.9 65.6 98.4
106 76.6 60.6 90.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#8
Phenol
Concen: 26.304 ng/ul
RT: 7.107 min Scan# 658
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00


Tgt Ion: 94 Resp: 114574
Ion Ratio Lower Upper
94 100
65 35.9 31.7 47.5
66 51.4 45.4 68.0

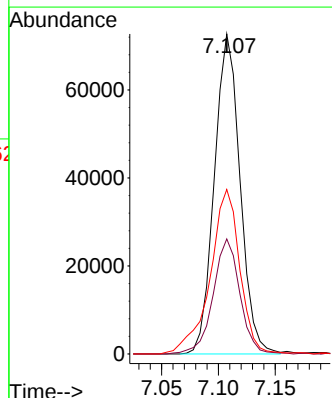



#10
Bis(2-Chloroethyl)ether
Concen: 26.051 ng/ul
RT: 7.337 min Scan# 680
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247




Tgt Ion: 93 Resp: 8536
Ion Ratio Lower Upper
93 100
63 89.7 71.7 107.5
95 31.3 26.3 39.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021

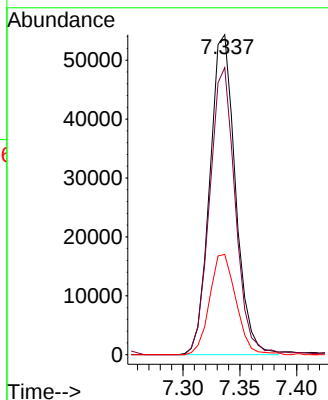


#12
2-Chlorophenol
Concen: 27.471 ng/ul
RT: 7.478 min Scan# 721
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00



Tgt Ion:128 Resp: 84107
Ion Ratio Lower Upper
128 100
64 59.4 49.4 74.2
130 32.4 26.8 40.2

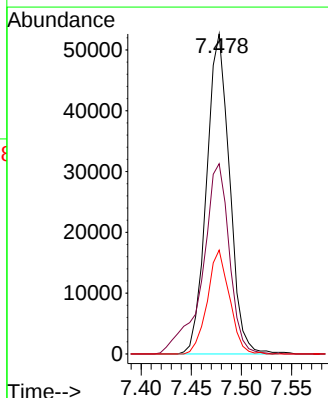







#13
2-Methylphenol
Concen: 25.846 ng/ul
RT: 8.354 min Scan# 81
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Instrument :
BNA_M
ClientSampleId :
SLCS247

Tgt Ion:108 Resp: 81620
Ion Ratio Lower Upper
108 100
107 91.8 70.2 105.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#14
2,2'-oxybis(1-Chloropropane)
Concen: 26.297 ng/ul m
RT: 8.431 min Scan# 883
Delta R.T. -0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00


Tgt Ion: 45 Resp: 148687
Ion Ratio Lower Upper
45 100
77 13.1 9.9 14.9
79 10.4 8.3 12.5





#16
Acetophenone
Concen: 26.296 ng/ul
RT: 8.737 min Scan# 918
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247



Tgt Ion: 105 Resp: 14418
Ion Ratio Lower Upper
105 100
77 90.8 73.1 109.7
51 38.7 30.5 45.7




Manual Integrations
APPROVED


Reviewed By : Jagrut Upadhyay 12/10/2021
Supervised By : mohammad ahmed 12/15/2021



#17
N-Nitroso-di-n-propylamine
Concen: 27.568 ng/ul
RT: 8.713 min Scan# 931
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Tgt Ion: 70 Resp: 82623
Ion Ratio Lower Upper
70 100
42 68.2 56.9 85.3
101 7.3 6.9 10.3
130 15.8 13.8 20.8









#18
4-Methylphenol
Concen: 26.138 ng/ul
RT: 8.684 min Scan# 909
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Instrument :
BNA_M
ClientSampleId :
SLCS247

Tgt Ion:108 Resp: 9031
Ion Ratio Lower Upper
108 100
107 114.9 87.4 131.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#19
Hexachloroethane
Concen: 26.733 ng/ul
RT: 8.984 min Scan# 977
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Tgt Ion:117 Resp: 41350
Ion Ratio Lower Upper
117 100
201 91.9 69.6 104.4
199 62.9 40.6 60.8#



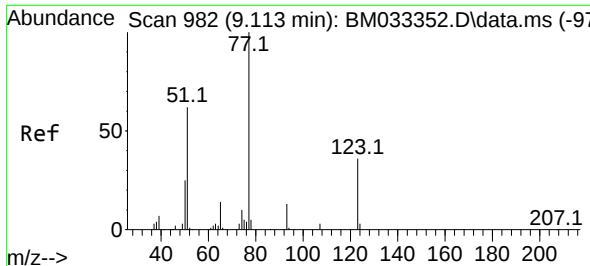





#22
Nitrobenzene
Concen: 28.340 ng/ul
RT: 9.113 min Scan# 90
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Instrument :
BNA_M
ClientSampleId :
SLCS247

Tgt Ion: 77 Resp: 123100
Ion Ratio Lower Upper
77 100
123 35.6 29.0 43.6
65 14.1 11.4 17.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021

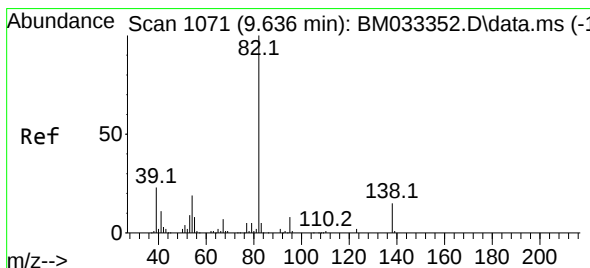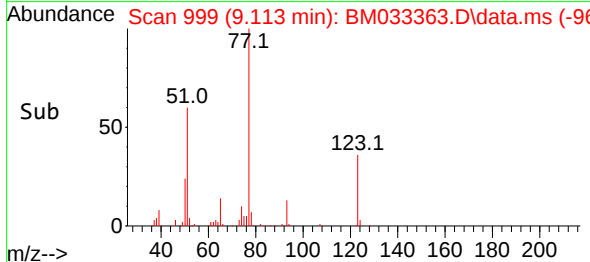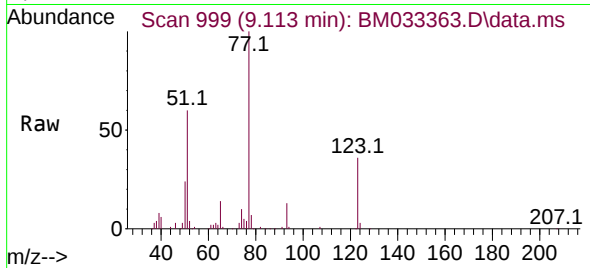

#23
Isophorone
Concen: 28.727 ng/ul
RT: 9.636 min Scan# 1088
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Tgt Ion: 82 Resp: 213682
Ion Ratio Lower Upper
82 100
95 8.4 6.5 9.7
138 15.7 11.8 17.8

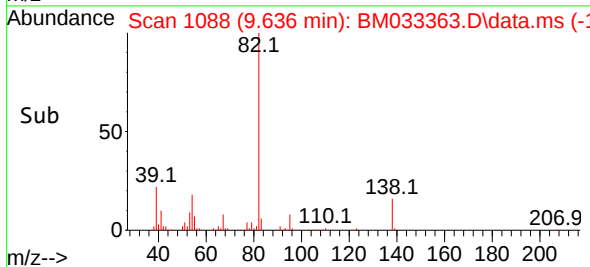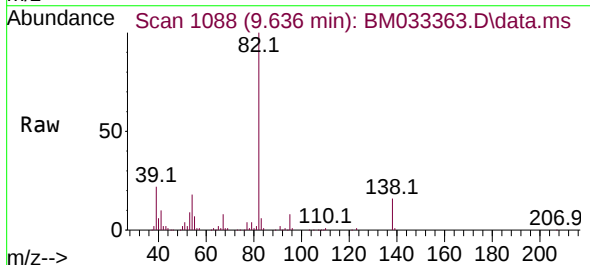







#25
2-Nitrophenol
Concen: 29.267 ng/ul
RT: 9.825 min Scan# 1103
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Instrument :
BNA_M
ClientSampleId :
SLCS247

Tgt Ion:139 Resp: 4723
Ion Ratio Lower Upper
139 100
65 72.1 59.0 88.6
109 42.9 37.2 55.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021

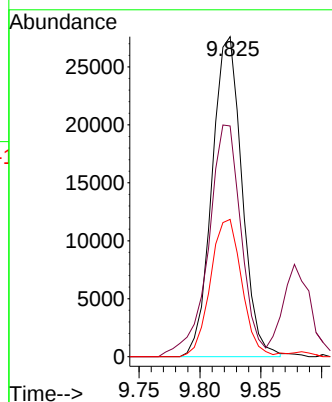

#26
2,4-Dimethylphenol
Concen: 26.760 ng/ul
RT: 9.878 min Scan# 1129
Delta R.T. -0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Tgt Ion:107 Resp: 104712
Ion Ratio Lower Upper
107 100
121 43.8 34.8 52.2
122 73.0 60.0 90.0



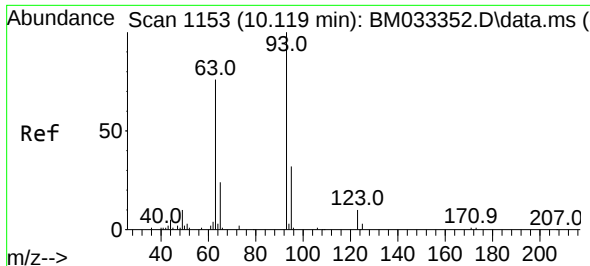





#27
Bis(2-Chloroethoxy)methane
Concen: 28.136 ng/ul
RT: 10.113 min Scan# 1153
Delta R.T. -0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Instrument :
BNA_M
ClientSampleId :
SLCS247

Tgt Ion: 93 Resp: 11770
Ion Ratio Lower Upper
93 100
95 32.5 25.3 37.9
123 10.9 7.9 11.9




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021

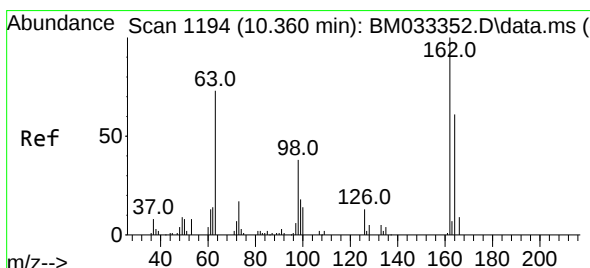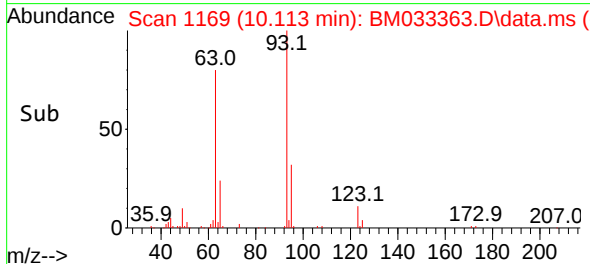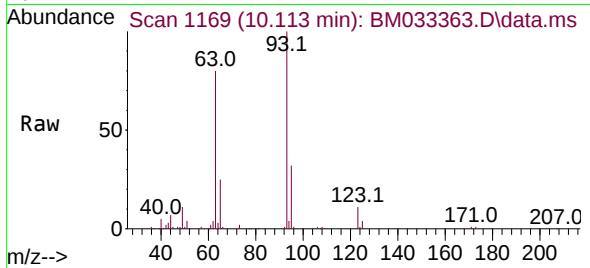

#29
2,4-Dichlorophenol
Concen: 28.560 ng/ul
RT: 10.354 min Scan# 1210
Delta R.T. -0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00


Tgt Ion:162 Resp: 83170
Ion Ratio Lower Upper
162 100
164 64.7 50.0 75.0
98 42.0 30.6 45.8

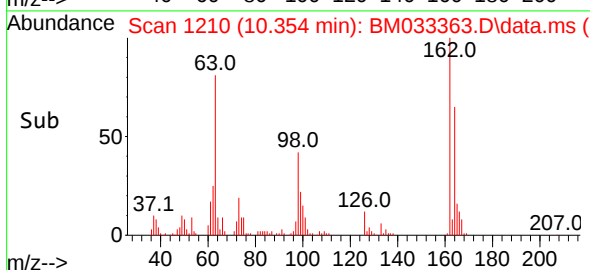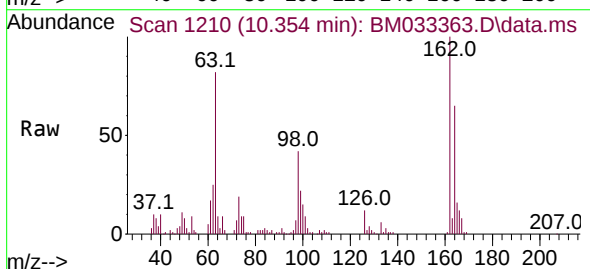



#30
Naphthalene
Concen: 27.781 ng/ul
RT: 10.754 min Scan# 1261
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247



Tgt Ion:128 Resp: 283084
Ion Ratio Lower Upper
128 100
129 11.0 9.1 13.7
127 13.4 10.2 15.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#32
4-Chloroaniline
Concen: 25.241 ng/ul
RT: 10.872 min Scan# 1298
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Tgt Ion:127 Resp: 108203
Ion Ratio Lower Upper
127 100
129 33.5 25.4 38.0

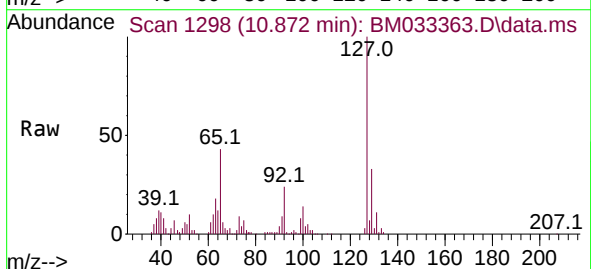







#33
Hexachlorobutadiene
Concen: 27.571 ng/ul
RT: 11.031 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Instrument :
BNA_M
ClientSampleId :
SLCS247

Tgt Ion:225 Resp: 58772
Ion Ratio Lower Upper
225 100
223 60.3 52.2 78.2
227 64.7 52.8 79.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021

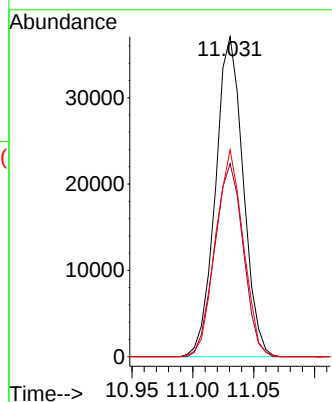

#34
Caprolactam
Concen: 30.124 ng/ul m
RT: 11.654 min Scan# 1431
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00


Tgt Ion:113 Resp: 29584
Ion Ratio Lower Upper
113 100
55 202.7 157.9 236.9
56 152.7 131.8 197.6

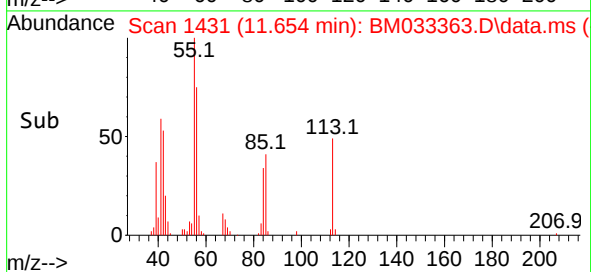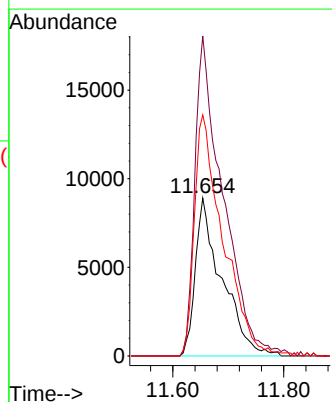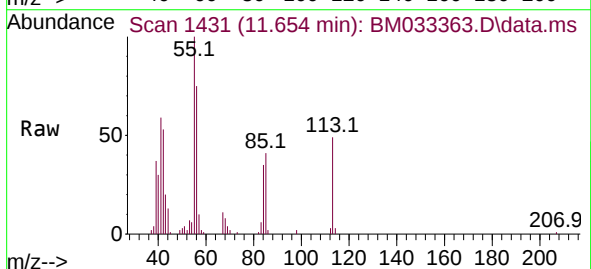



#35
4-Chloro-3-methylphenol
Concen: 30.398 ng/ul
RT: 11.989 min Scan# 1471
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247

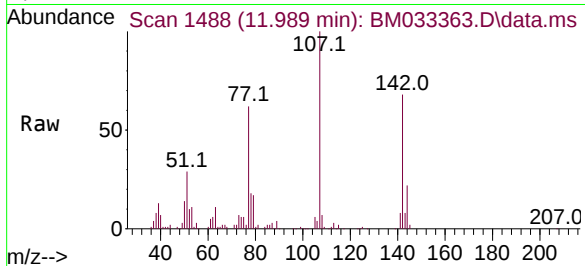


Tgt Ion:107 Resp: 103910
Ion Ratio Lower Upper
107 100
144 21.9 17.1 25.7
142 67.6 49.4 74.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021

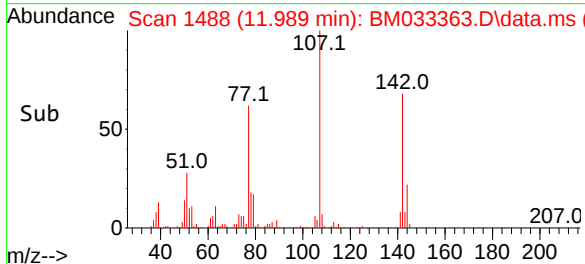


#36
2-Methylnaphthalene
Concen: 28.415 ng/ul
RT: 12.360 min Scan# 1551
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

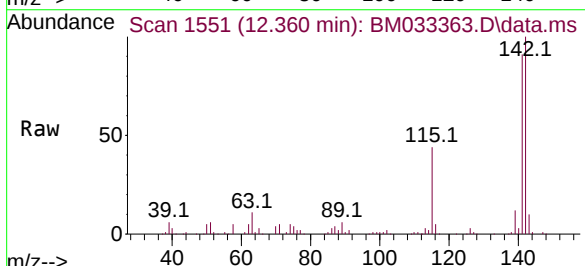

Tgt Ion:142 Resp: 196355
Ion Ratio Lower Upper
142 100
141 90.5 71.1 106.7









#37
1-Methylnaphthalene
Concen: 28.784 ng/ul
RT: 12.577 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Instrument :
BNA_M
ClientSampleId :
SLCS247

Tgt Ion:142 Resp: 206715
Ion Ratio Lower Upper
142 100
141 93.1 75.5 113.3
116 5.1 4.0 6.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021

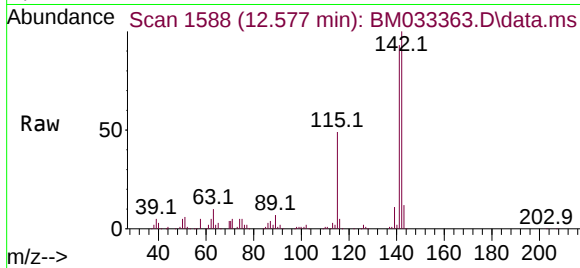

#39
1,2,4,5-Tetrachlorobenzene
Concen: 28.358 ng/ul
RT: 12.725 min Scan# 1613
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00


Tgt Ion:216 Resp: 107085
Ion Ratio Lower Upper
216 100
214 76.9 61.3 91.9
179 21.8 18.0 27.0
108 21.3 16.6 25.0

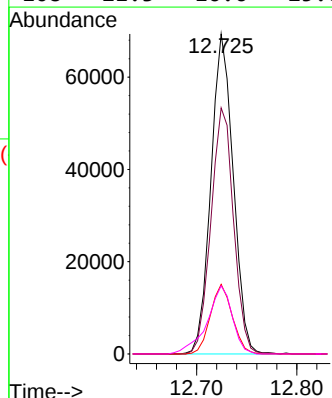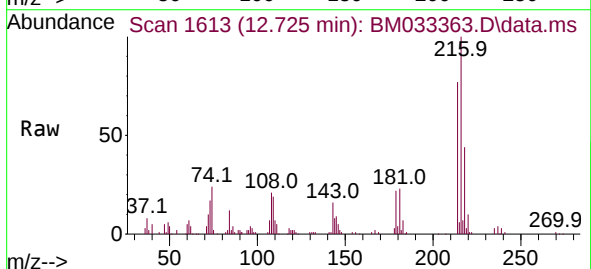



#40
Hexachlorocyclopentadiene
Concen: 30.875 ng/ul
RT: 12.701 min Scan# 1592
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247




Tgt Ion:237 Resp: 76090
Ion Ratio Lower Upper
237 100
235 60.5 50.6 76.0
272 12.2 9.6 14.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021




#41
2,4,6-Trichlorophenol
Concen: 30.714 ng/ul
RT: 12.972 min Scan# 1655
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Tgt Ion:196 Resp: 68272
Ion Ratio Lower Upper
196 100
198 97.8 78.9 118.3
200 32.8 23.7 35.5

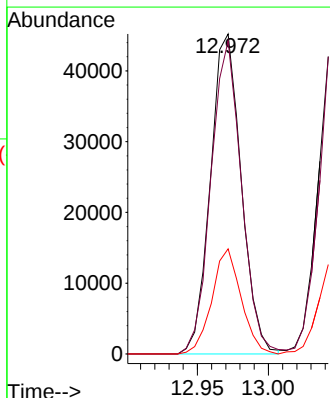



#42
2,4,5-Trichlorophenol
Concen: 30.905 ng/ul
RT: 13.048 min Scan# 1651
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247



Tgt Ion:196 Resp: 7442
Ion Ratio Lower Upper
196 100
198 92.7 82.2 123.2
200 30.1 27.9 41.9




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#43
1,1'-Biphenyl
Concen: 28.983 ng/ul
RT: 13.372 min Scan# 1723
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Tgt Ion:154 Resp: 277902
Ion Ratio Lower Upper
154 100
153 39.2 33.1 49.7
76 13.5 10.7 16.1





#44

2-Chloronaphthalene

Concen: 28.650 ng/ul

RT: 13.413 min Scan# 1

Delta R.T. 0.000 min

Lab File: BM033363.D

Acq: 09 Dec 2021 18:00

Instrument :

BNA_M

ClientSampleId :





SLCS247

Tgt Ion:	162	Resp:	211354
Ion Ratio	Lower	Upper	
162	100		
164	33.6	26.2	39.4
127	43.1	33.7	50.5

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021

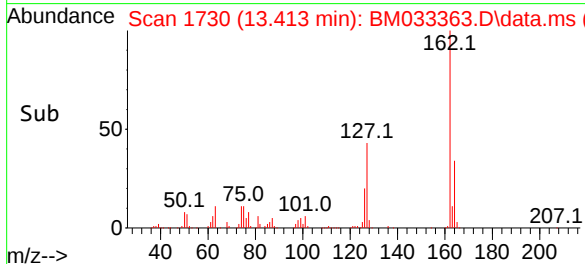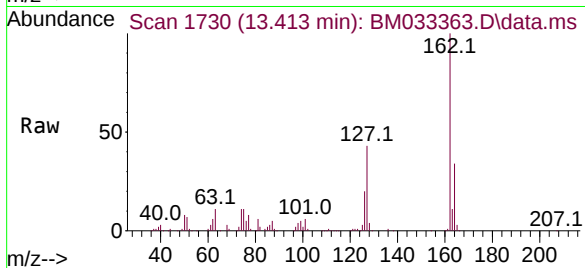

#45

2-Nitroaniline

Concen: 31.576 ng/ul




RT: 13.624 min Scan# 1766


Delta R.T. 0.000 min

Lab File: BM033363.D

Acq: 09 Dec 2021 18:00


Tgt Ion:	65	Resp:	83074
Ion Ratio	Lower	Upper	
65	100		
92	57.8	47.8	71.6
138	78.6	61.0	91.6

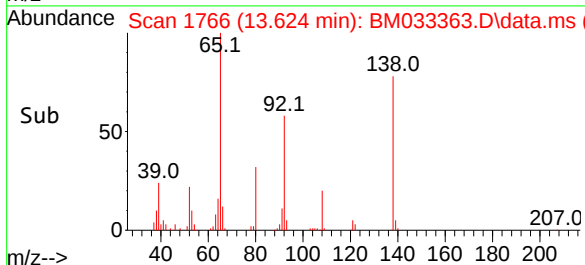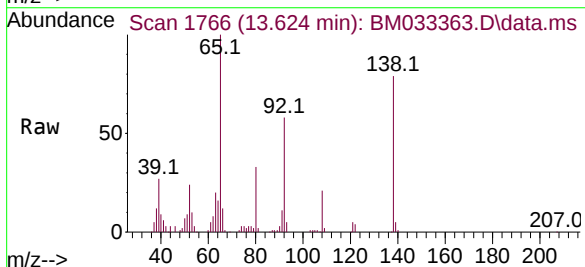



#47
Dimethylphthalate
Concen: 29.332 ng/ul
RT: 13.989 min Scan# 1811
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247




Tgt Ion:163 Resp: 272739
Ion Ratio Lower Upper
163 100
194 3.9 3.3 4.9
164 10.4 8.2 12.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021




#48
2,6-Dinitrotoluene
Concen: 31.289 ng/ul
RT: 14.113 min Scan# 1849
Delta R.T. -0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Tgt Ion:165 Resp: 56239
Ion Ratio Lower Upper
165 100
89 78.5 55.7 83.5
121 24.5 20.0 30.0

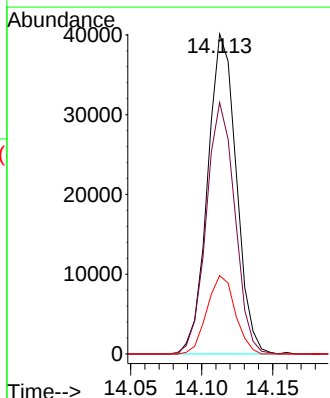



#50
Acenaphthylene
Concen: 29.650 ng/ul
RT: 14.260 min Scan# 11
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247



Tgt Ion:152 Resp: 358380
Ion Ratio Lower Upper
152 100
151 19.9 15.8 23.8
153 12.9 10.1 15.1




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#51
3-Nitroaniline
Concen: 30.650 ng/ul
RT: 14.448 min Scan# 1906
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00


Tgt Ion:138 Resp: 54227
Ion Ratio Lower Upper
138 100
108 12.9 10.8 16.2
92 140.0 110.6 166.0



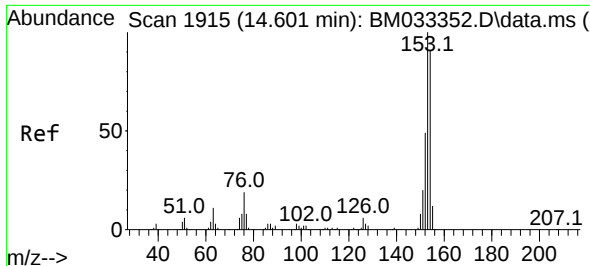

#52
Acenaphthene
Concen: 29.391 ng/ul
RT: 14.595 min Scan# 1915
Delta R.T. -0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247

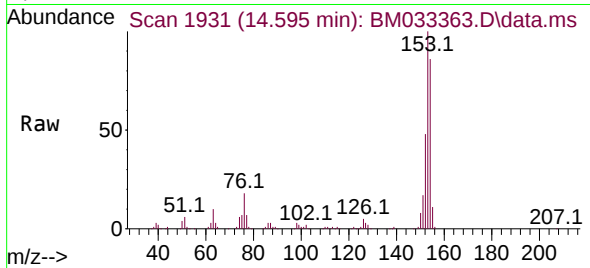


Tgt Ion:153 Resp: 235770
Ion Ratio Lower Upper
153 100
152 47.7 39.4 59.2
154 86.2 72.7 109.1

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021

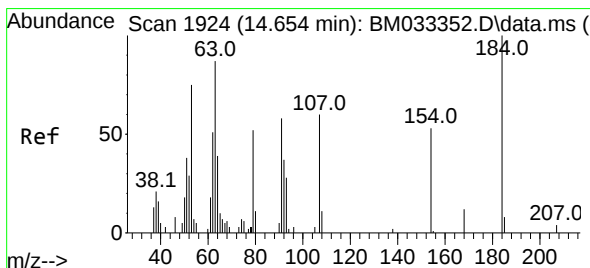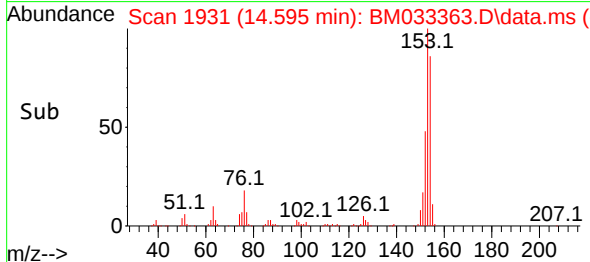


#53
2,4-Dinitrophenol
Concen: 26.898 ng/ul
RT: 14.654 min Scan# 1941
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

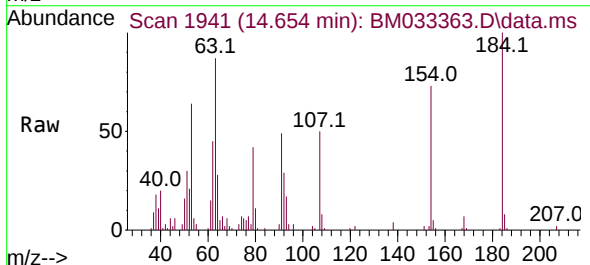


Tgt Ion:184 Resp: 28412
Ion Ratio Lower Upper
184 100
63 86.7 73.8 110.8
154 72.6 63.5 95.3

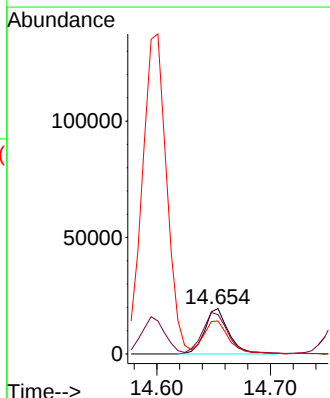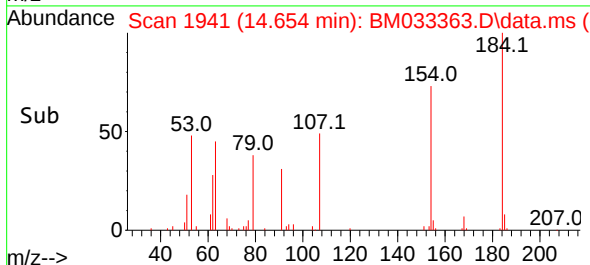



#55
4-Nitrophenol
Concen: 31.073 ng/ul
RT: 14.760 min Scan# 1942
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247



Tgt Ion:109 Resp: 57104
Ion Ratio Lower Upper
109 100
139 91.7 77.6 116.4
65 131.8 112.2 168.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#56
Dibenzofuran
Concen: 29.303 ng/ul
RT: 14.930 min Scan# 1988
Delta R.T. -0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Tgt Ion:168 Resp: 340878
Ion Ratio Lower Upper
168 100
139 42.5 34.0 51.0





#57
2,4-Dinitrotoluene
Concen: 31.944 ng/ul
RT: 14.901 min Scan# 1966
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Instrument :

BNA_M

ClientSampleId :





SLCS247

Tgt Ion:165 Resp: 84340
Ion Ratio Lower Upper
165 100
63 56.2 51.8 77.8
182 2.8 2.6 4.0

Manual Integrations




APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021

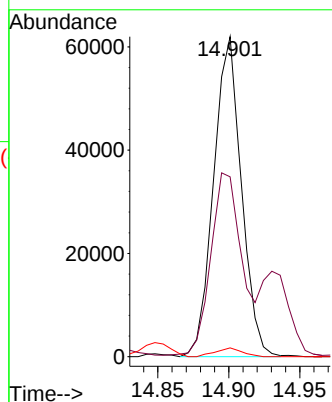

#58
2,3,4,6-Tetrachlorophenol
Concen: 31.758 ng/ul
RT: 15.160 min Scan# 2027
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00


Tgt Ion:232 Resp: 65011
Ion Ratio Lower Upper
232 100
131 51.4 41.4 62.2
130 2.8 2.0 3.0
166 30.8 27.4 41.0

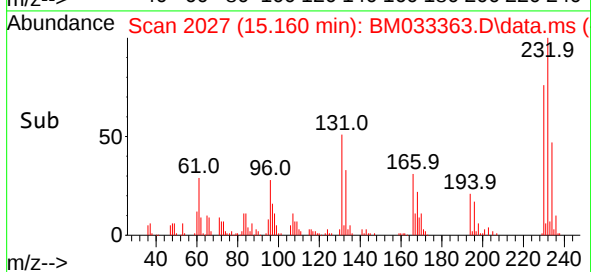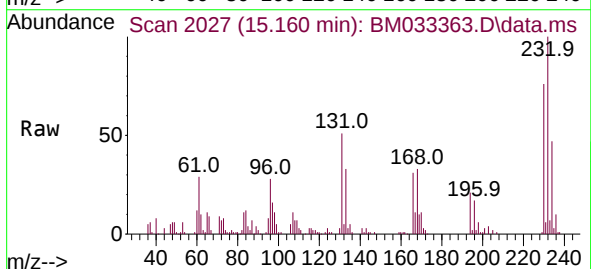



#59
Diethylphthalate
Concen: 30.560 ng/u1
RT: 15.348 min Scan# 2042
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247




Tgt Ion:149 Resp: 294915
Ion Ratio Lower Upper
149 100
177 20.4 17.1 25.7
150 12.2 9.9 14.9

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021




#61
Fluorene
Concen: 29.803 ng/u1
RT: 15.583 min Scan# 2099
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Tgt Ion:166 Resp: 285059
Ion Ratio Lower Upper
166 100
165 99.1 77.9 116.9
167 14.5 10.3 15.5





#62
 4-Chlorophenyl-phenylether
 Concen: 29.901 ng/ul
 RT: 15.571 min Scan# 2080
 Delta R.T. 0.000 min
 Lab File: BM033363.D
 Acq: 09 Dec 2021 18:00




Instrument :
 BNA_M
 ClientSampleId :
 SLCS247



Tgt Ion:204 Resp: 142668
 Ion Ratio Lower Upper
 204 100
 206 32.0 27.8 41.8
 141 67.4 54.9 82.3




Manual Integrations
 APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
 Supervised By :mohammad ahmed 12/15/2021



#63
 4-Nitroaniline
 Concen: 36.103 ng/ul
 RT: 15.607 min Scan# 2103
 Delta R.T. -0.006 min
 Lab File: BM033363.D
 Acq: 09 Dec 2021 18:00


Tgt Ion:138 Resp: 65592
 Ion Ratio Lower Upper
 138 100
 92 65.8 48.0 72.0
 108 113.9 89.5 134.3





#66
4,6-Dinitro-2-methylphenol
Concen: 24.797 ng/ul
RT: 15.660 min Scan# 2112
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247




Tgt Ion:198 Resp: 4263
Ion Ratio Lower Upper
198 100
182 5.4 4.2 6.2
77 35.6 26.3 39.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021




#67
N-Nitrosodiphenylamine
Concen: 28.642 ng/ul
RT: 15.789 min Scan# 2134
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Tgt Ion:169 Resp: 240844
Ion Ratio Lower Upper
169 100
168 66.8 52.9 79.3
167 37.1 29.9 44.9

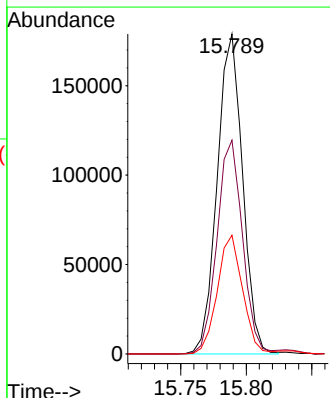



#68
4-Bromophenyl-phenylether
Concen: 28.274 ng/ul
RT: 16.465 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247




Tgt Ion:248 Resp: 8144
Ion Ratio Lower Upper
248 100
250 94.0 79.0 118.4
141 90.6 69.7 104.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021




#69
Hexachlorobenzene
Concen: 28.763 ng/ul
RT: 16.577 min Scan# 2268
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Tgt Ion:284 Resp: 95461
Ion Ratio Lower Upper
284 100
142 40.4 34.3 51.5
249 32.6 26.1 39.1

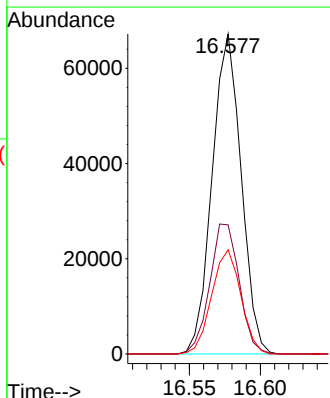



#70
Atrazine
Concen: 28.123 ng/ul
RT: 16.736 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247




Tgt Ion:200 Resp: 93834
Ion Ratio Lower Upper
200 100
173 26.3 20.6 30.8
215 46.9 36.9 55.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021




#71
Pentachlorophenol
Concen: 32.936 ng/ul
RT: 16.924 min Scan# 2327
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Tgt Ion:266 Resp: 61297
Ion Ratio Lower Upper
266 100
264 63.9 49.1 73.7
268 66.1 47.8 71.8





#72
Phenanthrene
Concen: 28.549 ng/u1
RT: 17.318 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247



Tgt Ion:178 Resp: 471015
Ion Ratio Lower Upper
178 100
179 15.5 11.7 17.5
176 19.3 15.1 22.7




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#74
Anthracene
Concen: 28.625 ng/u1
RT: 17.407 min Scan# 2409
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00


Tgt Ion:178 Resp: 478815
Ion Ratio Lower Upper
178 100
179 15.8 12.3 18.5
176 18.6 14.5 21.7

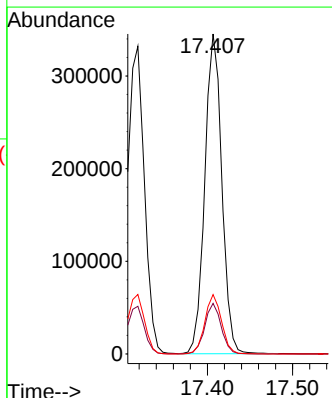



#75
1,2,3,4-Tetrachlorobenzene
Concen: 26.581 ng/uL
RT: 13.336 min Scan# 1700
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247




Tgt Ion:216 Resp: 109639
Ion Ratio Lower Upper
216 100
214 77.0 65.4 98.0
218 46.0 38.8 58.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021




#76
Pentachlorobenzene
Concen: 26.604 ng/uL
RT: 14.848 min Scan# 1974
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Tgt Ion:250 Resp: 108363
Ion Ratio Lower Upper
250 100
248 60.7 51.6 77.4
252 62.8 52.0 78.0

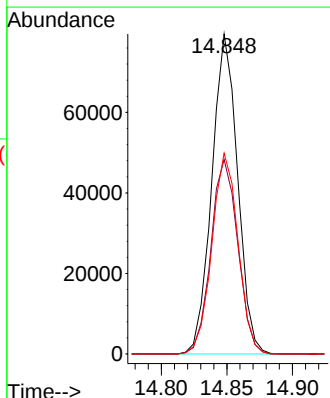



#77
Carbazole
Concen: 28.562 ng/ul
RT: 17.677 min Scan# 2439
Delta R.T. -0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247




Tgt Ion:167 Resp: 431820
Ion Ratio Lower Upper
167 100
166 21.3 16.9 25.3
139 13.6 10.5 15.7

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021




#78
Di-n-butylphthalate
Concen: 30.656 ng/ul
RT: 18.230 min Scan# 2549
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Tgt Ion:149 Resp: 520042
Ion Ratio Lower Upper
149 100
150 9.4 7.0 10.6
104 6.4 5.1 7.7

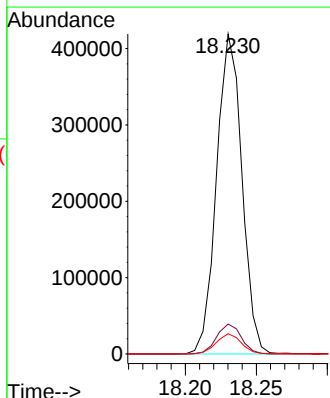



#80
Fluoranthene
Concen: 29.204 ng/u1
RT: 19.324 min Scan# 2718
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247



Tgt Ion:202 Resp: 570160
Ion Ratio Lower Upper
202 100
101 9.9 8.2 12.4
100 7.7 6.9 10.3




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#82
Pyrene
Concen: 29.299 ng/u1
RT: 19.689 min Scan# 2797
Delta R.T. 0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Tgt Ion:202 Resp: 598825
Ion Ratio Lower Upper
202 100
101 11.2 9.8 14.6
100 9.8 8.6 13.0

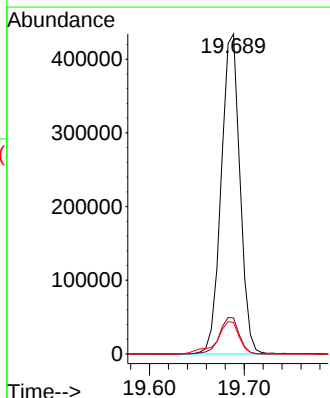



#83

Butylbenzylphthalate

Concen: 31.371 ng/ul

RT: 20.571 min Scan# 2930

Delta R.T. 0.000 min

Lab File: BM033363.D

Acq: 09 Dec 2021 18:00

Instrument :

BNA_M

ClientSampleId :

SLCS247

Tgt Ion:149 Resp: 245609

Ion Ratio Lower Upper

149 100





91 82.0 69.3 103.9

206 19.1 16.1 24.1

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021

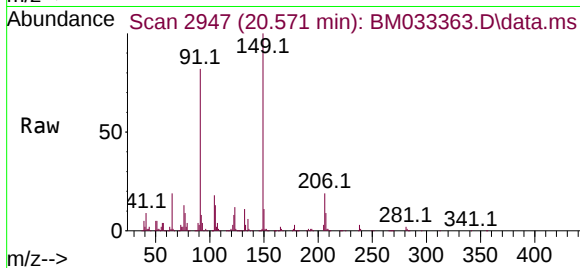

#84

3,3'-Dichlorobenzidine

Concen: 24.277 ng/ul

RT: 21.353 min Scan# 3080

Delta R.T. 0.000 min

Lab File: BM033363.D

Acq: 09 Dec 2021 18:00




Tgt Ion:252 Resp: 163525


Ion Ratio Lower Upper

252 100

254 64.4 49.4 74.2


126 12.0 8.2 12.4

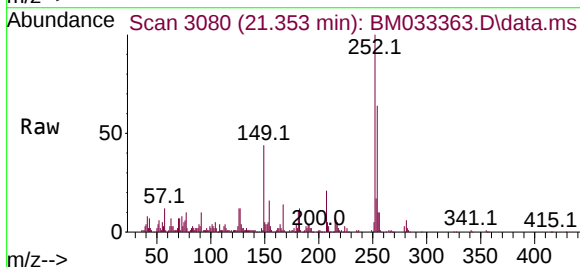



#85
Benzo(a)anthracene
Concen: 28.953 ng/ul
RT: 21.418 min Scan# 3074
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247



Tgt Ion:228 Resp: 563750
Ion Ratio Lower Upper
228 100
229 19.8 15.0 22.4
226 26.5 21.4 32.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#86
Bis(2-ethylhexyl)phthalate
Concen: 31.332 ng/ul
RT: 21.342 min Scan# 3078
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00


Tgt Ion:149 Resp: 352559
Ion Ratio Lower Upper
149 100
167 27.2 21.8 32.8
279 4.0 3.2 4.8





#87
Chrysene
Concen: 29.101 ng/ul
RT: 21.471 min Scan# 3100
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247



Tgt Ion:228 Resp: 556909
Ion Ratio Lower Upper
228 100
226 29.3 24.5 36.7
229 19.4 15.9 23.9




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#89
Di-n-octyl phthalate
Concen: 29.522 ng/ul
RT: 22.242 min Scan# 3231
Delta R.T. 0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Tgt Ion:149 Resp: 609285









#90
Benzo(b)fluoranthene
Concen: 29.486 ng/ul
RT: 23.053 min Scan# 3352
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00

Instrument :
BNA_M
ClientSampleId :
SLCS247

Tgt Ion:252 Resp: 56866
Ion Ratio Lower Upper
252 100
253 22.0 17.7 26.5
125 8.8 7.8 11.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#91
Benzo(k)fluoranthene
Concen: 30.247 ng/ul
RT: 23.100 min Scan# 3377
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00


Tgt Ion:252 Resp: 540114
Ion Ratio Lower Upper
252 100
253 21.3 17.6 26.4
125 8.6 7.4 11.2





#93
Benzo(a)pyrene
Concen: 29.826 ng/ul
RT: 23.659 min Scan# 3454
Delta R.T. 0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247




Tgt Ion:252 Resp: 55193
Ion Ratio Lower Upper
252 100
253 21.0 17.4 26.0
125 10.2 7.8 11.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021




#94
Indeno(1,2,3-cd)pyrene
Concen: 28.640 ng/ul
RT: 26.135 min Scan# 3893
Delta R.T. 0.000 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Tgt Ion:276 Resp: 576380
Ion Ratio Lower Upper
276 100
138 21.5 16.5 24.7
277 23.9 20.6 31.0

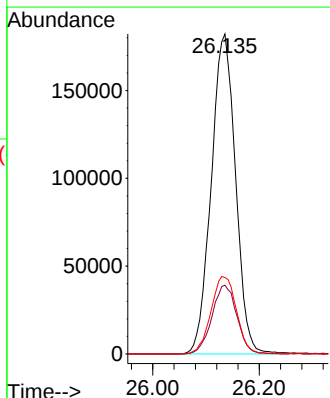



#95
Dibenzo(a,h)anthracene
Concen: 28.890 ng/ul
RT: 26.147 min Scan# 3877
Delta R.T. 0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00




Instrument :
BNA_M
ClientSampleId :
SLCS247




Tgt Ion:278 Resp: 50574
Ion Ratio Lower Upper
278 100
139 14.8 11.0 16.4
279 23.8 18.1 27.1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021



#96
Benzo(g,h,i)perylene
Concen: 28.949 ng/ul
RT: 26.865 min Scan# 4017
Delta R.T. 0.006 min
Lab File: BM033363.D
Acq: 09 Dec 2021 18:00



Tgt Ion:276 Resp: 496910
Ion Ratio Lower Upper
276 100
138 18.8 15.6 23.4
277 22.9 18.7 28.1

