

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033371.D
 Acq On : 09 Dec 2021 23:23
 Operator : CG/JU
 Sample : M4960-11DL3 1500X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGKS4DL3

Quant Time: Dec 10 01:16:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 09 13:25:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.907	152	46298	20.000	ng/ul	0.00
20) Naphthalene-d8	10.701	136	173719	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.530	164	108650	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.271	188	222151	20.000	ng/ul	0.00
79) Chrysene-d12	21.436	240	210604	20.000	ng/ul	0.00
88) Perylene-d12	23.753	264	220563	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	0.000	99	0	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	0.000	67	0	0.000	ng/ul	
11) 2-Chlorophenol-d4	0.000	132	0	0.000	ng/ul	
15) 4-Methylphenol-d8	0.000	113	0	0.000	ng/ul	
21) Nitrobenzene-d5	0.000	128	0	0.000	ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0	0.000	ng/ul	
31) 4-Chloroaniline-d4	0.000	131	0	0.000	ng/ul	
46) Dimethylphthalate-d6	0.000	166	0	0.000	ng/ul	
49) Acenaphthylene-d8	0.000	160	0	0.000	ng/ul	
54) 4-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
60) Fluorene-d10	0.000	176	0	0.000	ng/ul	
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/ul	
73) Anthracene-d10	0.000	188	0d	0.000	ng/ul	
81) Pyrene-d10	0.000	212	0d	0.000	ng/ul	
92) Benzo(a)pyrene-d12	0.000	264	0d	0.000	ng/ul	
Target Compounds						
32) 4-Chloroaniline	10.866	127	159343	39.126	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033371.D
Acq On : 09 Dec 2021 23:23
Operator : CG/JU
Sample : M4960-11DL3 1500X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGKS4DL3

Quant Time: Dec 10 01:16:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 09 13:25:37 2021
Response via : Initial Calibration

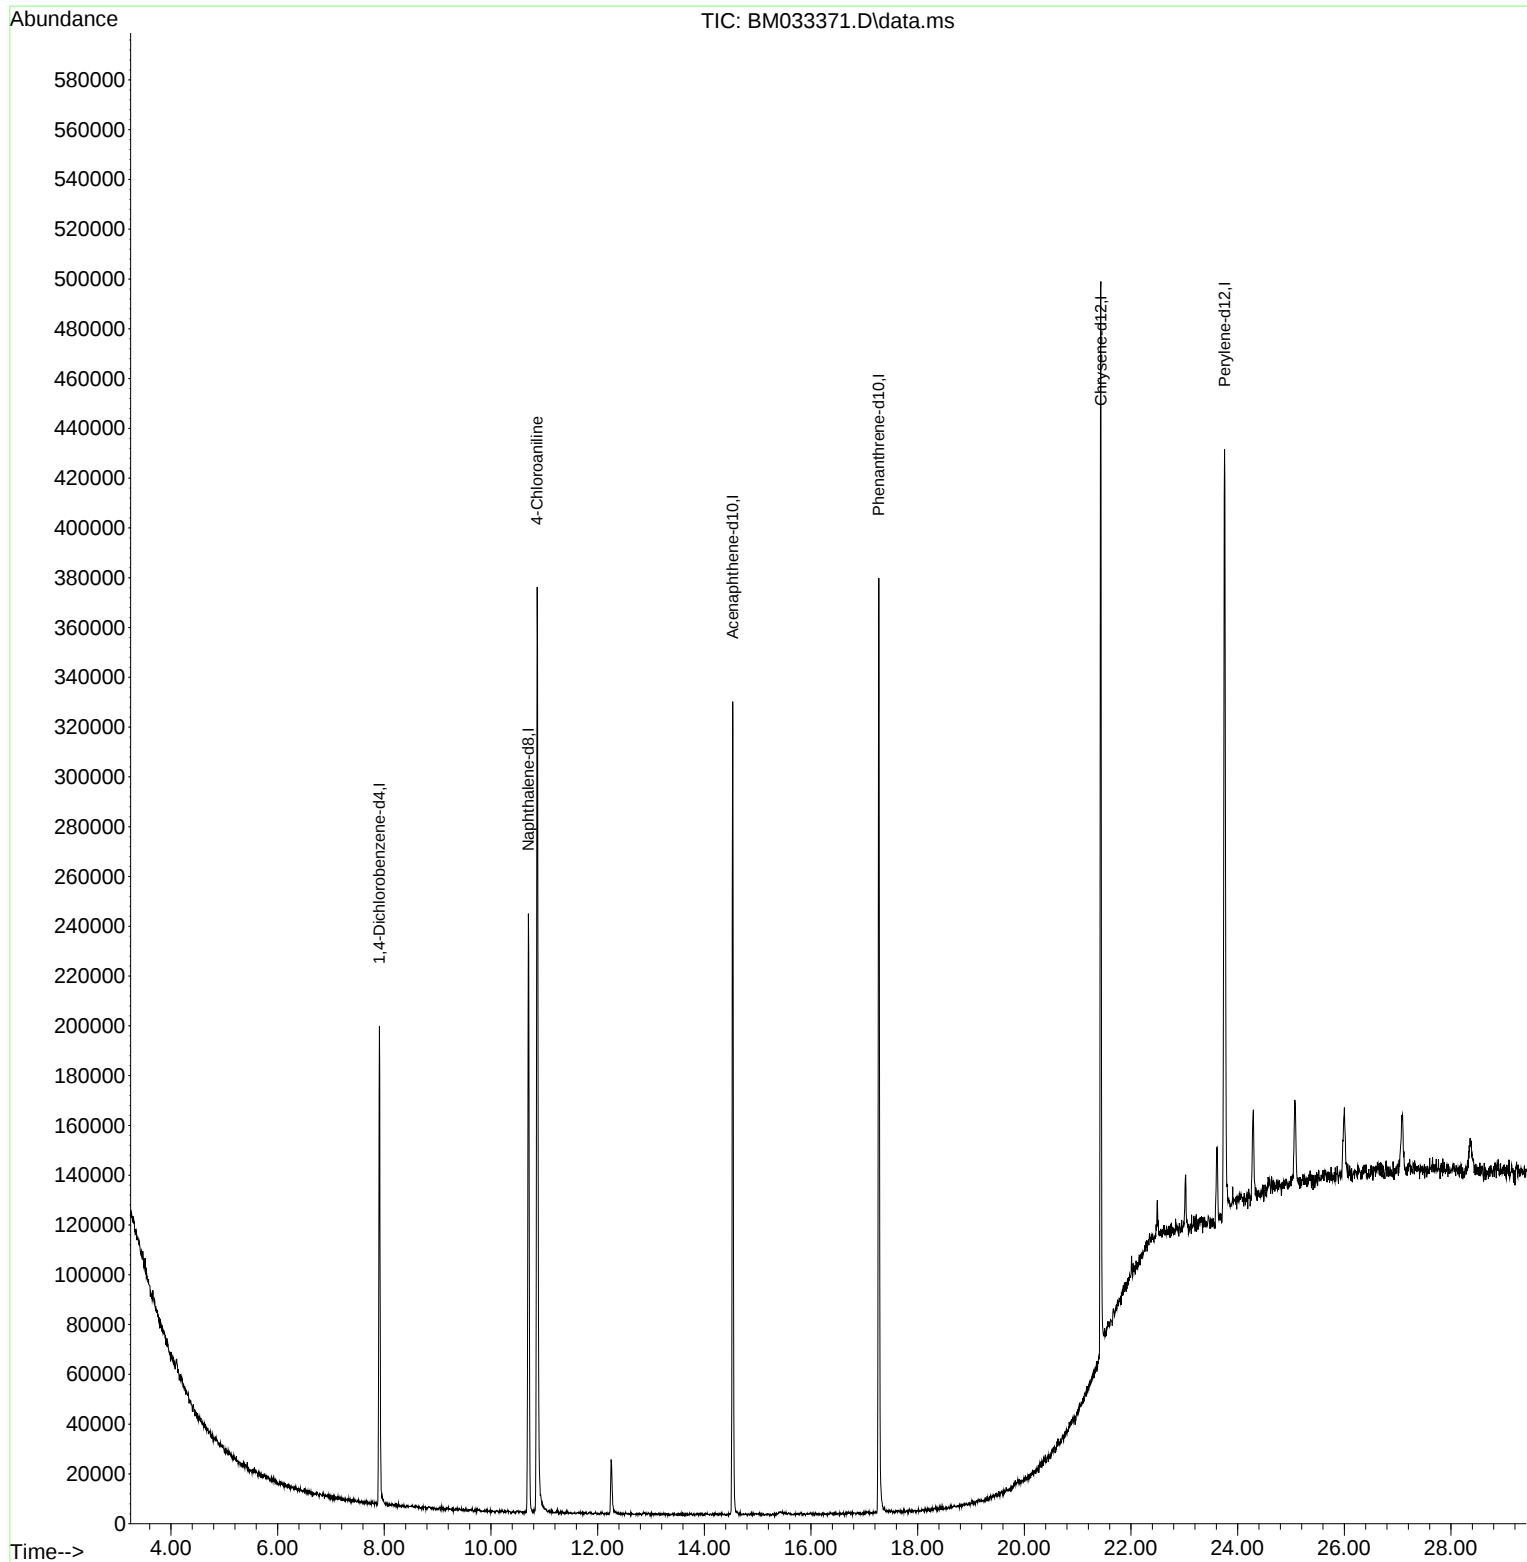

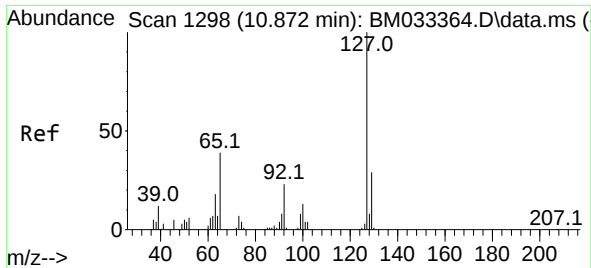

#32
 4-Chloroaniline
 Concen: 39.126 ng/ul
 RT: 10.866 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BM033371.D
 Acq: 09 Dec 2021 23:23

Instrument :
 BNA_M
 ClientSampleId :
 BGKS4DL3

Tgt Ion:127 Resp: 159343
 Ion Ratio Lower Upper
 127 100
 129 32.8 25.4 38.0

