

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033383.D
 Acq On : 10 Dec 2021 07:09
 Operator : CG/JU
 Sample : M4985-06
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5M9

Quant Time: Dec 10 12:57:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 09 13:25:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.907	152	59209	20.000	ng/ul	0.00
20) Naphthalene-d8	10.701	136	233916	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.530	164	150565	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.271	188	325320	20.000	ng/ul	0.00
79) Chrysene-d12	21.430	240	356492	20.000	ng/ul	0.00
88) Perylene-d12	23.753	264	353884	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.366	96	7033	4.464	ng/uL	0.00
4) Pyridine-d5	3.790	84	26134	5.721	ng/ul	0.00
7) Phenol-d5	7.078	99	30247	5.395	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.237	67	98849	26.930	ng/ul	0.00
11) 2-Chlorophenol-d4	7.442	132	82350	20.979	ng/ul	0.00
15) 4-Methylphenol-d8	8.613	113	54098	12.327	ng/ul	0.00
21) Nitrobenzene-d5	9.066	128	52629	27.728	ng/ul	0.00
24) 2-Nitrophenol-d4	9.789	143	52587	27.005	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.325	165	89380	24.287	ng/ul	0.00
31) 4-Chloroaniline-d4	10.842	131	85686	15.704	ng/ul	0.00
46) Dimethylphthalate-d6	13.942	166	334583	29.741	ng/ul	0.00
49) Acenaphthylene-d8	14.224	160	417482	29.936	ng/ul	0.00
54) 4-Nitrophenol-d4	14.765	143	5112	2.503	ng/ul	0.02
60) Fluorene-d10	15.518	176	297487	29.563	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.636	200	33913	17.272	ng/ul	0.00
73) Anthracene-d10	17.365	188	506004	31.472	ng/ul	0.00
81) Pyrene-d10	19.653	212	631351	31.688	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.606	264	590769	30.799	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.402	88	4006	2.284	ng/ul#	82
86) Bis(2-ethylhexyl)phtha...	21.336	149	73389	5.422	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033383.D
Acq On : 10 Dec 2021 07:09
Operator : CG/JU
Sample : M4985-06
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW5M9

Quant Time: Dec 10 12:57:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 09 13:25:37 2021
Response via : Initial Calibration




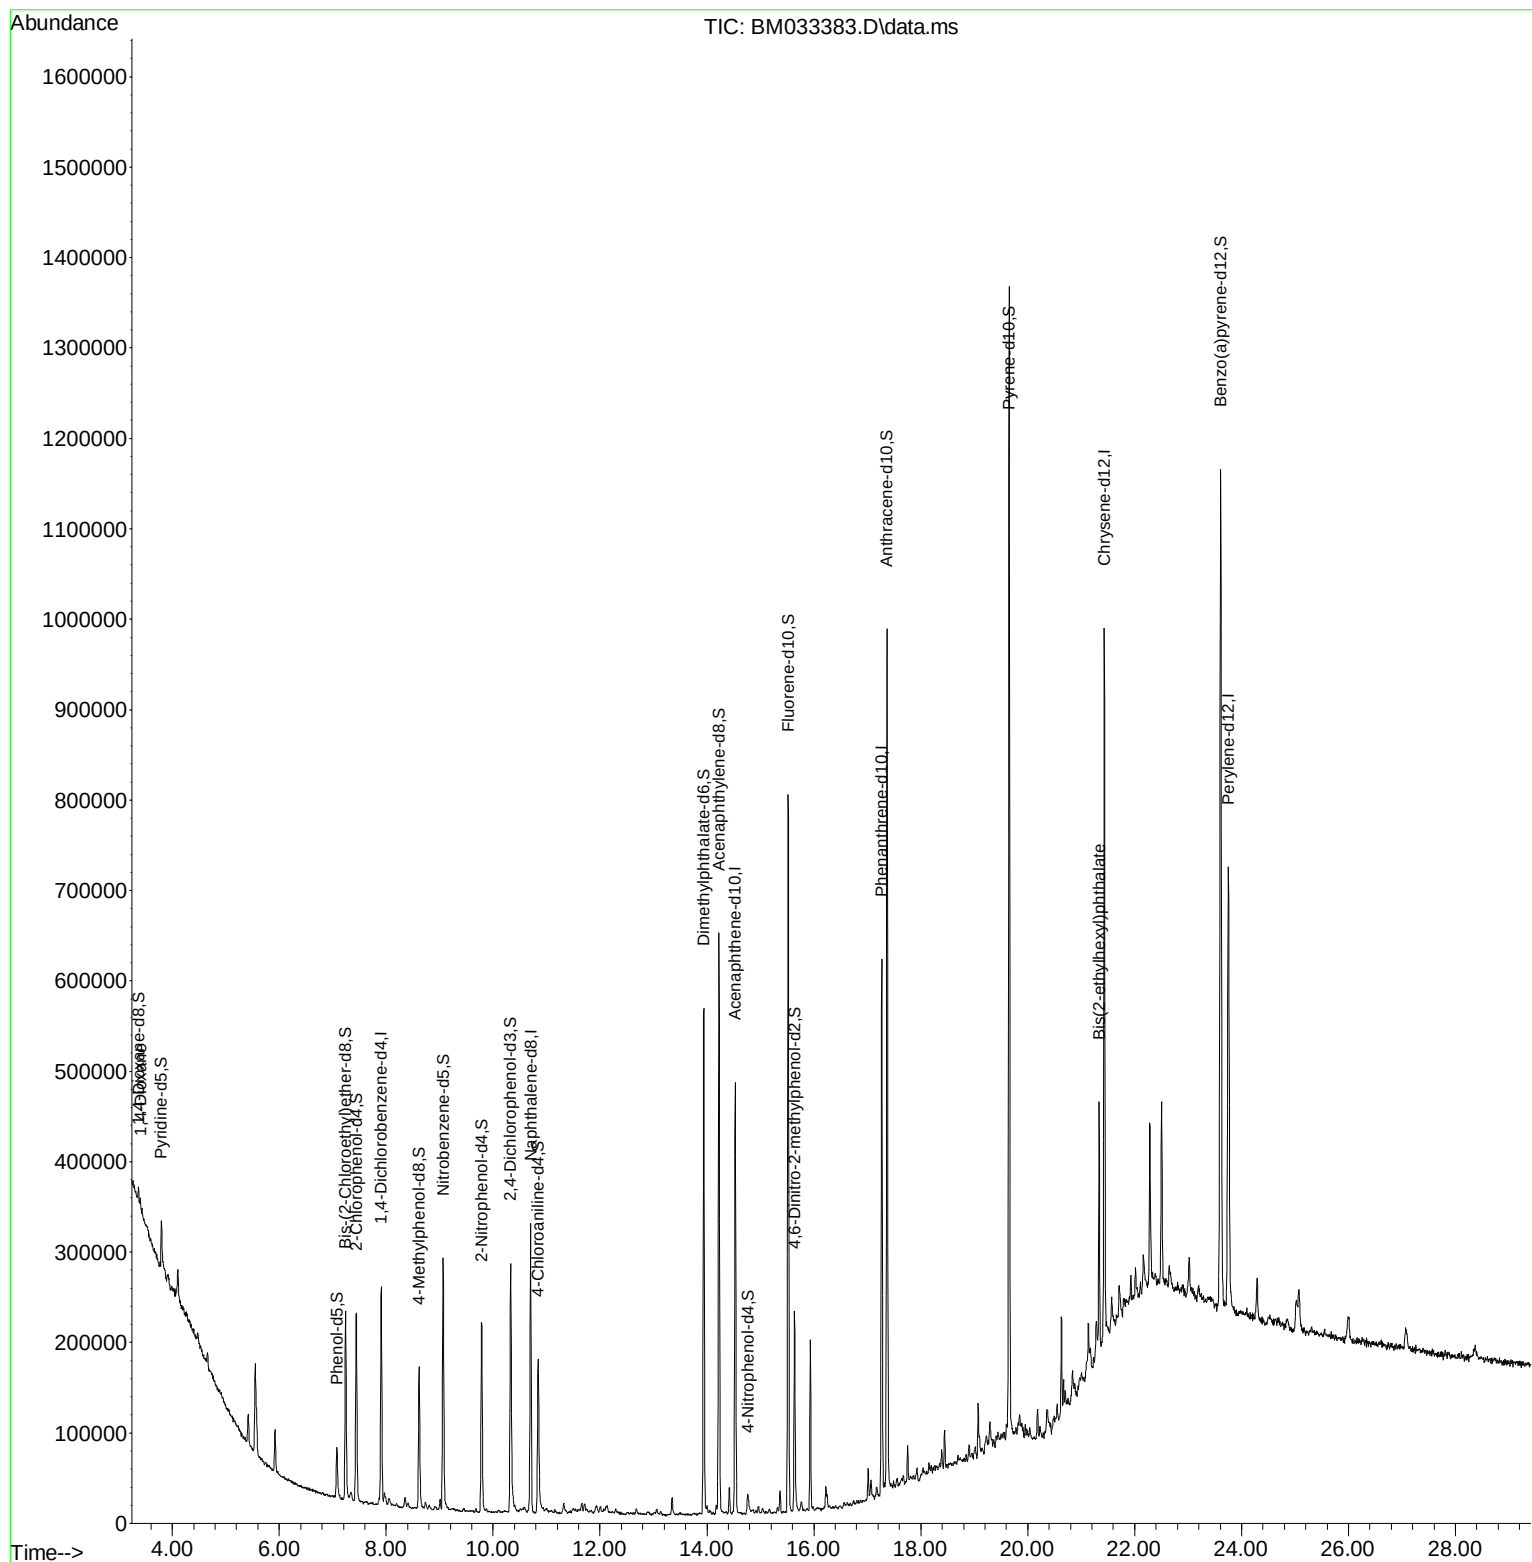


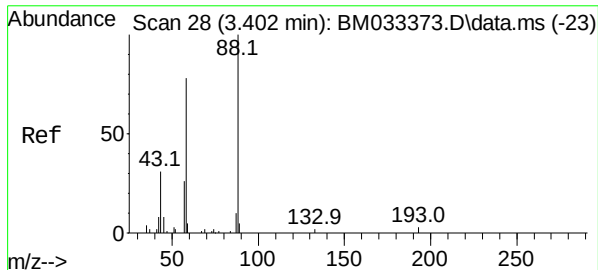

1,4-Dioxane
 Concen: 2.284 ng/uL
 RT: 3.402 min Scan# 21
 Delta R.T. 0.001 min
 Lab File: BM033383.D
 Acq: 10 Dec 2021 07:09

Instrument :
 BNA_M
 ClientSampleId :
 EW5M9

Tgt Ion: 88 Resp: 4006
 Ion Ratio Lower Upper
 88 100
 43 45.8 36.2 54.4
 58 60.3 68.5 102.7#

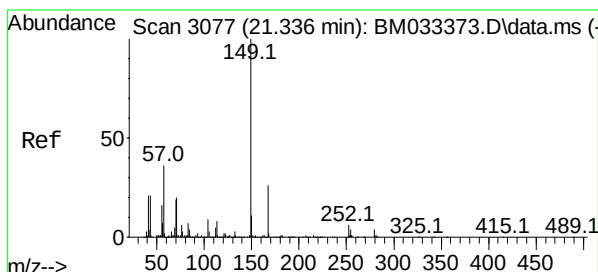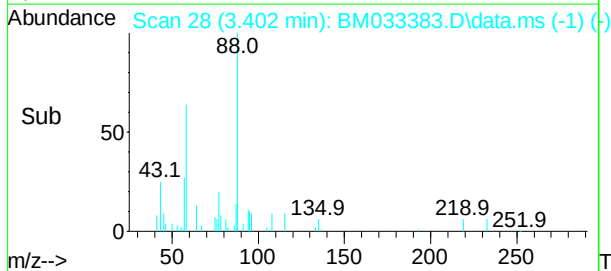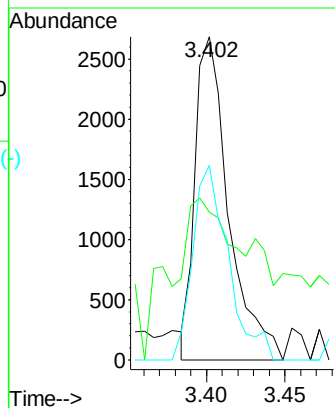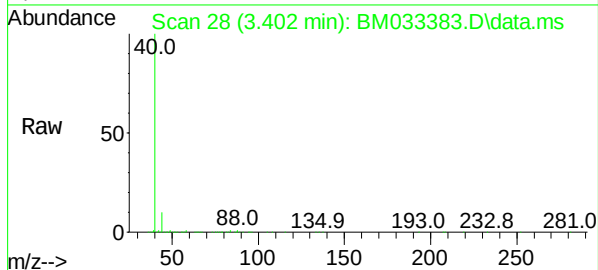

Bis(2-ethylhexyl)phthalate
 Concen: 5.422 ng/uL
 RT: 21.336 min Scan# 3077
 Delta R.T. -0.006 min
 Lab File: BM033383.D
 Acq: 10 Dec 2021 07:09

Tgt Ion: 149 Resp: 73389
 Ion Ratio Lower Upper
 149 100
 167 28.1 21.8 32.8
 279 3.9 3.2 4.8

