

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033384.D
 Acq On : 10 Dec 2021 07:45
 Operator : CG/JU
 Sample : M4985-02
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5P8

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/10/2021
 Supervised By :mohammad ahmed 12/15/2021

Quant Time: Dec 10 12:57:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 09 13:25:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.907	152	53638	20.000	ng/ul	0.00
20) Naphthalene-d8	10.701	136	216111	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.530	164	136936	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.271	188	304818	20.000	ng/ul	0.00
79) Chrysene-d12	21.430	240	345120	20.000	ng/ul	0.00
88) Perylene-d12	23.753	264	342059	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.366	96	7592	5.319	ng/uL	0.00
4) Pyridine-d5	3.796	84	20018m	4.837	ng/ul	0.01
7) Phenol-d5	7.078	99	33216	6.540	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.237	67	105385	31.693	ng/ul	0.00
11) 2-Chlorophenol-d4	7.442	132	90673	25.498	ng/ul	0.00
15) 4-Methylphenol-d8	8.613	113	59166	14.882	ng/ul	0.00
21) Nitrobenzene-d5	9.066	128	56134	32.012	ng/ul	0.00
24) 2-Nitrophenol-d4	9.783	143	55109	30.631	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.325	165	95432	28.068	ng/ul	0.00
31) 4-Chloroaniline-d4	10.842	131	102466	20.327	ng/ul	0.00
46) Dimethylphthalate-d6	13.942	166	365341	35.707	ng/ul	0.00
49) Acenaphthylene-d8	14.224	160	452702	35.692	ng/ul	0.00
54) 4-Nitrophenol-d4	14.771	143	5755m	3.098	ng/ul	0.02
60) Fluorene-d10	15.518	176	328796	35.927	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.642	200	37684	20.483	ng/ul	0.00
73) Anthracene-d10	17.365	188	583482	38.732	ng/ul	0.00
81) Pyrene-d10	19.653	212	741129	38.423	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.606	264	723510	39.023	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.402	88	2753	1.733	ng/uL#	71
86) Bis(2-ethylhexyl)phtha...	21.336	149	84039	6.413	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033384.D
Acq On : 10 Dec 2021 07:45
Operator : CG/JU
Sample : M4985-02
Misc :
ALS Vial : 39 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EW5P8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021

Quant Time: Dec 10 12:57:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 09 13:25:37 2021
Response via : Initial Calibration

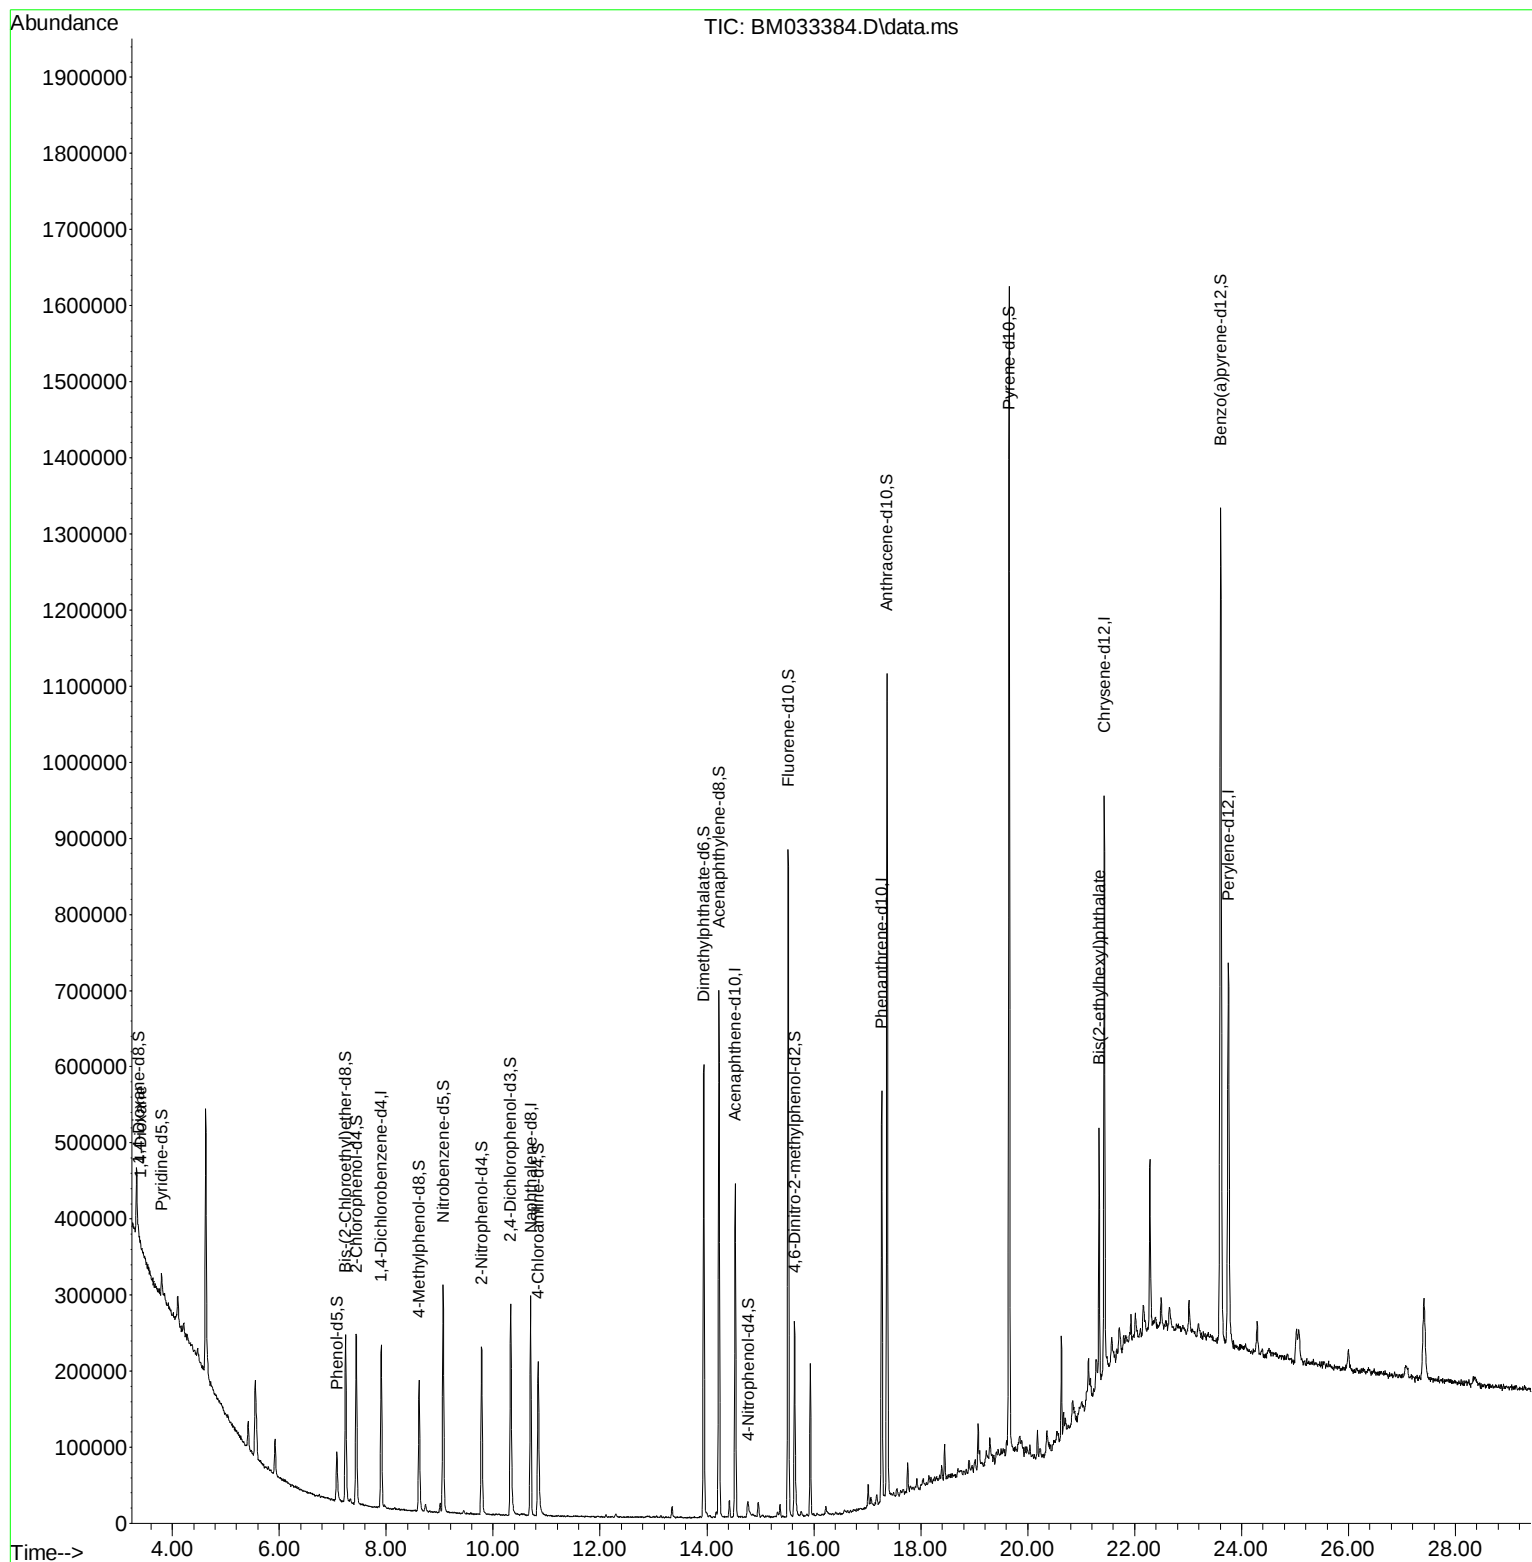

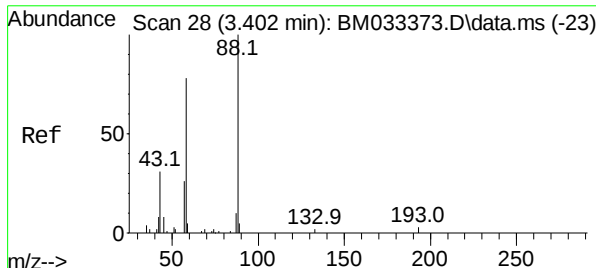





1,4-Dioxane
Concen: 1.733 ng/uL
RT: 3.402 min Scan# 21
Delta R.T. 0.001 min
Lab File: BM033384.D
Acq: 10 Dec 2021 07:45

Instrument :
BNA_M
ClientSampleId :
EW5P8

Tgt Ion:	88	Resp:	279
Ion	Ratio	Lower	Upper
88	100		
43	62.3	36.2	54.4
58	57.5	68.5	102.7

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :mohammad ahmed 12/15/2021

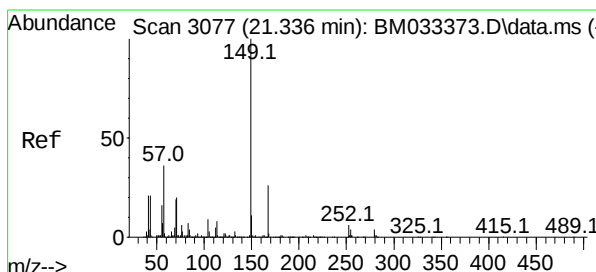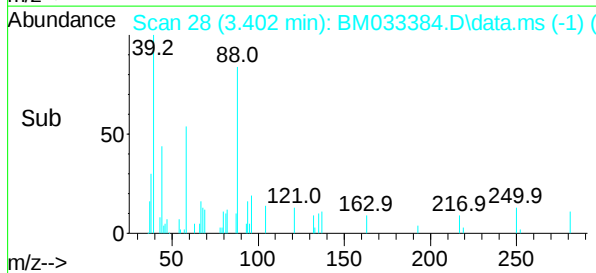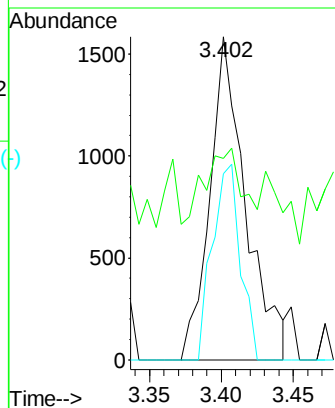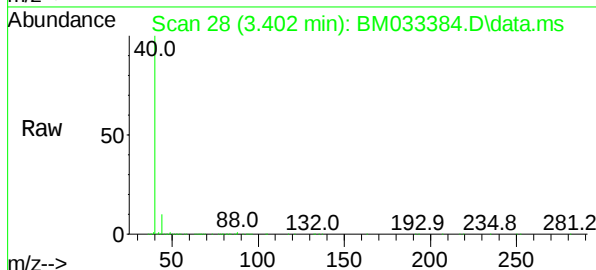

Bis(2-ethylhexyl)phthalate
Concen: 6.413 ng/uL
RT: 21.336 min Scan# 3077
Delta R.T. -0.006 min
Lab File: BM033384.D
Acq: 10 Dec 2021 07:45

Tgt Ion:	149	Resp:	84039
Ion	Ratio	Lower	Upper
149	100		
167	28.6	21.8	32.8
279	4.1	3.2	4.8

