

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033357.D
 Acq On : 09 Dec 2021 14:24
 Operator : CG/JU
 Sample : PB141247BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033357.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.366	19	22	29	rVB2	13980	20252	2.16%	0.194%
2	3.784	89	93	108	rBV	151453	243469	25.99%	2.337%
3	4.578	226	228	229	rBV2	1847	1318	0.14%	0.013%
4	5.113	317	319	325	rBV3	1238	2393	0.26%	0.023%
5	5.249	340	342	347	rVB4	1807	2356	0.25%	0.023%
6	5.643	408	409	411	rBV	1664	1181	0.13%	0.011%
7	5.890	449	451	453	rBV2	1076	1299	0.14%	0.012%
8	6.007	470	471	473	rBV	1278	1156	0.12%	0.011%
9	6.043	476	477	480	rBV3	1300	1027	0.11%	0.010%
10	6.137	491	493	495	rVV	1815	1154	0.12%	0.011%
11	6.166	495	498	500	rVB	1581	1613	0.17%	0.015%
12	6.460	546	548	549	rBV	1632	1181	0.13%	0.011%
13	6.884	619	620	623	rBV2	1493	1522	0.16%	0.015%
14	6.937	628	629	633	rVB2	988	1044	0.11%	0.010%
15	7.078	647	653	663	rBV	196954	326357	34.84%	3.132%
16	7.148	663	665	667	rVB2	1139	1167	0.12%	0.011%
17	7.243	675	681	690	rBV	137253	226850	24.21%	2.177%
18	7.396	705	707	708	rBV	1325	1298	0.14%	0.012%
19	7.443	709	715	726	rVB	192911	314944	33.62%	3.023%
20	7.554	731	734	736	rBV2	1268	1298	0.14%	0.012%
21	7.572	736	737	742	rVB2	1590	1728	0.18%	0.017%
22	7.613	742	744	746	rBV2	1273	1243	0.13%	0.012%
23	7.713	759	761	765	rVB5	1080	1309	0.14%	0.013%
24	7.907	785	794	804	rBV	143288	240107	25.63%	2.304%
25	8.201	842	844	846	rVB3	1522	1234	0.13%	0.012%
26	8.231	846	849	852	rBV3	1548	1942	0.21%	0.019%
27	8.390	873	876	880	rBV3	659	1117	0.12%	0.011%
28	8.619	908	915	925	rBV	213594	366675	39.14%	3.519%
29	8.707	929	930	934	rVB4	1585	1710	0.18%	0.016%
30	8.795	942	945	946	rVB2	1609	1079	0.12%	0.010%
31	9.072	985	992	1002	rBV	190051	329514	35.17%	3.162%
32	9.290	1027	1029	1032	rBV3	1294	1579	0.17%	0.015%
33	9.401	1046	1048	1051	rVB2	1166	1030	0.11%	0.010%
34	9.719	1100	1102	1105	rVB3	1033	1105	0.12%	0.011%
35	9.789	1108	1114	1125	rVB	153461	264401	28.22%	2.537%
36	9.907	1132	1134	1137	rBV2	1057	1201	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033357.D
 Acq On : 09 Dec 2021 14:24
 Operator : CG/JU
 Sample : PB141247BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

37	10.331	1200	1206	1218	rBV	192992	349026	37.26%	3.350%
38	10.707	1260	1270	1278	rBV	184959	316934	33.83%	3.042%
39	10.784	1281	1283	1286	rBV2	1146	1305	0.14%	0.013%
40	10.848	1286	1294	1306	rBV	183758	368548	39.34%	3.537%
41	11.089	1332	1335	1338	rBV4	1054	1307	0.14%	0.013%
42	11.260	1356	1364	1366	rVB3	901	1942	0.21%	0.019%
43	11.325	1373	1375	1380	rVV4	1161	1796	0.19%	0.017%
44	11.372	1380	1383	1386	rVB2	1119	1615	0.17%	0.015%
45	11.525	1407	1409	1412	rBV2	849	1077	0.11%	0.010%
46	11.989	1486	1488	1495	rVV2	903	1575	0.17%	0.015%
47	12.283	1537	1538	1540	rBV2	1432	1116	0.12%	0.011%
48	12.301	1540	1541	1543	rVV2	1654	1706	0.18%	0.016%
49	12.325	1543	1545	1547	rVB3	1672	1361	0.15%	0.013%
50	12.483	1570	1572	1575	rVV2	849	1168	0.12%	0.011%
51	12.607	1590	1593	1595	rBV3	999	1143	0.12%	0.011%
52	12.836	1630	1632	1634	rVB	1161	1033	0.11%	0.010%
53	12.854	1634	1635	1638	rBV2	1255	1167	0.12%	0.011%
54	13.436	1731	1734	1735	rBV3	956	1065	0.11%	0.010%
55	13.472	1738	1740	1743	rVB	1208	1040	0.11%	0.010%
56	13.513	1743	1747	1748	rBV2	1466	1713	0.18%	0.016%
57	13.942	1814	1820	1831	rVV	377084	533378	56.93%	5.119%
58	14.019	1831	1833	1836	rVB4	1386	1393	0.15%	0.013%
59	14.230	1862	1869	1878	rBV	414540	603348	64.40%	5.790%
60	14.289	1878	1879	1883	rVV2	1156	1422	0.15%	0.014%
61	14.395	1894	1897	1899	rVB3	1082	1056	0.11%	0.010%
62	14.536	1915	1921	1929	rBV	269907	402529	42.97%	3.863%
63	14.748	1951	1957	1974	rBV	102812	227536	24.29%	2.184%
64	14.860	1974	1976	1981	rVB4	2618	3342	0.36%	0.032%
65	14.960	1992	1993	1996	rVV2	1657	1587	0.17%	0.015%
66	15.524	2083	2089	2099	rBV	509620	735726	78.53%	7.061%
67	15.642	2103	2109	2120	rVV	143617	220593	23.55%	2.117%
68	15.713	2120	2121	2123	rVV	2127	1182	0.13%	0.011%
69	15.901	2151	2153	2157	rBV2	909	1095	0.12%	0.011%
70	15.942	2157	2160	2162	rBV2	1455	1800	0.19%	0.017%
71	16.013	2169	2172	2173	rBV3	1421	1189	0.13%	0.011%
72	16.089	2182	2185	2186	rBV3	1697	1715	0.18%	0.016%
73	16.666	2281	2283	2286	rVB3	1164	1215	0.13%	0.012%
74	16.695	2286	2288	2290	rBV3	883	1125	0.12%	0.011%
75	16.742	2295	2296	2299	rVV2	1250	1181	0.13%	0.011%
76	16.795	2302	2305	2308	rVV4	756	1046	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033357.D
 Acq On : 09 Dec 2021 14:24
 Operator : CG/JU
 Sample : PB141247BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

77	17.007	2338	2341	2344	rBV4	937	1434	0.15%	0.014%
78	17.160	2365	2367	2370	rVB2	1259	1124	0.12%	0.011%
79	17.271	2381	2386	2394	rBV	317757	471781	50.36%	4.528%
80	17.371	2397	2403	2415	rBV	551663	801017	85.50%	7.687%
81	17.795	2472	2475	2477	rVB2	1017	1180	0.13%	0.011%
82	17.942	2498	2500	2502	rVV2	1571	1041	0.11%	0.010%
83	17.971	2502	2505	2506	rVV3	1115	1246	0.13%	0.012%
84	17.983	2506	2507	2511	rVB3	1522	1249	0.13%	0.012%
85	18.148	2532	2535	2536	rBV	1266	1362	0.15%	0.013%
86	18.212	2543	2546	2548	rBV2	1067	1117	0.12%	0.011%
87	18.283	2554	2558	2559	rVB3	1113	1259	0.13%	0.012%
88	18.295	2559	2560	2563	rBV3	1547	1444	0.15%	0.014%
89	18.342	2567	2568	2571	rBV3	1172	1150	0.12%	0.011%
90	18.595	2610	2611	2613	rBV2	1522	1337	0.14%	0.013%
91	18.659	2619	2622	2624	rBV4	1191	1353	0.14%	0.013%
92	18.701	2627	2629	2631	rVB3	1794	1485	0.16%	0.014%
93	19.071	2689	2692	2694	rBV3	2780	3042	0.32%	0.029%
94	19.230	2714	2719	2722	rBV6	5113	7792	0.83%	0.075%
95	19.295	2726	2730	2733	rBV3	5361	8140	0.87%	0.078%
96	19.377	2743	2744	2746	rBV2	1816	1502	0.16%	0.014%
97	19.659	2786	2792	2801	rBV	651424	936830	100.00%	8.991%
98	21.436	3089	3094	3103	rBV	398900	538025	57.43%	5.163%
99	23.612	3457	3464	3472	rBV	476150	936073	99.92%	8.984%
100	23.759	3483	3489	3501	rVB	257461	526961	56.25%	5.057%


Sum of corrected areas: 10419892

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033357.D
Acq On : 09 Dec 2021 14:24
Operator : CG/JU
Sample : PB141247BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK247

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

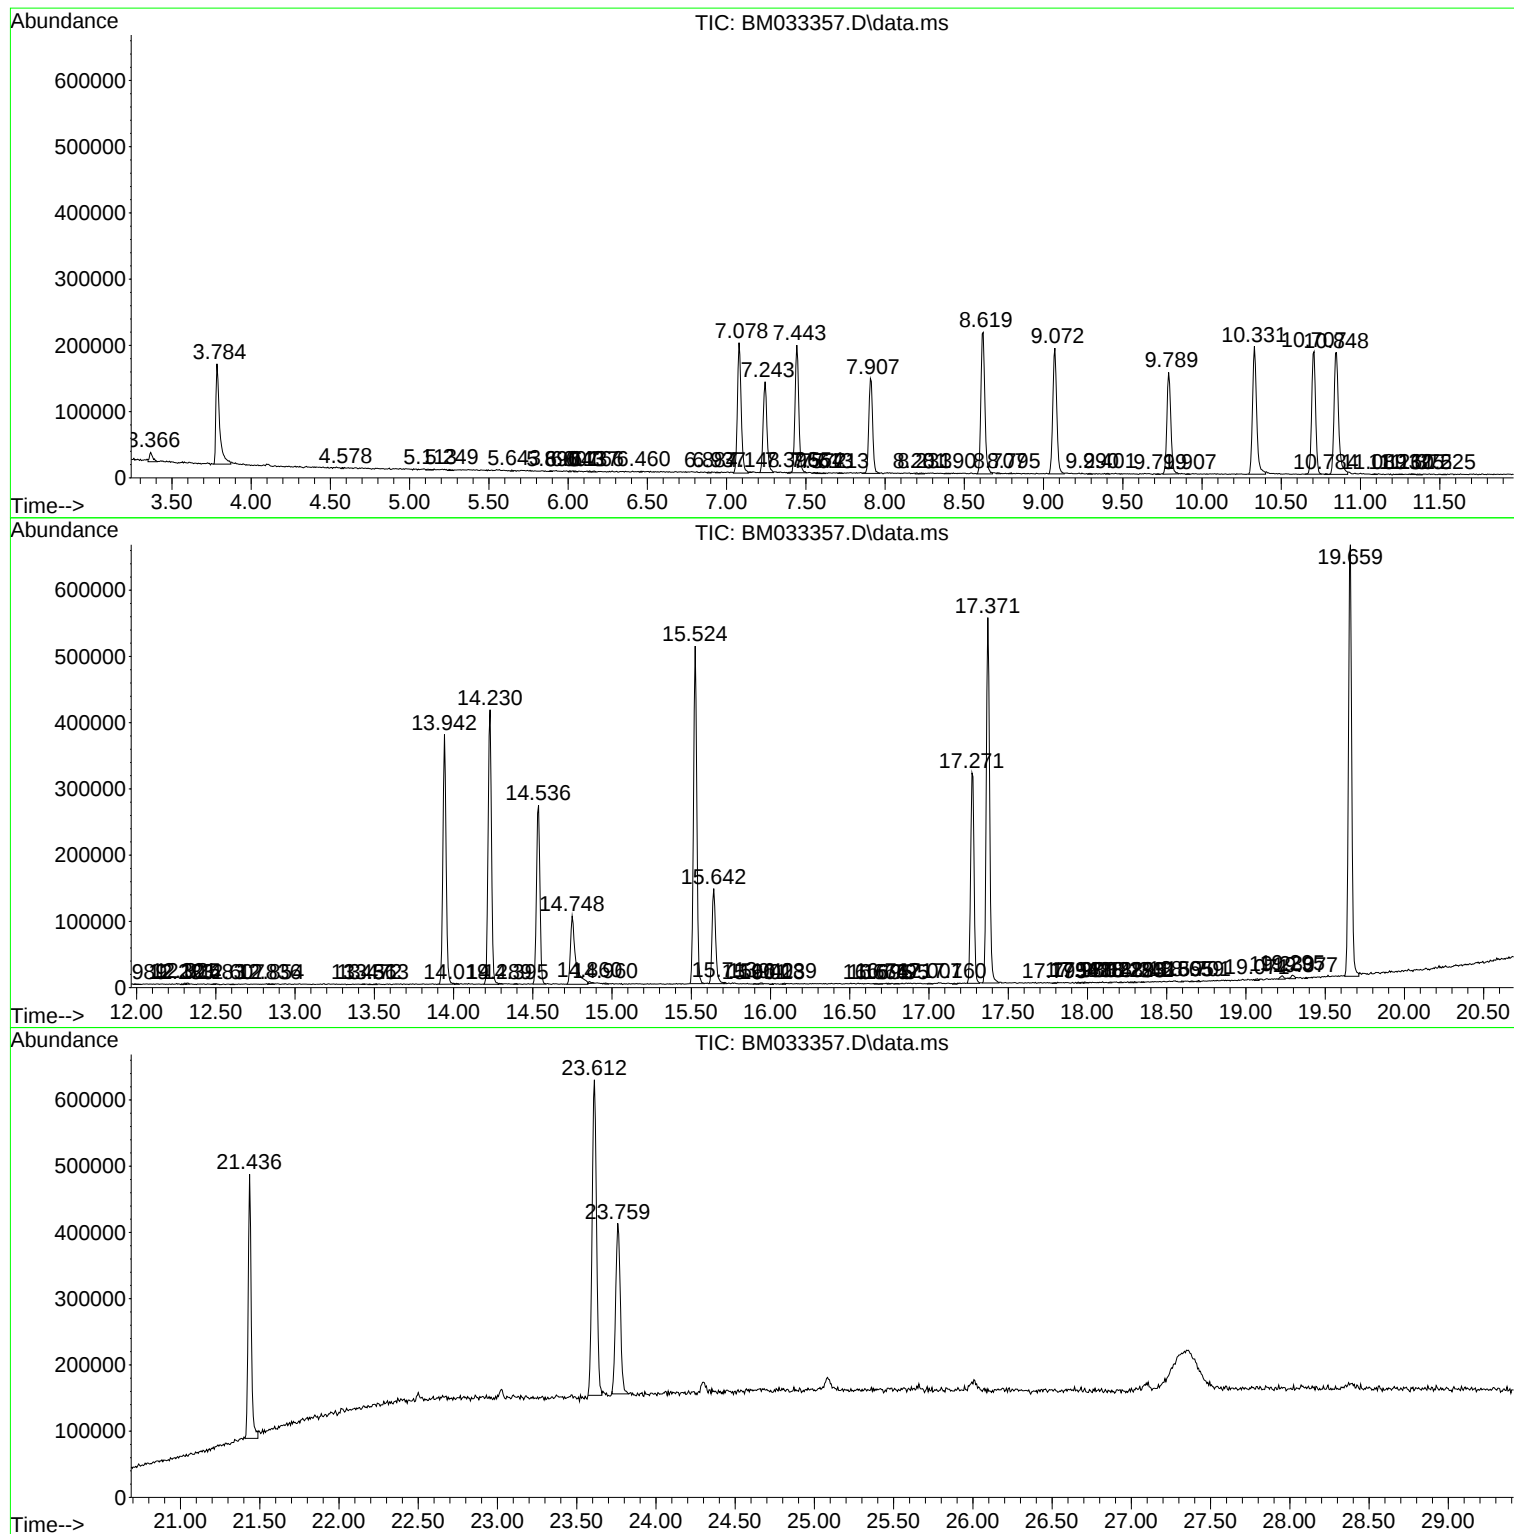

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033357.D
Acq On : 09 Dec 2021 14:24
Operator : CG/JU
Sample : PB141247BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK247

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033357.D
Acq On : 09 Dec 2021 14:24
Operator : CG/JU
Sample : PB141247BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK247

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc