

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033365.D
 Acq On : 09 Dec 2021 19:48
 Operator : CG/JU
 Sample : PB141232BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.784	90	93	105	rBV	161989	248424	25.69%	2.194%
2	6.490	552	553	555	rVB	1731	1181	0.12%	0.010%
3	6.548	561	563	566	rBV3	1094	1519	0.16%	0.013%
4	6.960	629	633	634	rBV	2480	2528	0.26%	0.022%
5	7.078	647	653	662	rVV	210136	343228	35.50%	3.031%
6	7.243	675	681	690	rBV	146000	242985	25.13%	2.146%
7	7.442	709	715	724	rVV	207288	336651	34.82%	2.973%
8	7.531	728	730	734	rVB5	1334	1422	0.15%	0.013%
9	7.742	765	766	770	rVV2	1610	1578	0.16%	0.014%
10	7.778	770	772	775	rVB3	1369	1578	0.16%	0.014%
11	7.907	788	794	802	rBV	178199	293879	30.39%	2.595%
12	8.166	836	838	844	rVB4	1495	1485	0.15%	0.013%
13	8.460	886	888	893	rBV4	1521	1559	0.16%	0.014%
14	8.619	905	915	924	rBV	234290	398584	41.22%	3.520%
15	8.889	958	961	962	rBV2	1473	1455	0.15%	0.013%
16	9.072	983	992	1001	rBV	200687	351668	36.37%	3.105%
17	9.360	1039	1041	1045	rVV2	1089	1187	0.12%	0.010%
18	9.401	1045	1048	1053	rVB2	1482	2512	0.26%	0.022%
19	9.442	1053	1055	1057	rBV3	1481	1203	0.12%	0.011%
20	9.572	1075	1077	1082	rBV2	1279	1660	0.17%	0.015%
21	9.625	1082	1086	1092	rVB3	1361	2385	0.25%	0.021%
22	9.725	1100	1103	1108	rBV4	1031	1607	0.17%	0.014%
23	9.789	1108	1114	1125	rVV	170764	290273	30.02%	2.563%
24	9.866	1125	1127	1130	rVB2	1276	1364	0.14%	0.012%
25	9.984	1145	1147	1150	rVB2	1171	1349	0.14%	0.012%
26	10.331	1199	1206	1222	rBV	207213	383201	39.63%	3.384%
27	10.631	1253	1257	1259	rBV2	790	1092	0.11%	0.010%
28	10.701	1261	1269	1276	rBV	226040	389894	40.32%	3.443%
29	10.848	1287	1294	1308	rBV	202809	398251	41.19%	3.517%
30	10.978	1315	1316	1321	rVB2	1519	1924	0.20%	0.017%
31	11.013	1321	1322	1325	rVV3	1473	1470	0.15%	0.013%
32	11.054	1328	1329	1332	rVV2	1062	1074	0.11%	0.009%
33	11.142	1340	1344	1345	rVV2	1495	1454	0.15%	0.013%
34	11.160	1345	1347	1351	rVV4	1171	1578	0.16%	0.014%
35	11.201	1351	1354	1357	rVV3	889	1239	0.13%	0.011%
36	11.454	1396	1397	1401	rVB2	1445	1418	0.15%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033365.D
 Acq On : 09 Dec 2021 19:48
 Operator : CG/JU
 Sample : PB141232BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

37	11.501	1401	1405	1407	rBV2	1042	1160	0.12%	0.010%
38	11.654	1426	1431	1433	rBV4	700	1146	0.12%	0.010%
39	11.795	1452	1455	1460	rVV2	1143	1291	0.13%	0.011%
40	12.289	1537	1539	1540	rVV	1700	1155	0.12%	0.010%
41	12.313	1540	1543	1546	rVV3	2683	3764	0.39%	0.033%
42	12.501	1572	1575	1578	rVB3	1126	1146	0.12%	0.010%
43	12.589	1584	1590	1591	rBV3	1236	1748	0.18%	0.015%
44	12.625	1593	1596	1599	rVB2	833	1227	0.13%	0.011%
45	12.683	1605	1606	1609	rVB2	1338	1127	0.12%	0.010%
46	12.748	1613	1617	1618	rVB3	1397	1542	0.16%	0.014%
47	12.777	1618	1622	1623	rBV	1396	1155	0.12%	0.010%
48	12.942	1647	1650	1652	rBV3	1115	1365	0.14%	0.012%
49	13.448	1732	1736	1740	rVB4	832	1181	0.12%	0.010%
50	13.513	1745	1747	1749	rBV2	1410	1076	0.11%	0.010%
51	13.619	1762	1765	1767	rBV3	1005	1207	0.12%	0.011%
52	13.942	1814	1820	1832	rBV	387688	556876	57.59%	4.918%
53	14.160	1854	1857	1859	rVB2	1055	1082	0.11%	0.010%
54	14.230	1862	1869	1878	rBV	406774	637098	65.89%	5.626%
55	14.536	1914	1921	1930	rBV	317968	492601	50.94%	4.350%
56	14.748	1951	1957	1976	rBV2	113002	252653	26.13%	2.231%
57	14.889	1979	1981	1983	rVV3	2999	2922	0.30%	0.026%
58	14.913	1983	1985	1987	rVV3	2141	2447	0.25%	0.022%
59	14.960	1991	1993	1996	rVV3	2045	2326	0.24%	0.021%
60	15.107	2015	2018	2021	rBV2	1405	1476	0.15%	0.013%
61	15.271	2042	2046	2050	rBV3	1184	2483	0.26%	0.022%
62	15.336	2054	2057	2060	rBV2	936	1490	0.15%	0.013%
63	15.524	2081	2089	2101	rBV	533919	778384	80.50%	6.874%
64	15.642	2101	2109	2122	rVV2	146237	215910	22.33%	1.907%
65	15.754	2127	2128	2130	rBV2	1543	1494	0.15%	0.013%
66	15.942	2156	2160	2161	rBV3	1474	1475	0.15%	0.013%
67	16.024	2172	2174	2179	rVB2	1122	1272	0.13%	0.011%
68	16.083	2179	2184	2188	rBV4	1203	2046	0.21%	0.018%
69	16.407	2236	2239	2242	rVB3	1543	2051	0.21%	0.018%
70	16.430	2242	2243	2246	rBV3	1015	1141	0.12%	0.010%
71	16.542	2257	2262	2263	rBV3	1321	1803	0.19%	0.016%
72	16.571	2263	2267	2272	rVB5	1729	2547	0.26%	0.022%
73	16.636	2275	2278	2280	rBV3	966	1095	0.11%	0.010%
74	16.765	2296	2300	2304	rVB4	889	1609	0.17%	0.014%
75	16.918	2324	2326	2331	rVB4	972	1532	0.16%	0.014%
76	16.960	2331	2333	2337	rBV4	986	1391	0.14%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033365.D
 Acq On : 09 Dec 2021 19:48
 Operator : CG/JU
 Sample : PB141232BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

77	17.060	2347	2350	2352	rBV4	1804	1628	0.17%	0.014%
78	17.177	2367	2370	2373	rVV4	1178	1323	0.14%	0.012%
79	17.230	2375	2379	2380	rBV2	1122	1377	0.14%	0.012%
80	17.271	2380	2386	2395	rVV	401973	570171	58.97%	5.035%
81	17.371	2397	2403	2415	rVV	575261	837373	86.60%	7.395%
82	17.448	2415	2416	2419	rVV3	1823	1697	0.18%	0.015%
83	17.771	2470	2471	2473	rBV2	1228	1062	0.11%	0.009%
84	17.895	2490	2492	2495	rVB2	1196	1062	0.11%	0.009%
85	18.177	2539	2540	2543	rBV2	1290	1586	0.16%	0.014%
86	18.289	2557	2559	2561	rBV3	1115	1127	0.12%	0.010%
87	18.377	2570	2574	2577	rVV5	1102	1889	0.20%	0.017%
88	18.454	2585	2587	2588	rBV2	1506	1108	0.11%	0.010%
89	18.706	2629	2630	2632	rBV2	1987	1372	0.14%	0.012%
90	18.854	2652	2655	2657	rBV3	1124	1387	0.14%	0.012%
91	18.871	2657	2658	2661	rBV3	1697	1560	0.16%	0.014%
92	18.959	2671	2673	2677	rVB4	2363	2100	0.22%	0.019%
93	19.130	2700	2702	2703	rBV2	2561	1748	0.18%	0.015%
94	19.224	2715	2718	2723	rBV5	6434	9619	0.99%	0.085%
95	19.295	2726	2730	2733	rVV4	5020	6894	0.71%	0.061%
96	19.653	2785	2791	2800	rBV	692822	965344	99.83%	8.525%
97	19.936	2837	2839	2842	rBV3	3058	3311	0.34%	0.029%
98	21.436	3089	3094	3102	rBV	482588	619804	64.10%	5.473%
99	23.612	3457	3464	3472	rVB	496615	966951	100.00%	8.539%
100	23.759	3483	3489	3498	rVB2	308466	618316	63.94%	5.460%




Sum of corrected areas: 11324162

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033365.D
Acq On : 09 Dec 2021 19:48
Operator : CG/JU
Sample : PB141232BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK232

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

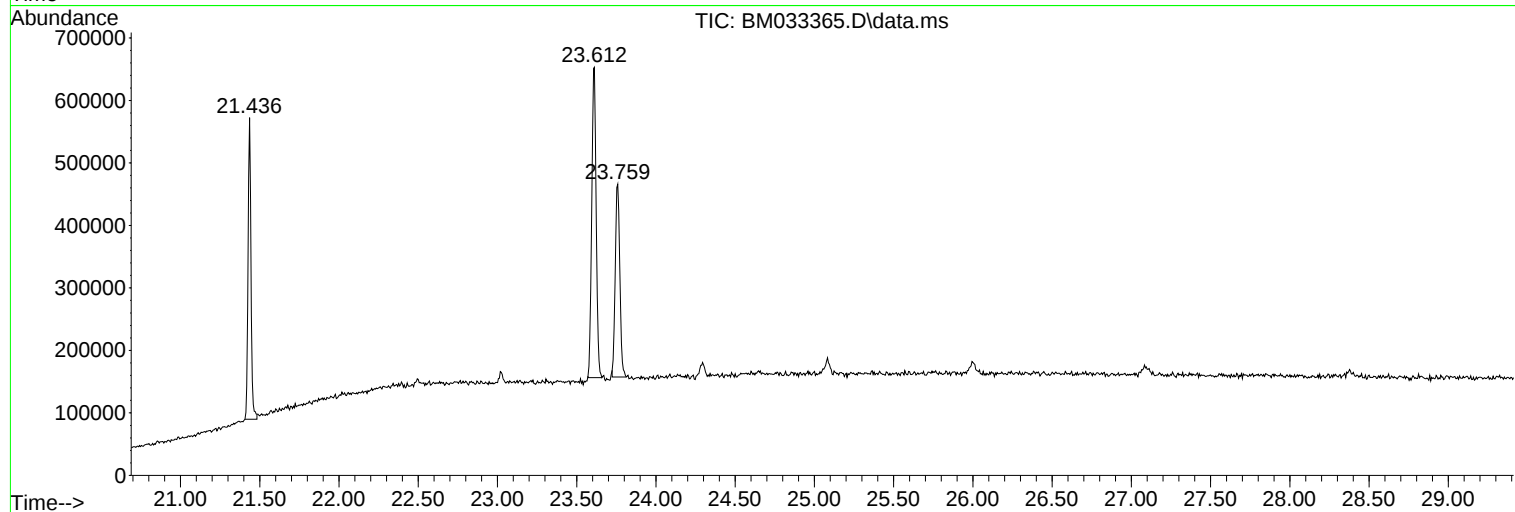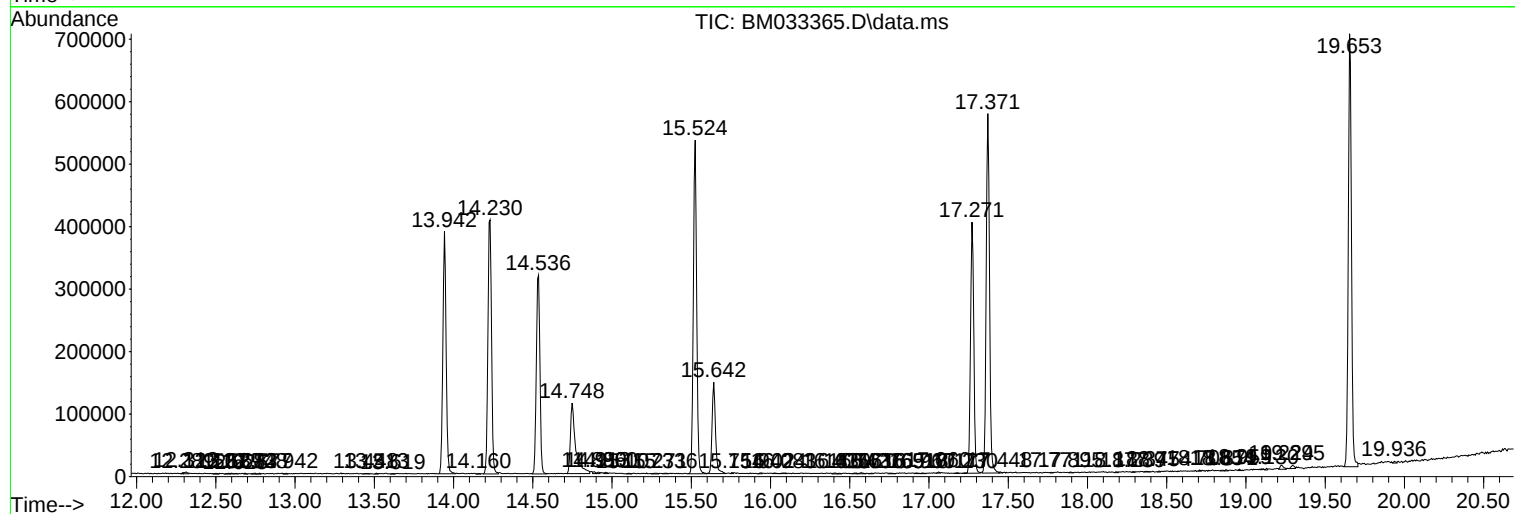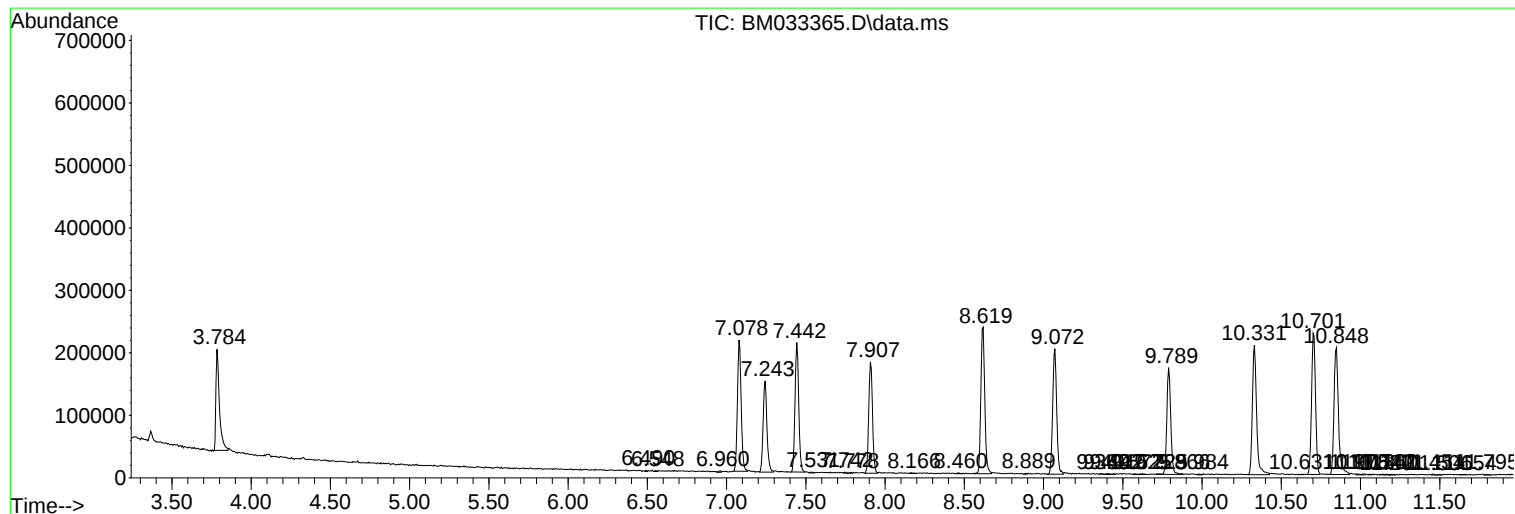

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033365.D
Acq On : 09 Dec 2021 19:48
Operator : CG/JU
Sample : PB141232BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK232

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033365.D
Acq On : 09 Dec 2021 19:48
Operator : CG/JU
Sample : PB141232BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK232

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc