

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033366.D
 Acq On : 09 Dec 2021 20:24
 Operator : CG/JU
 Sample : PB141265BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033366.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.784	90	93	104	rBV	161091	252574	27.39%	2.274%
2	5.854	443	445	446	rVB2	2364	1334	0.14%	0.012%
3	6.084	482	484	485	rBV2	1472	1210	0.13%	0.011%
4	6.696	586	588	590	rVB2	2175	1464	0.16%	0.013%
5	6.713	590	591	592	rBV	1446	981	0.11%	0.009%
6	7.007	638	641	642	rBV2	1441	1110	0.12%	0.010%
7	7.078	647	653	662	rBV	208168	348848	37.83%	3.141%
8	7.243	675	681	691	rBV	146050	237496	25.75%	2.138%
9	7.396	705	707	709	rBV3	1081	1091	0.12%	0.010%
10	7.443	709	715	726	rVB	204957	336109	36.45%	3.026%
11	7.760	766	769	772	rBV3	1130	1539	0.17%	0.014%
12	7.907	787	794	804	rVB	180751	290691	31.52%	2.617%
13	8.125	829	831	834	rBV2	1634	1453	0.16%	0.013%
14	8.225	845	848	849	rBV2	1742	1660	0.18%	0.015%
15	8.237	849	850	854	rVV3	826	1115	0.12%	0.010%
16	8.501	891	895	898	rVB3	1470	1711	0.19%	0.015%
17	8.613	908	914	928	rBV	229880	391438	42.45%	3.524%
18	8.725	931	933	936	rVV2	1738	1346	0.15%	0.012%
19	8.748	936	937	942	rVB2	1146	1187	0.13%	0.011%
20	8.948	969	971	973	rBV2	943	1133	0.12%	0.010%
21	9.072	985	992	999	rBV	202684	354107	38.40%	3.188%
22	9.295	1028	1030	1033	rVB3	1308	1384	0.15%	0.012%
23	9.325	1033	1035	1037	rBV	994	976	0.11%	0.009%
24	9.460	1057	1058	1062	rVB3	1064	1016	0.11%	0.009%
25	9.548	1071	1073	1077	rVB	1033	1540	0.17%	0.014%
26	9.790	1106	1114	1123	rBV	171998	291888	31.65%	2.628%
27	9.854	1123	1125	1126	rVV	1664	1186	0.13%	0.011%
28	9.907	1129	1134	1136	rVB2	1228	1344	0.15%	0.012%
29	10.048	1154	1158	1161	rBV4	882	1234	0.13%	0.011%
30	10.107	1167	1168	1172	rVB2	1577	1566	0.17%	0.014%
31	10.331	1200	1206	1218	rBV	208859	379558	41.16%	3.417%
32	10.472	1228	1230	1233	rVB3	1269	1229	0.13%	0.011%
33	10.701	1262	1269	1277	rBV	223852	391311	42.43%	3.523%
34	10.789	1282	1284	1286	rVV	1833	1247	0.14%	0.011%
35	10.842	1286	1293	1312	rVV	204594	402392	43.64%	3.623%
36	10.978	1315	1316	1320	rVV2	2048	2317	0.25%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033366.D
 Acq On : 09 Dec 2021 20:24
 Operator : CG/JU
 Sample : PB141265BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

37	11.042	1323	1327	1328	rVB3	1407	1901	0.21%	0.017%
38	11.066	1328	1331	1332	rBV2	1110	1279	0.14%	0.012%
39	11.101	1334	1337	1344	rVB5	1254	2417	0.26%	0.022%
40	11.219	1354	1357	1360	rBV3	942	1429	0.15%	0.013%
41	11.395	1386	1387	1391	rBV2	1016	1062	0.12%	0.010%
42	11.754	1443	1448	1449	rVB2	1516	1738	0.19%	0.016%
43	11.778	1449	1452	1455	rBV3	1178	1621	0.18%	0.015%
44	12.131	1509	1512	1514	rBV2	1463	1558	0.17%	0.014%
45	12.307	1537	1542	1550	rVB5	2058	5045	0.55%	0.045%
46	12.595	1589	1591	1594	rVV3	1167	1393	0.15%	0.013%
47	12.631	1594	1597	1601	rVB3	1006	1334	0.14%	0.012%
48	12.707	1607	1610	1613	rVB3	715	1150	0.12%	0.010%
49	12.889	1639	1641	1644	rVB2	1162	1049	0.11%	0.009%
50	13.207	1691	1695	1698	rBV3	957	1174	0.13%	0.011%
51	13.572	1754	1757	1762	rVB3	1087	1522	0.17%	0.014%
52	13.730	1780	1784	1787	rVB3	1140	1518	0.16%	0.014%
53	13.772	1787	1791	1793	rBV2	1123	1346	0.15%	0.012%
54	13.942	1814	1820	1829	rBV	390963	547271	59.35%	4.927%
55	14.007	1829	1831	1837	rVB2	1481	2403	0.26%	0.022%
56	14.089	1842	1845	1847	rVB2	879	1136	0.12%	0.010%
57	14.230	1862	1869	1879	rBV	419269	630582	68.38%	5.677%
58	14.336	1886	1887	1892	rVB3	860	1132	0.12%	0.010%
59	14.530	1913	1920	1931	rBV	327539	487731	52.89%	4.391%
60	14.748	1948	1957	1980	rBV	109070	250508	27.17%	2.255%
61	14.895	1980	1982	1985	rVV3	2096	2887	0.31%	0.026%
62	14.924	1985	1987	1991	rVB4	1527	1992	0.22%	0.018%
63	15.083	2012	2014	2018	rBV3	1115	1425	0.15%	0.013%
64	15.524	2082	2089	2104	rVB	519773	762675	82.71%	6.867%
65	15.642	2104	2109	2119	rVV	147195	210533	22.83%	1.896%
66	15.730	2122	2124	2127	rVV2	1520	1674	0.18%	0.015%
67	15.766	2127	2130	2131	rVV3	1911	1998	0.22%	0.018%
68	15.807	2134	2137	2140	rVB4	901	1056	0.11%	0.010%
69	15.936	2155	2159	2163	rVB4	2073	2687	0.29%	0.024%
70	15.966	2163	2164	2168	rBV2	1244	1272	0.14%	0.011%
71	16.548	2262	2263	2269	rVB2	1182	1098	0.12%	0.010%
72	16.595	2269	2271	2275	rBV2	1140	1166	0.13%	0.010%
73	17.060	2349	2350	2353	rVV2	1798	1254	0.14%	0.011%
74	17.089	2353	2355	2358	rVB	1287	1457	0.16%	0.013%
75	17.118	2358	2360	2363	rBV2	842	1025	0.11%	0.009%
76	17.177	2368	2370	2376	rBV4	884	1437	0.16%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033366.D
 Acq On : 09 Dec 2021 20:24
 Operator : CG/JU
 Sample : PB141265BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

77	17.271	2380	2386	2394	rBV	395356	561537	60.89%	5.056%
78	17.371	2397	2403	2415	rVV2	568800	820668	89.00%	7.389%
79	17.454	2415	2417	2419	rVV3	1286	1190	0.13%	0.011%
80	17.477	2419	2421	2426	rVB3	1356	1628	0.18%	0.015%
81	17.654	2449	2451	2455	rBV4	921	1504	0.16%	0.014%
82	17.754	2464	2468	2470	rBV4	1553	2226	0.24%	0.020%
83	17.889	2489	2491	2494	rBV2	1032	1500	0.16%	0.014%
84	18.018	2510	2513	2515	rBV3	1741	1872	0.20%	0.017%
85	18.077	2520	2523	2524	rBV2	1590	1334	0.14%	0.012%
86	18.265	2553	2555	2557	rVB3	1545	1180	0.13%	0.011%
87	18.371	2572	2573	2576	rBV2	2014	2264	0.25%	0.020%
88	18.454	2586	2587	2588	rBV	1601	1006	0.11%	0.009%
89	18.630	2614	2617	2619	rBV4	1470	1159	0.13%	0.010%
90	18.695	2625	2628	2629	rBV3	1244	1417	0.15%	0.013%
91	18.924	2665	2667	2672	rBV4	1912	2448	0.27%	0.022%
92	19.007	2679	2681	2682	rBV	1699	1073	0.12%	0.010%
93	19.036	2684	2686	2688	rBV3	1155	1111	0.12%	0.010%
94	19.224	2714	2718	2722	rVB4	4793	6998	0.76%	0.063%
95	19.265	2722	2725	2726	rBV3	1707	1331	0.14%	0.012%
96	19.301	2726	2731	2733	rBV4	6342	9278	1.01%	0.084%
97	19.654	2786	2791	2802	rBV	669190	922148	100.00%	8.303%
98	21.436	3089	3094	3102	rBV	450658	609537	66.10%	5.488%
99	23.606	3457	3463	3471	rBV	468621	907533	98.42%	8.171%
100	23.759	3483	3489	3496	rVB2	300020	590121	63.99%	5.313%




Sum of corrected areas: 11106783

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033366.D
Acq On : 09 Dec 2021 20:24
Operator : CG/JU
Sample : PB141265BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK265

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

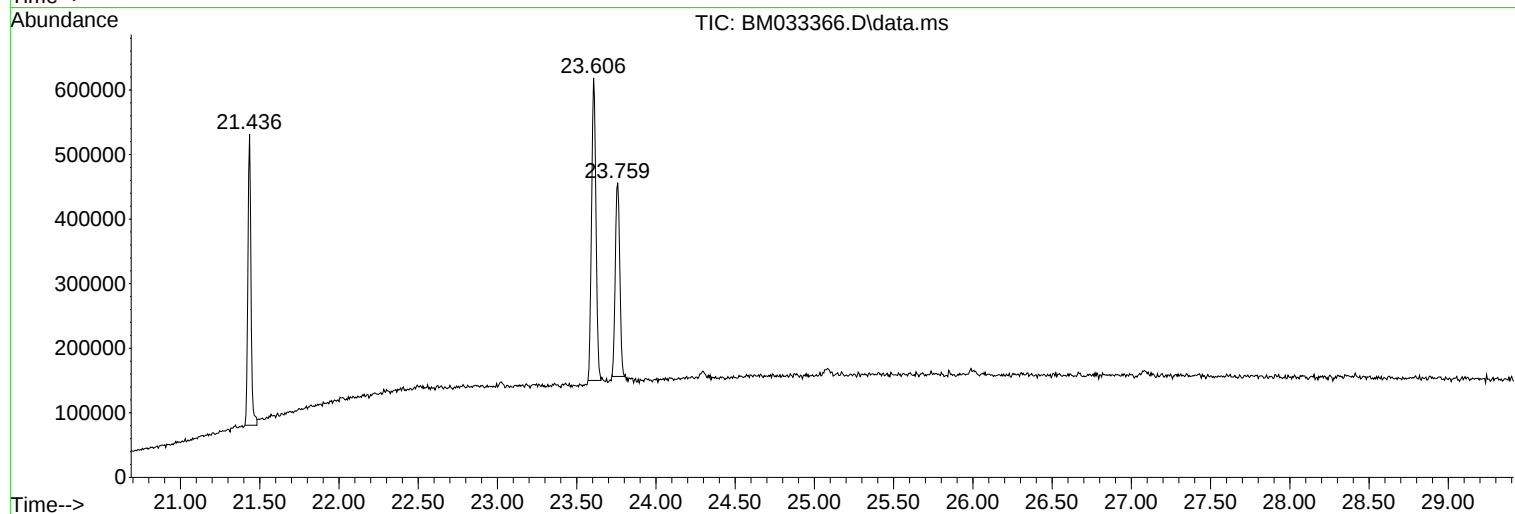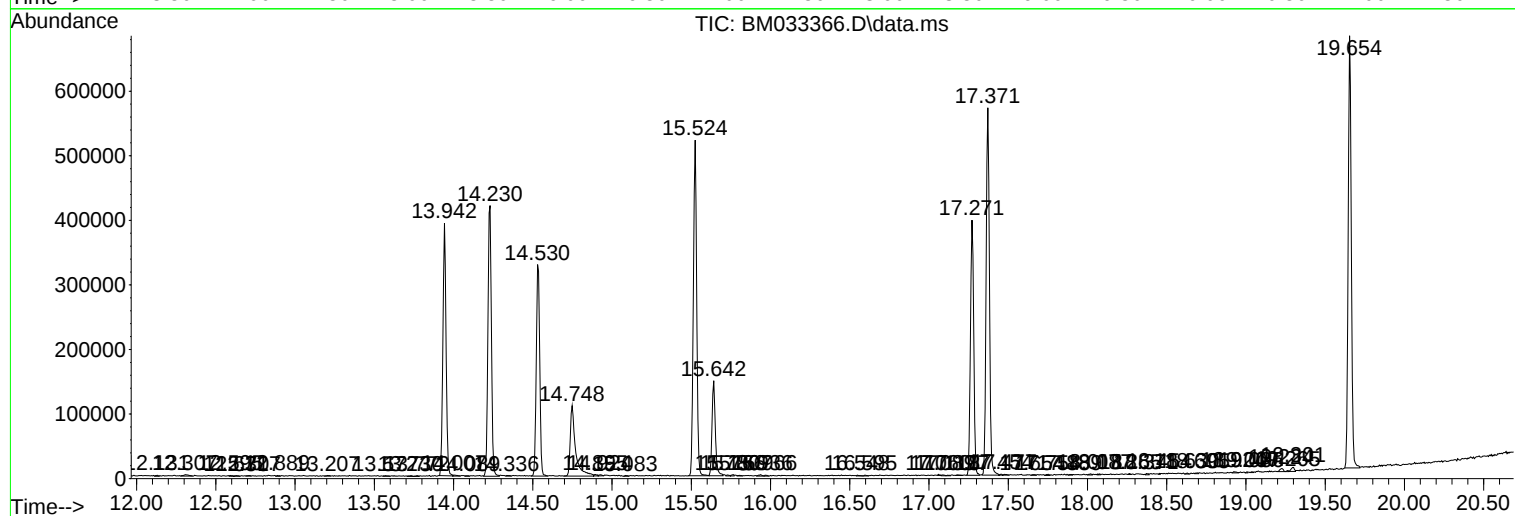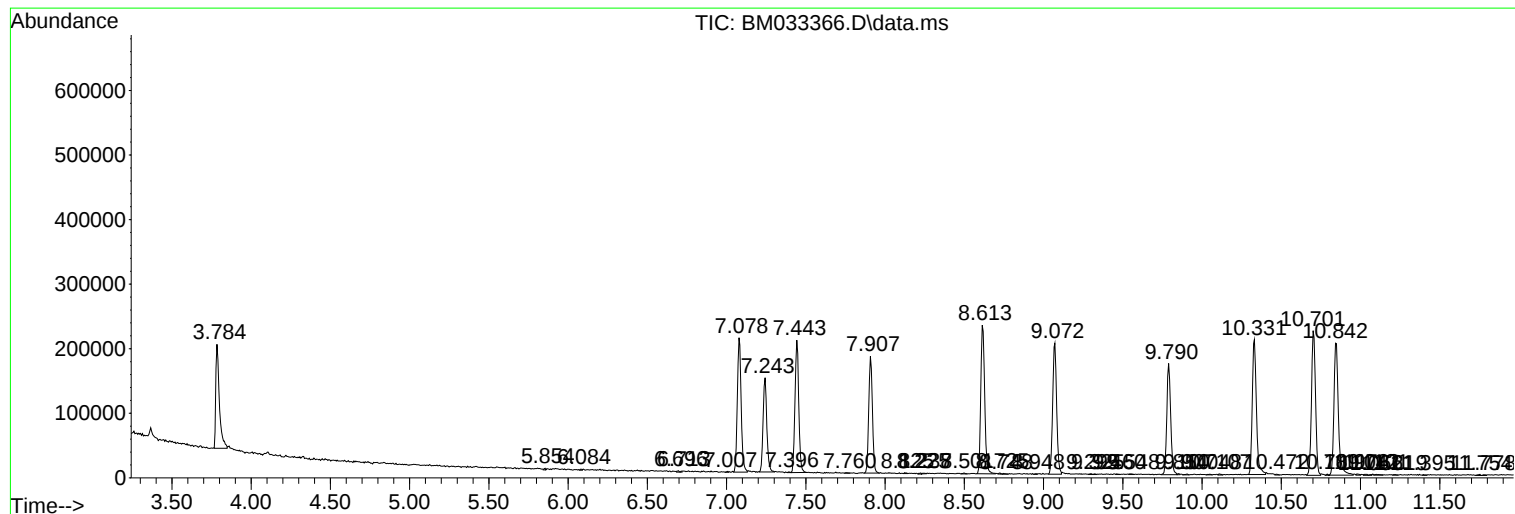

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033366.D
Acq On : 09 Dec 2021 20:24
Operator : CG/JU
Sample : PB141265BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK265

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033366.D
Acq On : 09 Dec 2021 20:24
Operator : CG/JU
Sample : PB141265BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK265

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc