

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033371.D
 Acq On : 09 Dec 2021 23:23
 Operator : CG/JU
 Sample : M4960-11DL3 1500X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGKS4DL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.525	557	559	562	rBV	1728	1799	0.26%	0.046%
2	6.654	580	581	584	rBV2	1867	2166	0.32%	0.055%
3	6.737	593	595	600	rVB3	1468	1665	0.24%	0.042%
4	6.790	602	604	606	rBV2	1355	1520	0.22%	0.039%
5	6.984	635	637	639	rVB3	1665	1222	0.18%	0.031%
6	7.007	639	641	643	rBV	1444	1307	0.19%	0.033%
7	7.619	742	745	746	rBV	1330	1030	0.15%	0.026%
8	7.690	755	757	759	rBV2	1214	1050	0.15%	0.027%
9	7.766	768	770	772	rBV2	1708	1637	0.24%	0.042%
10	7.907	788	794	811	rBV	192345	326030	47.46%	8.300%
11	8.290	857	859	863	rVB3	923	1119	0.16%	0.028%
12	8.413	878	880	883	rBV2	847	932	0.14%	0.024%
13	8.584	908	909	911	rBV	1080	839	0.12%	0.021%
14	8.607	911	913	916	rVV	938	936	0.14%	0.024%
15	8.654	919	921	924	rBV2	884	841	0.12%	0.021%
16	8.784	942	943	946	rBV3	1005	1050	0.15%	0.027%
17	9.272	1024	1026	1030	rVB3	1597	1832	0.27%	0.047%
18	9.401	1046	1048	1053	rVV2	1106	1604	0.23%	0.041%
19	9.484	1058	1062	1063	rBV	951	976	0.14%	0.025%
20	9.613	1080	1084	1087	rBV4	607	1140	0.17%	0.029%
21	9.648	1087	1090	1093	rVB	1501	1618	0.24%	0.041%
22	9.742	1105	1106	1110	rBV	1136	1190	0.17%	0.030%
23	10.013	1149	1152	1153	rBV	960	1077	0.16%	0.027%
24	10.095	1163	1166	1167	rBV2	921	1021	0.15%	0.026%
25	10.207	1184	1185	1187	rVV2	1212	883	0.13%	0.022%
26	10.260	1190	1194	1197	rBV3	903	1280	0.19%	0.033%
27	10.625	1252	1256	1257	rBV2	911	998	0.15%	0.025%
28	10.701	1262	1269	1278	rBV	240701	417251	60.73%	10.622%
29	10.866	1290	1297	1307	rBV	370981	687010	100.00%	17.490%
30	11.137	1342	1343	1346	rVB2	1268	1112	0.16%	0.028%
31	11.301	1367	1371	1373	rBV3	1288	1327	0.19%	0.034%
32	11.336	1375	1377	1380	rBV2	1128	1076	0.16%	0.027%
33	11.619	1420	1425	1427	rVB3	717	1102	0.16%	0.028%
34	11.778	1450	1452	1456	rVB3	930	945	0.14%	0.024%
35	12.060	1497	1500	1502	rBV2	1030	1062	0.15%	0.027%
36	12.254	1528	1533	1541	rBV2	21635	41908	6.10%	1.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033371.D
 Acq On : 09 Dec 2021 23:23
 Operator : CG/JU
 Sample : M4960-11DL3 1500X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGKS4DL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

37	12.307	1541	1542	1545	rVB3	1207	897	0.13%	0.023%
38	12.842	1630	1633	1634	rBV2	834	855	0.12%	0.022%
39	12.860	1634	1636	1638	rVV	1130	1033	0.15%	0.026%
40	12.883	1638	1640	1643	rVB3	915	893	0.13%	0.023%
41	13.136	1680	1683	1686	rVB2	880	869	0.13%	0.022%
42	13.295	1707	1710	1713	rVB2	834	1217	0.18%	0.031%
43	13.325	1713	1715	1720	rBV3	920	1391	0.20%	0.035%
44	13.442	1732	1735	1738	rBV3	801	856	0.12%	0.022%
45	13.548	1749	1753	1755	rVV4	897	940	0.14%	0.024%
46	13.754	1785	1788	1792	rVB3	966	1368	0.20%	0.035%
47	14.025	1832	1834	1838	rBV3	893	1401	0.20%	0.036%
48	14.113	1847	1849	1853	rBV	675	964	0.14%	0.025%
49	14.154	1853	1856	1860	rVB3	944	1317	0.19%	0.034%
50	14.277	1874	1877	1879	rBV	1083	1023	0.15%	0.026%
51	14.530	1912	1920	1930	rVV	326532	514863	74.94%	13.108%
52	15.042	2006	2007	2010	rVB3	991	935	0.14%	0.024%
53	15.230	2037	2039	2042	rVB4	758	862	0.13%	0.022%
54	15.283	2042	2048	2051	rBV2	960	1587	0.23%	0.040%
55	15.436	2072	2074	2076	rVV	958	1061	0.15%	0.027%
56	15.466	2077	2079	2082	rVB2	1147	943	0.14%	0.024%
57	15.572	2096	2097	2102	rBV3	601	890	0.13%	0.023%
58	15.683	2113	2116	2120	rVB4	738	1159	0.17%	0.030%
59	15.813	2134	2138	2141	rVB3	1422	2237	0.33%	0.057%
60	15.860	2141	2146	2147	rBV2	803	1005	0.15%	0.026%
61	15.913	2152	2155	2157	rBV	776	1007	0.15%	0.026%
62	16.083	2181	2184	2185	rBV2	1031	966	0.14%	0.025%
63	16.213	2203	2206	2209	rVB2	1267	1379	0.20%	0.035%
64	16.324	2223	2225	2227	rBV3	781	927	0.13%	0.024%
65	16.371	2229	2233	2235	rVV3	1005	1375	0.20%	0.035%
66	16.513	2253	2257	2260	rVB3	917	1529	0.22%	0.039%
67	16.607	2272	2273	2276	rVB2	1439	929	0.14%	0.024%
68	16.771	2297	2301	2302	rVB2	1581	1377	0.20%	0.035%
69	16.789	2302	2304	2306	rBV2	1130	1256	0.18%	0.032%
70	16.813	2306	2308	2313	rVB4	737	1489	0.22%	0.038%
71	16.918	2323	2326	2327	rVB2	939	934	0.14%	0.024%
72	16.971	2331	2335	2336	rVB2	1022	1061	0.15%	0.027%
73	17.271	2379	2386	2400	rBV	375716	585948	85.29%	14.917%
74	17.371	2402	2403	2408	rVB2	1667	1909	0.28%	0.049%
75	17.642	2446	2449	2452	rBV3	939	1202	0.17%	0.031%
76	17.748	2466	2467	2470	rBV2	1261	982	0.14%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033371.D
 Acq On : 09 Dec 2021 23:23
 Operator : CG/JU
 Sample : M4960-11DL3 1500X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGKS4DL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

77	17.795	2473	2475	2480	rVB3	969	1449	0.21%	0.037%
78	17.848	2482	2484	2488	rVB4	1103	1109	0.16%	0.028%
79	17.930	2497	2498	2503	rVB2	702	963	0.14%	0.025%
80	17.977	2505	2506	2510	rBV3	786	1181	0.17%	0.030%
81	18.107	2526	2528	2532	rVB2	1012	1075	0.16%	0.027%
82	18.154	2534	2536	2539	rVB2	1356	1152	0.17%	0.029%
83	18.183	2539	2541	2542	rBV2	1374	902	0.13%	0.023%
84	18.265	2553	2555	2557	rBV2	1130	934	0.14%	0.024%
85	18.313	2561	2563	2565	rVV2	767	861	0.13%	0.022%
86	18.336	2565	2567	2569	rVB2	1443	878	0.13%	0.022%
87	18.407	2575	2579	2580	rBV4	1148	986	0.14%	0.025%
88	18.471	2588	2590	2593	rBV2	1601	1201	0.17%	0.031%
89	18.612	2612	2614	2616	rBV3	1526	1168	0.17%	0.030%
90	18.665	2619	2623	2624	rBV2	727	1033	0.15%	0.026%
91	18.812	2646	2648	2650	rVB3	1378	1167	0.17%	0.030%
92	18.954	2669	2672	2674	rBV2	1026	1012	0.15%	0.026%
93	19.018	2681	2683	2685	rVV3	1806	1468	0.21%	0.037%
94	19.060	2688	2690	2692	rBV3	1146	863	0.13%	0.022%
95	19.354	2738	2740	2741	rBV2	1315	1301	0.19%	0.033%
96	19.518	2766	2768	2769	rVB	2118	1067	0.16%	0.027%
97	19.659	2790	2792	2794	rBV2	1876	1149	0.17%	0.029%
98	19.759	2807	2809	2810	rBV2	2244	1348	0.20%	0.034%
99	21.436	3088	3094	3103	rBV	433011	631535	91.93%	16.078%
100	23.753	3482	3488	3495	rBV3	302208	615801	89.63%	15.677%


Sum of corrected areas: 3927994

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033371.D
Acq On : 09 Dec 2021 23:23
Operator : CG/JU
Sample : M4960-11DL3 1500X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGKS4DL3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

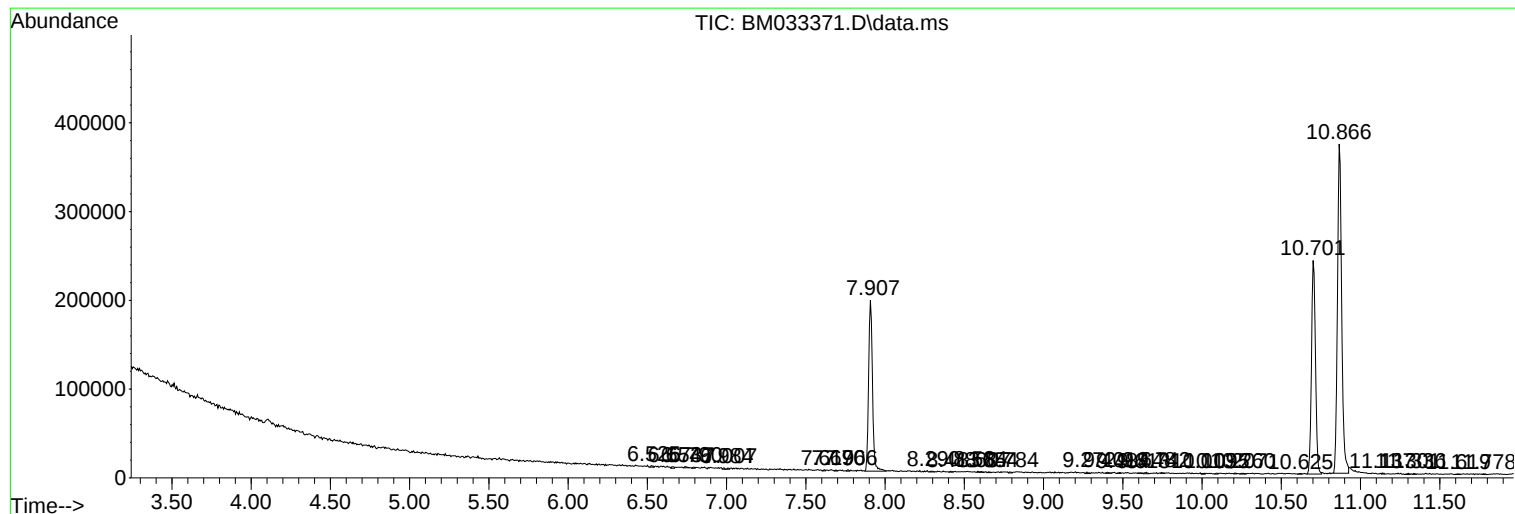

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033371.D
Acq On : 09 Dec 2021 23:23
Operator : CG/JU
Sample : M4960-11DL3 1500X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGKS4DL3










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.254	2.01 ng/ul	41908	Naphthalene-d8	10.701

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		4-Chloroaniline, N-isopropylidene	167	C9H10ClN	040938-43-0	47
2		3-Chloro-1H-indazole	152	C7H5ClN2	029110-74-5	43
3		Benzonitrile, 2-amino-5-chloro-	152	C7H5ClN2	005922-60-1	38
4		1H-Indazole, 5-chloro-	152	C7H5ClN2	000698-26-0	38
5		Benzofuran, 7-chloro-	152	C8H5ClO	024410-55-7	38

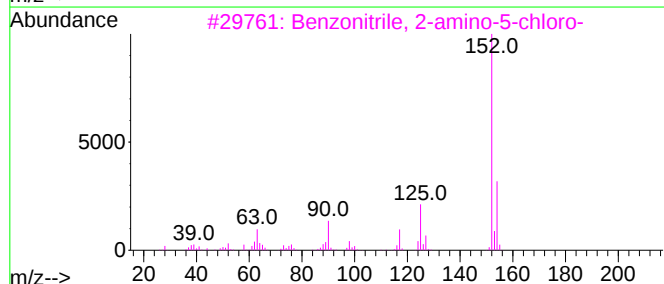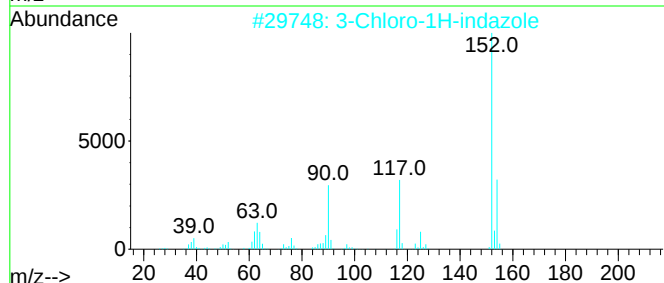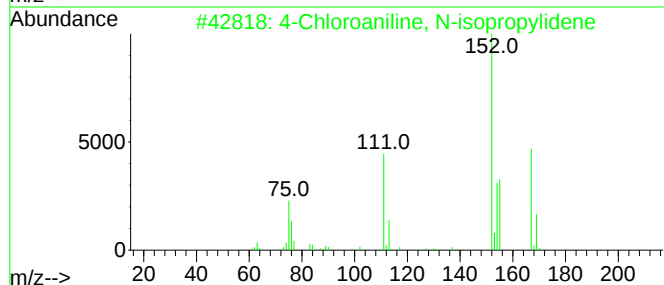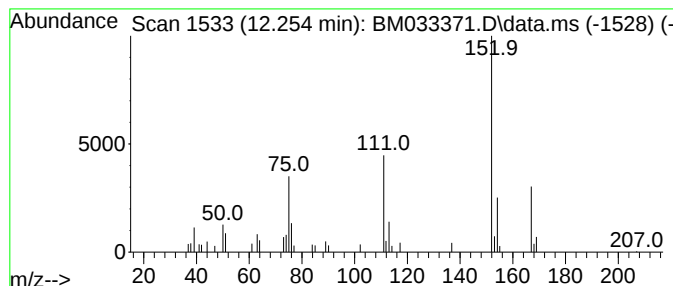

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033371.D
Acq On : 09 Dec 2021 23:23
Operator : CG/JU
Sample : M4960-11DL3 1500X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGKS4DL3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	12.254	2.0	ng/u1	41908	2	10.701	417251	20.0