

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033374.D
 Acq On : 10 Dec 2021 01:47
 Operator : CG/JU
 Sample : PB141276BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK276

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033374.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.784	90	93	105	rVB	202727	325613	25.16%	2.299%
2	7.078	647	653	661	rBV	276954	446459	34.49%	3.153%
3	7.243	675	681	691	rVB	188082	317371	24.52%	2.241%
4	7.443	708	715	726	rBV	257103	433018	33.46%	3.058%
5	7.672	752	754	755	rBV	2205	1310	0.10%	0.009%
6	7.907	788	794	802	rBV	192362	310352	23.98%	2.192%
7	8.049	816	818	820	rVB3	2185	1663	0.13%	0.012%
8	8.178	838	840	842	rVB2	2242	1544	0.12%	0.011%
9	8.278	855	857	860	rVB2	2429	1711	0.13%	0.012%
10	8.613	907	914	927	rBV	308540	514839	39.78%	3.635%
11	9.066	985	991	1001	rBV	267784	458197	35.40%	3.236%
12	9.254	1020	1023	1025	rBV3	1128	1295	0.10%	0.009%
13	9.372	1041	1043	1047	rBV3	1336	2128	0.16%	0.015%
14	9.790	1107	1114	1125	rVB	211716	371452	28.70%	2.623%
15	9.913	1134	1135	1138	rBV2	1602	1589	0.12%	0.011%
16	10.325	1198	1205	1219	rBV	272139	500010	38.63%	3.531%
17	10.413	1219	1220	1226	rVB5	2460	3234	0.25%	0.023%
18	10.513	1236	1237	1240	rVB2	1832	1501	0.12%	0.011%
19	10.643	1257	1259	1262	rVB2	1405	1358	0.10%	0.010%
20	10.701	1262	1269	1278	rBV	245347	421137	32.54%	2.974%
21	10.760	1278	1279	1285	rVB2	1330	2072	0.16%	0.015%
22	10.843	1286	1293	1307	rBV	273843	519086	40.11%	3.665%
23	11.466	1397	1399	1401	rBV	1672	1761	0.14%	0.012%
24	11.566	1413	1416	1417	rBV	1481	1343	0.10%	0.009%
25	11.590	1417	1420	1423	rVB4	1138	1472	0.11%	0.010%
26	11.878	1466	1469	1472	rVB2	1471	1663	0.13%	0.012%
27	12.301	1535	1541	1544	rBV5	3388	6246	0.48%	0.044%
28	13.460	1733	1738	1739	rVB	1487	1590	0.12%	0.011%
29	13.489	1739	1743	1744	rVB2	1276	1420	0.11%	0.010%
30	13.619	1761	1765	1768	rBV3	875	1394	0.11%	0.010%
31	13.942	1814	1820	1827	rBV	527335	731813	56.54%	5.168%
32	14.084	1841	1844	1846	rBV2	1439	1399	0.11%	0.010%
33	14.154	1854	1856	1858	rBV	1731	1502	0.12%	0.011%
34	14.225	1862	1868	1882	rBV	565675	846444	65.40%	5.977%
35	14.531	1914	1920	1927	rBV	359252	527147	40.73%	3.722%
36	14.742	1950	1956	1974	rBV	165535	348658	26.94%	2.462%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033374.D
 Acq On : 10 Dec 2021 01:47
 Operator : CG/JU
 Sample : PB141276BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK276

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

37	14.966	1990	1994	1997	rVB4	2387	3223	0.25%	0.023%
38	15.001	1997	2000	2003	rVB4	1814	2878	0.22%	0.020%
39	15.031	2003	2005	2006	rBV3	1453	1296	0.10%	0.009%
40	15.525	2081	2089	2100	rVV	667352	1012848	78.25%	7.152%
41	15.636	2103	2108	2121	rBV	220058	331594	25.62%	2.342%
42	15.772	2127	2131	2134	rVB5	2021	2851	0.22%	0.020%
43	15.936	2156	2159	2162	rVB3	2396	3230	0.25%	0.023%
44	16.330	2225	2226	2231	rVB3	1067	1345	0.10%	0.009%
45	16.448	2243	2246	2249	rVB3	1092	1385	0.11%	0.010%
46	16.601	2271	2272	2276	rBV3	1243	1485	0.11%	0.010%
47	17.060	2346	2350	2355	rVB4	1846	3214	0.25%	0.023%
48	17.272	2380	2386	2393	rBV	425156	613821	47.42%	4.334%
49	17.372	2396	2403	2415	rVV	780843	1115726	86.20%	7.879%
50	18.271	2554	2556	2561	rBV2	1482	2119	0.16%	0.015%
51	18.330	2564	2566	2568	rVV	1501	1606	0.12%	0.011%
52	18.789	2642	2644	2646	rBV3	1276	1353	0.10%	0.010%
53	18.913	2662	2665	2668	rVB4	2709	2685	0.21%	0.019%
54	18.942	2668	2670	2672	rBV3	1903	2029	0.16%	0.014%
55	19.136	2699	2703	2707	rBV5	1737	3313	0.26%	0.023%
56	19.171	2707	2709	2712	rBV4	1658	1595	0.12%	0.011%
57	19.224	2714	2718	2724	rBV4	8381	12794	0.99%	0.090%
58	19.289	2724	2729	2734	rBV4	8231	14110	1.09%	0.100%
59	19.654	2785	2791	2798	rBV	971699	1294309	100.00%	9.140%
60	21.430	3088	3093	3102	rBV	482910	673156	52.01%	4.753%
61	23.606	3456	3463	3476	rVB2	685157	1292442	99.86%	9.126%
62	23.753	3482	3488	3500	rVB2	319911	654268	50.55%	4.620%




Sum of corrected areas: 14161466

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033374.D
Acq On : 10 Dec 2021 01:47
Operator : CG/JU
Sample : PB141276BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK276

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

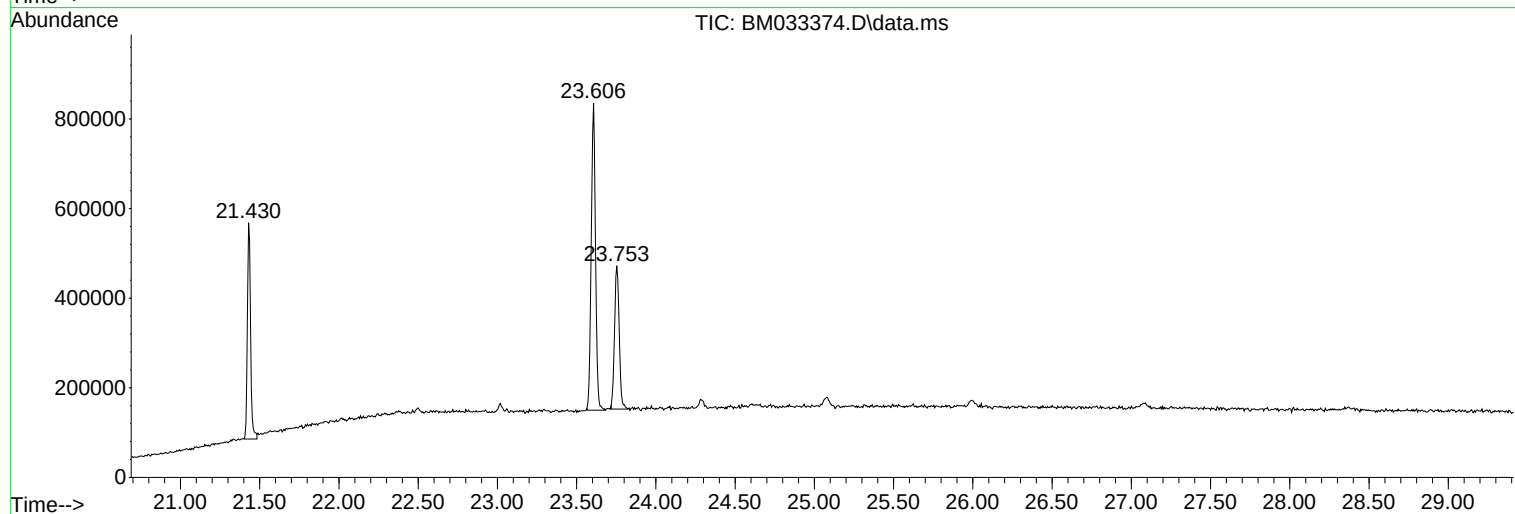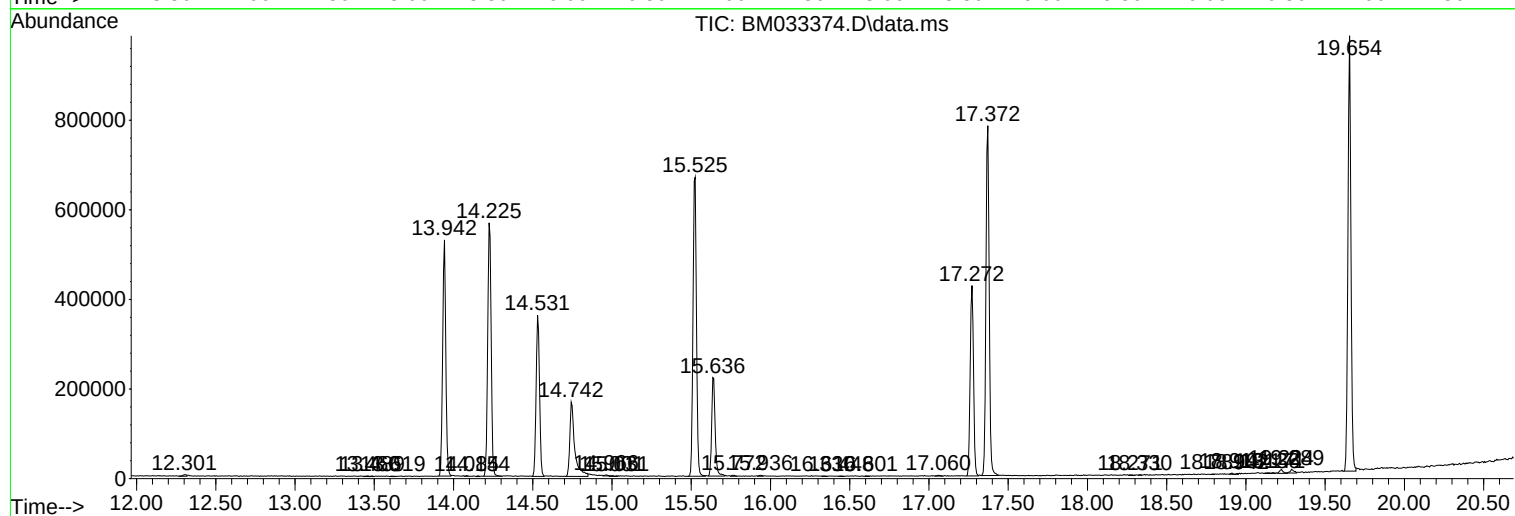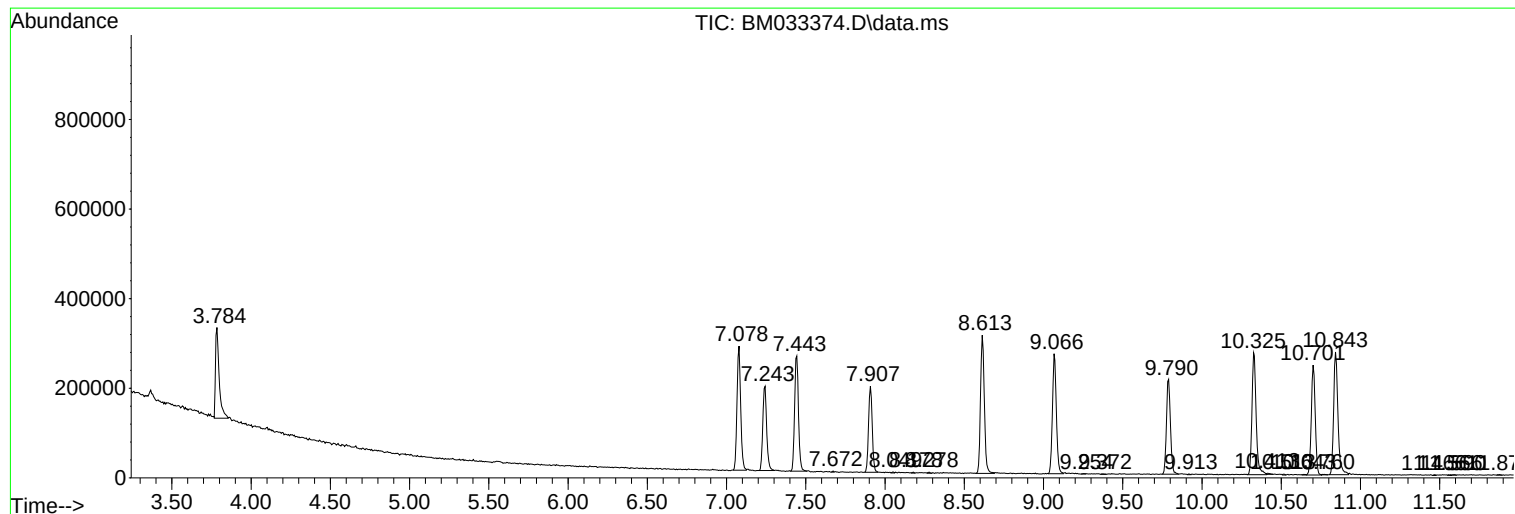

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033374.D
Acq On : 10 Dec 2021 01:47
Operator : CG/JU
Sample : PB141276BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK276

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033374.D
Acq On : 10 Dec 2021 01:47
Operator : CG/JU
Sample : PB141276BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK276

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
