

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033375.D
 Acq On : 10 Dec 2021 02:23
 Operator : CG/JU
 Sample : PB141278BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK278

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033375.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.784	90	93	105	rVB	176404	265565	23.98%	2.165%
2	7.078	646	653	664	rBV	226195	372406	33.63%	3.037%
3	7.237	675	680	692	rVB	150835	257690	23.27%	2.101%
4	7.443	708	715	725	rVB	217708	358788	32.40%	2.926%
5	7.907	787	794	801	rBV	189724	310871	28.07%	2.535%
6	8.613	908	914	927	rBV	246922	416565	37.61%	3.397%
7	8.895	958	962	965	rBV3	1337	2133	0.19%	0.017%
8	9.066	985	991	999	rBV	213925	373057	33.69%	3.042%
9	9.307	1030	1032	1036	rVB2	980	1149	0.10%	0.009%
10	9.425	1050	1052	1054	rBV	1465	1289	0.12%	0.011%
11	9.789	1108	1114	1126	rVB	178426	306341	27.66%	2.498%
12	10.325	1198	1205	1220	rBV	220929	407232	36.77%	3.321%
13	10.701	1262	1269	1278	rVB	247503	417632	37.71%	3.405%
14	10.842	1285	1293	1307	rBV	216451	428155	38.66%	3.491%
15	10.931	1307	1308	1311	rVV2	3347	3050	0.28%	0.025%
16	10.960	1311	1313	1315	rVV2	1952	1392	0.13%	0.011%
17	10.989	1315	1318	1322	rVV5	989	1433	0.13%	0.012%
18	11.683	1433	1436	1441	rBV2	1272	2319	0.21%	0.019%
19	11.725	1441	1443	1445	rBV2	1211	1249	0.11%	0.010%
20	12.289	1535	1539	1540	rBV2	1297	1489	0.13%	0.012%
21	12.395	1553	1557	1562	rVB4	795	1213	0.11%	0.010%
22	12.689	1605	1607	1611	rVB3	1089	1401	0.13%	0.011%
23	12.730	1611	1614	1616	rBV3	1319	1589	0.14%	0.013%
24	12.813	1624	1628	1631	rVB2	1263	2092	0.19%	0.017%
25	12.854	1631	1635	1637	rBV	1761	2496	0.23%	0.020%
26	13.342	1714	1718	1720	rBV2	1304	1299	0.12%	0.011%
27	13.530	1749	1750	1753	rBV2	1742	1448	0.13%	0.012%
28	13.607	1762	1763	1768	rVB3	1021	1363	0.12%	0.011%
29	13.942	1814	1820	1828	rBV	414572	596389	53.85%	4.863%
30	14.224	1862	1868	1877	rBV	455745	669781	60.48%	5.461%
31	14.401	1896	1898	1901	rVV2	1127	1363	0.12%	0.011%
32	14.530	1914	1920	1928	rVB	363759	530185	47.87%	4.323%
33	14.742	1951	1956	1976	rBV	121357	279356	25.23%	2.278%
34	14.954	1990	1992	1994	rBV3	1690	1464	0.13%	0.012%
35	15.413	2067	2070	2074	rVB4	1044	1290	0.12%	0.011%
36	15.524	2082	2089	2099	rVV	548368	827689	74.74%	6.749%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
 Data File : BM033375.D
 Acq On : 10 Dec 2021 02:23
 Operator : CG/JU
 Sample : PB141278BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK278

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
 Title : SVOA CALIBRATION

37	15.595	2099	2101	2103	rVV3	1614	1989	0.18%	0.016%
38	15.636	2103	2108	2125	rVV	172504	266102	24.03%	2.170%
39	15.754	2125	2128	2136	rVB5	2242	4855	0.44%	0.040%
40	15.865	2144	2147	2151	rVB3	1584	1648	0.15%	0.013%
41	15.895	2151	2152	2156	rBV3	1081	1172	0.11%	0.010%
42	15.936	2156	2159	2163	rBV4	2543	2811	0.25%	0.023%
43	16.013	2169	2172	2176	rVB4	904	1343	0.12%	0.011%
44	16.442	2243	2245	2248	rBV3	1510	1385	0.13%	0.011%
45	16.718	2289	2292	2295	rBV3	1075	1333	0.12%	0.011%
46	16.830	2309	2311	2314	rBV3	1109	1286	0.12%	0.010%
47	16.977	2334	2336	2341	rBV2	962	1377	0.12%	0.011%
48	17.065	2347	2351	2352	rBV3	1019	1330	0.12%	0.011%
49	17.271	2380	2386	2393	rBV	436537	615669	55.59%	5.020%
50	17.371	2396	2403	2417	rBV	624732	914169	82.55%	7.454%
51	17.565	2431	2436	2437	rBV2	1770	1997	0.18%	0.016%
52	17.642	2446	2449	2450	rVB3	1454	1423	0.13%	0.012%
53	17.683	2454	2456	2458	rBV3	1044	1232	0.11%	0.010%
54	17.977	2505	2506	2508	rBV	1428	1156	0.10%	0.009%
55	18.112	2528	2529	2532	rVB3	1380	1191	0.11%	0.010%
56	18.230	2548	2549	2554	rVB2	1238	1532	0.14%	0.012%
57	18.318	2561	2564	2566	rBV3	1114	1483	0.13%	0.012%
58	18.359	2568	2571	2574	rBV3	920	1382	0.12%	0.011%
59	18.512	2596	2597	2600	rVB3	1668	1292	0.12%	0.011%
60	18.542	2600	2602	2603	rBV	2462	1501	0.14%	0.012%
61	18.559	2603	2605	2606	rBV	1142	1125	0.10%	0.009%
62	18.606	2609	2613	2614	rBV3	2097	3017	0.27%	0.025%
63	18.671	2620	2624	2625	rBV2	2401	2307	0.21%	0.019%
64	18.742	2633	2636	2637	rBV3	1716	1483	0.13%	0.012%
65	18.801	2640	2646	2647	rBV5	1400	2607	0.24%	0.021%
66	19.036	2685	2686	2689	rBV3	1445	1391	0.13%	0.011%
67	19.106	2696	2698	2700	rBV3	2045	2403	0.22%	0.020%
68	19.224	2714	2718	2722	rBV5	6002	10125	0.91%	0.083%
69	19.301	2726	2731	2734	rVV3	5476	8987	0.81%	0.073%
70	19.330	2734	2736	2740	rVB4	2063	2809	0.25%	0.023%
71	19.389	2745	2746	2748	rBV2	3506	2772	0.25%	0.023%
72	19.653	2785	2791	2804	rBV2	774329	1055503	95.31%	8.607%
73	21.430	3088	3093	3102	rBV	496384	681110	61.50%	5.554%
74	23.606	3456	3463	3471	rBV2	567877	1107446	100.00%	9.030%
75	23.753	3482	3488	3501	rVB	342563	699982	63.21%	5.708%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033375.D
Acq On : 10 Dec 2021 02:23
Operator : CG/JU
Sample : PB141278BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK278

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Title : SVOA CALIBRATION




Sum of corrected areas: 12263948

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033375.D
Acq On : 10 Dec 2021 02:23
Operator : CG/JU
Sample : PB141278BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK278

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

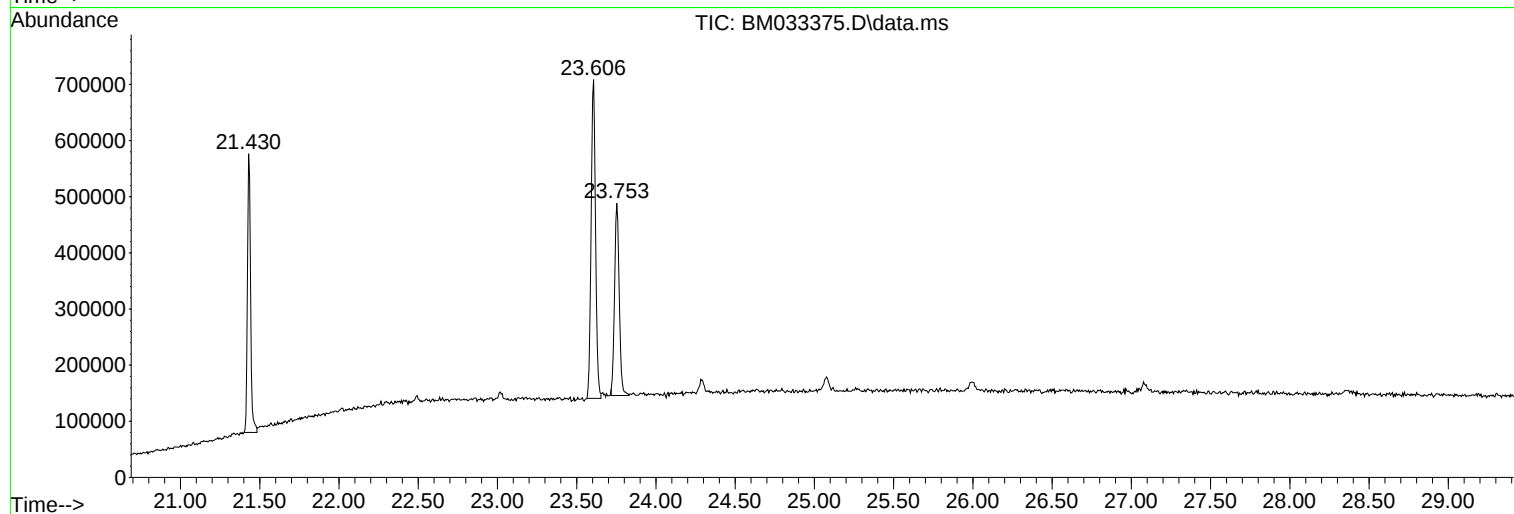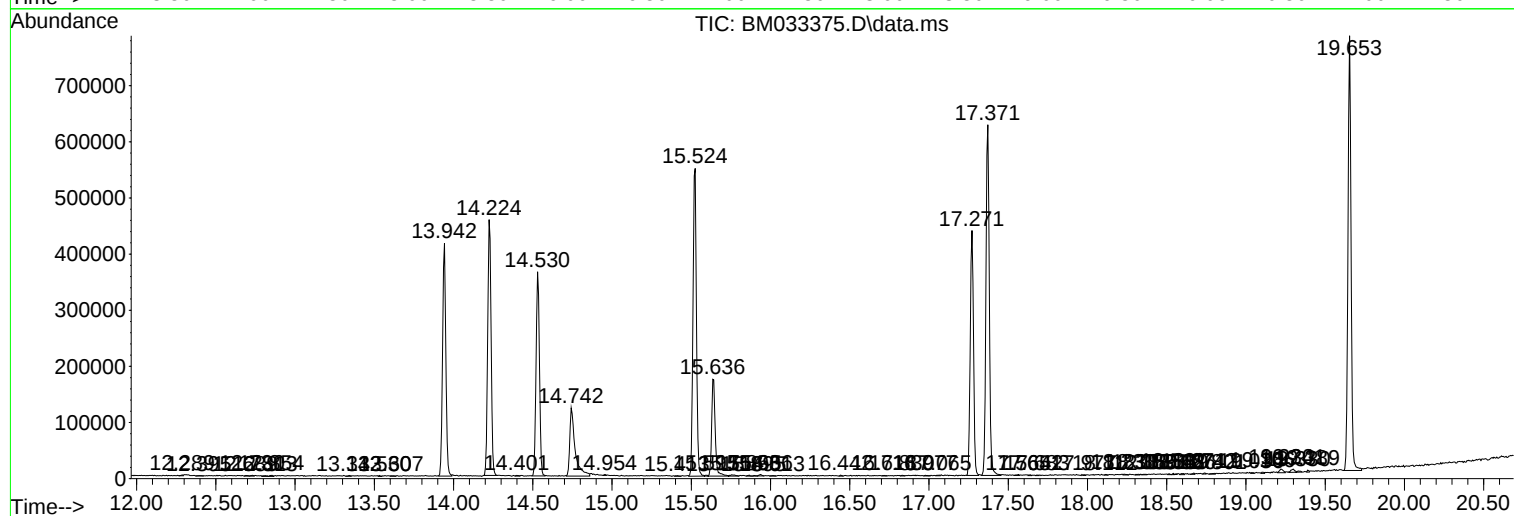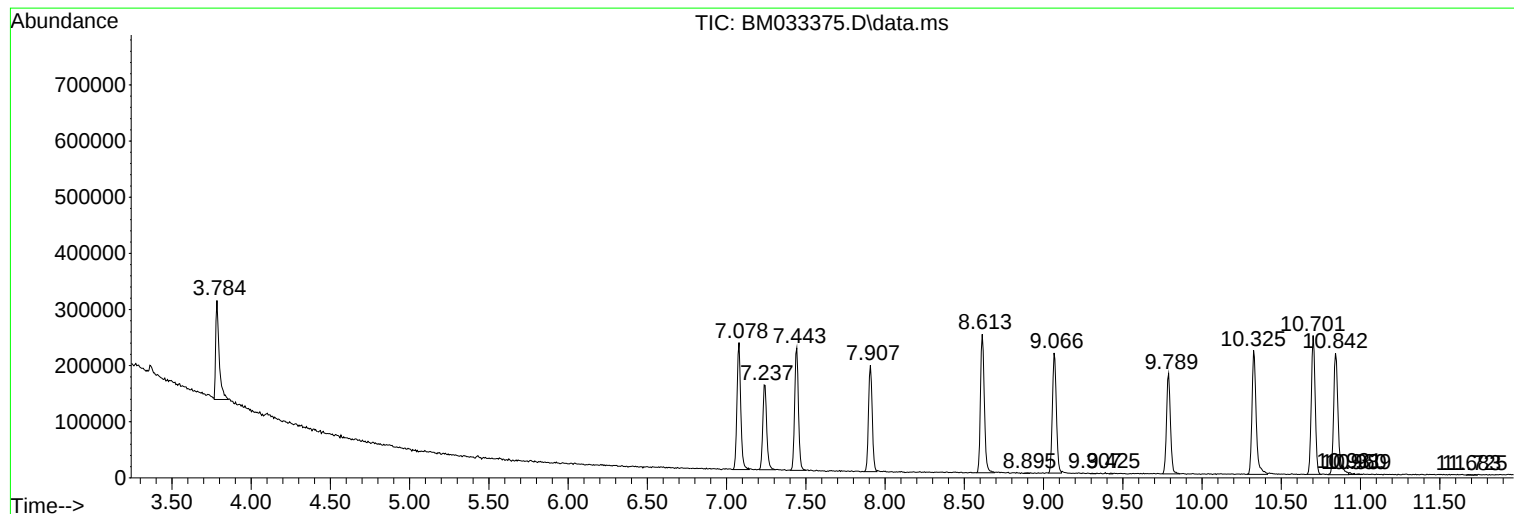

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033375.D
Acq On : 10 Dec 2021 02:23
Operator : CG/JU
Sample : PB141278BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK278

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120921\
Data File : BM033375.D
Acq On : 10 Dec 2021 02:23
Operator : CG/JU
Sample : PB141278BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK278

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc