




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121421\
 Data File : BM033462.D
 Acq On : 15 Dec 2021 04:59
 Operator : CG/JU
 Sample : M4985-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5S5

Manual IntegrationsAPPROVED

Quant Time: Dec 15 06:45:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 01:00:55 2021
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/15/2021
 Supervised By :mohammad ahmed 12/24/2021

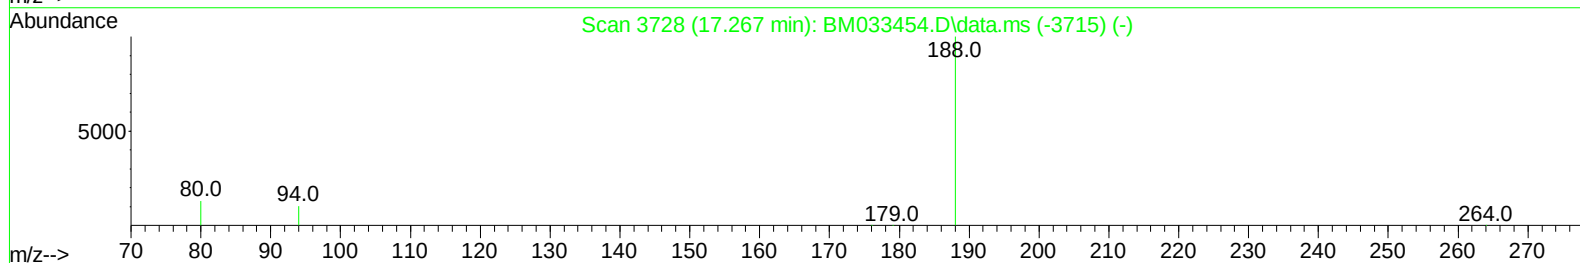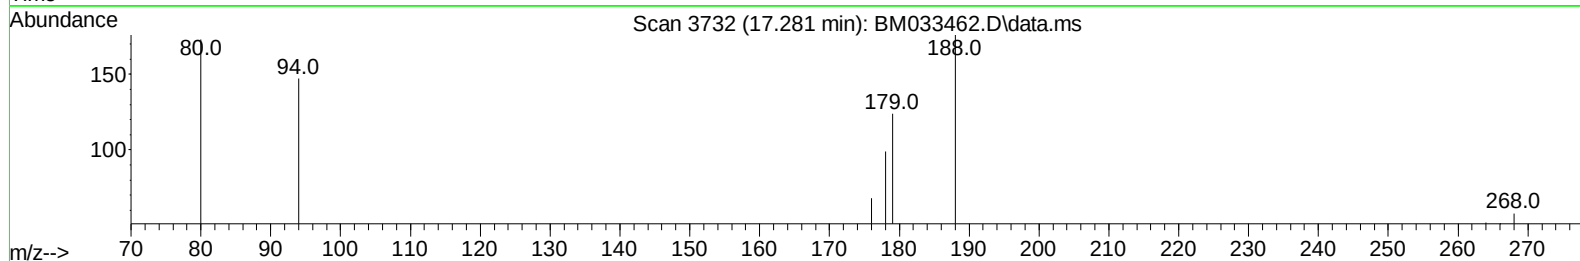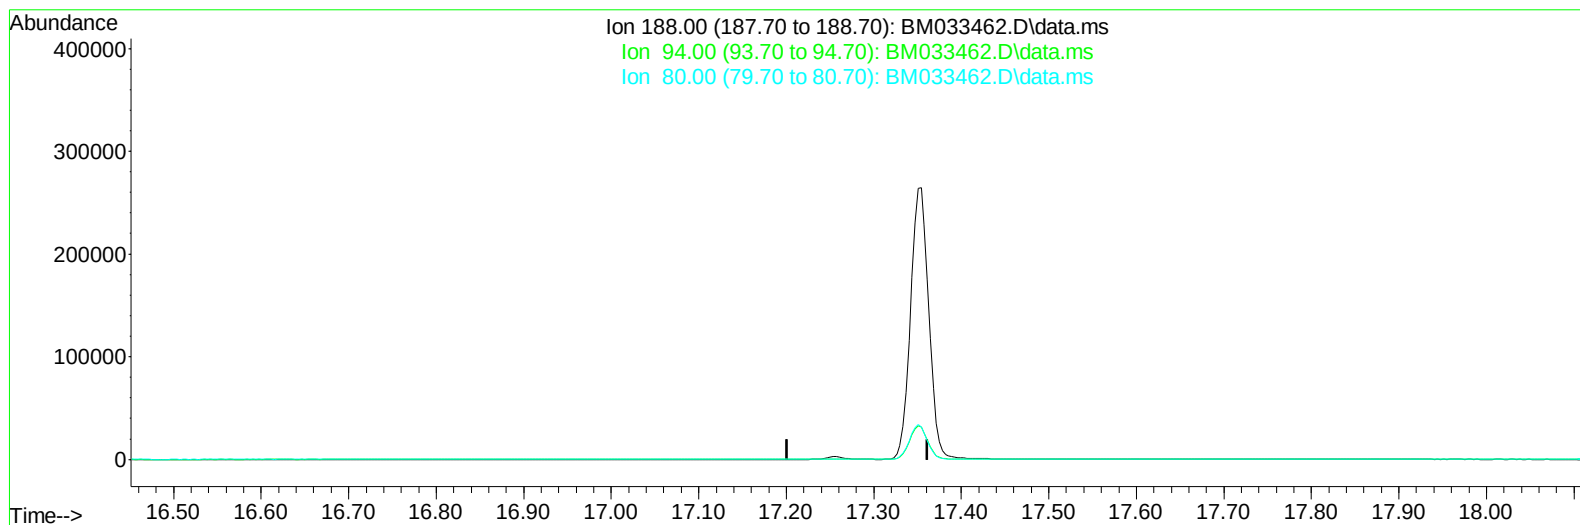

TIC: BM033462.D\data.ms

(13) Phenanthrene-d10 (I)

17.281min (-17.281) 0.00 ng/ul

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	13.30	0.00#
80.00	15.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121421\
Data File : BM033462.D
Acq On : 15 Dec 2021 04:59
Operator : CG/JU
Sample : M4985-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW5S5

Manual IntegrationsAPPROVED

Quant Time: Dec 15 06:45:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 01:00:55 2021
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/15/2021
Supervised By :mohammad ahmed 12/24/2021

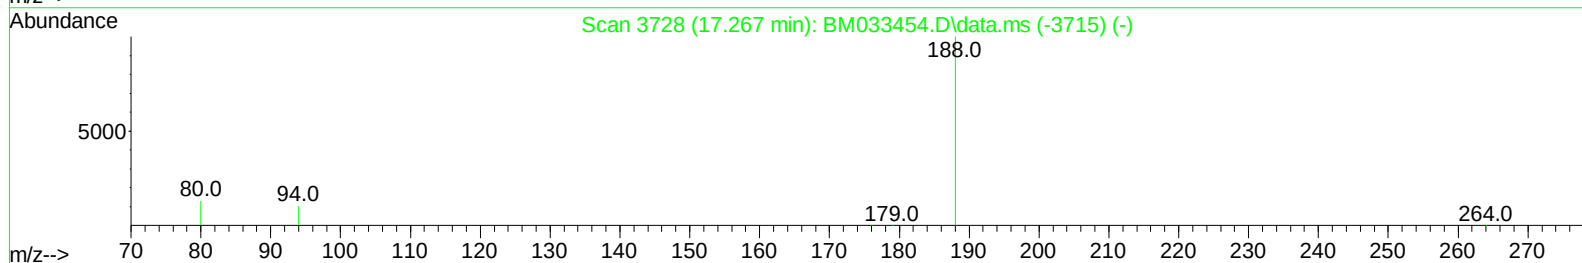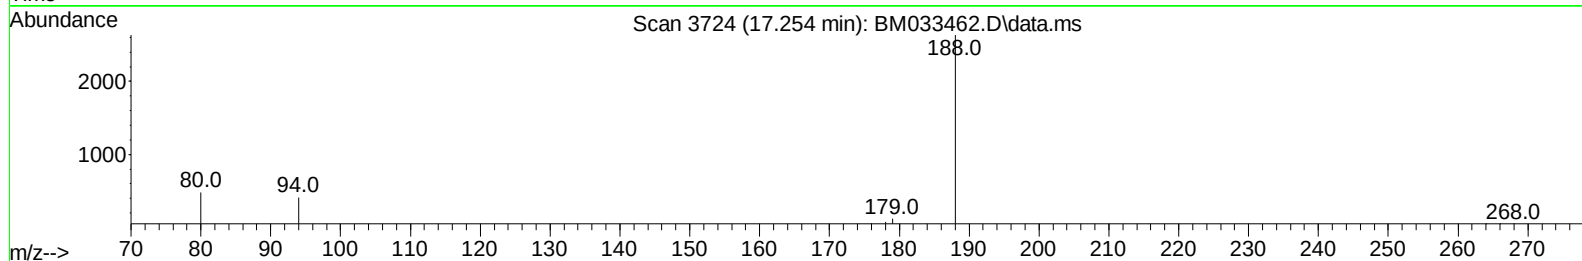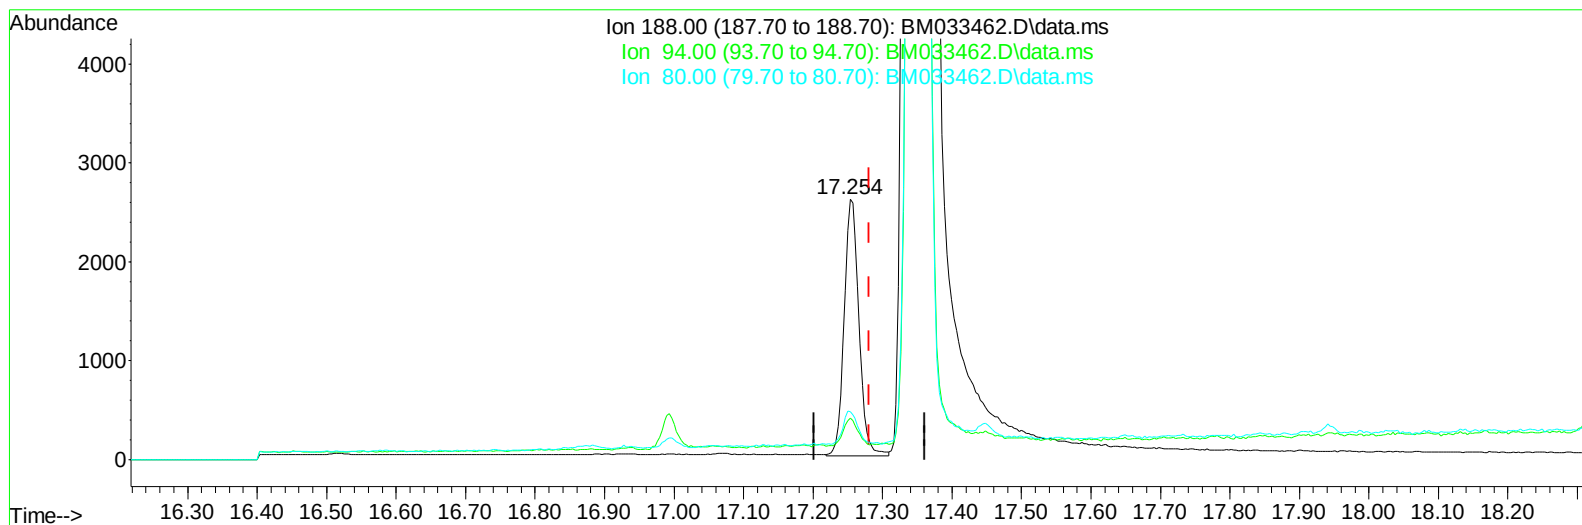

TIC: BM033462.D\data.ms

(13) Phenanthrene-d10 (I)

17.254min (-0.028) 0.40 ng/ul m

response 3827

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.30	15.76
80.00	15.50	18.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121421\
 Data File : BM033462.D
 Acq On : 15 Dec 2021 04:59
 Operator : CG/JU
 Sample : M4985-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5S5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/15/2021
 Supervised By :mohammad ahmed 12/24/2021

Quant Time: Dec 15 06:45:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 01:00:55 2021
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.894	152		752	0.40	ng/ul	-0.02
4) Naphthalene-d8	10.684	136		2079	0.40	ng/ul	-0.02
9) Acenaphthene-d10	14.515	164		1553	0.40	ng/ul	-0.02
13) Phenanthrene-d10	17.254	188		3827m	0.40	ng/ul	-0.03
17) Chrysene-d12	21.427	240		4174	0.40	ng/ul	0.00
23) Perylene-d12	23.735	264		3886	0.40	ng/ul	#-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.358	96		3105	5.10	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.276	152		1277	0.49	ng/ul	-0.03
18) Fluoranthene-d10	19.277	212		6110	0.67	ng/ul	-0.01
Target Compounds							Qvalue
5) Naphthalene	10.733	128		541	0.07	ng/ul#	83
7) 2-Methylnaphthalene	12.353	142		89	0.02	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121421\
Data File : BM033462.D
Acq On : 15 Dec 2021 04:59
Operator : CG/JU
Sample : M4985-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW5S5

Manual IntegrationsAPPROVED

Quant Time: Dec 15 06:45:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 01:00:55 2021
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/15/2021
Supervised By :mohammad ahmed 12/24/2021

