

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121421\
 Data File : BM033466.D
 Acq On : 15 Dec 2021 07:21
 Operator : CG/JU
 Sample : M4985-12
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW5Q6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/16/2021
 Supervised By :mohammad ahmed 12/24/2021

Quant Time: Dec 16 02:32:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 01:00:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.894	152	815	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.684	136	2192	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.515	164	1618	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.254	188	3845m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.427	240	4106	0.400	ng/ul	0.00
23) Perylene-d12	23.732	264	3887	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	3044	4.609	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.281	152	1240	0.448	ng/ul	-0.02
18) Fluoranthene-d10	19.277	212	5745	0.643	ng/ul	-0.01
Target Compounds						
5) Naphthalene	10.734	128	425	0.053	ng/ul#	Qvalue 72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121421\
Data File : BM033466.D
Acq On : 15 Dec 2021 07:21
Operator : CG/JU
Sample : M4985-12
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EW5Q6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/16/2021
Supervised By :mohammad ahmed 12/24/2021


Quant Time: Dec 16 02:32:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 01:00:55 2021
Response via : Initial Calibration

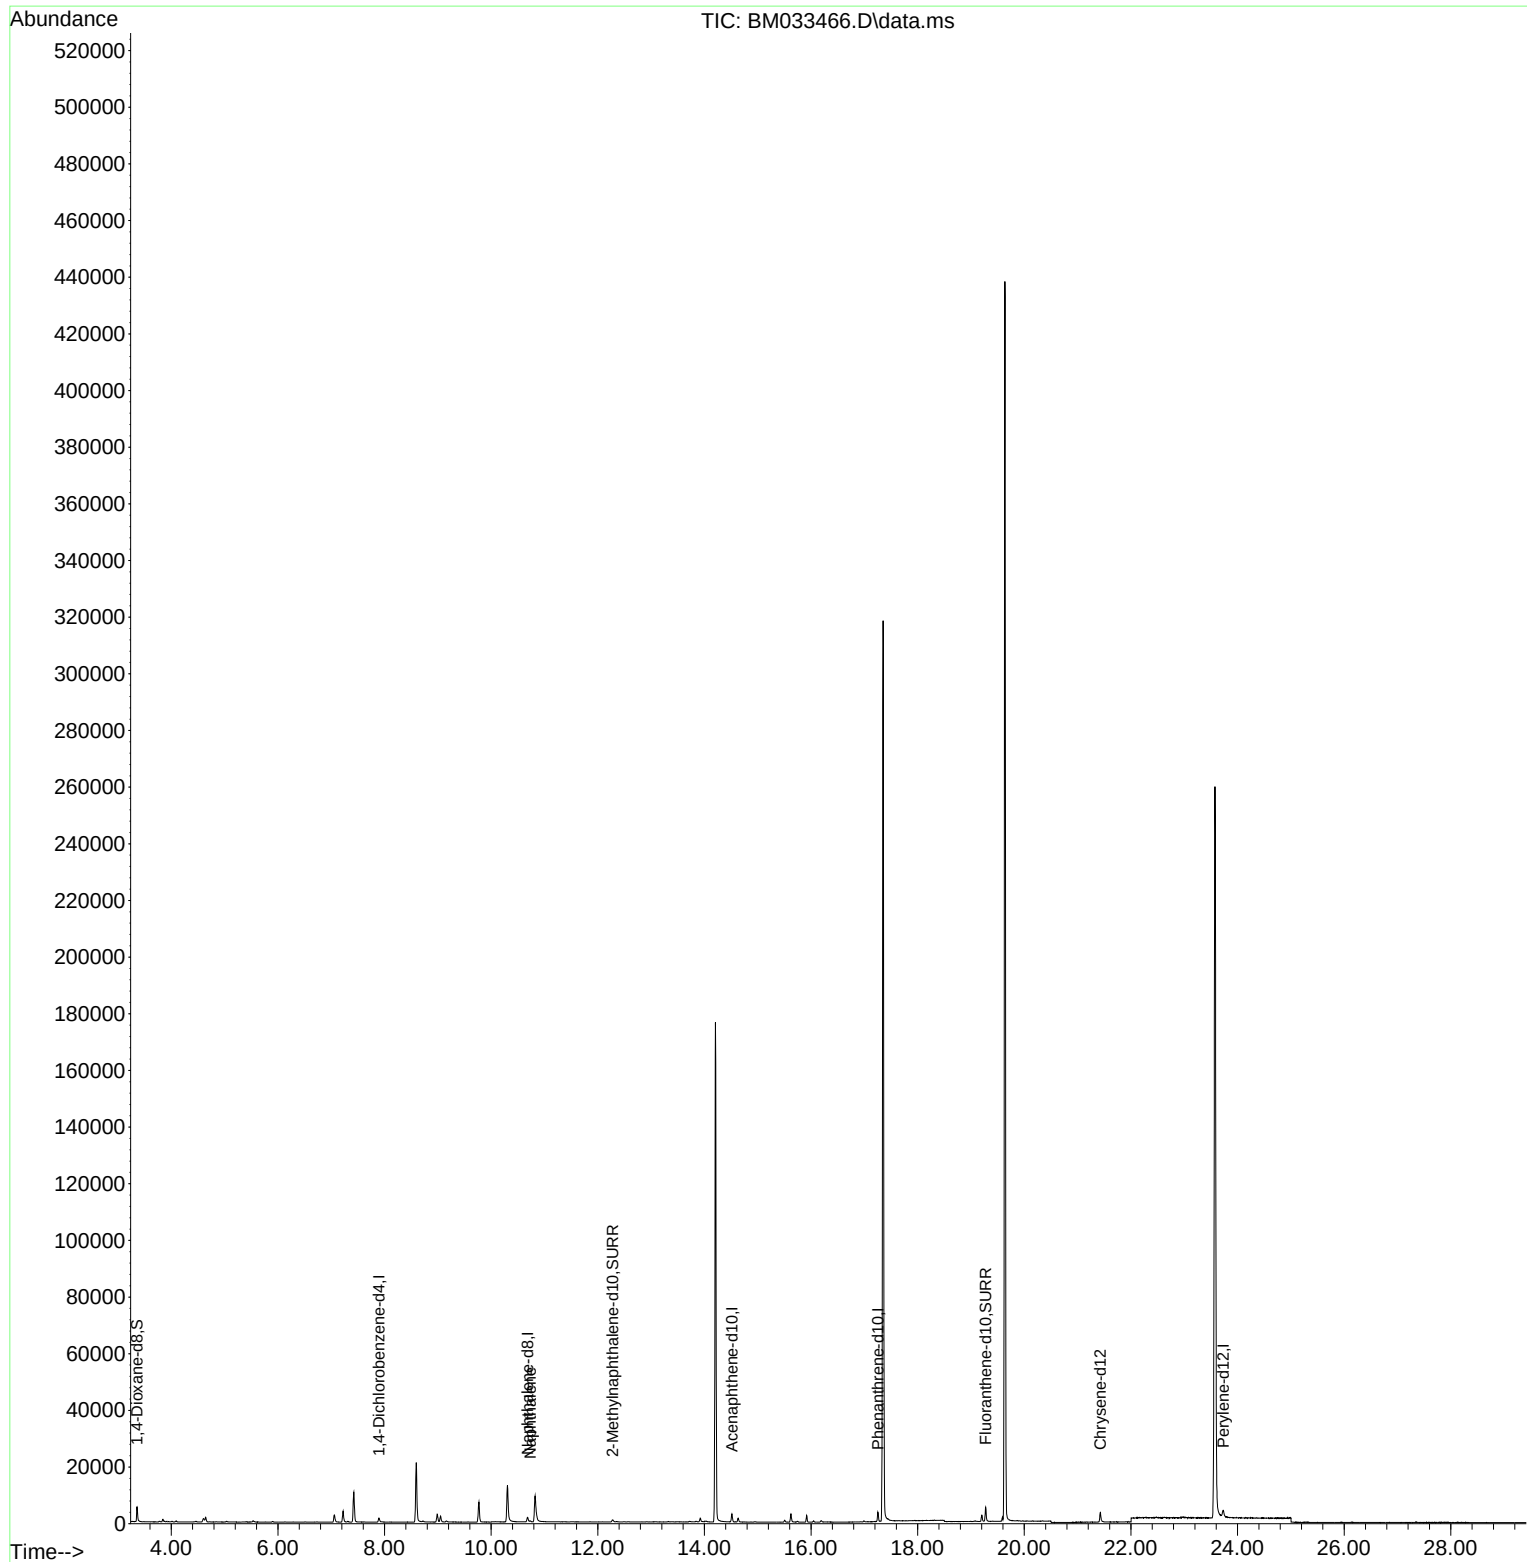

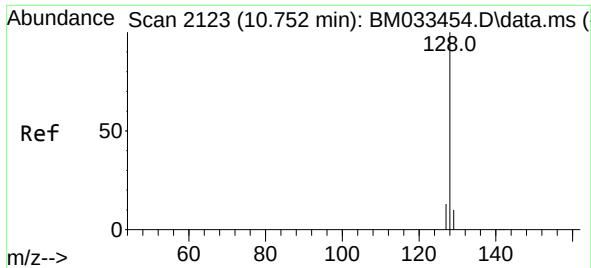

#5
Naphthalene
Concen: 0.053 ng/ul
RT: 10.734 min Scan# 2119
Delta R.T. -0.022 min
Lab File: BM033466.D
Acq: 15 Dec 2021 07:21

Instrument :
BNA_M
ClientSampleId :
EW5Q6

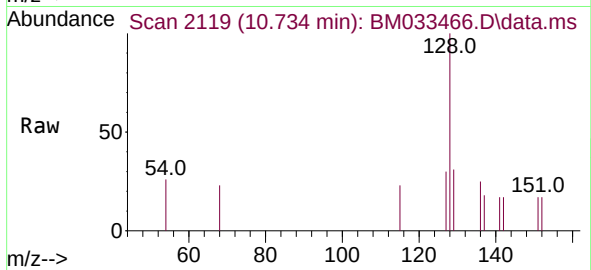

Tgt Ion:128 Resp: 429
Ion Ratio Lower Upper
128 100
129 31.0 13.4 20.2
127 29.6 15.2 22.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/16/2021
Supervised By :mohammad ahmed 12/24/2021

