

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121421\
 Data File : BM033478.D
 Acq On : 15 Dec 2021 14:33
 Operator : CG/JU
 Sample : PB141294BS
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS294

Quant Time: Dec 16 02:34:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 01:00:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.901	152	512	0.400	ng/ul	0.00
4) Naphthalene-d8	0.000	136	0	0.000	ng/ul	-10.71
9) Acenaphthene-d10	0.000	164	0	0.000	ng/ul	-14.53
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.28
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.44
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.75
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.361	96	322	0.776	ng/ul	0.00
6) 2-Methylnaphthalene-d10	0.000	152	0	0.000	ng/ul	
18) Fluoranthene-d10	0.000	212	0	0.000	ng/ul	
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.393	88	1075	1.983	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121421\
Data File : BM033478.D
Acq On : 15 Dec 2021 14:33
Operator : CG/JU
Sample : PB141294BS
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLCS294

Quant Time: Dec 16 02:34:07 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 01:00:55 2021
Response via : Initial Calibration

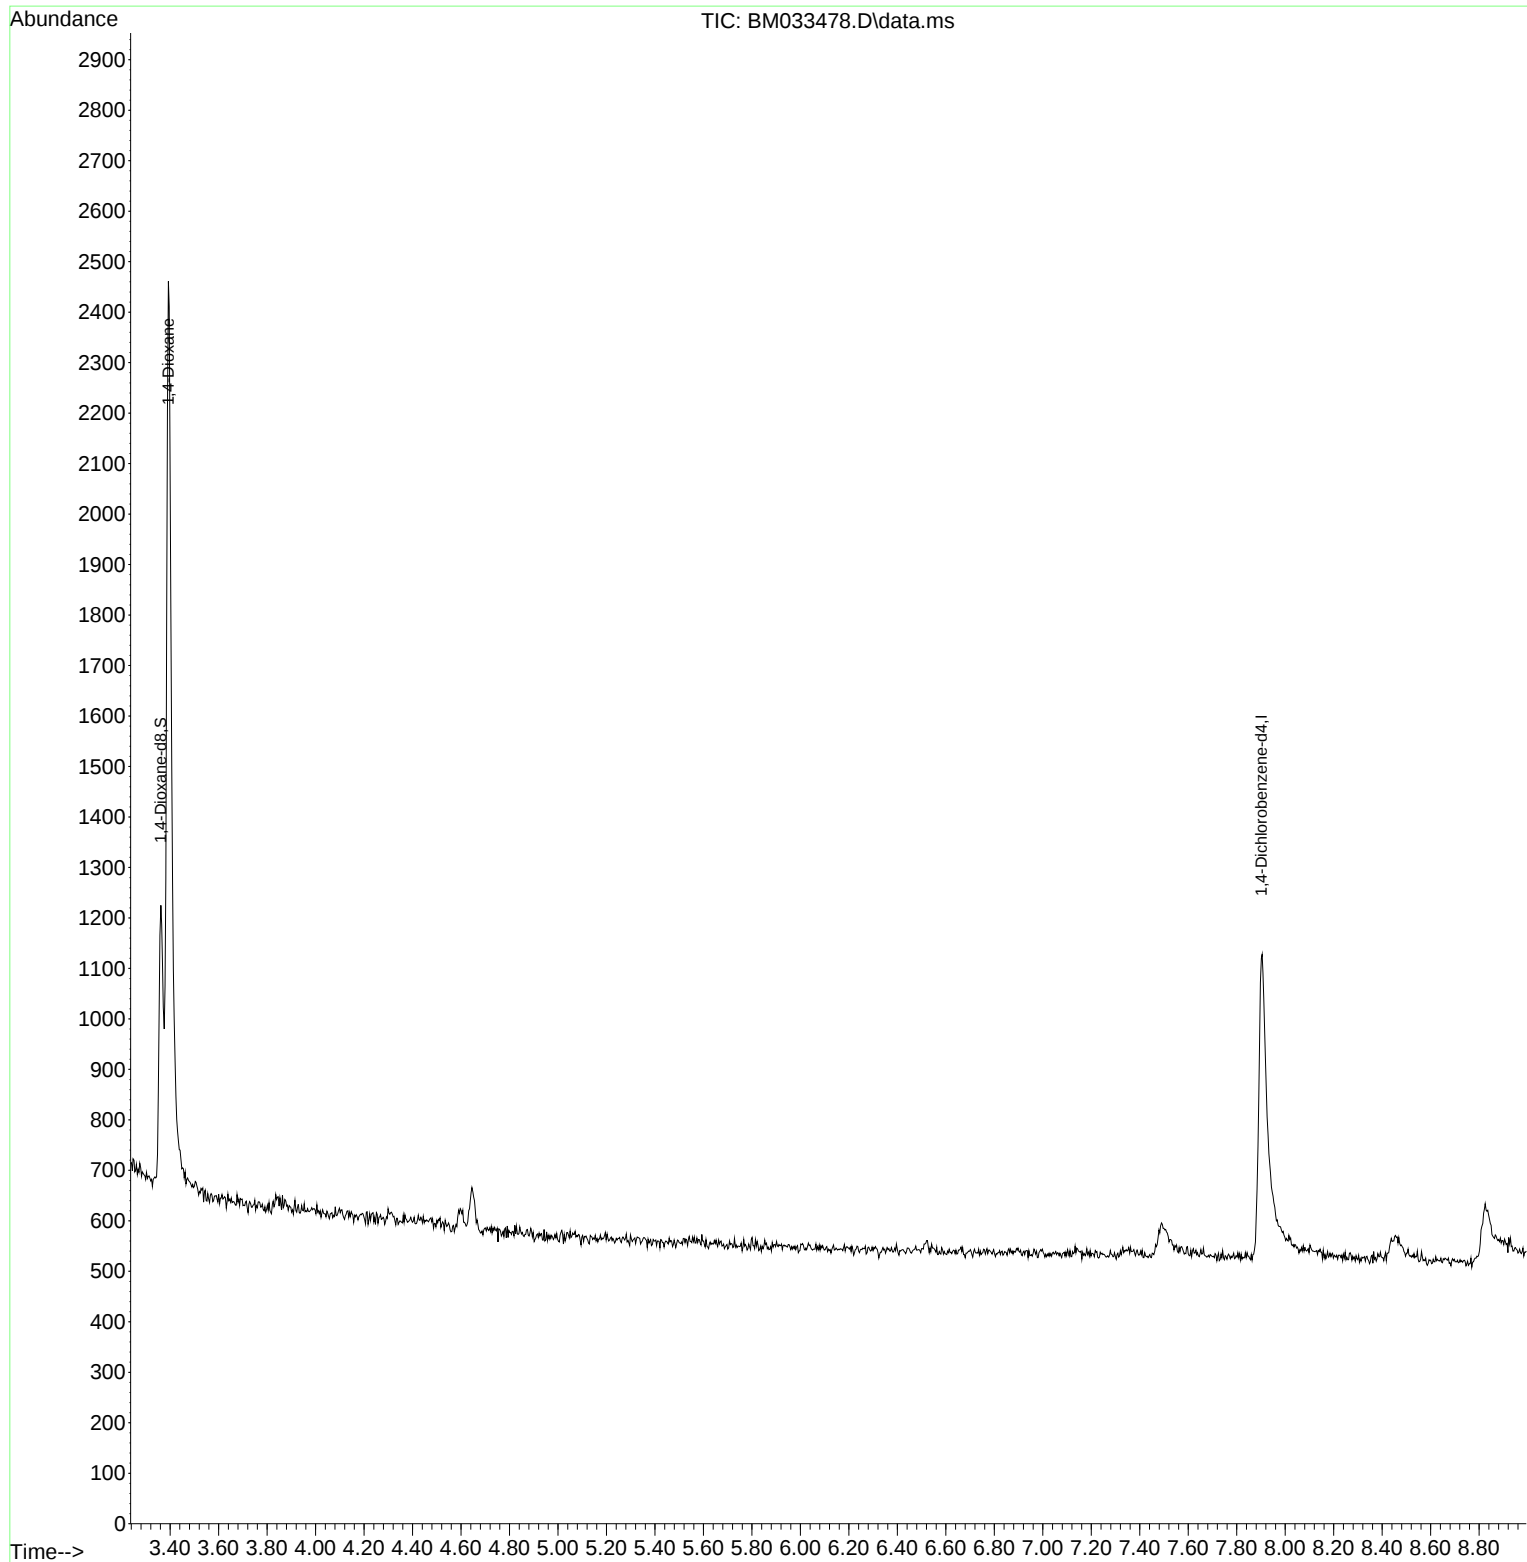

Abundance Scan 48 (3.399 min): BM033471.D\data.ms (-36)

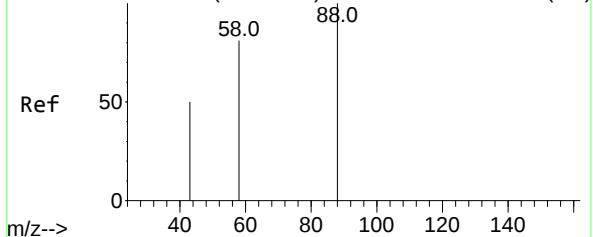

#2

1,4-Dioxane

Concen: 1.983 ng/ul

RT: 3.393 min Scan# 4

Delta R.T. -0.010 min

Lab File: BM033478.D

Acq: 15 Dec 2021 14:33


Instrument :

BNA_M

ClientSampleId :

SLCS294

Abundance Scan 46 (3.393 min): BM033478.D\data.ms

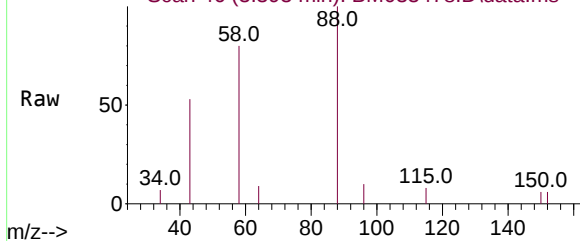

Tgt Ion: 88 Resp: 1075


Ion Ratio Lower Upper

88 100

43 52.9 49.7 74.5

58 79.5 52.5 78.7#

Abundance

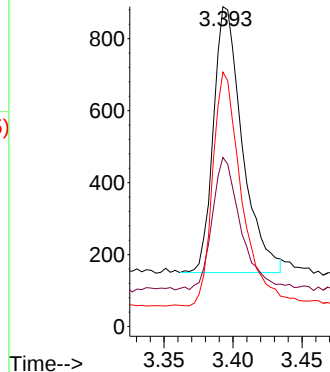

Abundance Scan 46 (3.393 min): BM033478.D\data.ms (-35)

