
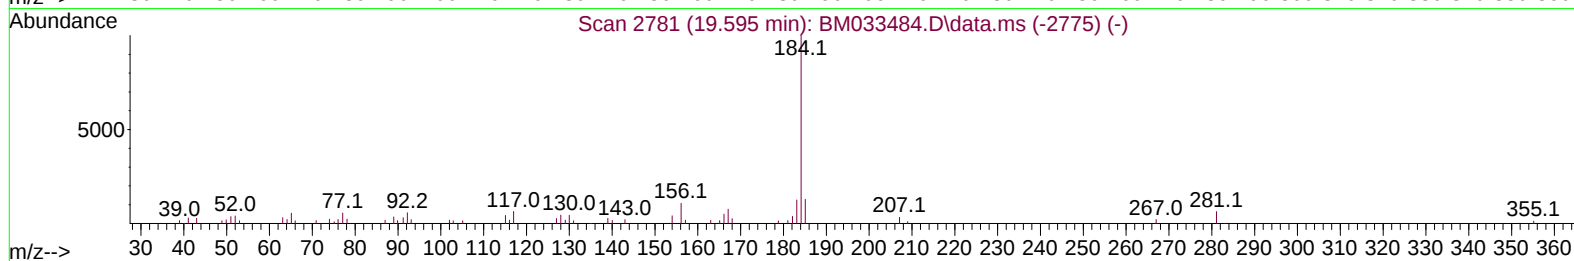
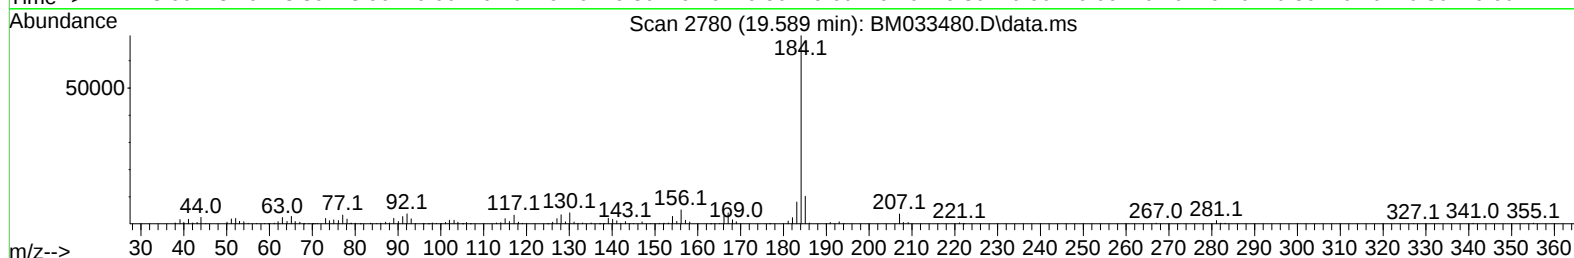


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121621\
Data File : BM033480.D
Acq On : 16 Dec 2021 11:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 17:45:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 17:10:15 2021
Response via : Initial Calibration

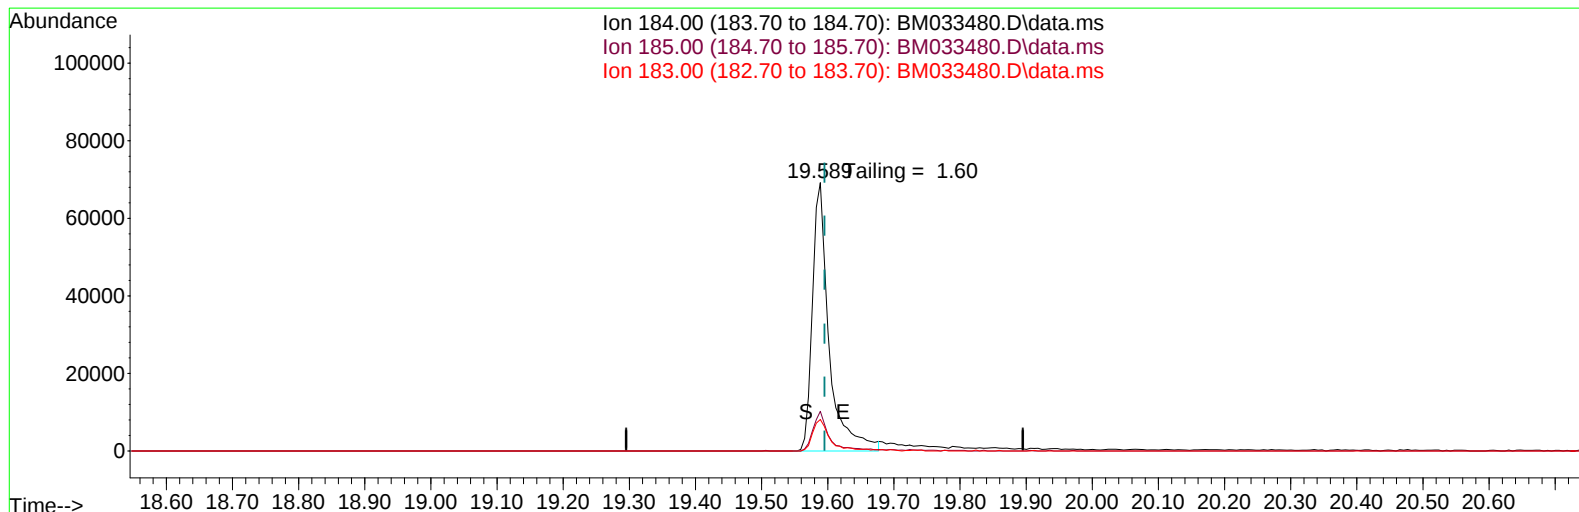

TIC: BM033480.D\data.ms




(77) Benzidine

19.589min (-0.006) 0.00 ng

response 127450

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.81
183.00	12.10	11.76
0.00	0.00	0.00

Quant Time: Dec 16 17:45:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 17:10:15 2021
Response via : Initial Calibration

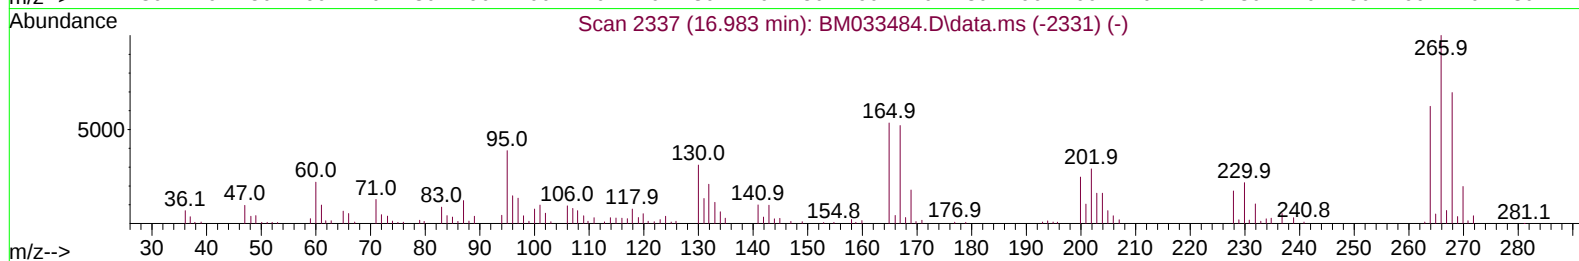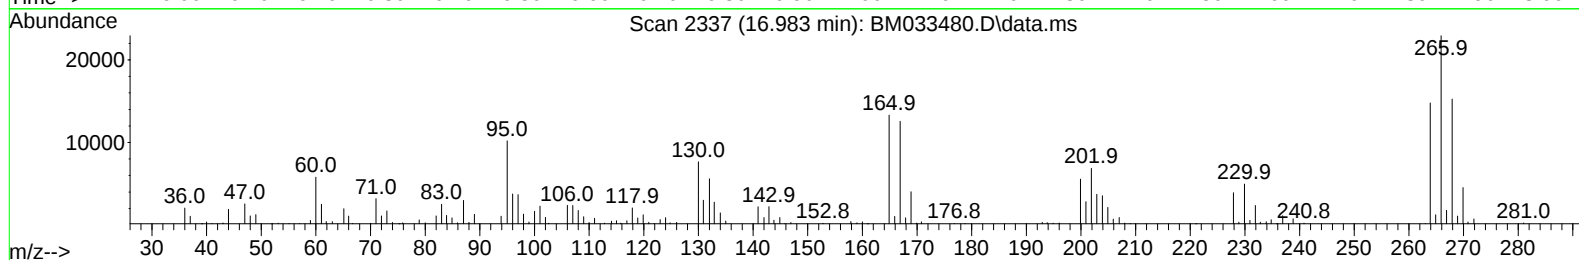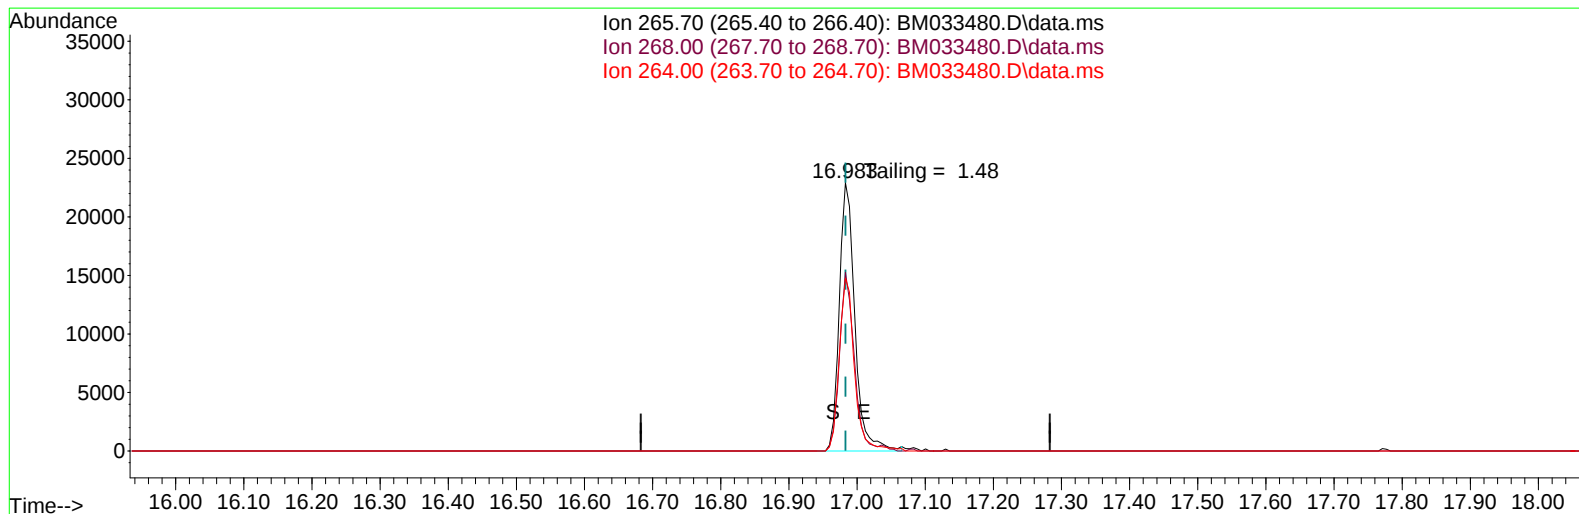

TIC: BM033480.D\data.ms

(70) **Pentachlorophenol (C)**

16.983min (-0.000) 0.00 ng

response **36365**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	66.53
264.00	61.40	64.47
0.00	0.00	0.00