

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121621\
 Data File : BM033489.D
 Acq On : 16 Dec 2021 17:59
 Operator : CG/JU
 Sample : PB141339BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB141339BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.502	379	385	402	rBV	570656	876421	45.26%	9.739%
2	7.108	651	658	674	rBV	556023	925390	47.79%	10.283%
3	7.937	793	799	809	rVB	141847	230640	11.91%	2.563%
4	9.113	989	999	1018	rBV	519473	907676	46.88%	10.086%
5	10.749	1270	1277	1291	rBV	157532	292563	15.11%	3.251%
6	13.207	1688	1695	1713	rBV	1184073	1827113	94.36%	20.304%
7	14.584	1923	1929	1943	rBV	242313	371420	19.18%	4.127%
8	16.078	2176	2183	2198	rBV	537121	834777	43.11%	9.276%
9	17.336	2391	2397	2407	rBV	245444	386065	19.94%	4.290%
10	19.954	2836	2842	2854	rBV	1582127	1936222	100.00%	21.516%
11	21.513	3103	3107	3118	rBV2	165352	273105	14.11%	3.035%
12	23.936	3515	3519	3529	rVB	65229	137585	7.11%	1.529%




Sum of corrected areas: 8998977

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121621\
Data File : BM033489.D
Acq On : 16 Dec 2021 17:59
Operator : CG/JU
Sample : PB141339BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

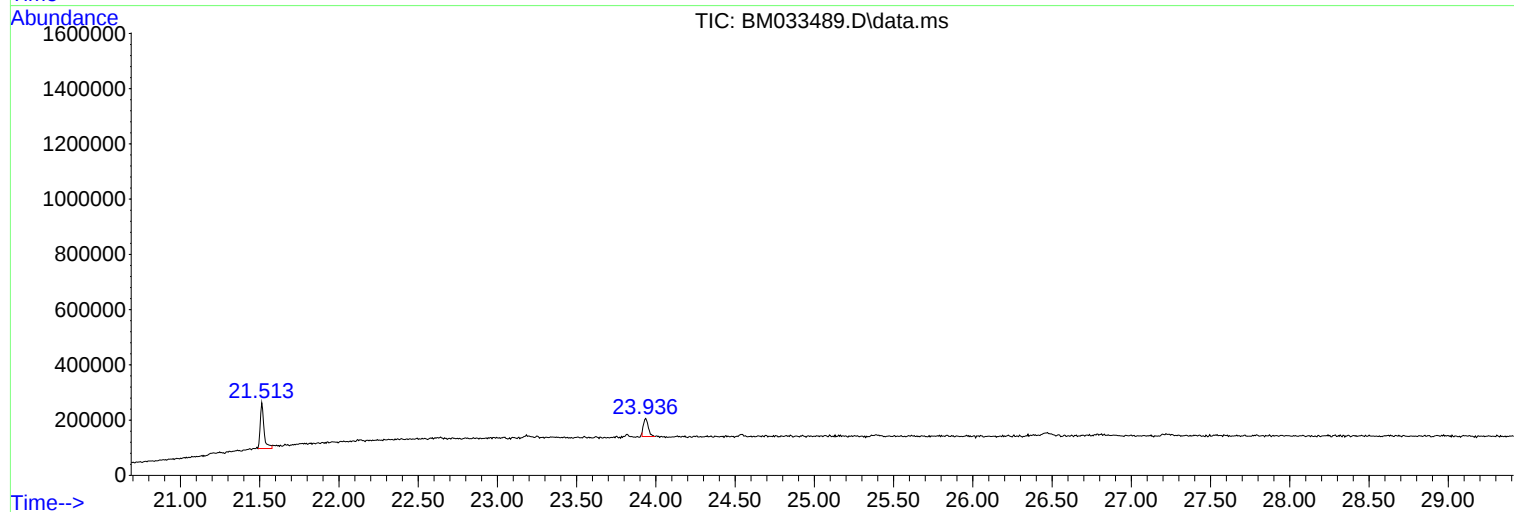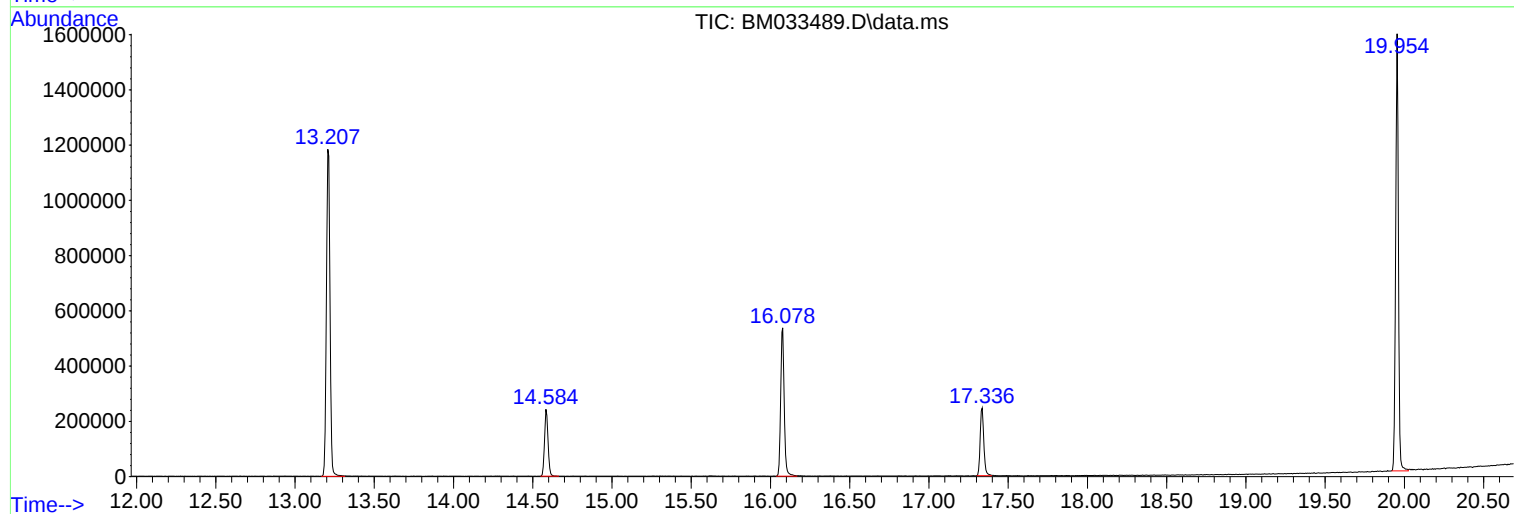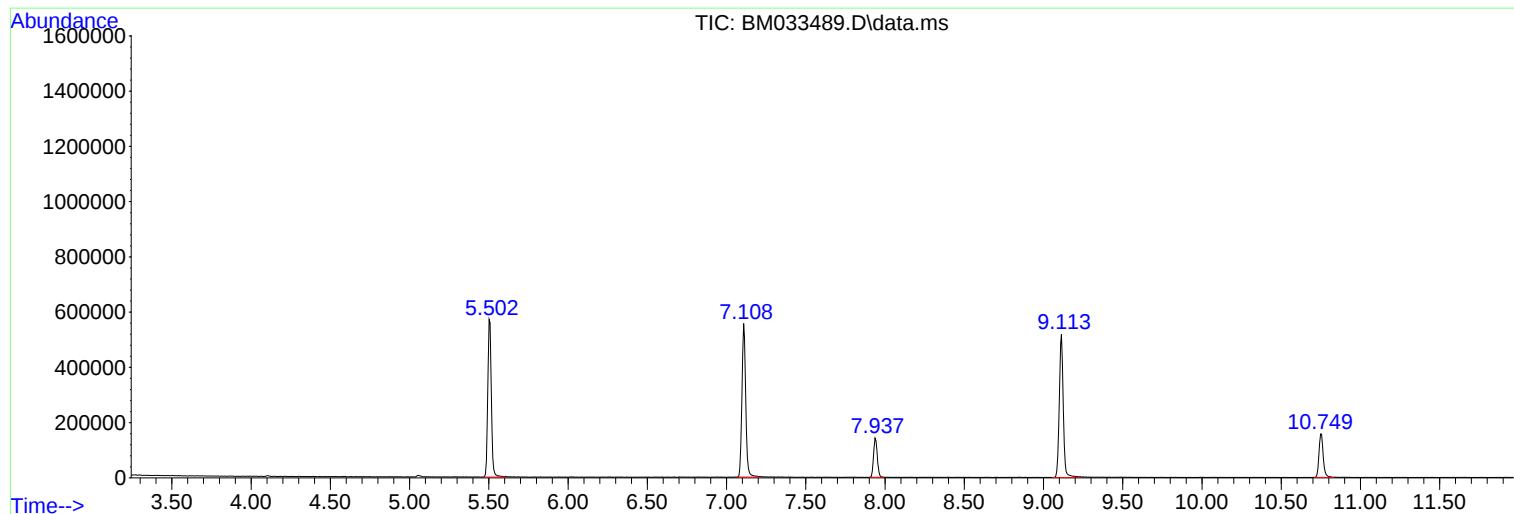

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121621\
Data File : BM033489.D
Acq On : 16 Dec 2021 17:59
Operator : CG/JU
Sample : PB141339BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121621\
Data File : BM033489.D
Acq On : 16 Dec 2021 17:59
Operator : CG/JU
Sample : PB141339BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------