

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121621\
 Data File : BM033490.D
 Acq On : 16 Dec 2021 18:36
 Operator : CG/JU
 Sample : PB141485BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB141485BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.501	379	385	401	rBV	692351	1052611	66.05%	12.861%
2	7.107	652	658	671	rBV	668992	1104114	69.28%	13.490%
3	7.937	791	799	808	rBV	111976	186296	11.69%	2.276%
4	9.113	991	999	1014	rBV	416795	724992	45.49%	8.858%
5	10.754	1270	1278	1295	rBV	128648	241639	15.16%	2.952%
6	13.207	1689	1695	1707	rBV	937740	1457571	91.46%	17.809%
7	14.583	1923	1929	1939	rVB	190080	300376	18.85%	3.670%
8	16.077	2176	2183	2201	rBV	655195	1000322	62.77%	12.222%
9	17.336	2391	2397	2409	rBV	197055	308680	19.37%	3.772%
10	19.953	2836	2842	2855	rBV	1282567	1593669	100.00%	19.472%
11	21.518	3103	3108	3120	rBV	130224	214223	13.44%	2.617%




Sum of corrected areas: 8184493

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121621\
Data File : BM033490.D
Acq On : 16 Dec 2021 18:36
Operator : CG/JU
Sample : PB141485BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141485BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

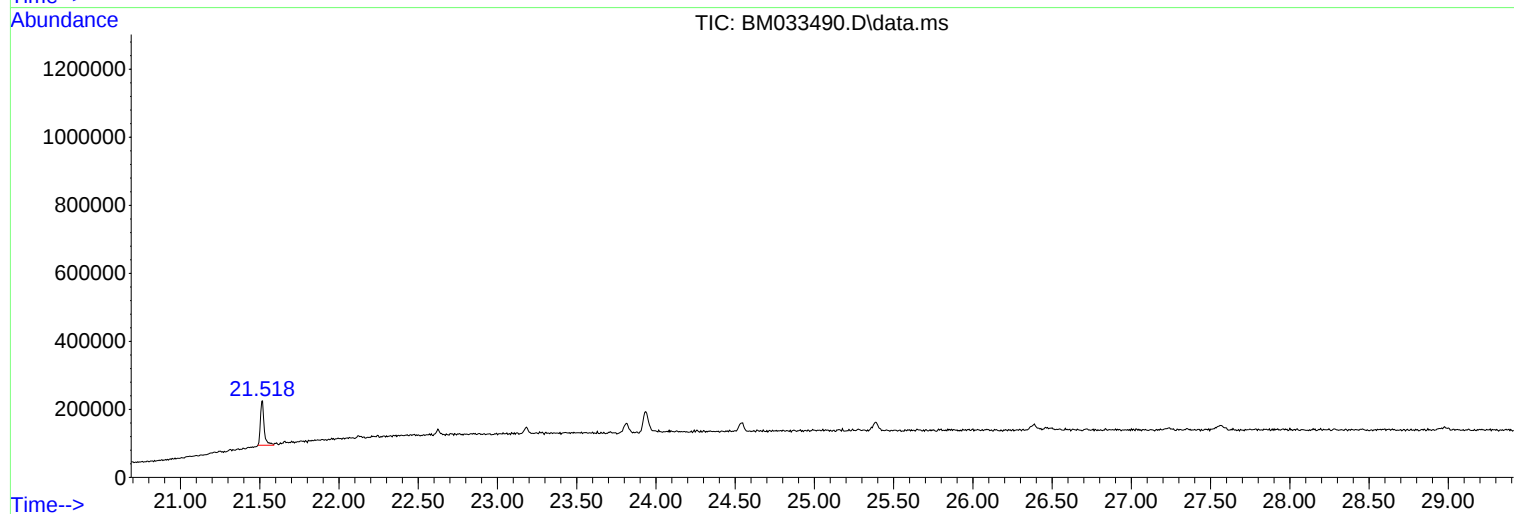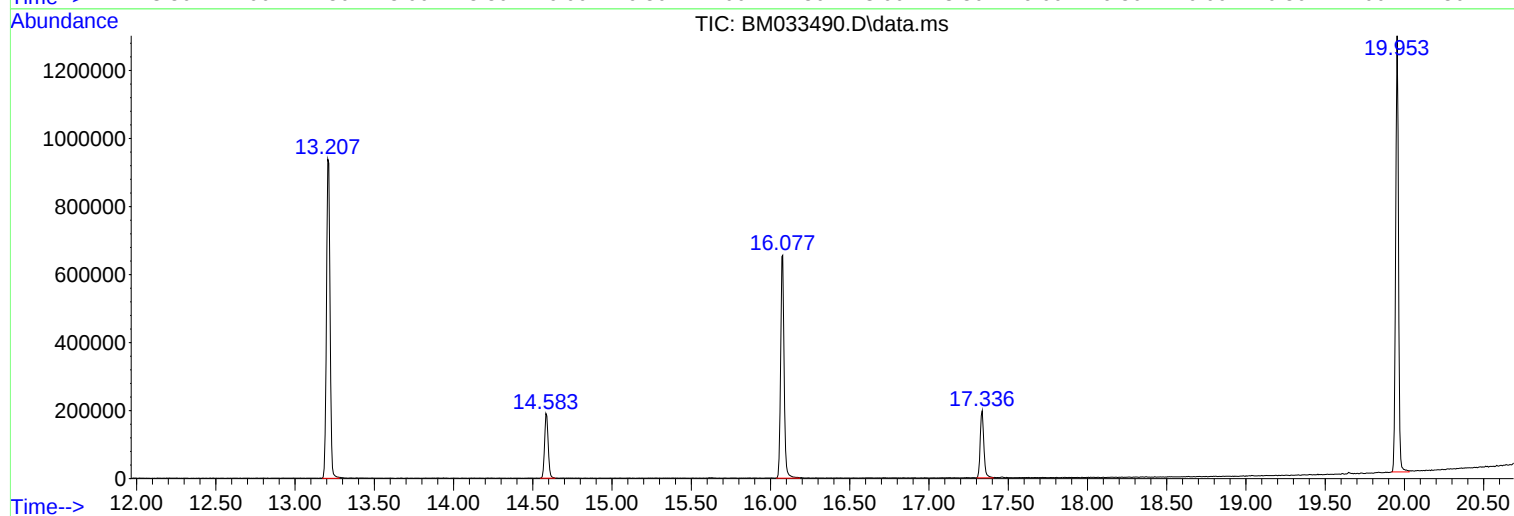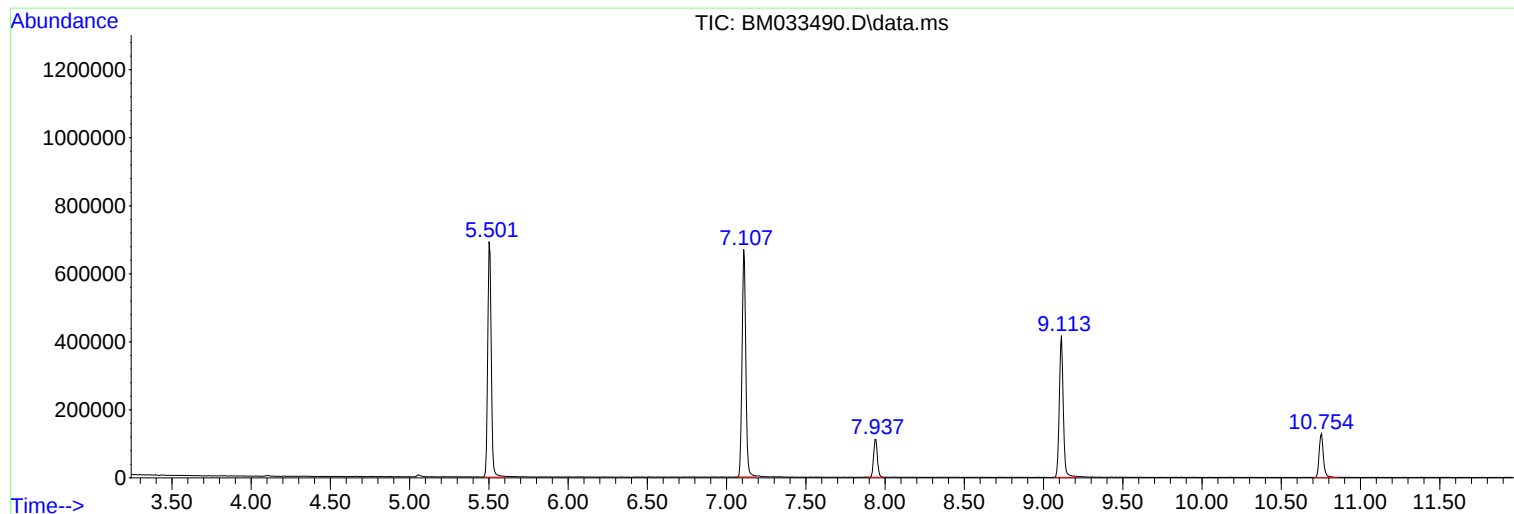

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121621\
Data File : BM033490.D
Acq On : 16 Dec 2021 18:36
Operator : CG/JU
Sample : PB141485BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141485BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121621\
Data File : BM033490.D
Acq On : 16 Dec 2021 18:36
Operator : CG/JU
Sample : PB141485BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141485BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------