
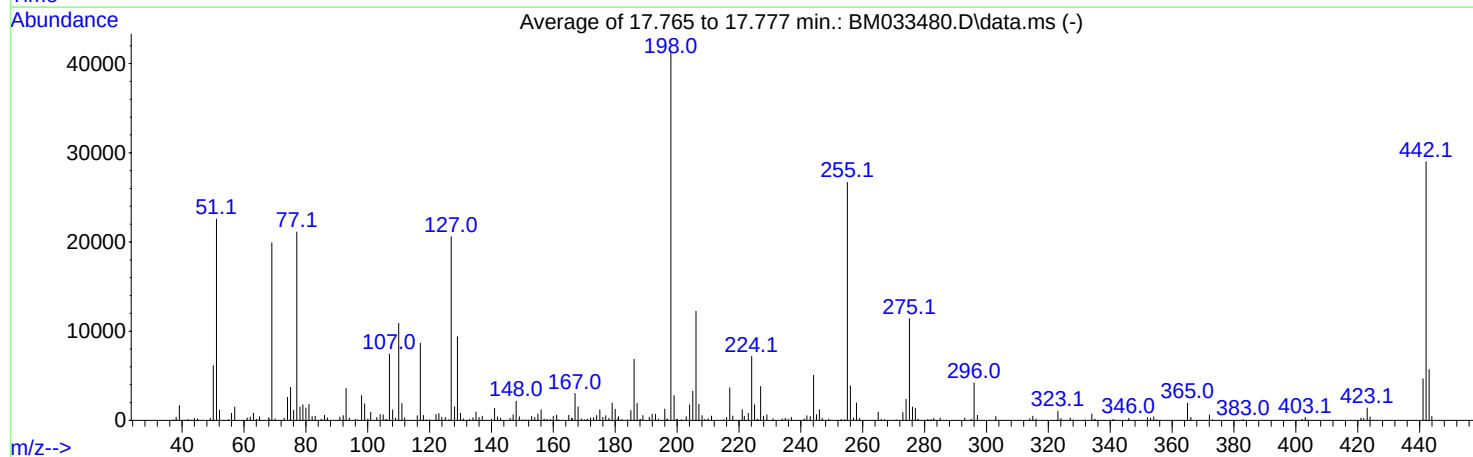


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121621\
 Data File : BM033480.D
 Acq On : 16 Dec 2021 11:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 08 01:18:09 2021

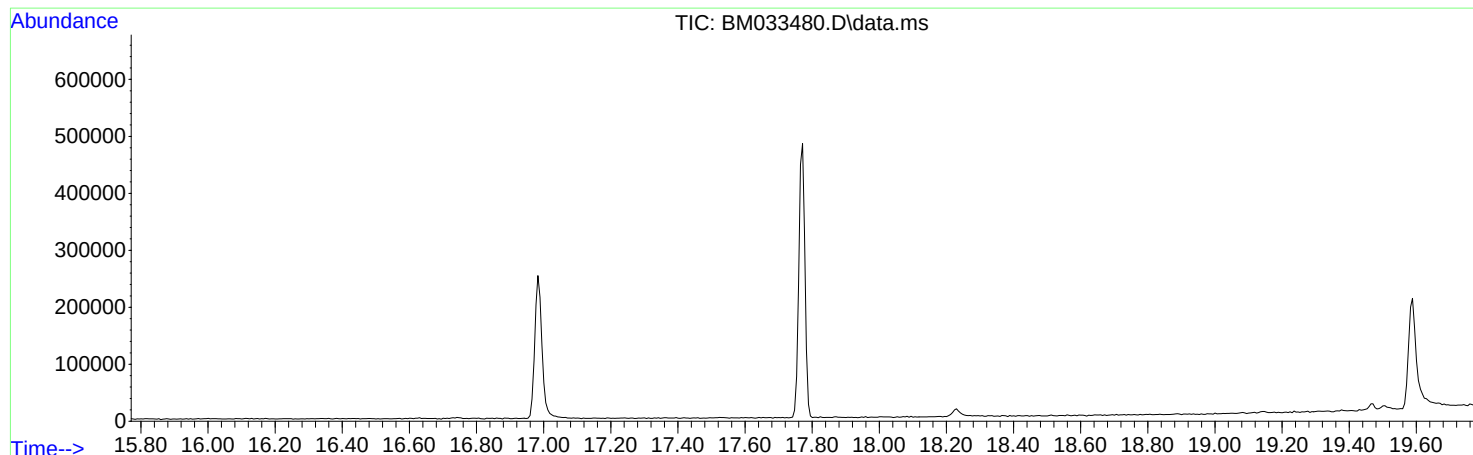




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.7	22559	PASS
68	69	0.00	2	1.5	300	PASS
69	198	0.00	100	48.3	19905	PASS
70	69	0.00	2	0.8	161	PASS
127	198	10	80	49.9	20592	PASS
197	198	0.00	2	0.4	149	PASS
198	198	100	100	100.0	41240	PASS
199	198	5	9	6.7	2781	PASS
275	198	10	60	27.7	11411	PASS
365	198	1	100	4.7	1920	PASS
441	198	0.01	100	11.3	4663	PASS
442	442	50	100	100.0	28995	PASS
443	442	15	24	19.6	5689	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121621\
 Data File : BM033480.D
 Acq On : 16 Dec 2021 11:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Dec 16 17:45:23 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 17:10:15 2021
 Response via : Initial Calibration

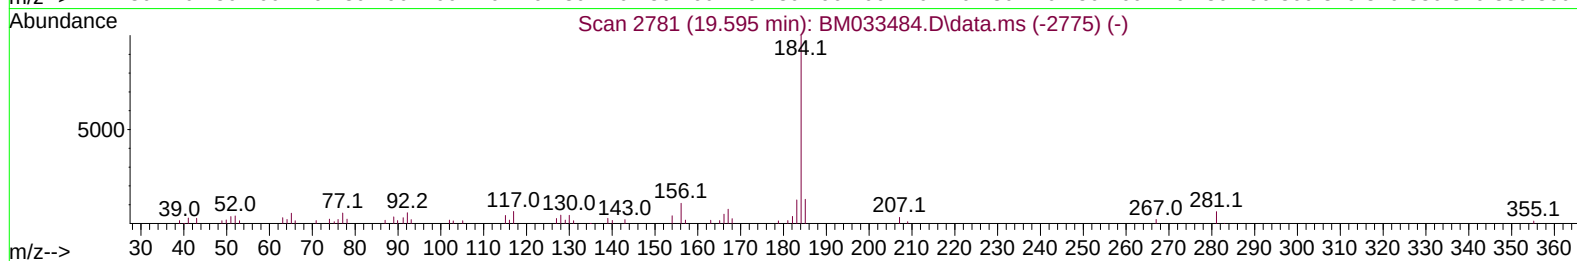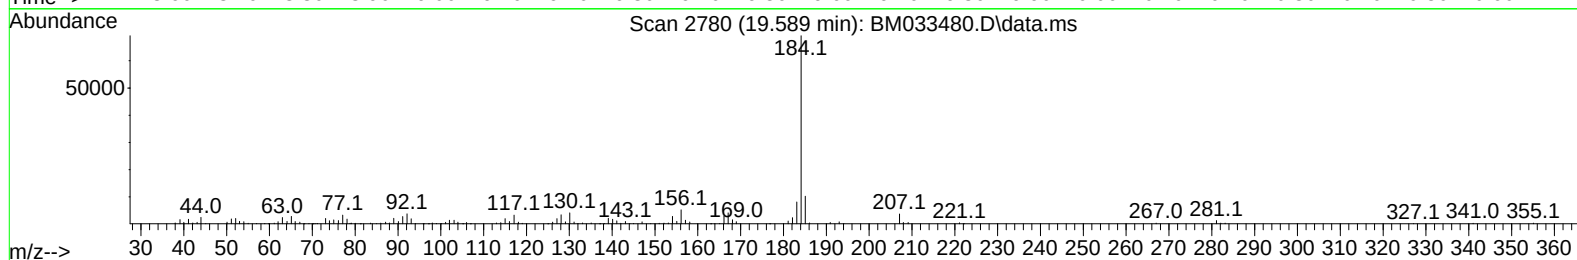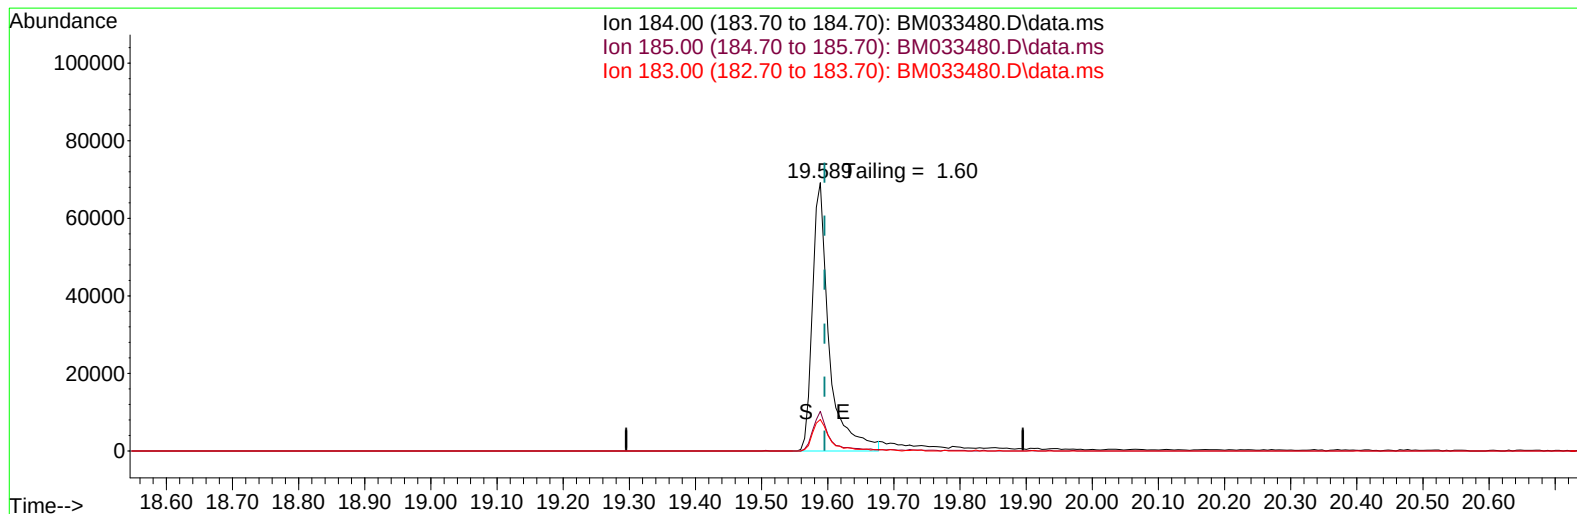

TIC: BM033480.D\data.ms

(77) Benzidine

19.589min (-0.006) 0.00 ng


response 127450

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.81
183.00	12.10	11.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121621\
Data File : BM033480.D
Acq On : 16 Dec 2021 11:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 16 17:45:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 17:10:15 2021
Response via : Initial Calibration

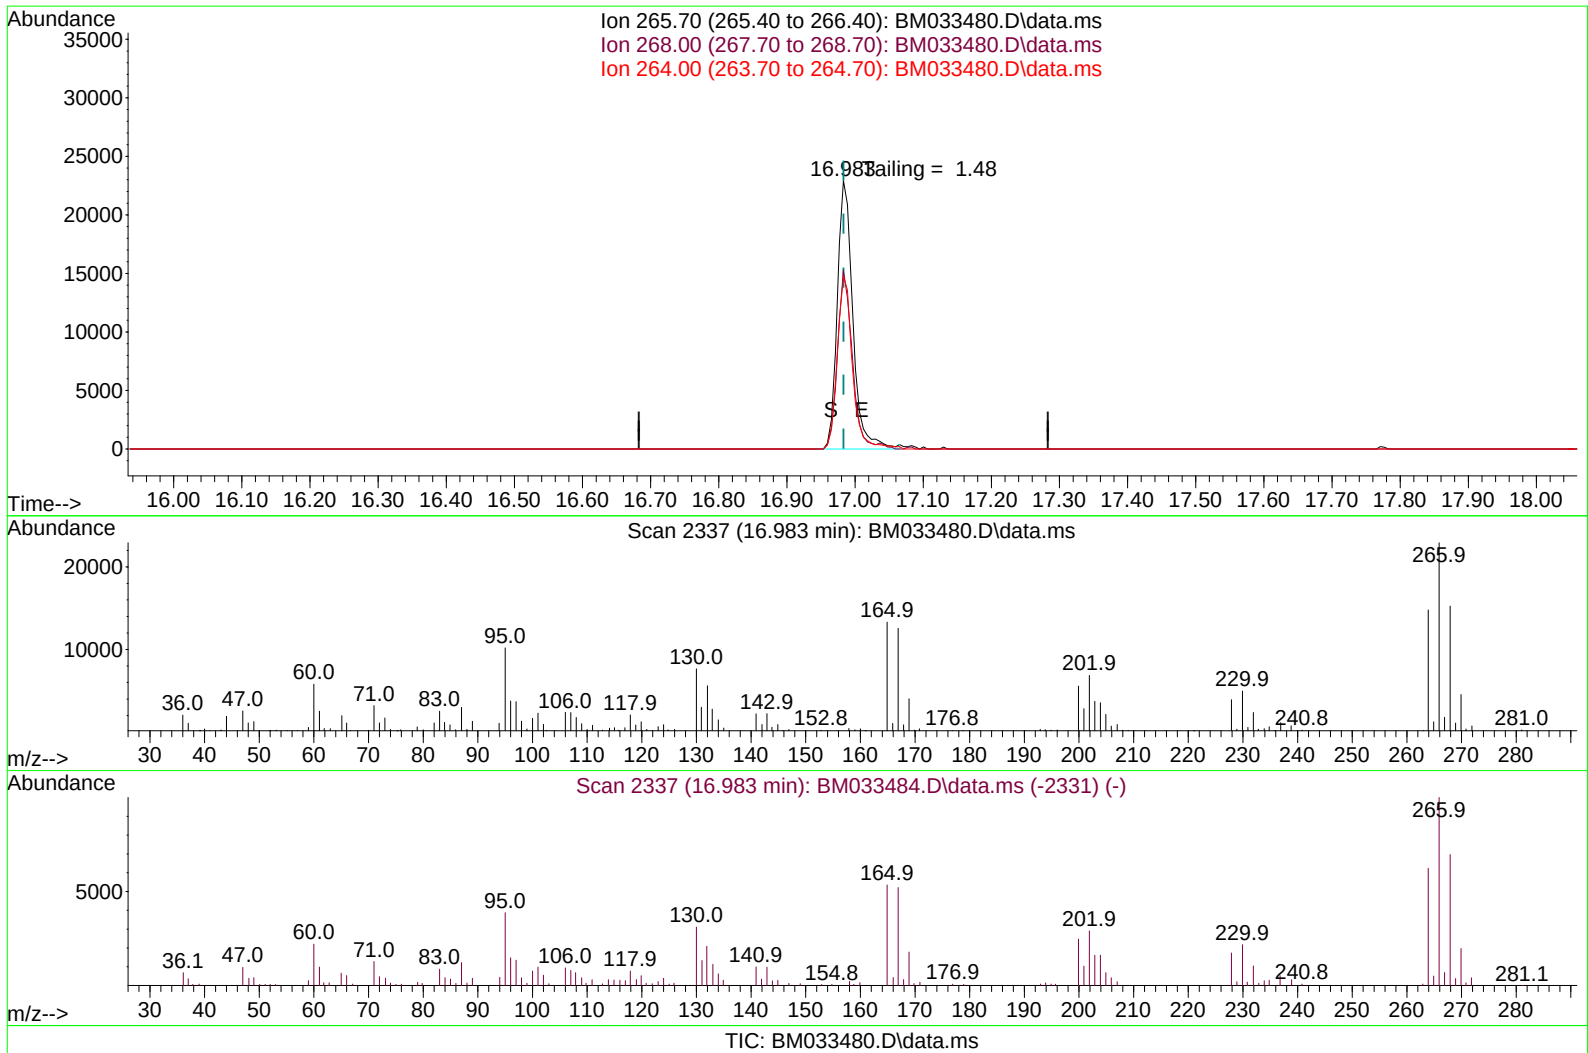

(70) Pentachlorophenol (C)

16.983min (-0.000) 0.00 ng

response 36365

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	66.53
264.00	61.40	64.47
0.00	0.00	0.00

Instrument :
BNA_M
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/16/2021	BNA_M	<u>BM033480.D</u>
Compound Name	Response	Retention Time
DDT	116431	20.81
DDD	4148	20.37
DDE	745	19.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4893	121324	4.03

Instrument :
BNA_M
ClientSampleId :
DFTPP