
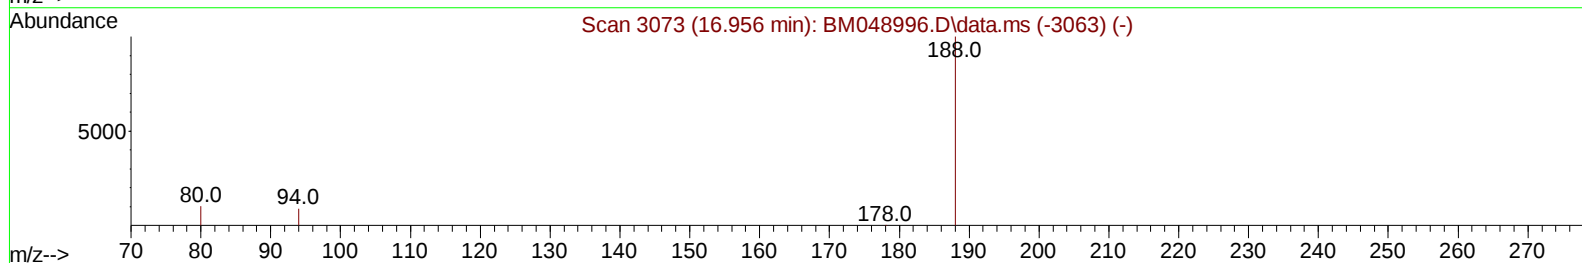
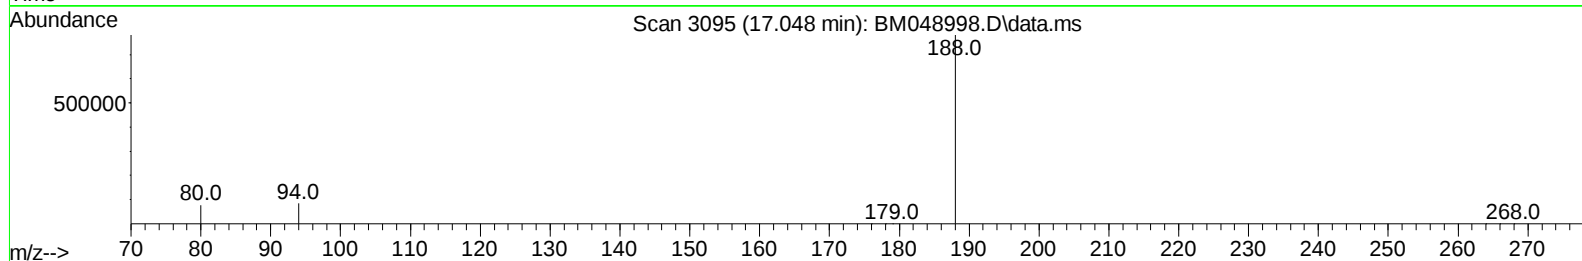


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM048998.D
Acq On : 16 Dec 2024 11:11
Operator : RC/JU
Sample : PB165614BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 16 11:44:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

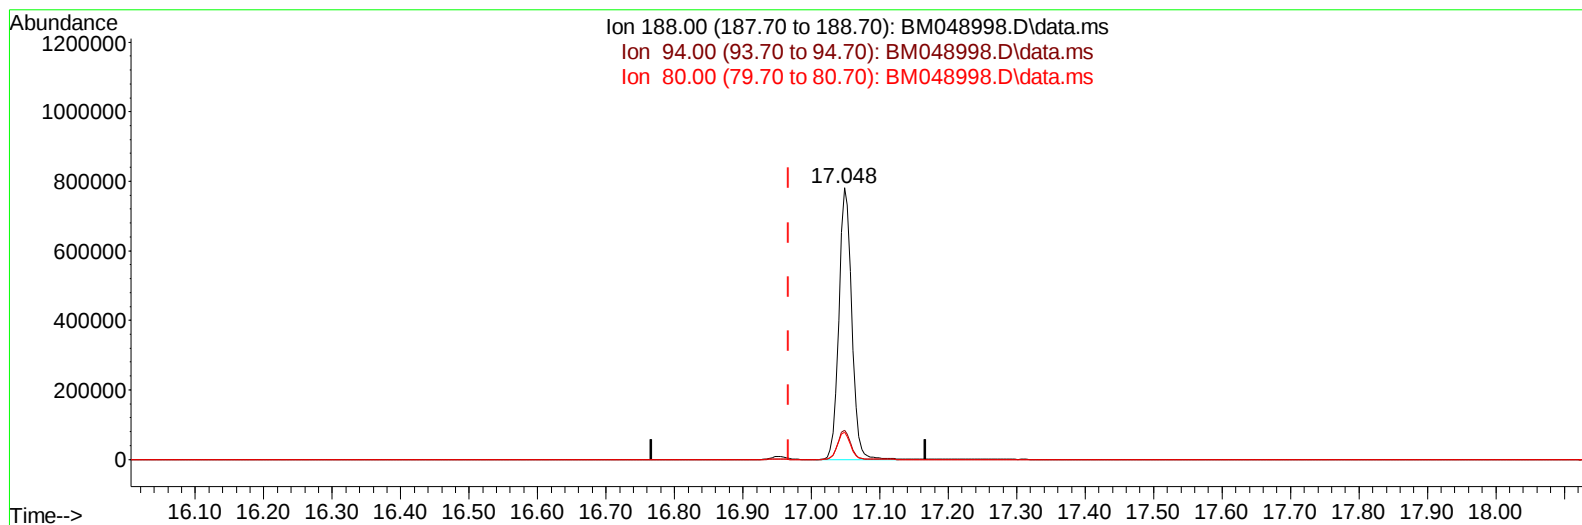

TIC: BM048998.D\data.ms

(13) Phenanthrene-d10 (I)




17.048min (+ 0.081) 0.40 ng/ul

response 1020195

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	10.83
80.00	13.90	9.99#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM048998.D
Acq On : 16 Dec 2024 11:11
Operator : RC/JU
Sample : PB165614BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 16 11:44:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

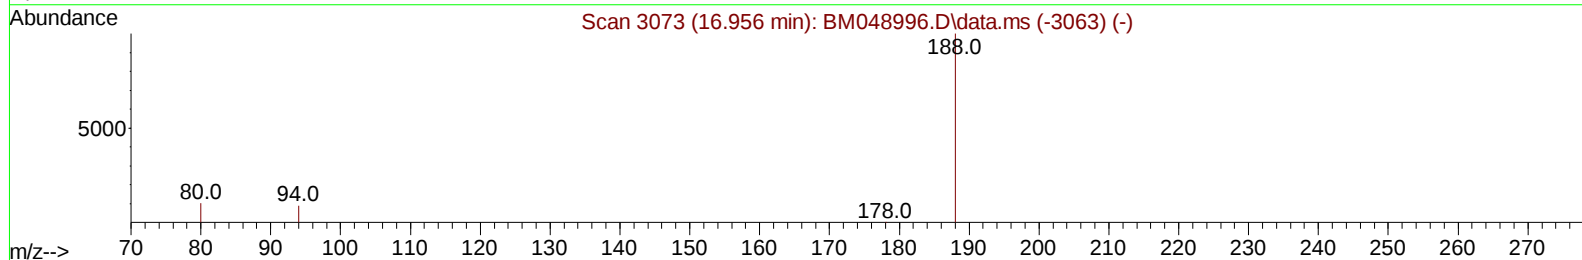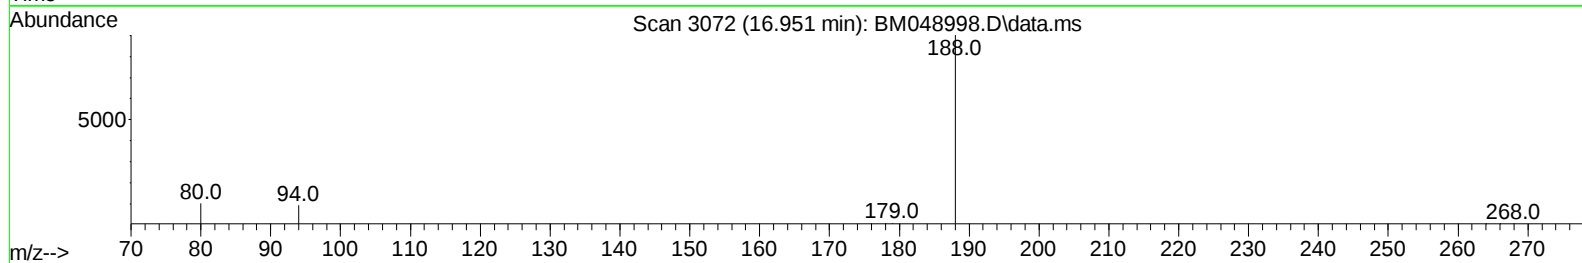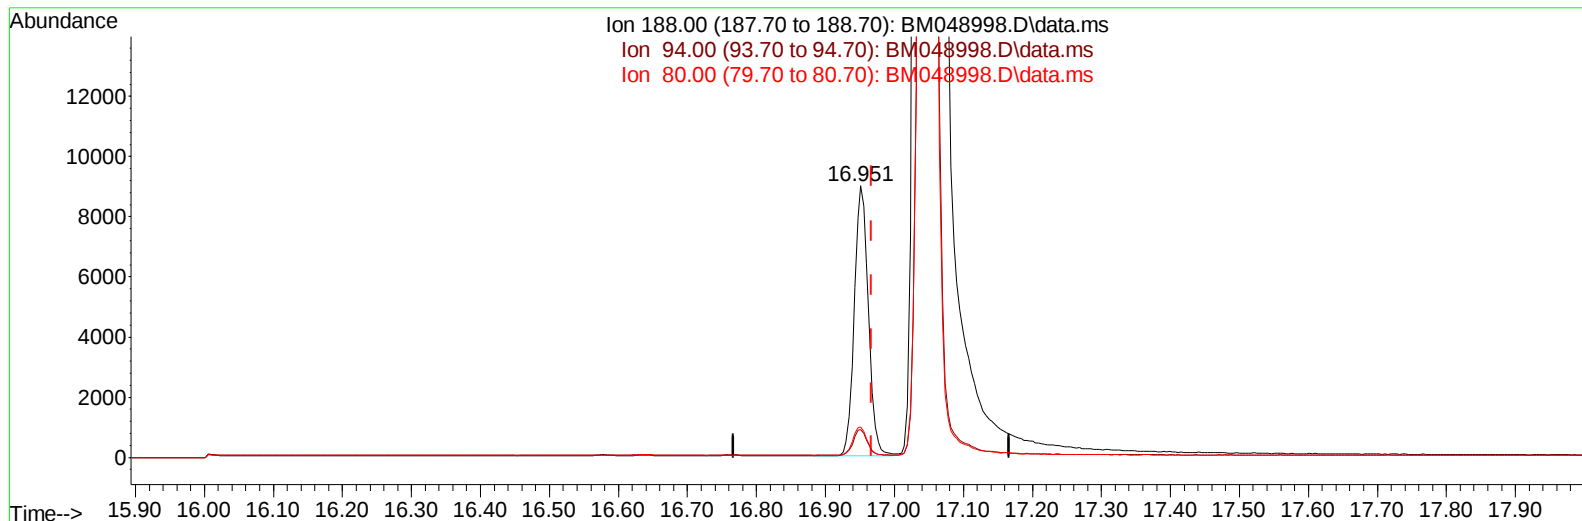

TIC: BM048998.D\data.ms

(13) Phenanthrene-d10 (I)




16.951min (-0.016) 0.40 ng/ul m

response 12751

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	10.24
80.00	13.90	11.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM048998.D
Acq On : 16 Dec 2024 11:11
Operator : RC/JU
Sample : PB165614BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 16 11:44:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

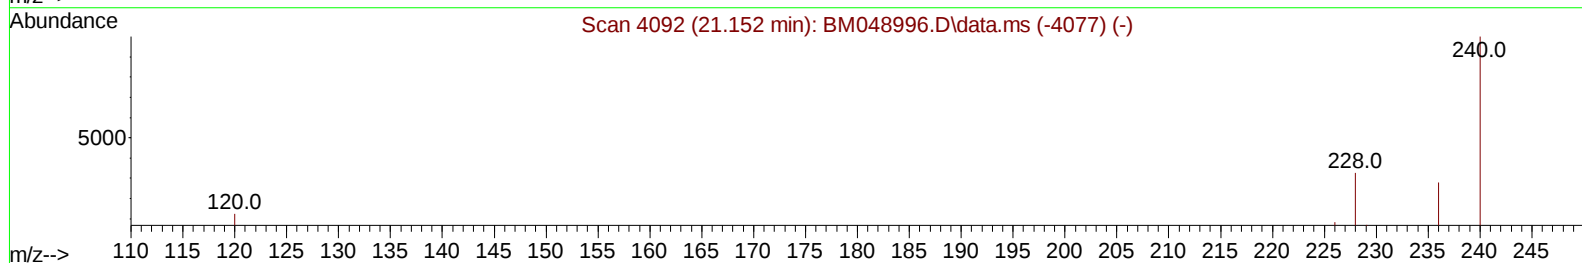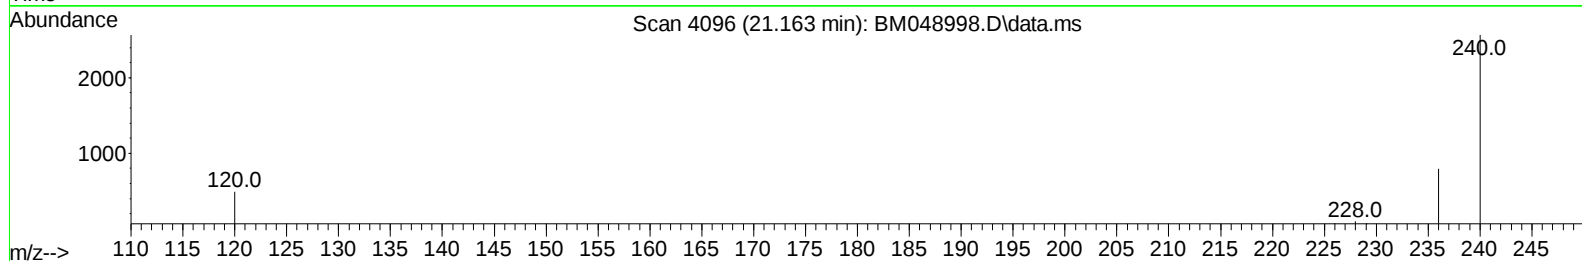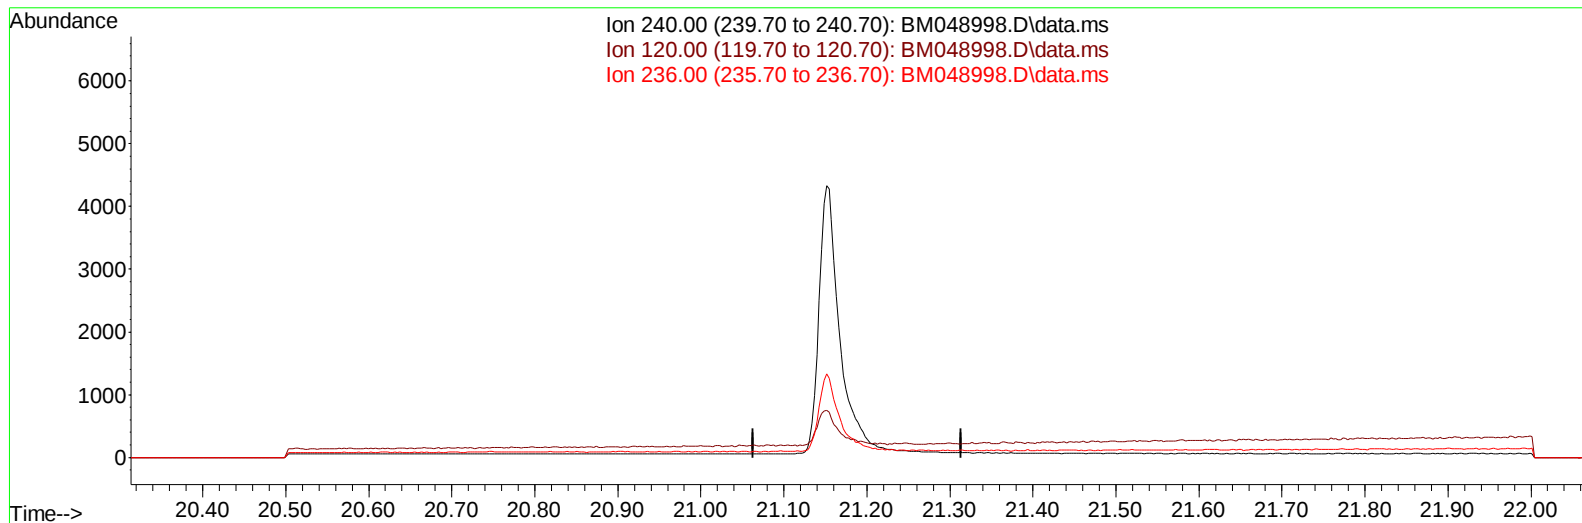

TIC: BM048998.D\data.ms

(17) Chrysene-d12




21.164min (-21.164) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	18.30	0.00#
236.00	30.50	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM048998.D
Acq On : 16 Dec 2024 11:11
Operator : RC/JU
Sample : PB165614BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 16 11:44:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

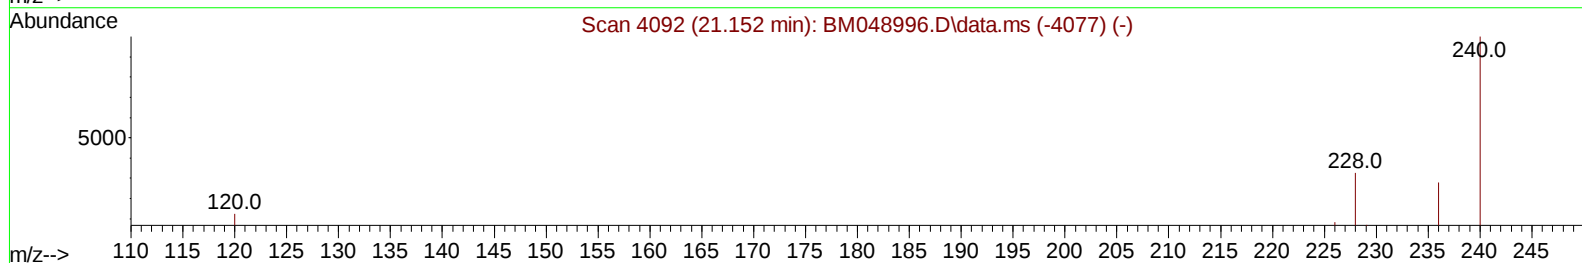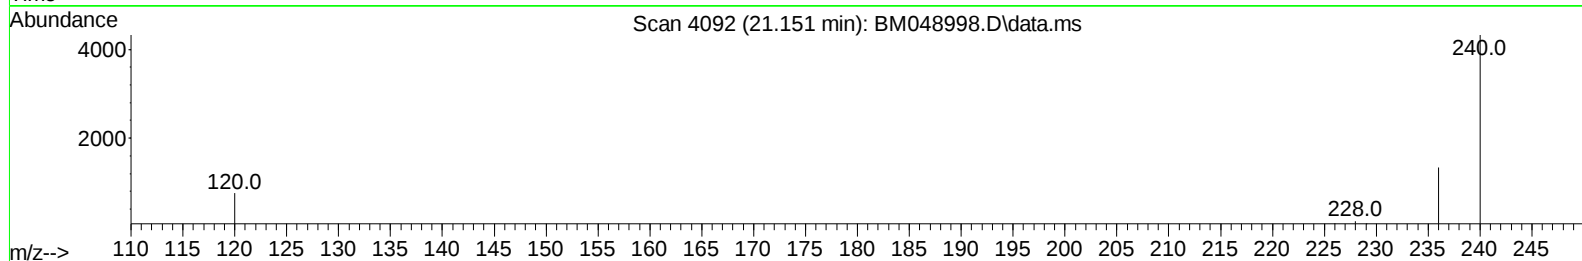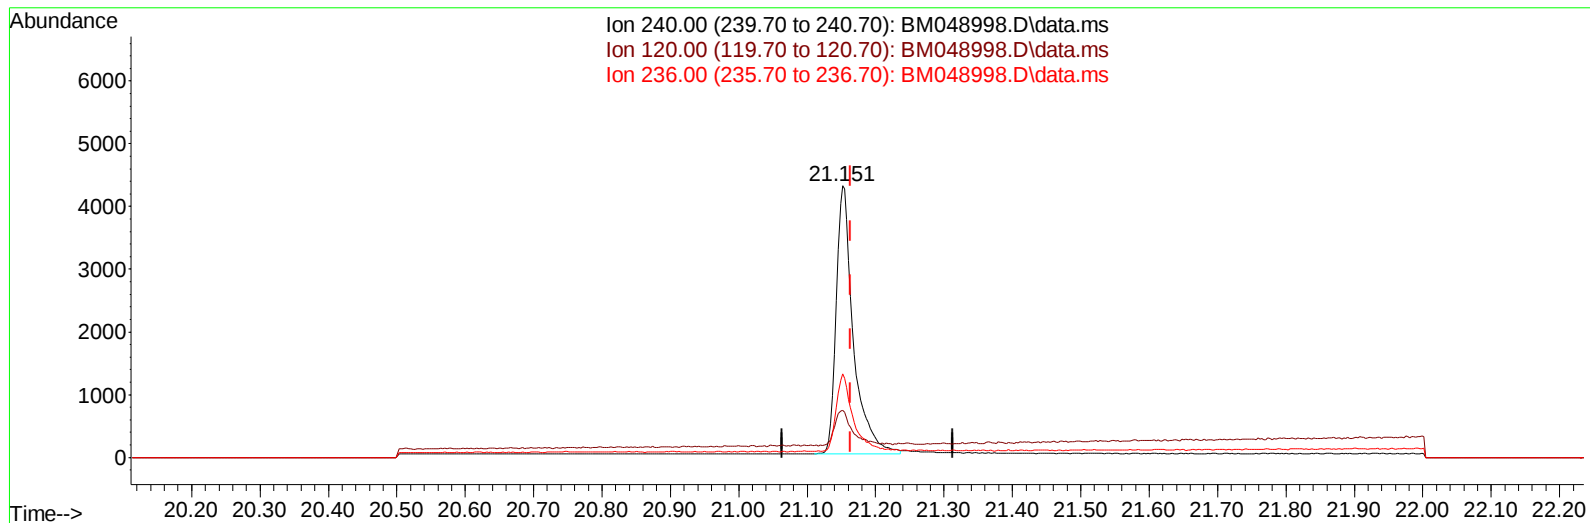

TIC: BM048998.D\data.ms

(17) Chrysene-d12




21.151min (-0.012) 0.40 ng/ul m

response 7464

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	18.30	17.43
236.00	30.50	30.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM048998.D
Acq On : 16 Dec 2024 11:11
Operator : RC/JU
Sample : PB165614BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 16 11:44:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

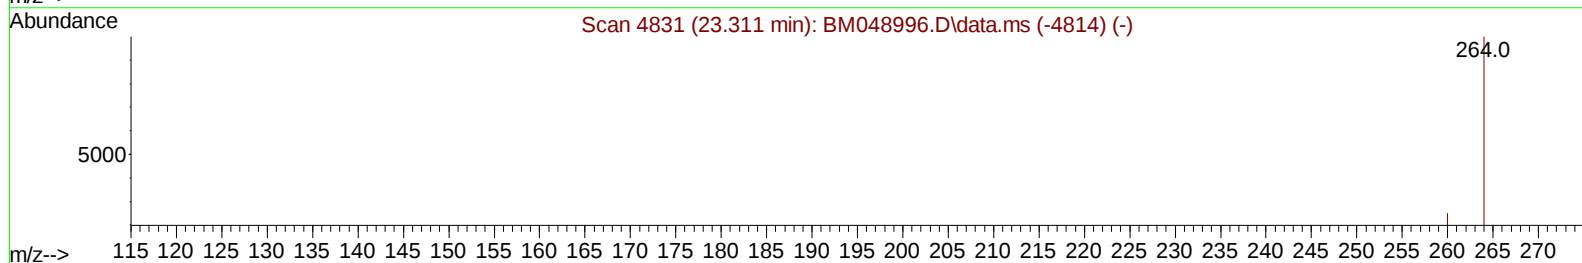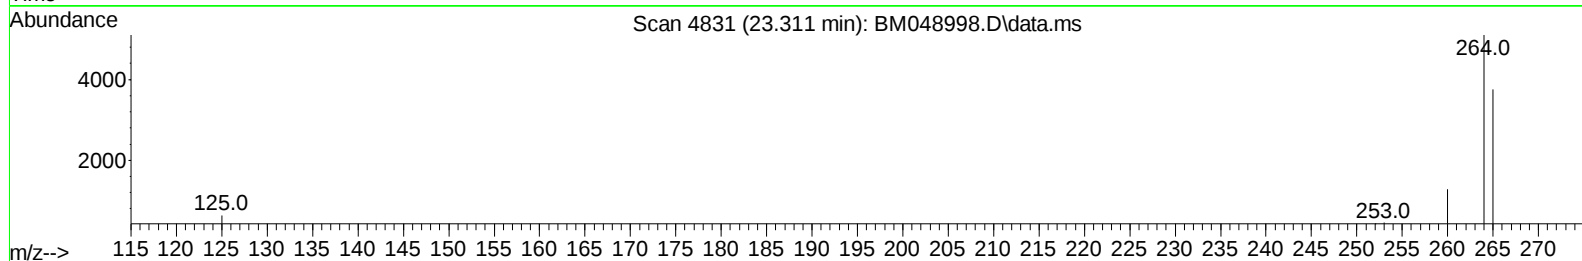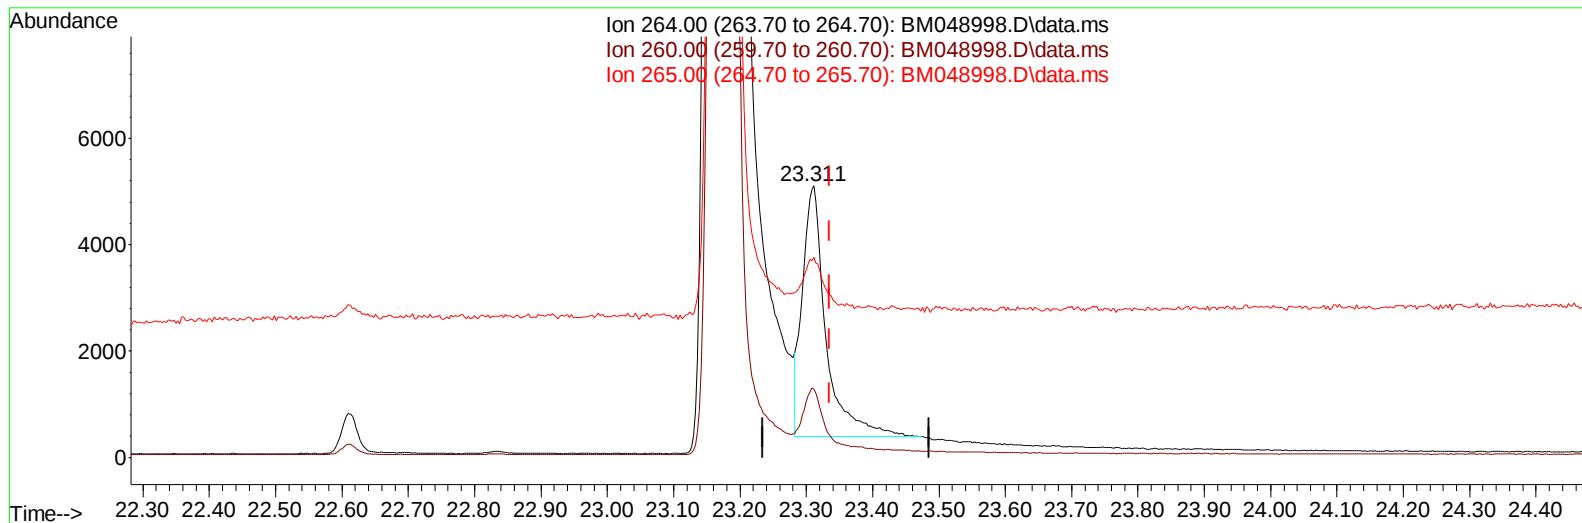

TIC: BM048998.D\data.ms

(23) Perylene-d12 (I)




23.311min (-0.024) 0.40 ng/u1

response 11823

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	25.05
265.00	82.60	73.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM048998.D
Acq On : 16 Dec 2024 11:11
Operator : RC/JU
Sample : PB165614BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 16 11:44:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

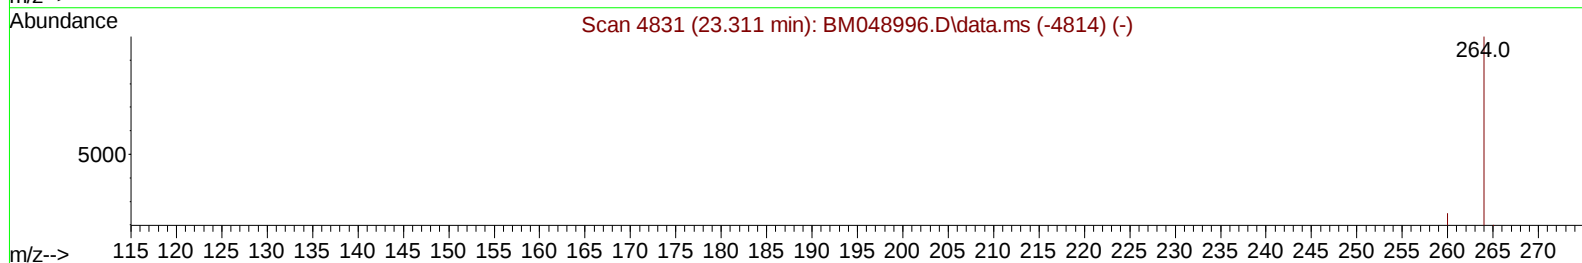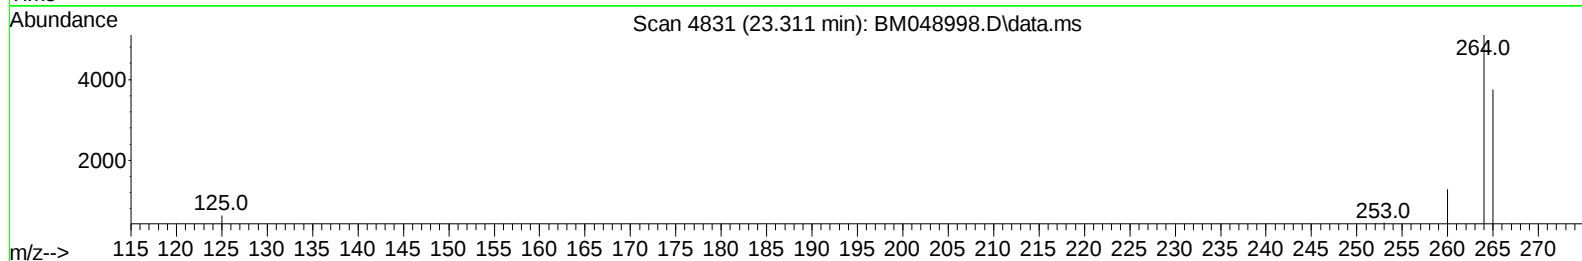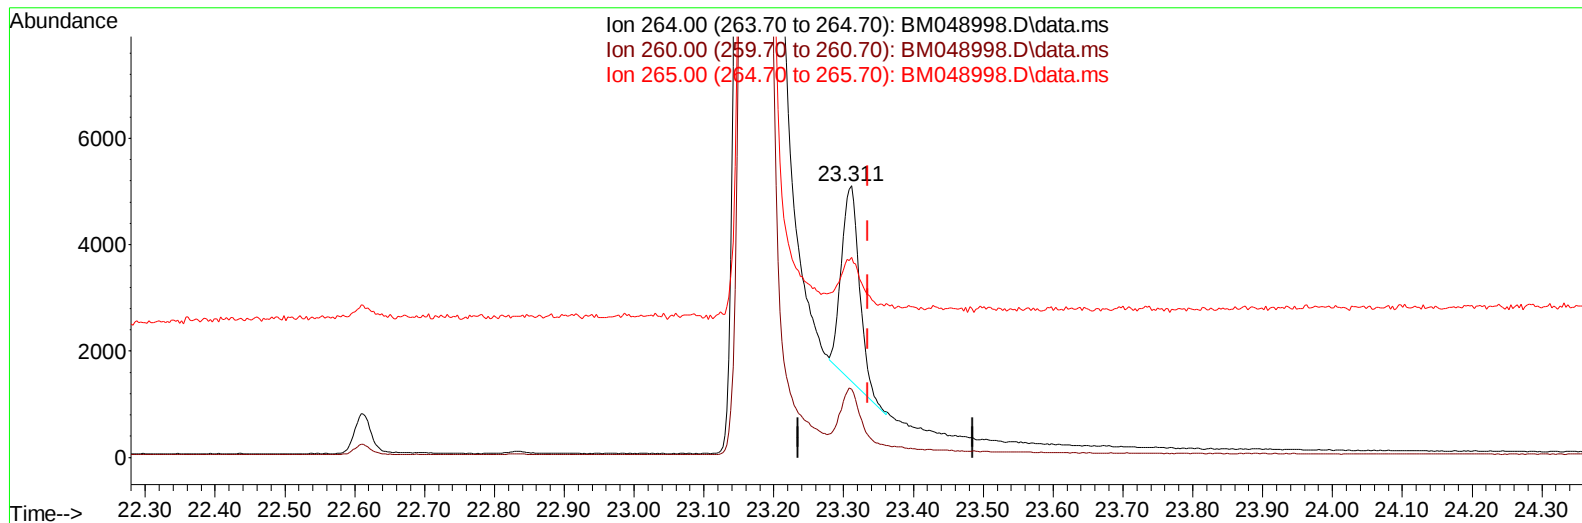

TIC: BM048998.D\data.ms

(23) Perylene-d12 (I)

23.311min (-0.024) 0.40 ng/ul m

response 6493

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	25.05
265.00	82.60	73.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
 Data File : BM048998.D
 Acq On : 16 Dec 2024 11:11
 Operator : RC/JU
 Sample : PB165614BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 16 11:44:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 09 17:52:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.573	152	4526	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.337	136	12247	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.206	164	6279	0.400	ng/ul	-0.02
13) Phenanthrene-d10	16.951	188	12751m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.151	240	7464m	0.400	ng/ul	-0.01
23) Perylene-d12	23.311	264	6493m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	32467	6.138	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.943	152	5003	0.320	ng/ul	0.00
18) Fluoranthene-d10	18.988	212	8526	0.382	ng/ul	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM048998.D
Acq On : 16 Dec 2024 11:11
Operator : RC/JU
Sample : PB165614BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 16 11:44:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

