
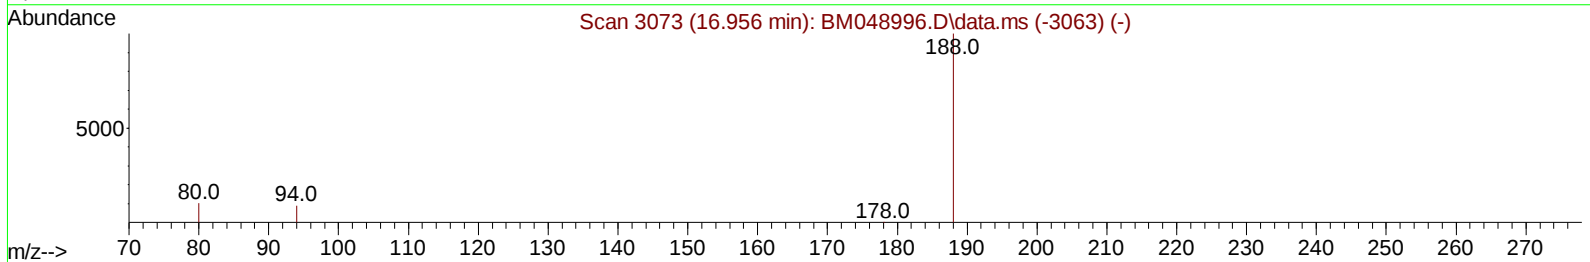
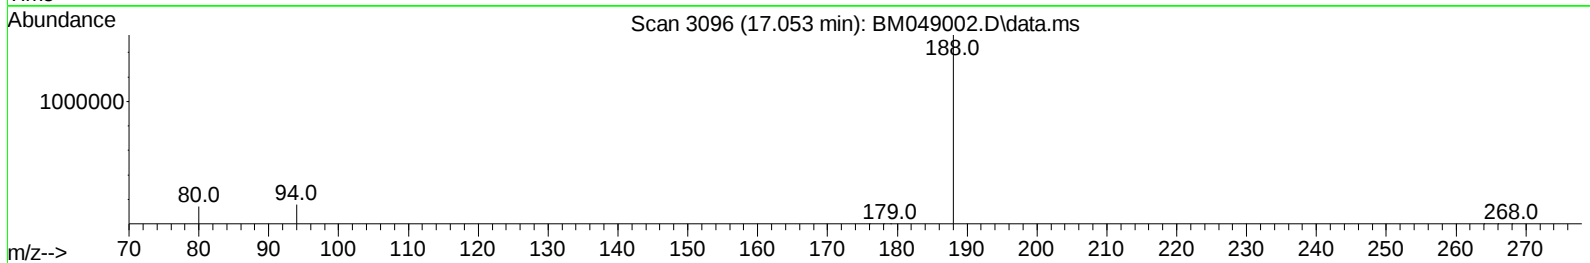


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049002.D
Acq On : 16 Dec 2024 13:35
Operator : RC/JU
Sample : P5247-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Dec 16 14:04:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

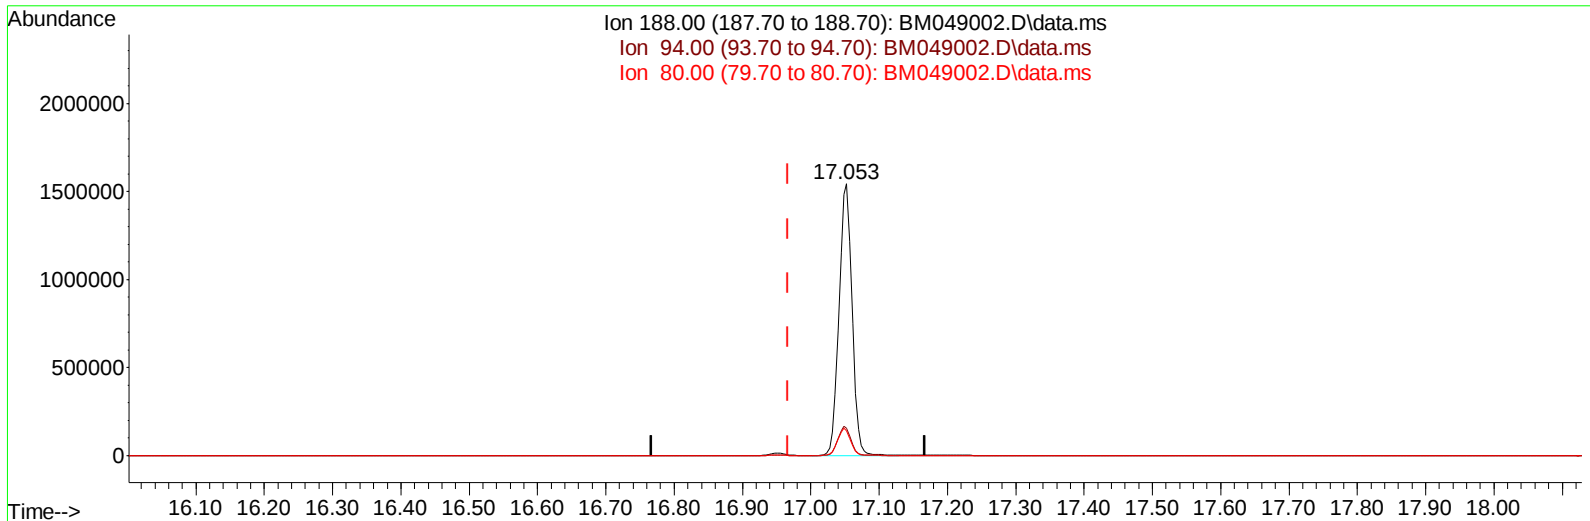




TIC: BM049002.D\data.ms

(13) Phenanthrene-d10 (I)**17.053min (+ 0.086) 0.40 ng/u1****response 2032683**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	10.03
80.00	13.90	9.15#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049002.D
Acq On : 16 Dec 2024 13:35
Operator : RC/JU
Sample : P5247-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Dec 16 14:04:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

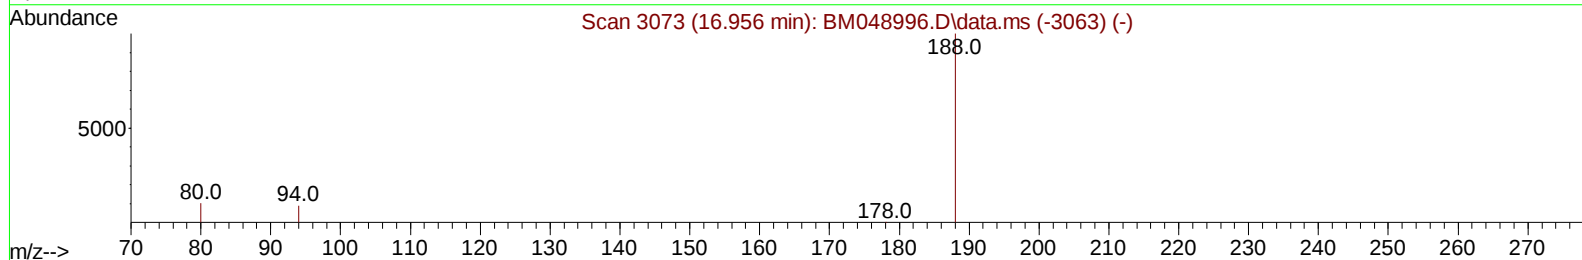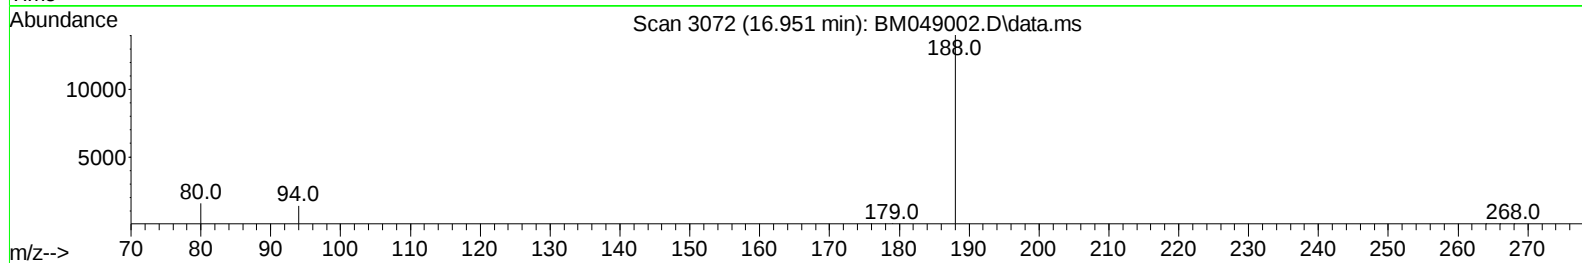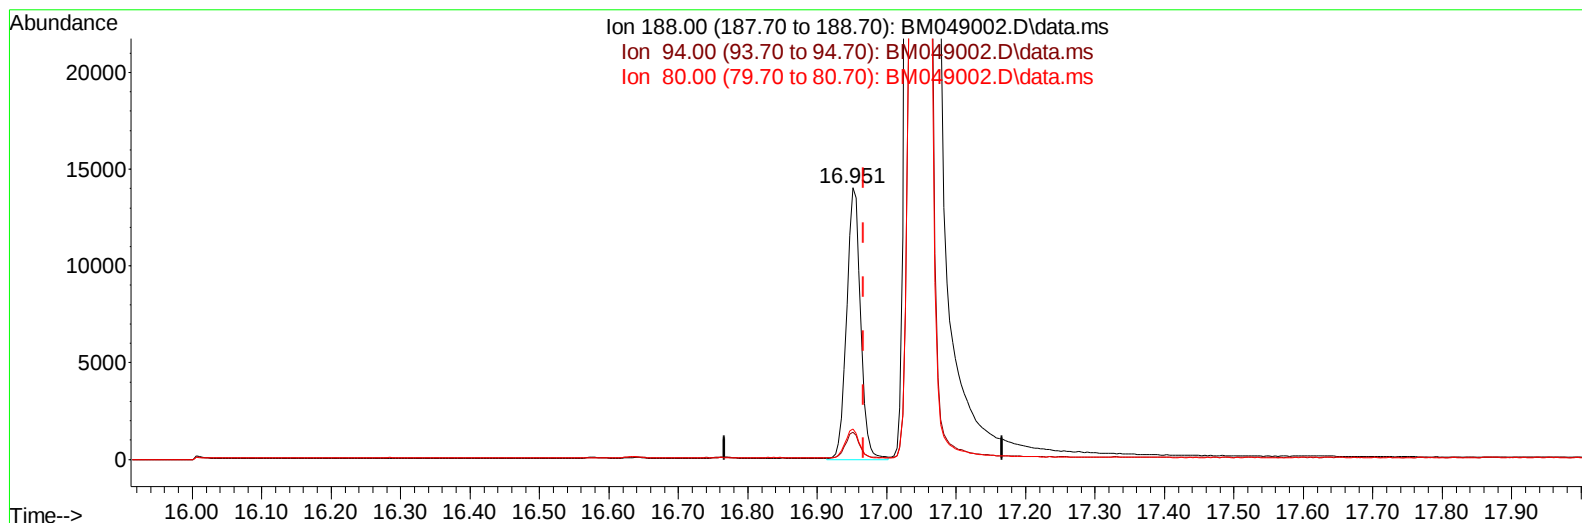




TIC: BM049002.D\data.ms

(13) Phenanthrene-d10 (I)**16.951min (-0.015) 0.40 ng/ul m****response 19424**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	10.00
80.00	13.90	11.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049002.D
Acq On : 16 Dec 2024 13:35
Operator : RC/JU
Sample : P5247-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Dec 16 14:04:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

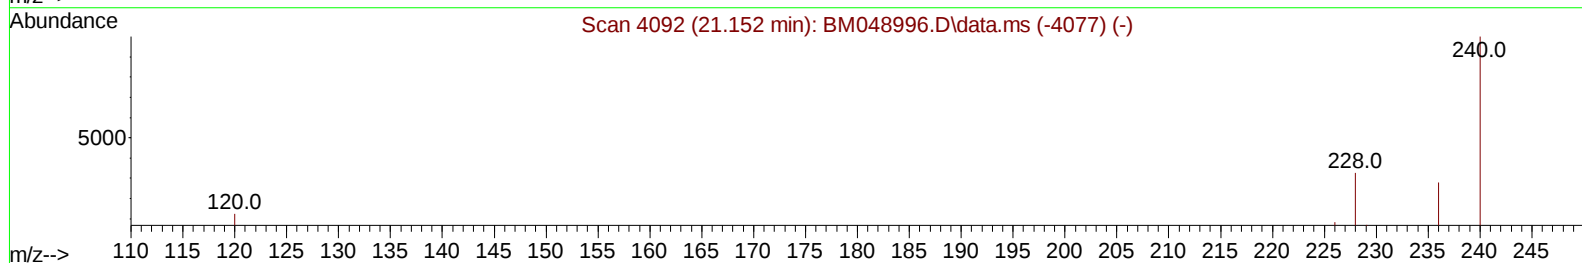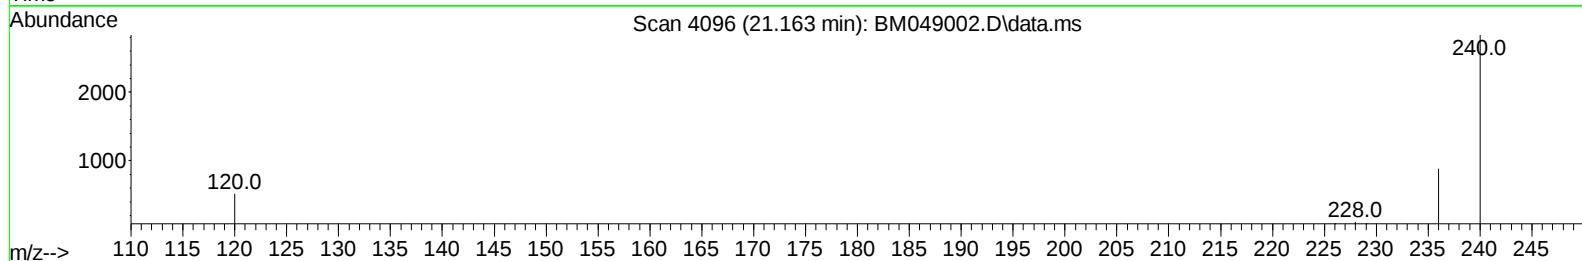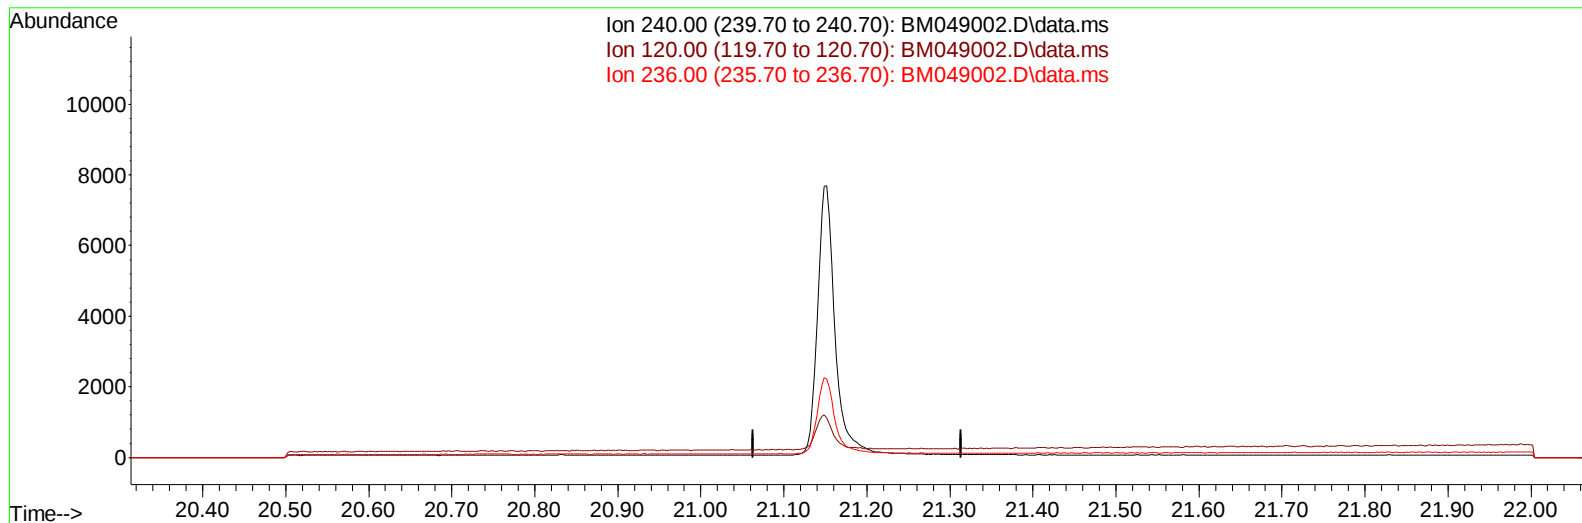

TIC: BM049002.D\data.ms

(17) Chrysene-d12




21.164min (-21.164) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	18.30	0.00#
236.00	30.50	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049002.D
Acq On : 16 Dec 2024 13:35
Operator : RC/JU
Sample : P5247-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Dec 16 14:04:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

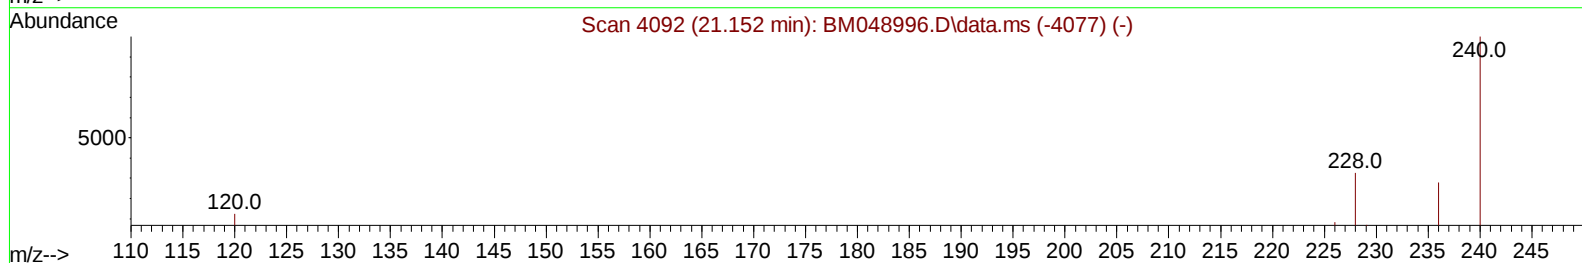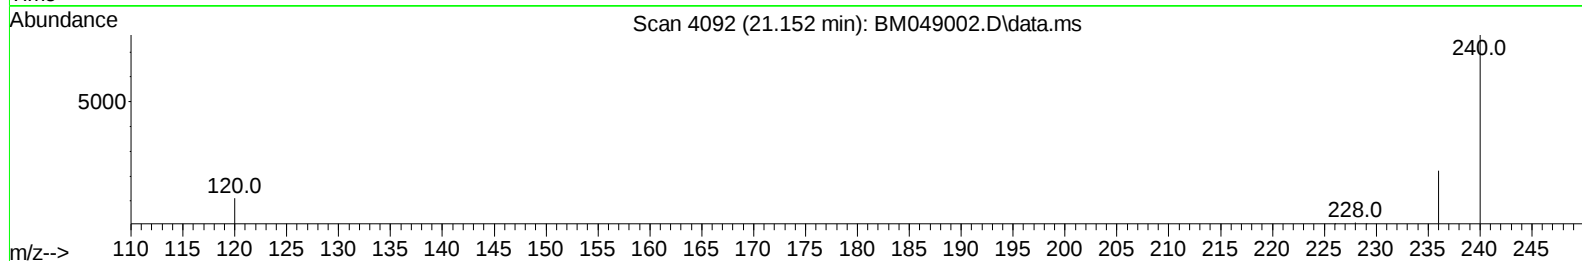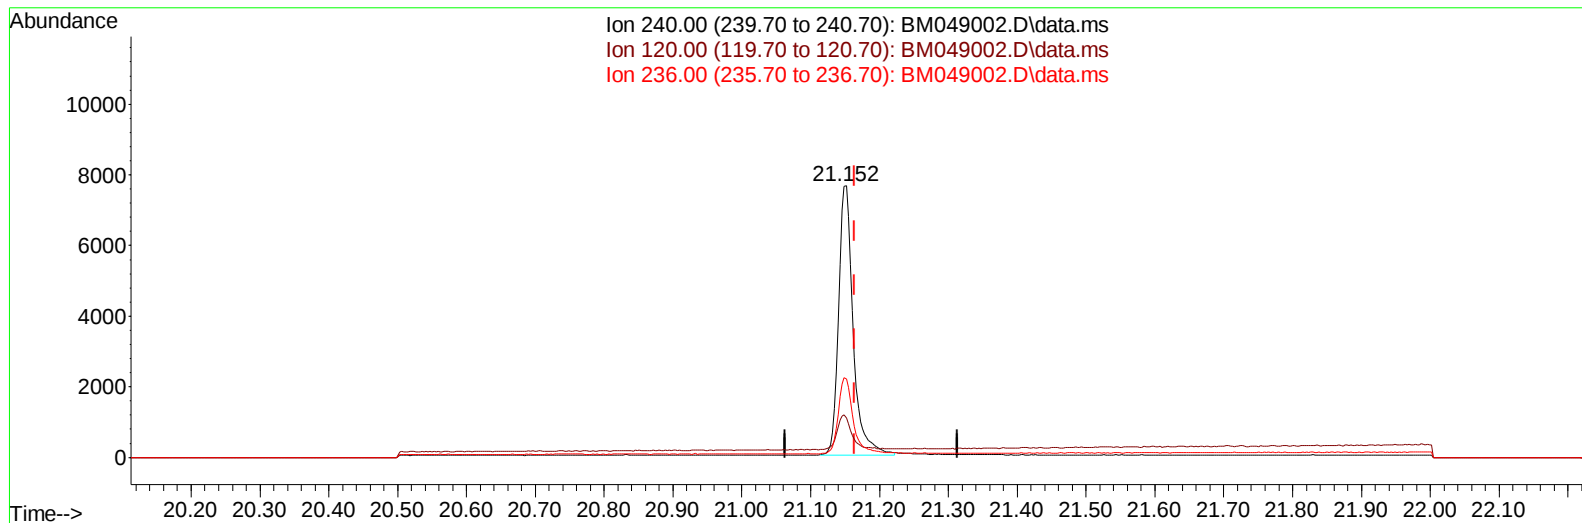

TIC: BM049002.D\data.ms

(17) Chrysene-d12




21.152min (-0.012) 0.40 ng/ul m

response 11215

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	18.30	14.62#
236.00	30.50	28.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049002.D
Acq On : 16 Dec 2024 13:35
Operator : RC/JU
Sample : P5247-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Dec 16 14:04:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

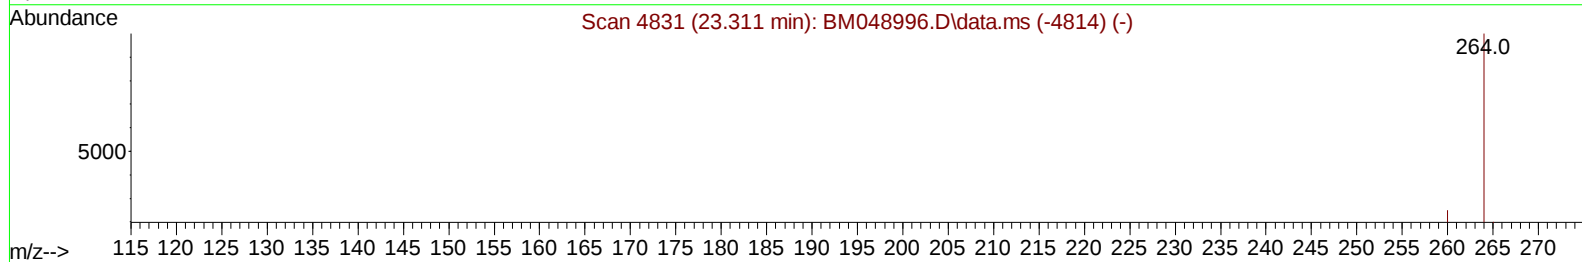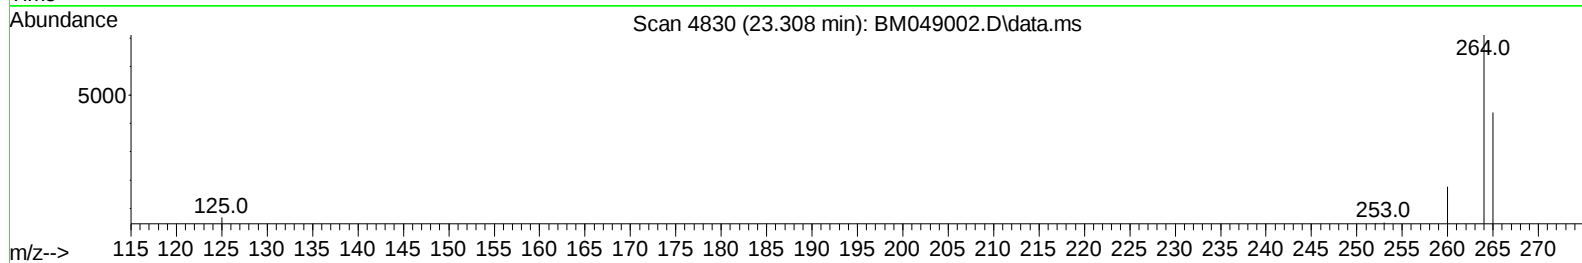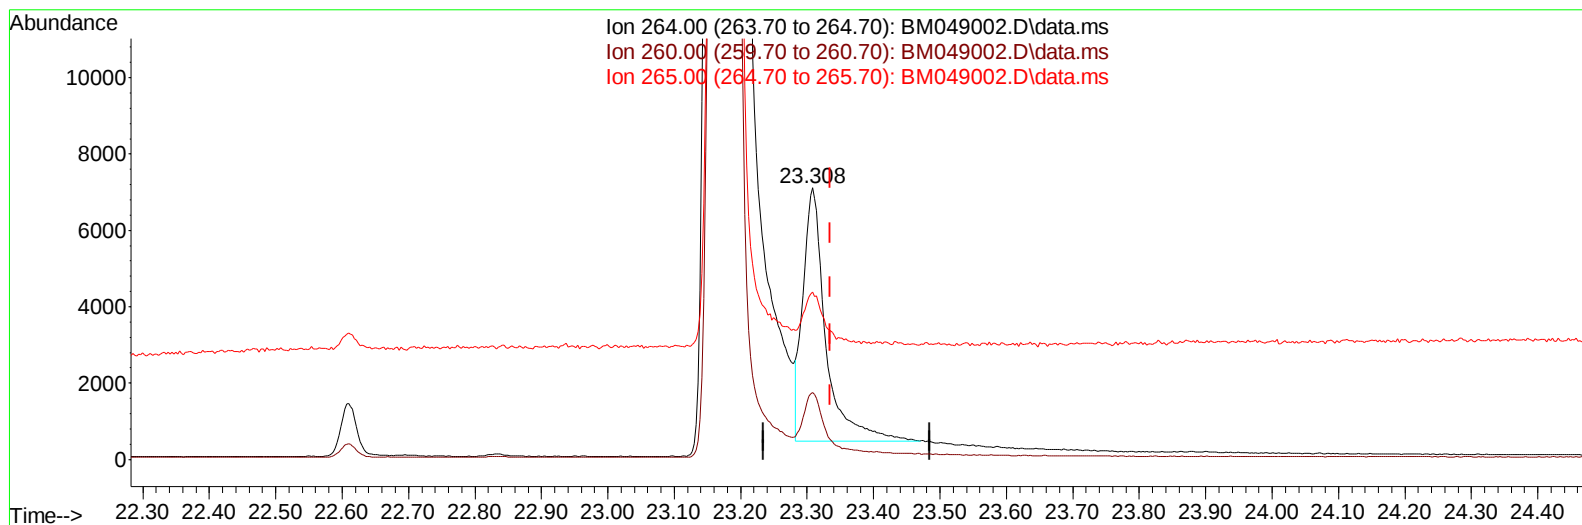

TIC: BM049002.D\data.ms

(23) Perylene-d12 (I)




23.308min (-0.027) 0.40 ng/u1

response 16100

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	24.74
265.00	82.60	61.66#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049002.D
Acq On : 16 Dec 2024 13:35
Operator : RC/JU
Sample : P5247-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Dec 16 14:04:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

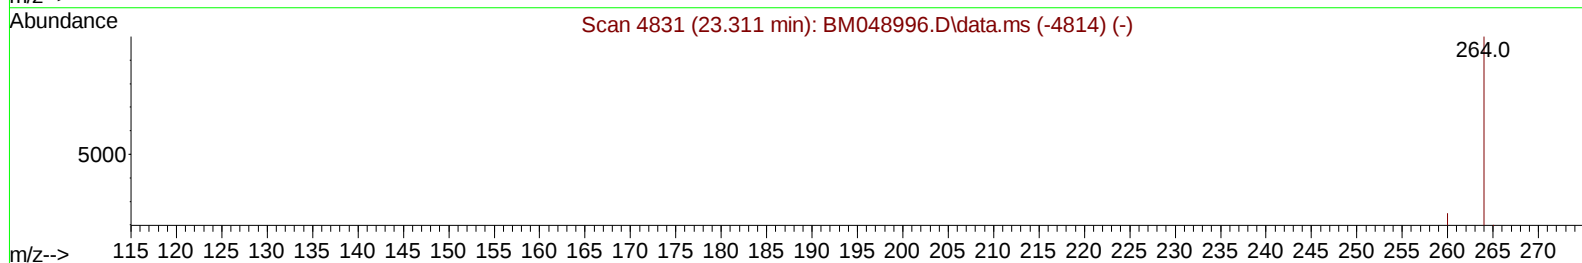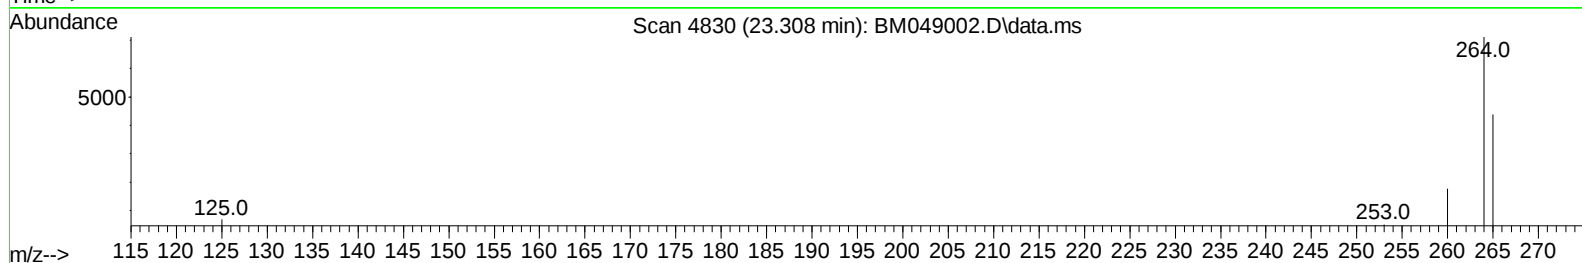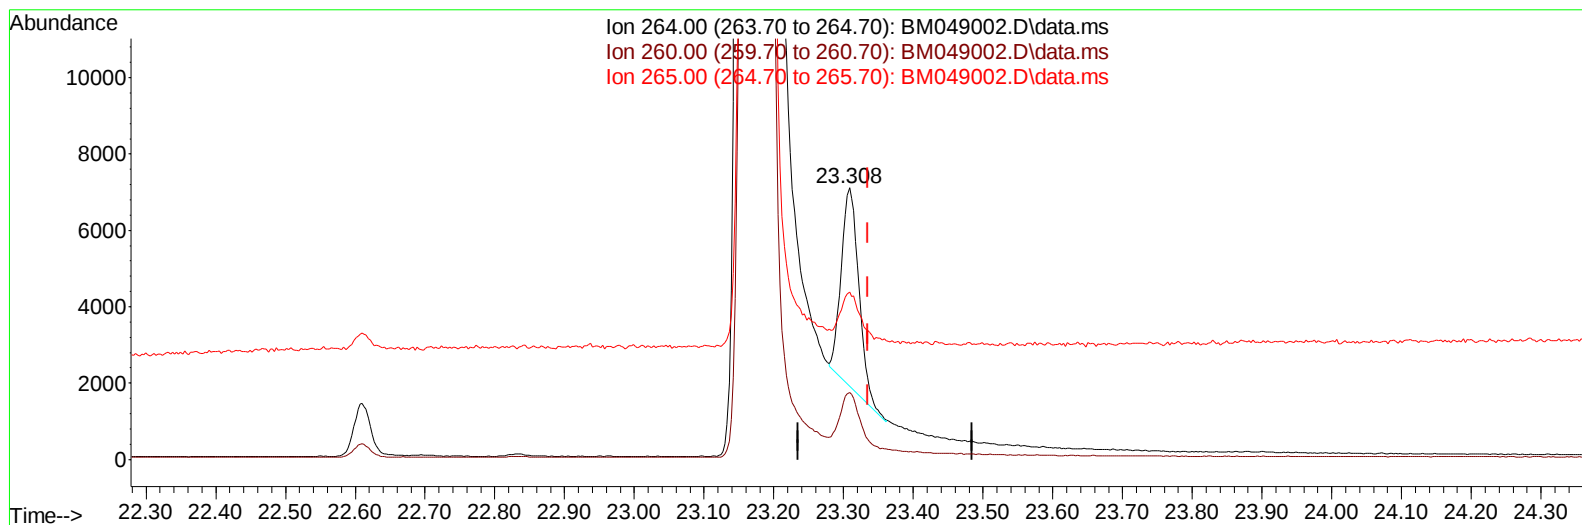

TIC: BM049002.D\data.ms

(23) Perylene-d12 (I)

23.308min (-0.027) 0.40 ng/ul m

response 8992

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	24.74
265.00	82.60	61.66#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
 Data File : BM049002.D
 Acq On : 16 Dec 2024 13:35
 Operator : RC/JU
 Sample : P5247-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Dec 16 14:04:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 09 17:52:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.573	152	5607	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.337	136	16858	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.206	164	9212	0.400	ng/ul	-0.02
13) Phenanthrene-d10	16.951	188	19424m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.152	240	11215m	0.400	ng/ul	-0.01
23) Perylene-d12	23.308	264	8992m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	59323	9.053	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.937	152	7411	0.345	ng/ul	0.00
18) Fluoranthene-d10	18.984	212	17086	0.510	ng/ul	-0.02
Target Compounds						Qvalue
2) 1,4-Dioxane	3.185	88	6246	0.824	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049002.D
Acq On : 16 Dec 2024 13:35
Operator : RC/JU
Sample : P5247-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Dec 16 14:04:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

