
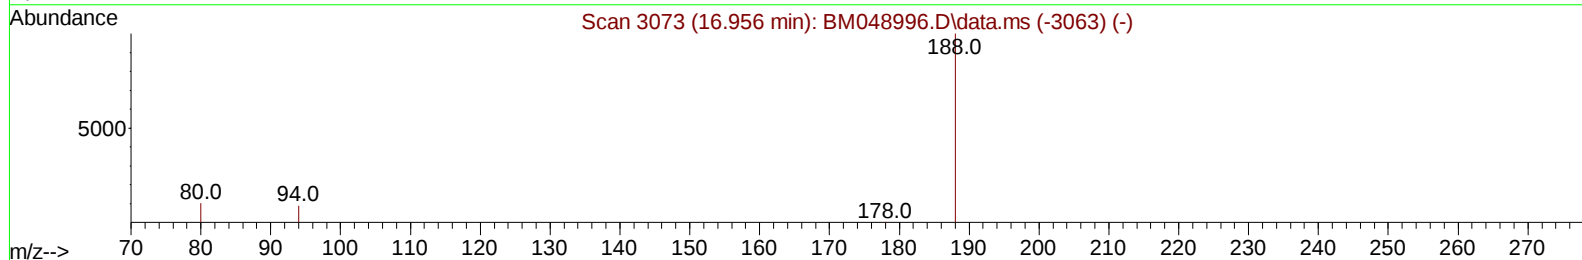
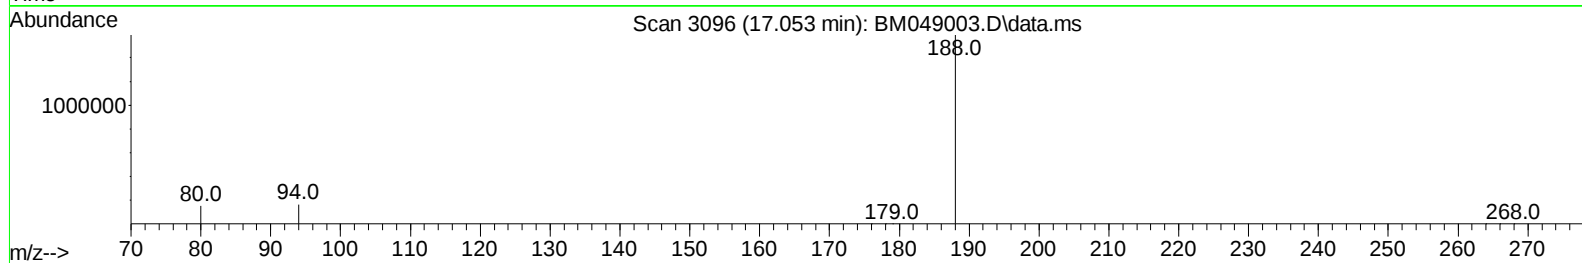


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049003.D
Acq On : 16 Dec 2024 14:10
Operator : RC/JU
Sample : P5247-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Dec 16 15:21:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

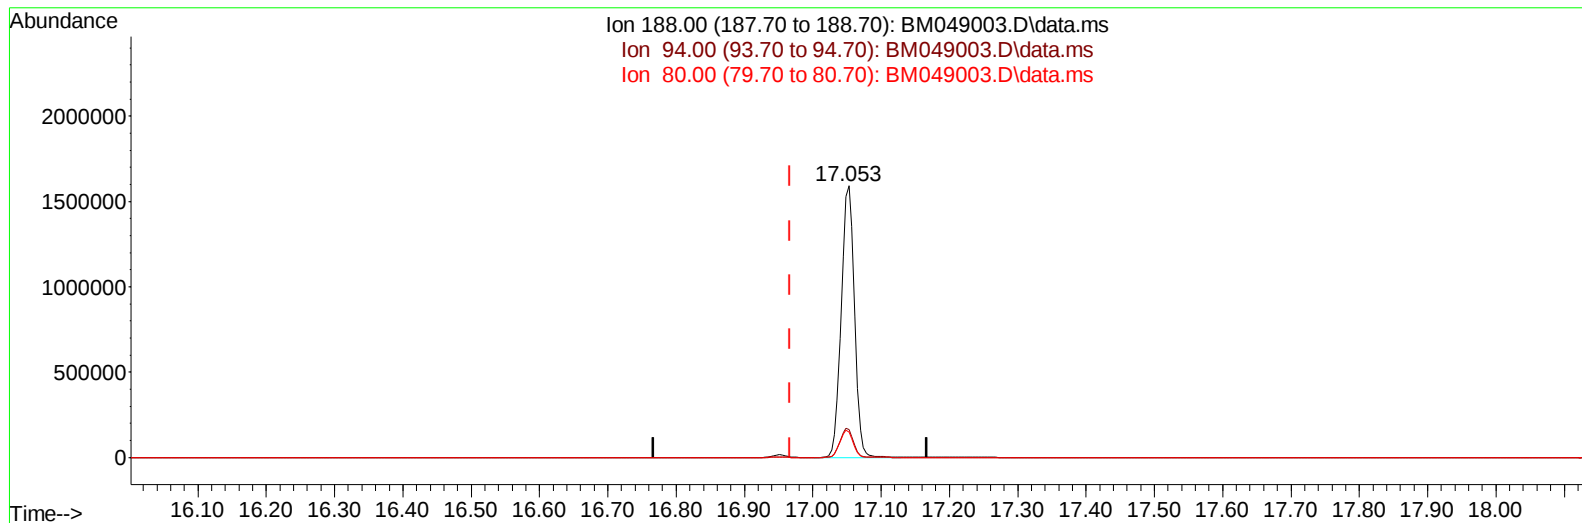

TIC: BM049003.D\data.ms

(13) Phenanthrene-d10 (I)




17.053min (+ 0.086) 0.40 ng/u1

response 2128879

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	10.25
80.00	13.90	9.35#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049003.D
Acq On : 16 Dec 2024 14:10
Operator : RC/JU
Sample : P5247-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Dec 16 15:21:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

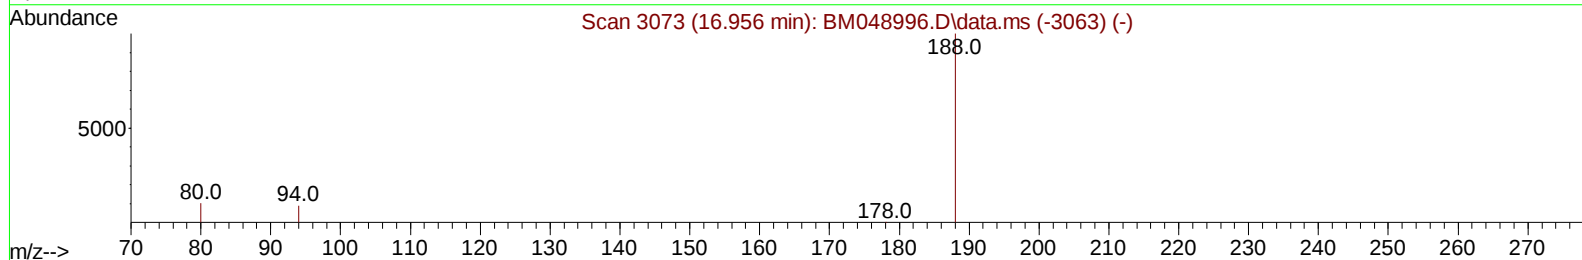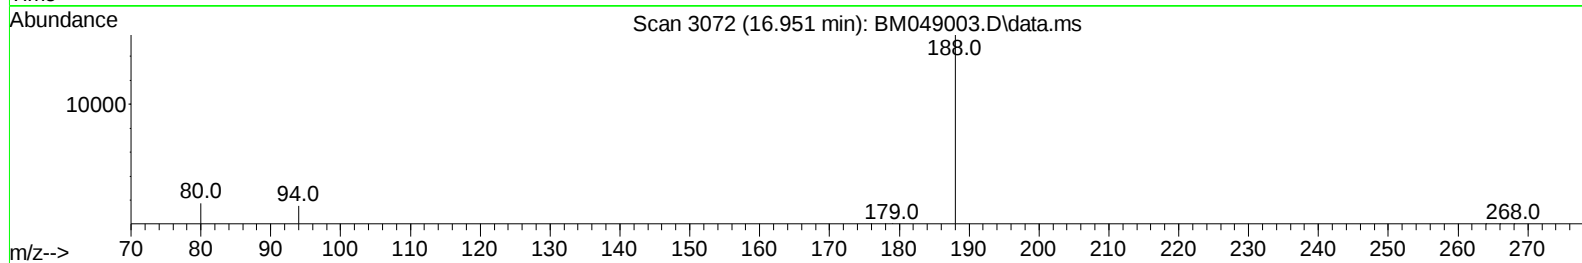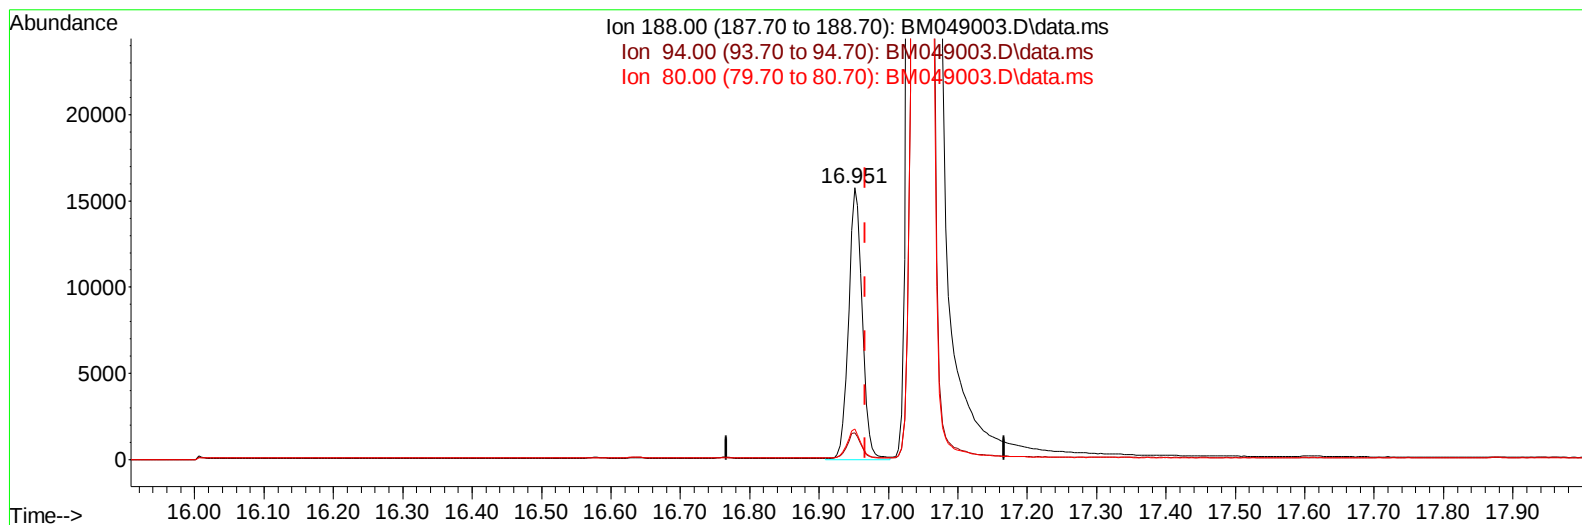




TIC: BM049003.D\data.ms

(13) Phenanthrene-d10 (I)**16.951min (-0.015) 0.40 ng/ul m****response 21337**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	9.87
80.00	13.90	11.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049003.D
Acq On : 16 Dec 2024 14:10
Operator : RC/JU
Sample : P5247-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Dec 16 15:21:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

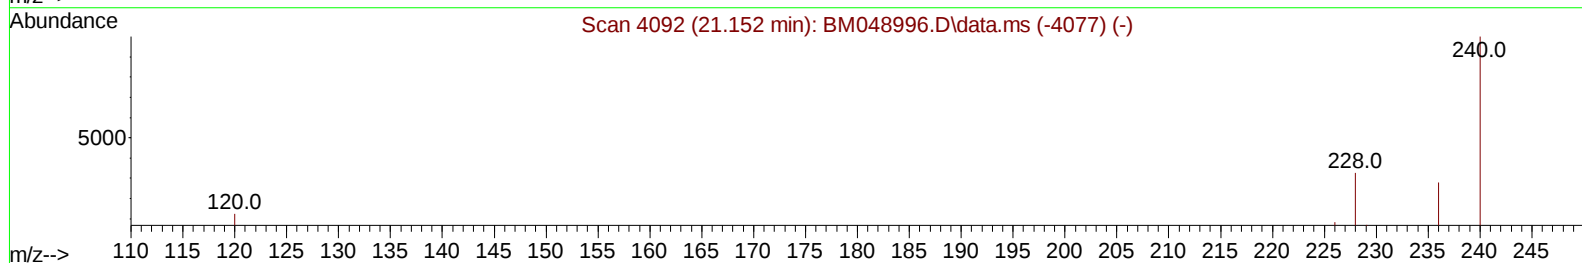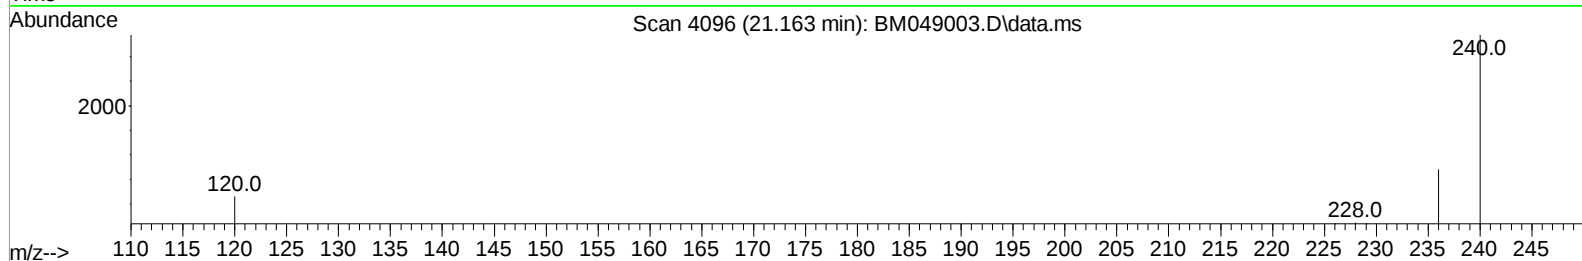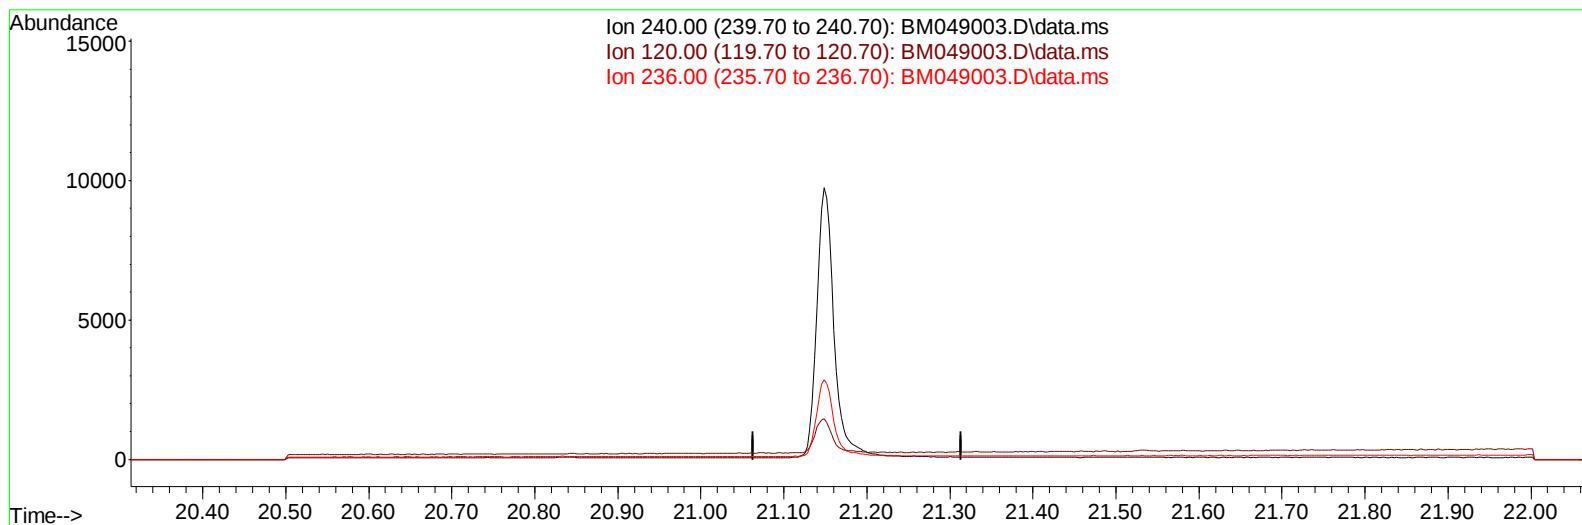

TIC: BM049003.D\data.ms

(17) Chrysene-d12




21.164min (-21.164) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	18.30	0.00#
236.00	30.50	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049003.D
Acq On : 16 Dec 2024 14:10
Operator : RC/JU
Sample : P5247-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Dec 16 15:21:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

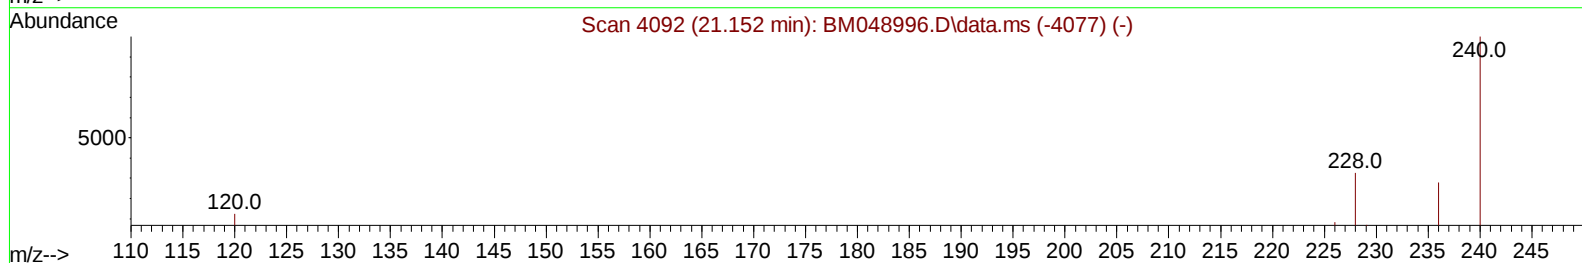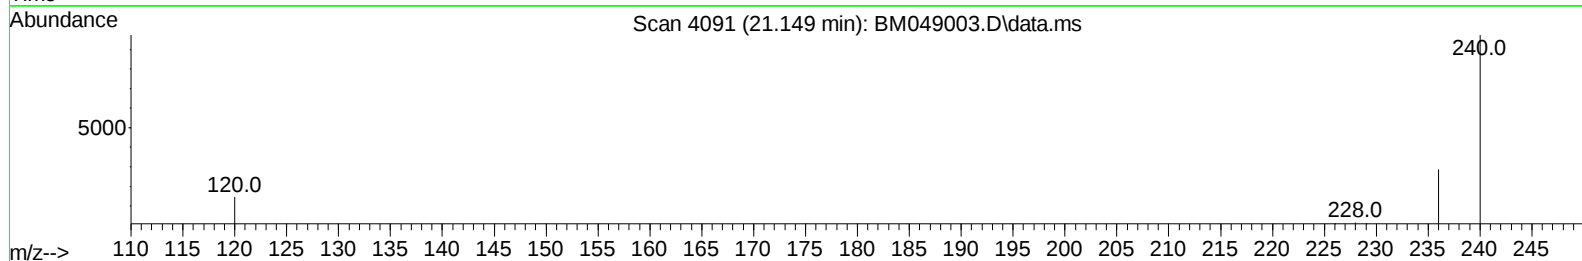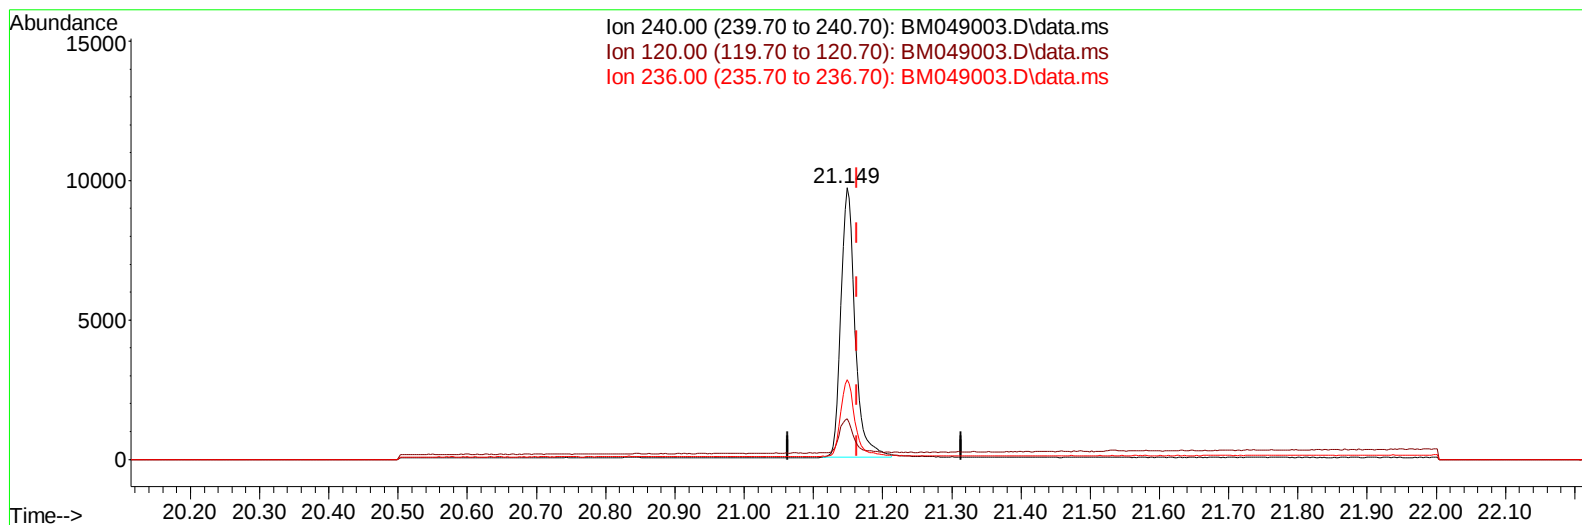

TIC: BM049003.D\data.ms

(17) Chrysene-d12




21.149min (-0.015) 0.40 ng/ul m

response 13887

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	18.30	14.95
236.00	30.50	29.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049003.D
Acq On : 16 Dec 2024 14:10
Operator : RC/JU
Sample : P5247-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Dec 16 15:21:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

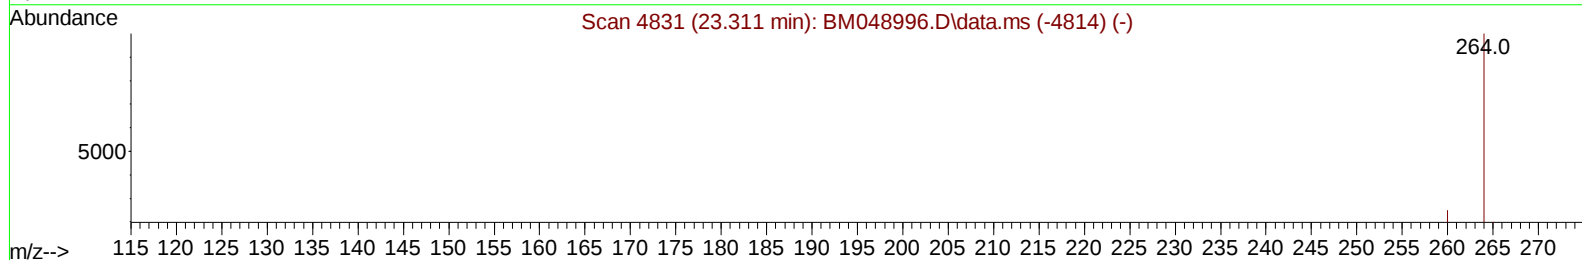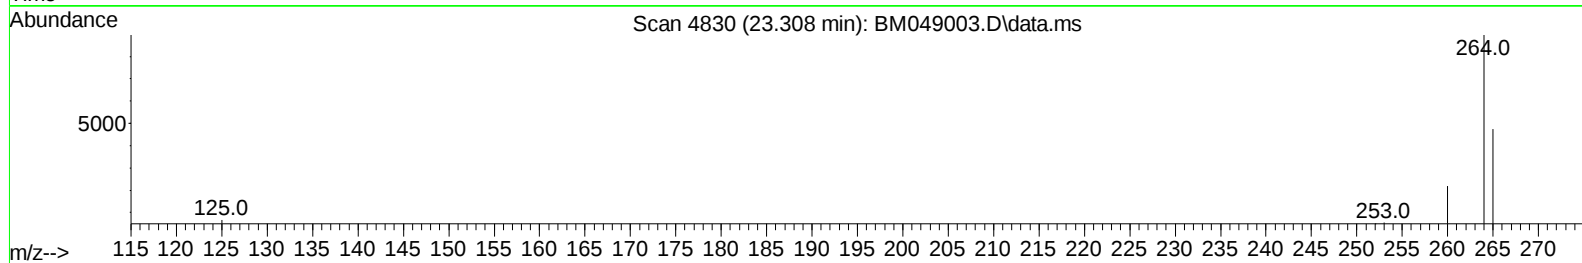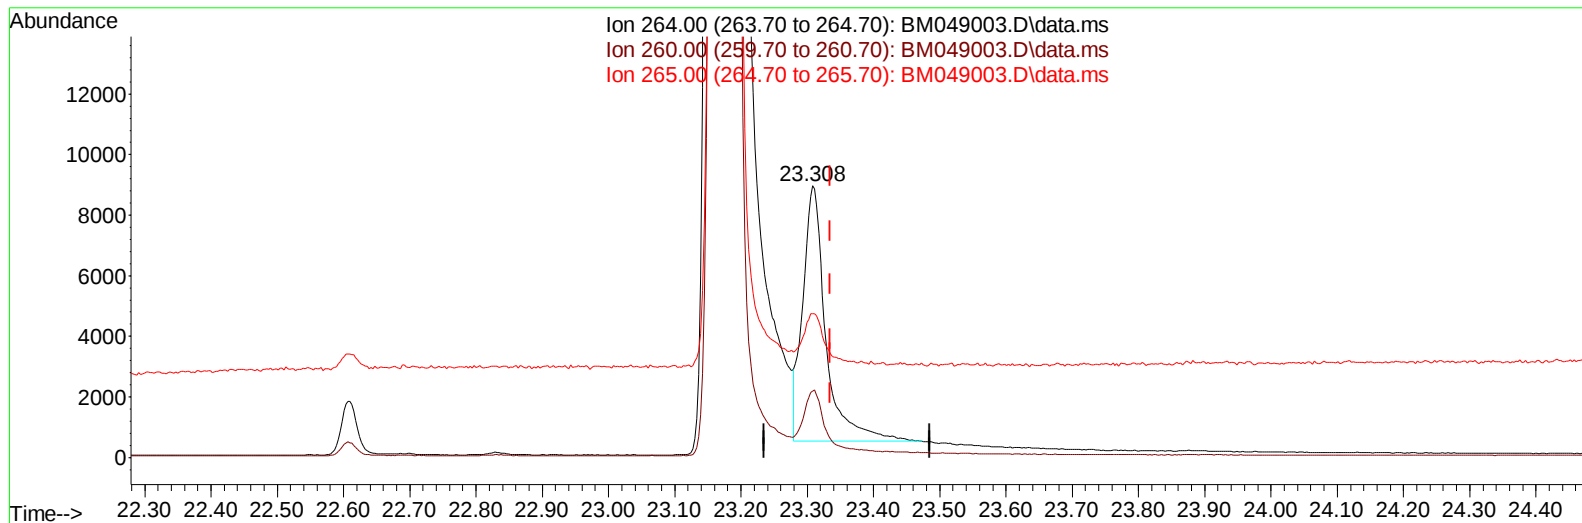

TIC: BM049003.D\data.ms

(23) Perylene-d12 (I)




23.308min (-0.027) 0.40 ng/ul

response 20393

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	24.33
265.00	82.60	52.83#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049003.D
Acq On : 16 Dec 2024 14:10
Operator : RC/JU
Sample : P5247-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Dec 16 15:21:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

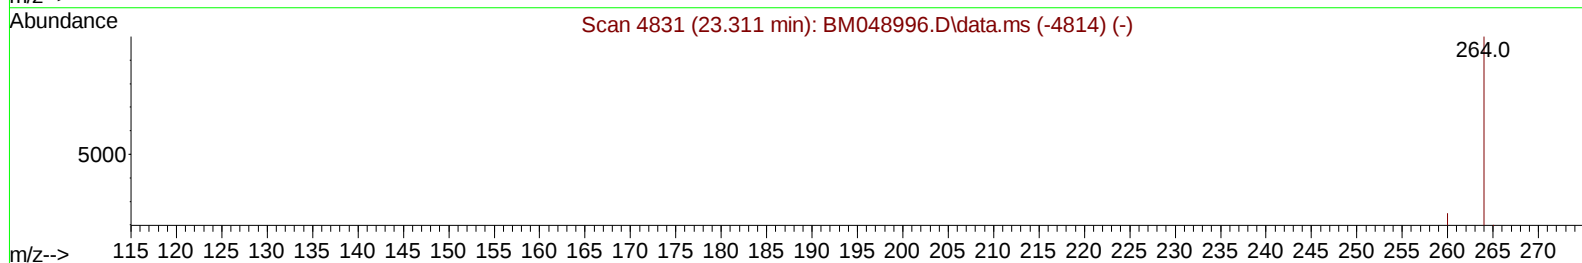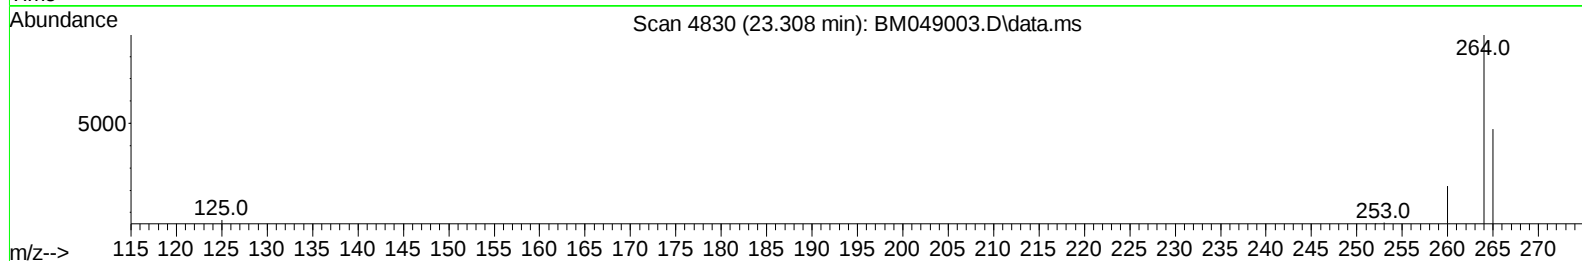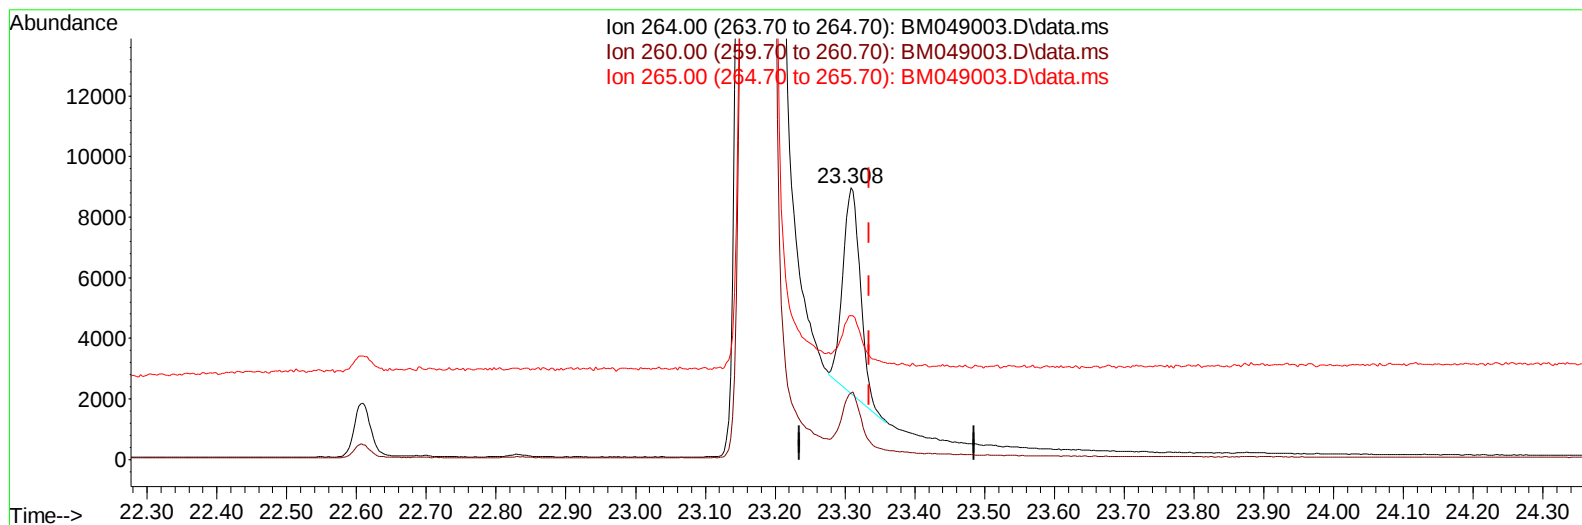

TIC: BM049003.D\data.ms

(23) Perylene-d12 (I)

23.308min (-0.027) 0.40 ng/ul m

response 11836

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	24.33
265.00	82.60	52.83#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
 Data File : BM049003.D
 Acq On : 16 Dec 2024 14:10
 Operator : RC/JU
 Sample : P5247-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: Dec 16 15:21:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 09 17:52:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.573	152	5871	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.337	136	17666	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.206	164	9857	0.400	ng/ul	-0.02
13) Phenanthrene-d10	16.951	188	21337m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.149	240	13887m	0.400	ng/ul	-0.01
23) Perylene-d12	23.308	264	11836m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	31437	4.582	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.937	152	7451	0.331	ng/ul	0.00
18) Fluoranthene-d10	18.984	212	19175	0.462	ng/ul	-0.02
Target Compounds						Qvalue
2) 1,4-Dioxane	3.185	88	5909	0.744	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049003.D
Acq On : 16 Dec 2024 14:10
Operator : RC/JU
Sample : P5247-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Dec 16 15:21:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

