
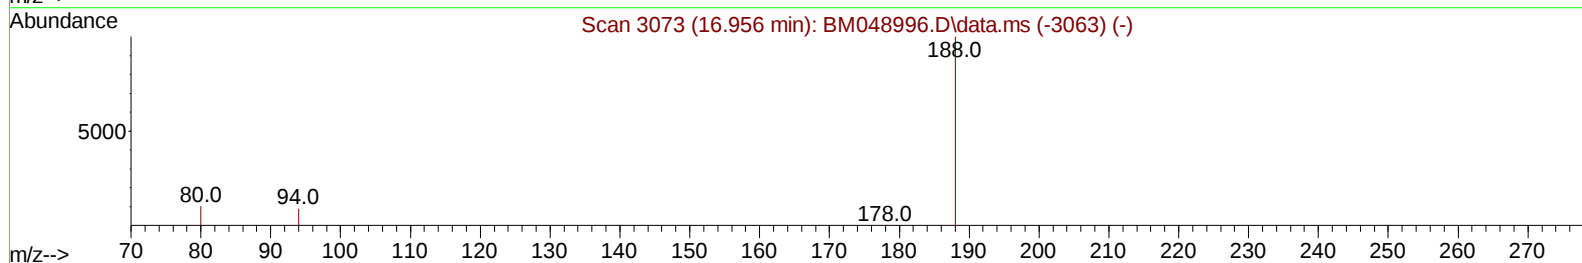
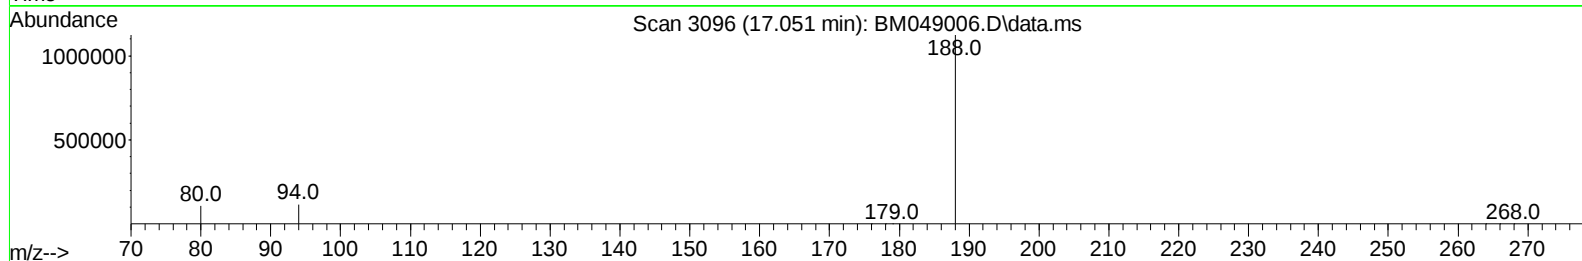


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049006.D
Acq On : 16 Dec 2024 15:58
Operator : RC/JU
Sample : P5228-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 16 17:34:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

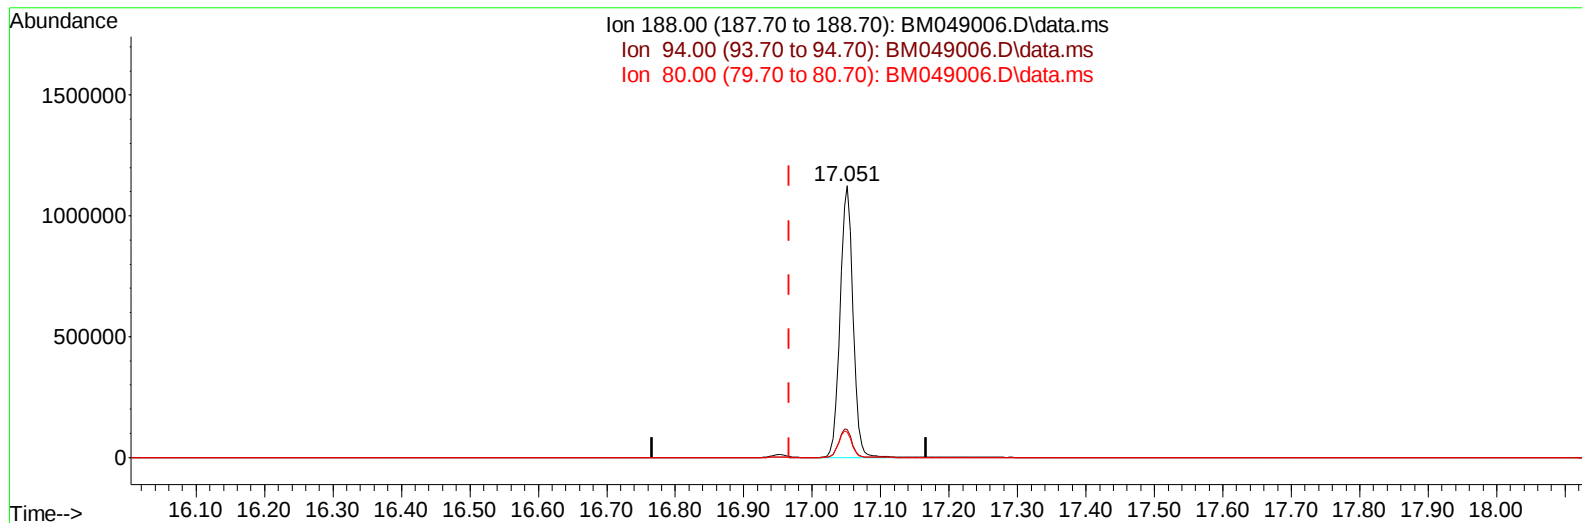




TIC: BM049006.D\data.ms

(13) Phenanthrene-d10 (I)**17.051min (+ 0.085) 0.40 ng/u1****response 1471287**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	10.30
80.00	13.90	9.40#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049006.D
Acq On : 16 Dec 2024 15:58
Operator : RC/JU
Sample : P5228-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 16 17:34:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

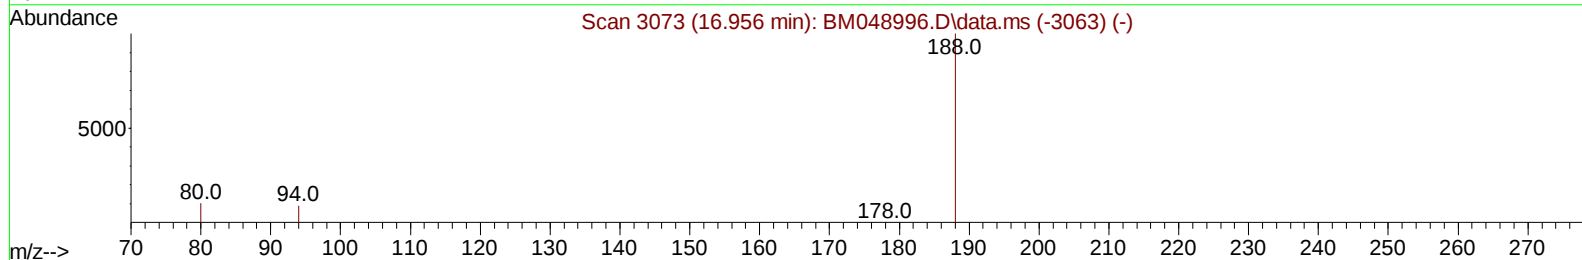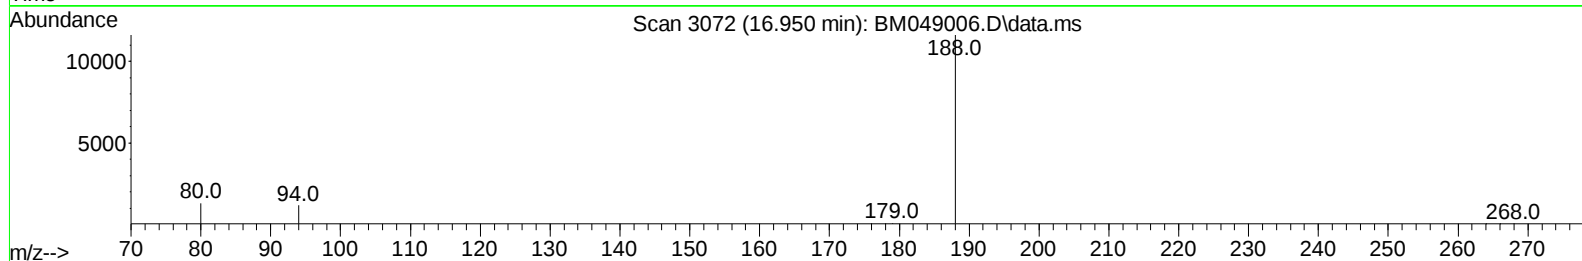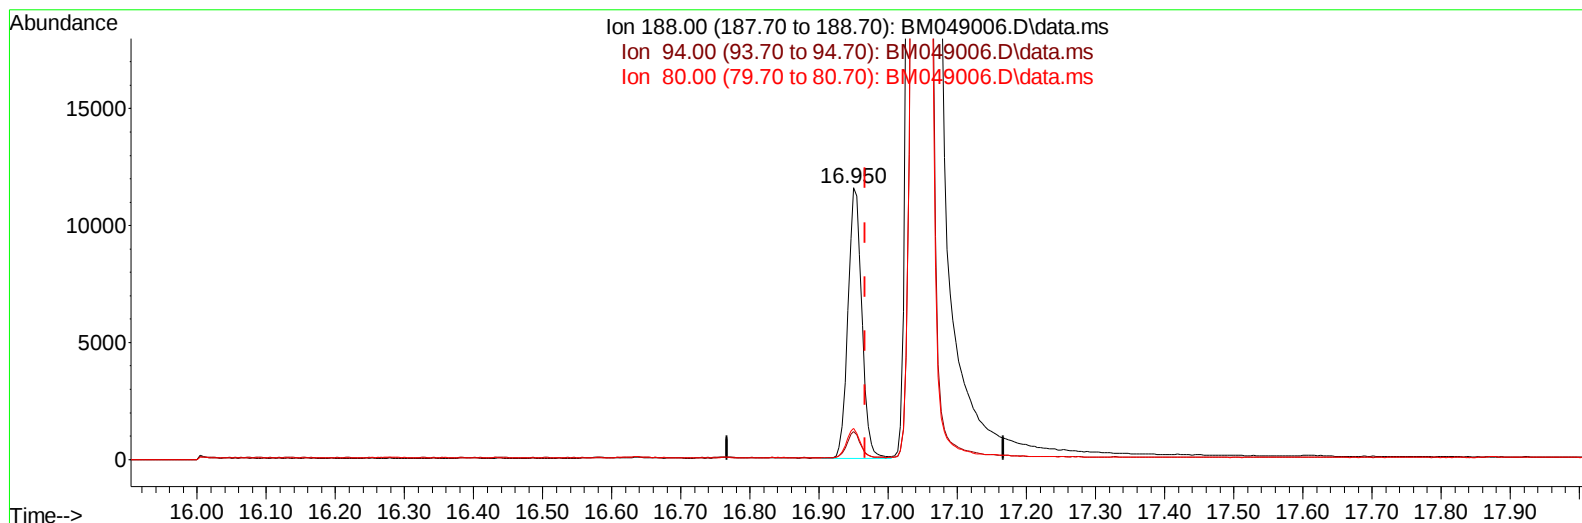

TIC: BM049006.D\data.ms

(13) Phenanthrene-d10 (I)




16.950min (-0.017) 0.40 ng/ul m

response 16182

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	10.21
80.00	13.90	11.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049006.D
Acq On : 16 Dec 2024 15:58
Operator : RC/JU
Sample : P5228-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 16 17:34:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

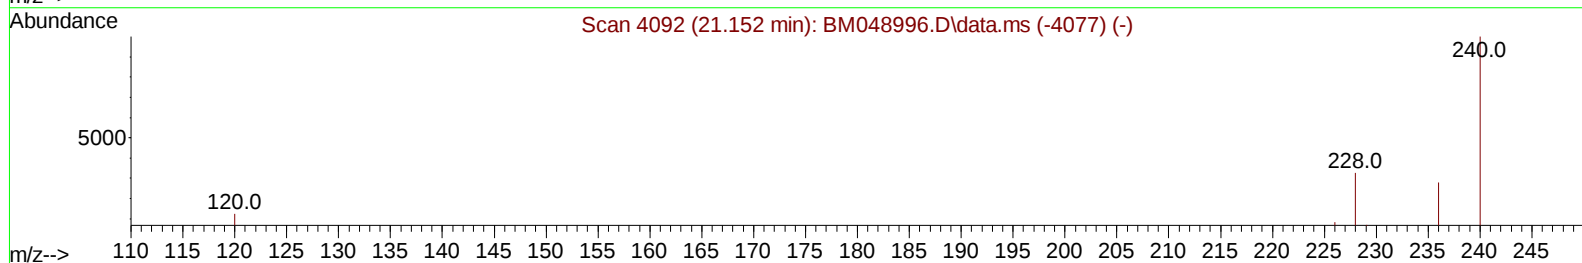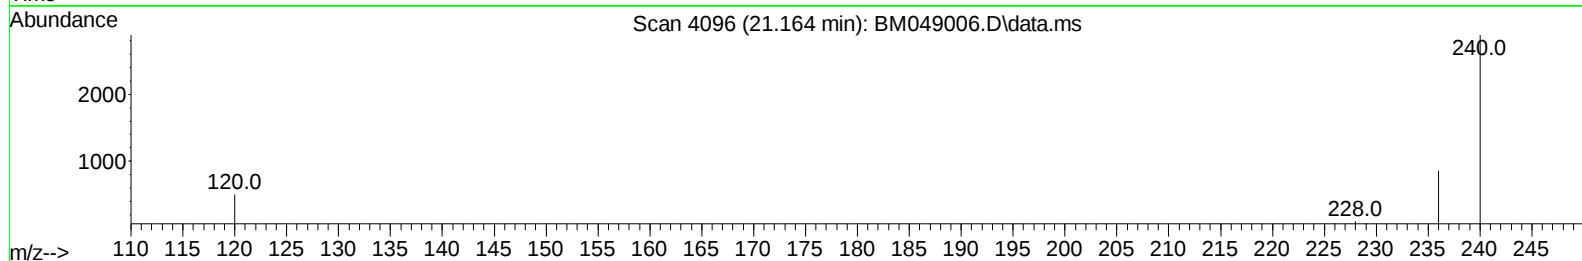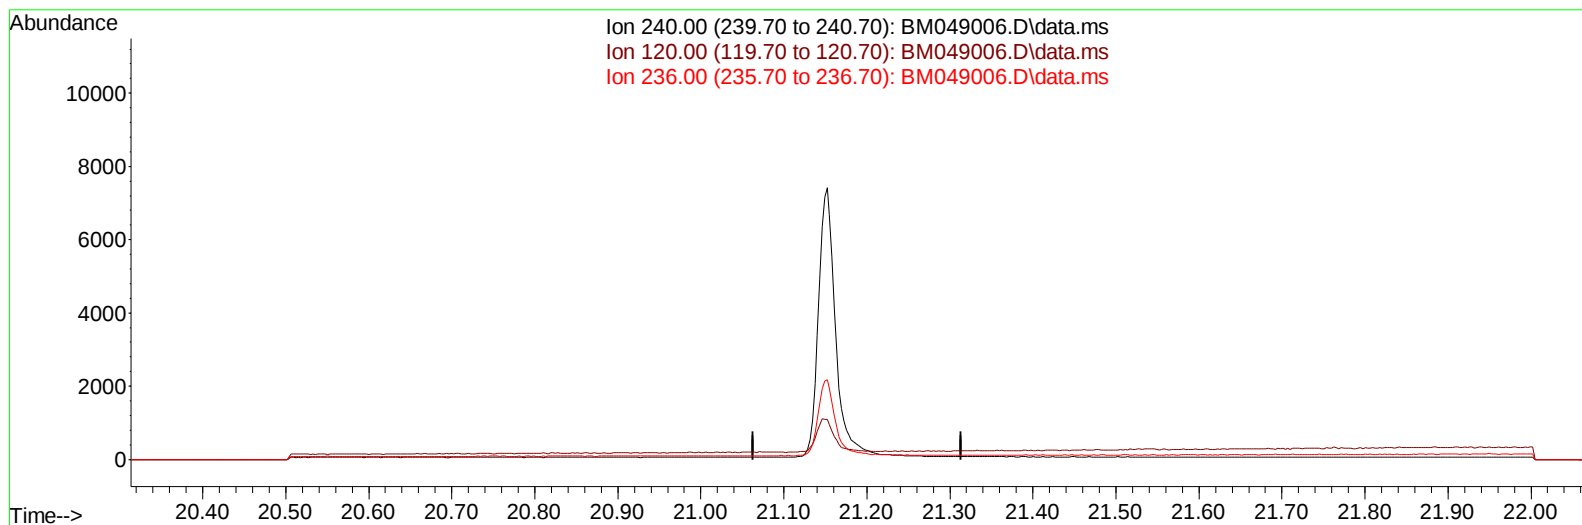

TIC: BM049006.D\data.ms

(17) Chrysene-d12




21.164min (-21.164) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	18.30	0.00#
236.00	30.50	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049006.D
Acq On : 16 Dec 2024 15:58
Operator : RC/JU
Sample : P5228-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 16 17:34:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

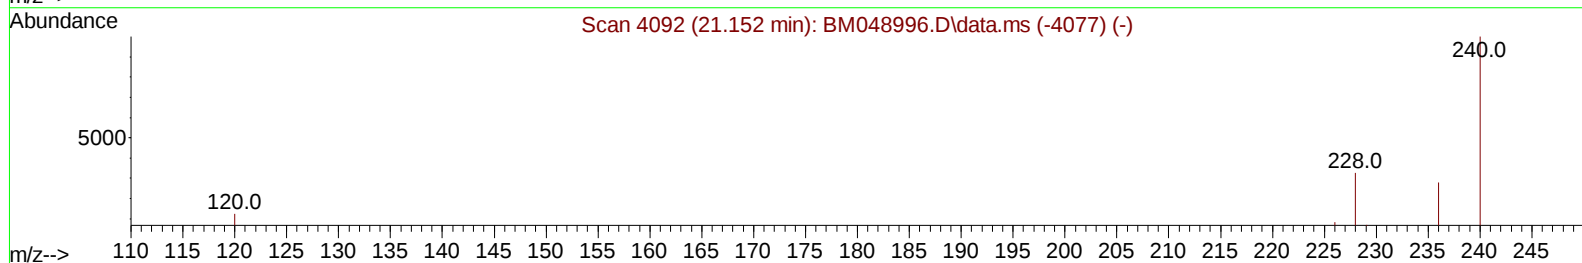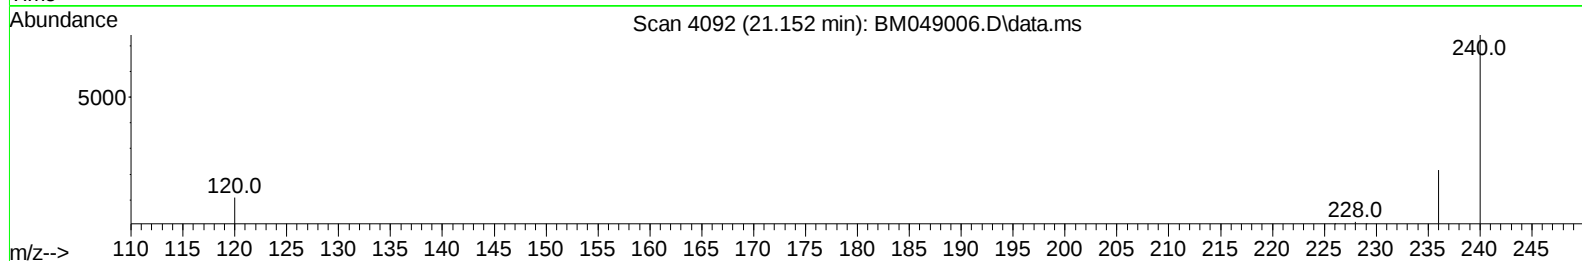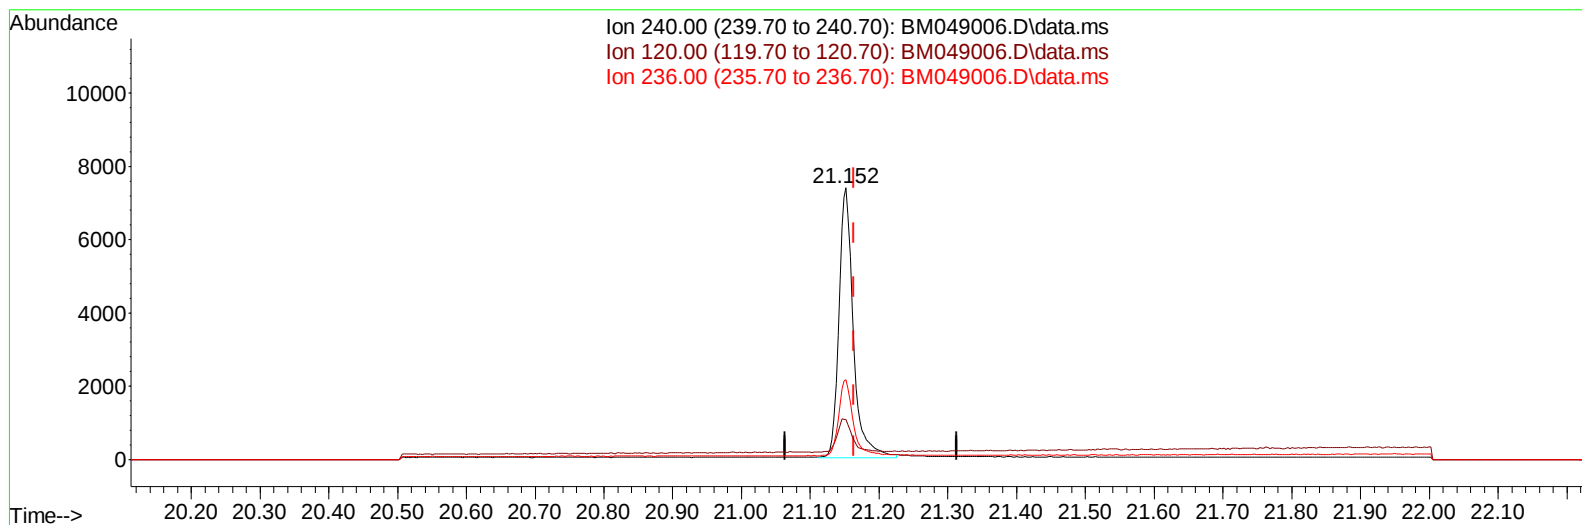




TIC: BM049006.D\data.ms

(17) Chrysene-d12**21.152min (-0.012) 0.40 ng/ul m****response 10668**

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	18.30	14.72
236.00	30.50	29.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049006.D
Acq On : 16 Dec 2024 15:58
Operator : RC/JU
Sample : P5228-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 16 17:34:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

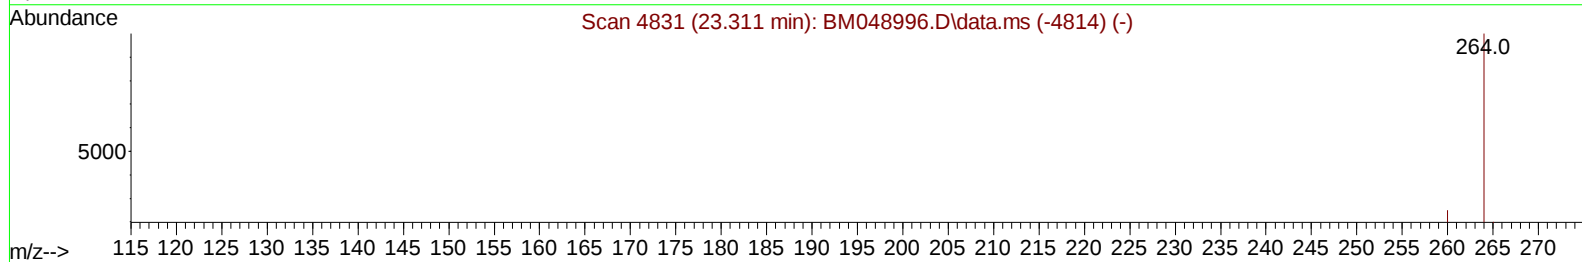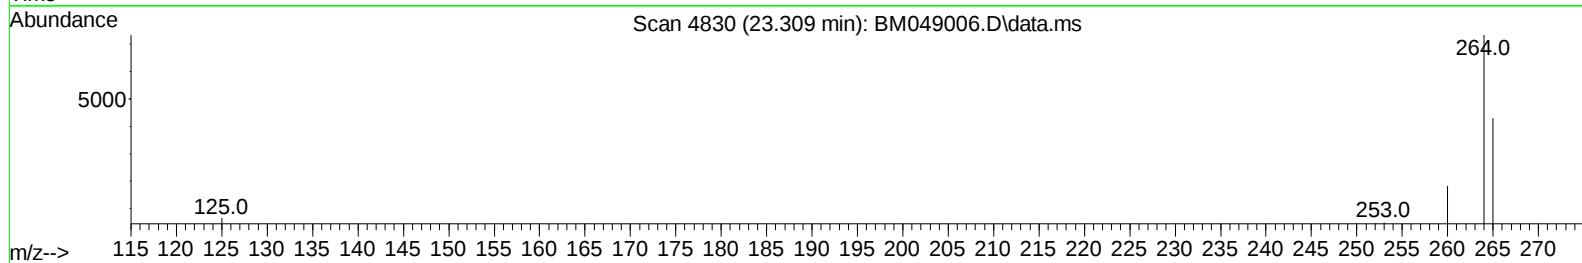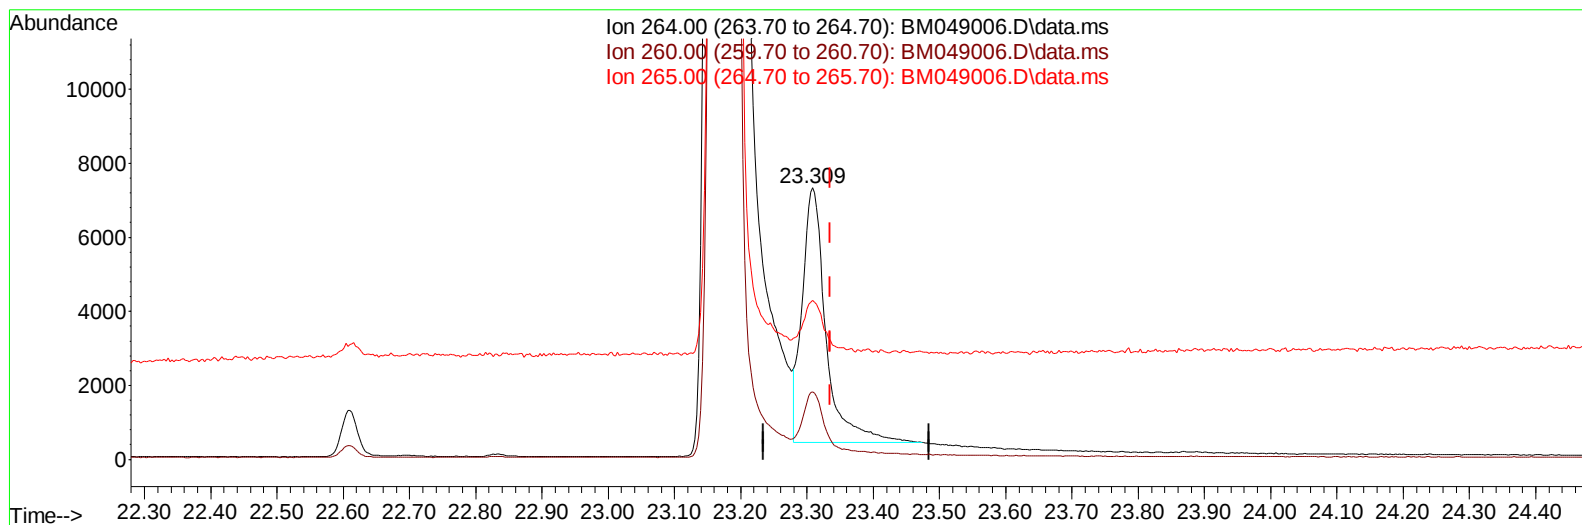

TIC: BM049006.D\data.ms

(23) Perylene-d12 (I)




23.309min (-0.026) 0.40 ng/ul

response 17012

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	24.95
265.00	82.60	58.70#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049006.D
Acq On : 16 Dec 2024 15:58
Operator : RC/JU
Sample : P5228-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 16 17:34:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

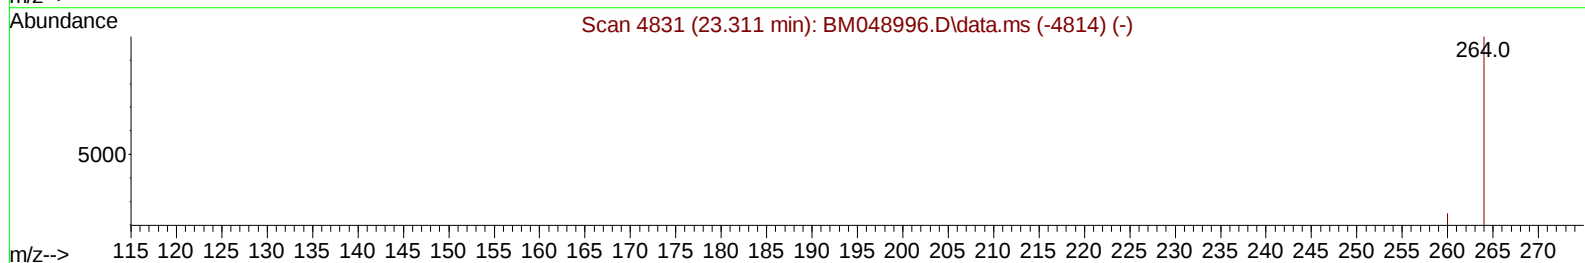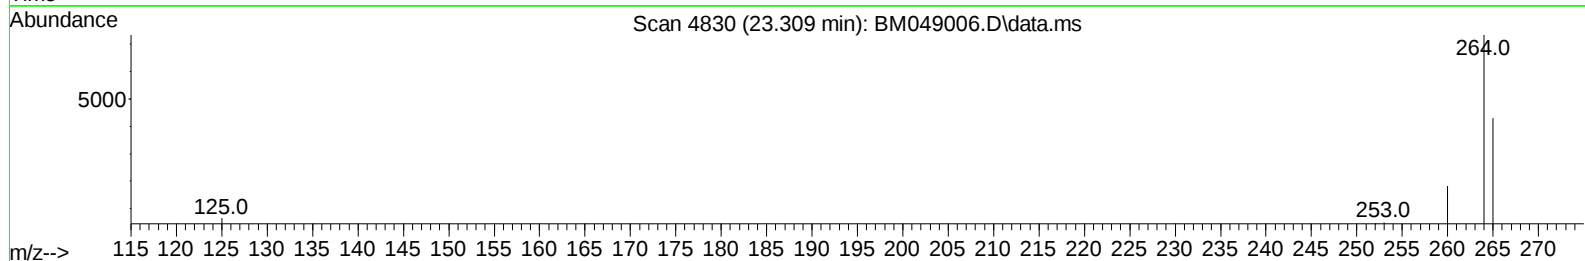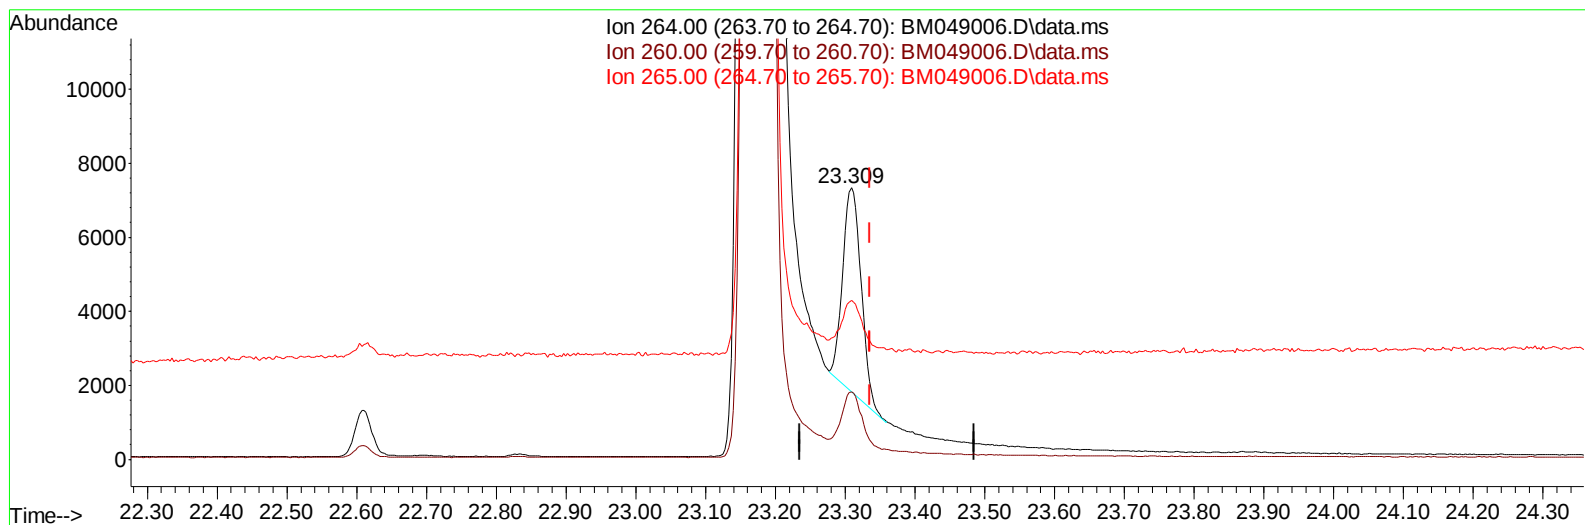

TIC: BM049006.D\data.ms

(23) Perylene-d12 (I)

23.309min (-0.026) 0.40 ng/ul m

response 10094

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	24.95
265.00	82.60	58.70#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
 Data File : BM049006.D
 Acq On : 16 Dec 2024 15:58
 Operator : RC/JU
 Sample : P5228-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 16 17:34:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 09 17:52:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.573	152	5504	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.336	136	15435	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.205	164	7949	0.400	ng/ul	-0.02
13) Phenanthrene-d10	16.950	188	16182m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.152	240	10668m	0.400	ng/ul	-0.01
23) Perylene-d12	23.309	264	10094m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	29009	4.510	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.936	152	5434	0.276	ng/ul	-0.01
18) Fluoranthene-d10	18.987	212	12852	0.403	ng/ul	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049006.D
Acq On : 16 Dec 2024 15:58
Operator : RC/JU
Sample : P5228-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 16 17:34:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

