

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
 Data File : BM049000.D
 Acq On : 16 Dec 2024 12:23
 Operator : RC/JU
 Sample : P5228-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2AT0

Quant Time: Dec 16 12:52:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 09 17:52:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.573	152	5960	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.337	136	17616	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.206	164	9551	0.400	ng/ul	-0.02
13) Phenanthrene-d10	16.952	188	19259m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.152	240	10450m	0.400	ng/ul	-0.01
23) Perylene-d12	23.309	264	8725m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.152	96	35276	5.064	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.932	152	9763	0.435	ng/ul	-0.01
18) Fluoranthene-d10	18.984	212	17409	0.558	ng/ul	-0.02
Target Compounds						Qvalue
5) Naphthalene	10.387	128	1145	0.025	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121624\
Data File : BM049000.D
Acq On : 16 Dec 2024 12:23
Operator : RC/JU
Sample : P5228-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AT0


Quant Time: Dec 16 12:52:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

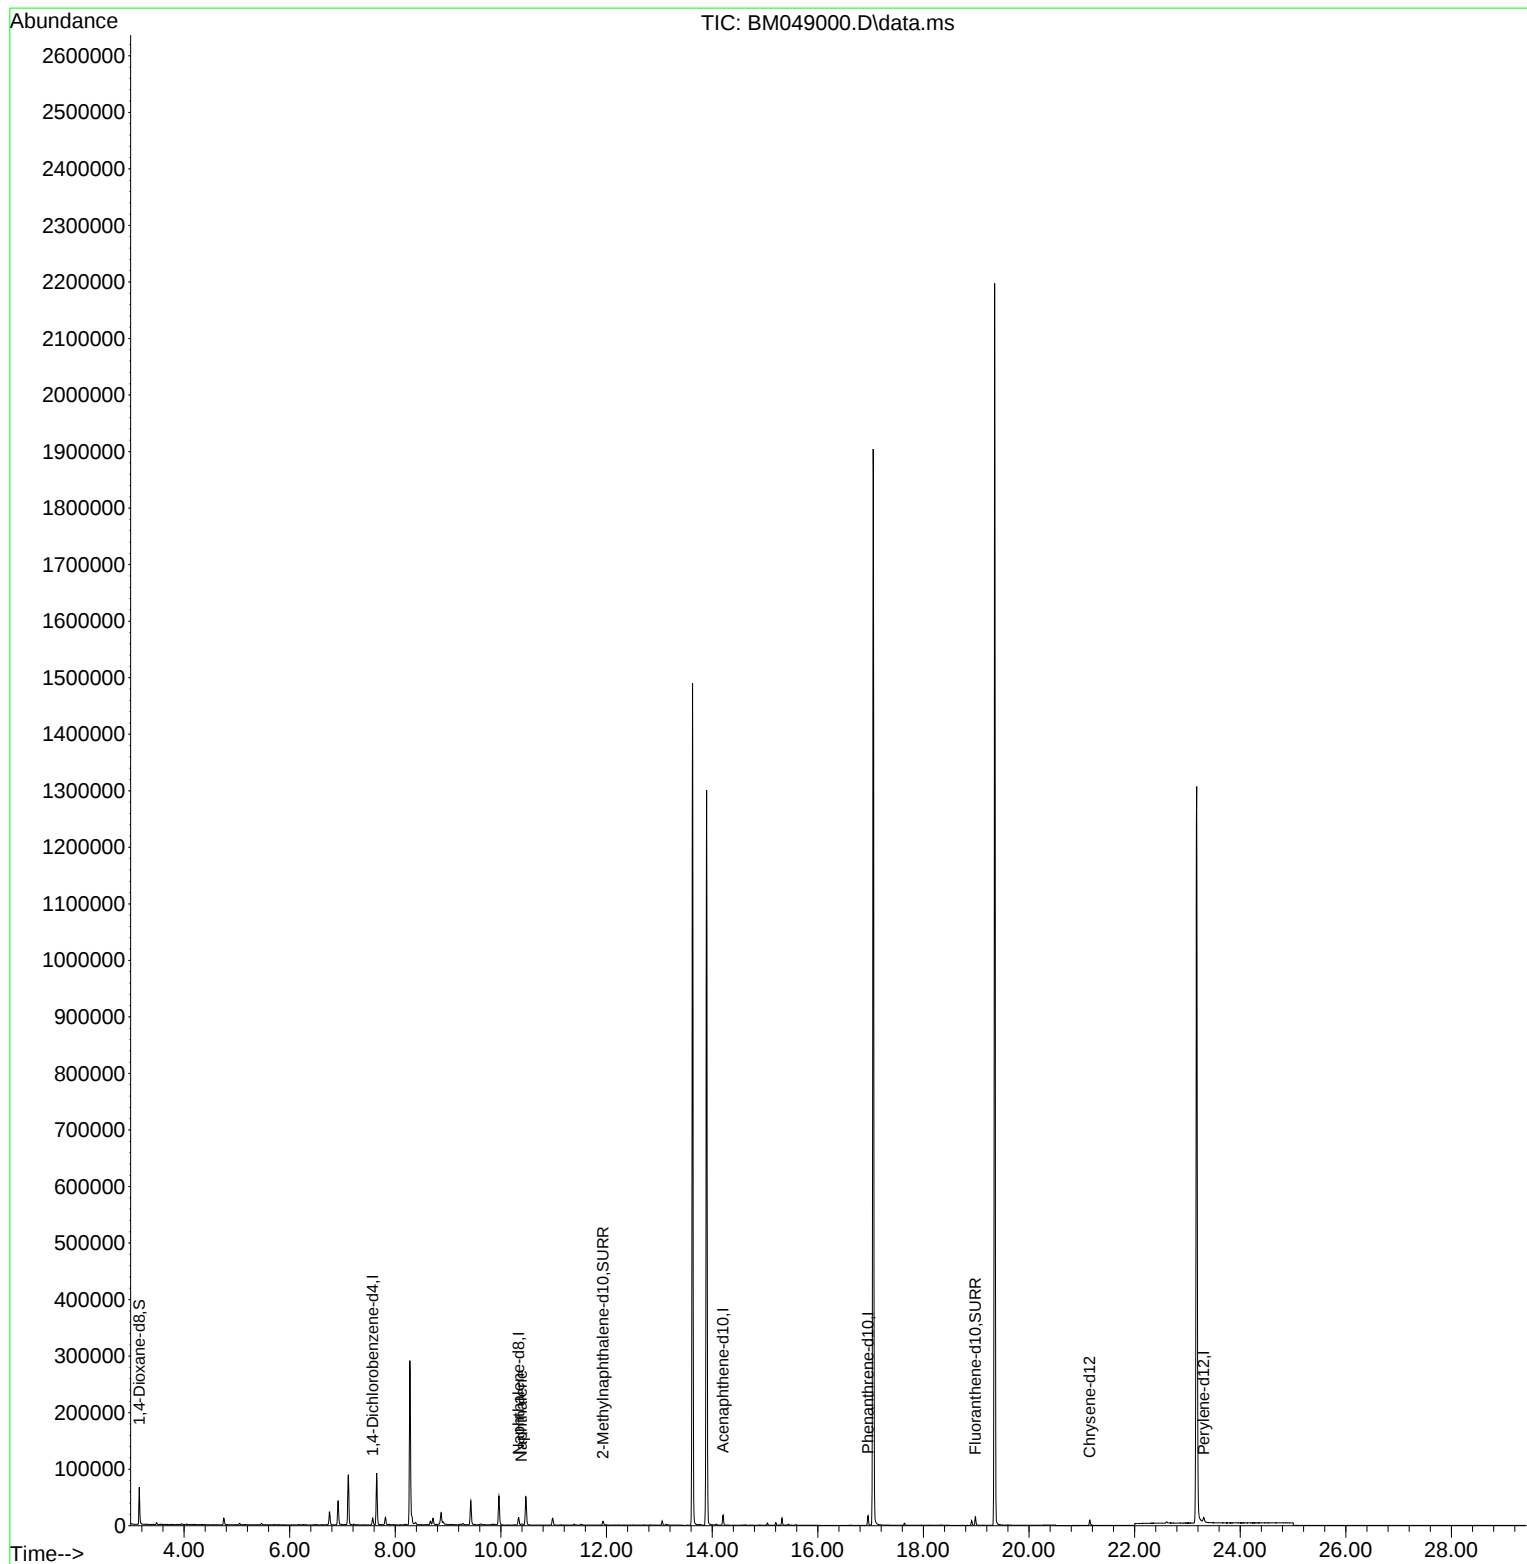

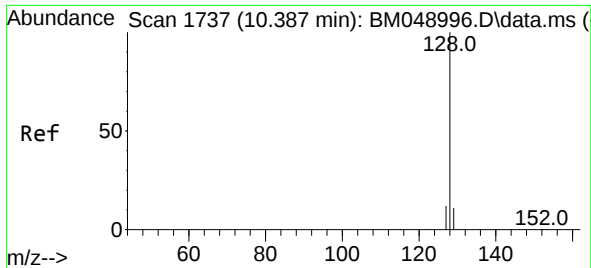

#5
Naphthalene
Concen: 0.025 ng/ul
RT: 10.387 min Scan# 11
Delta R.T. -0.015 min
Lab File: BM049000.D
Acq: 16 Dec 2024 12:23

Instrument :
BNA_M
ClientSampleId :
E2AT0

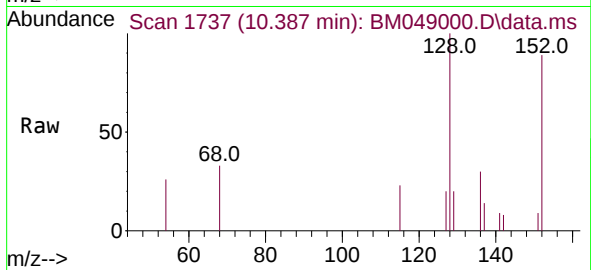

Tgt Ion:128 Resp: 1145
Ion Ratio Lower Upper
128 100
129 20.5 9.4 14.2#
127 19.6 10.6 16.0#

