

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012022\
 Data File : BM033812.D
 Acq On : 21 Jan 2022 05:39
 Operator : CG/JU
 Sample : N1199-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F39

Quant Time: Jan 21 06:13:12 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM010422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 21 01:34:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	3634	0.400	ng/ul	0.00
4) Naphthalene-d8	10.760	136	13785	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.583	164	8160	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.319	188	14227	0.400	ng/ul	0.00
17) Chrysene-d12	21.482	240	7919	0.400	ng/ul #	0.00
23) Perylene-d12	23.882	264	7931	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	16212	4.188	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.348	152	7420	0.396	ng/ul	0.00
18) Fluoranthene-d10	19.341	212	13094	0.534	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	16.972	266	273	0.049	ng/ul	95
24) Benzo(b)fluoranthene	23.148	252	746	0.021	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012022\
Data File : BM033812.D
Acq On : 21 Jan 2022 05:39
Operator : CG/JU
Sample : N1199-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F39

Quant Time: Jan 21 06:13:12 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM010422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 21 01:34:59 2022
Response via : Initial Calibration




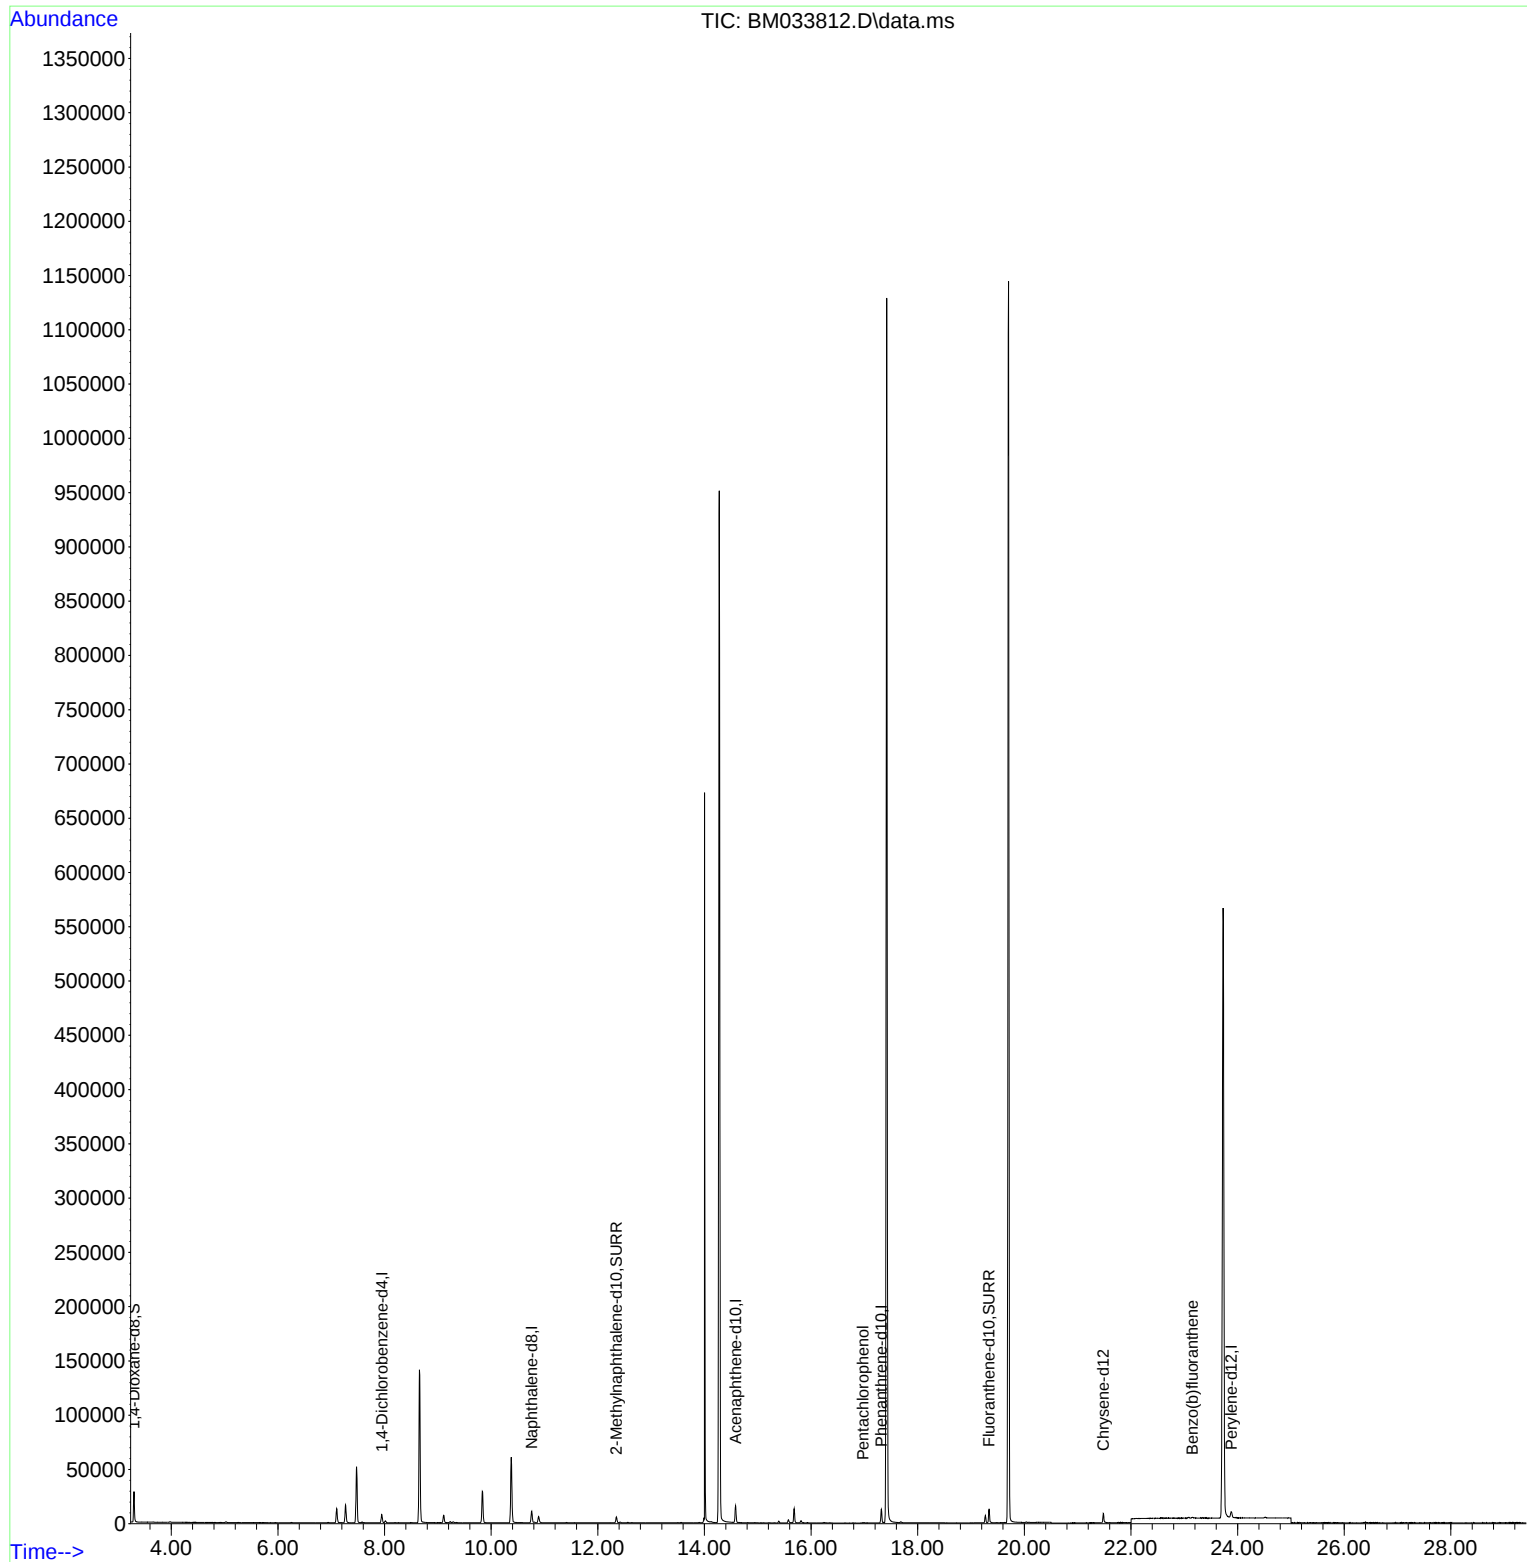


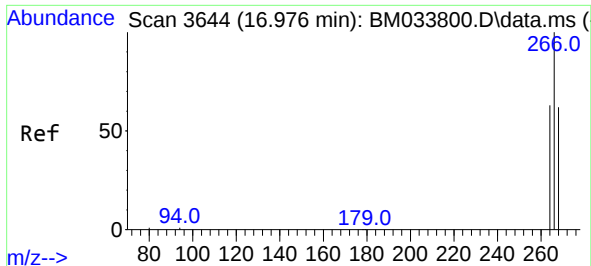

#14
Pentachlorophenol
Concen: 0.049 ng/ul
RT: 16.972 min Scan# 30
Delta R.T. -0.003 min
Lab File: BM033812.D
Acq: 21 Jan 2022 05:39

Instrument :
BNA_M
ClientSampleId :
C0F39

Tgt Ion:266 Resp: 273
Ion Ratio Lower Upper
266 100
264 64.8 51.4 77.0
268 59.7 53.1 79.7

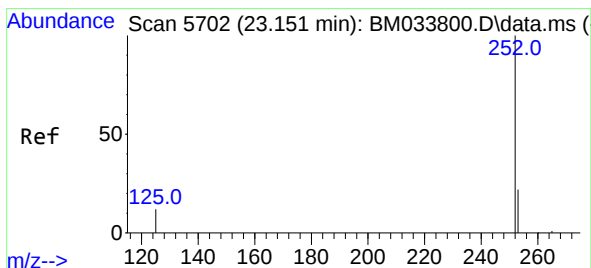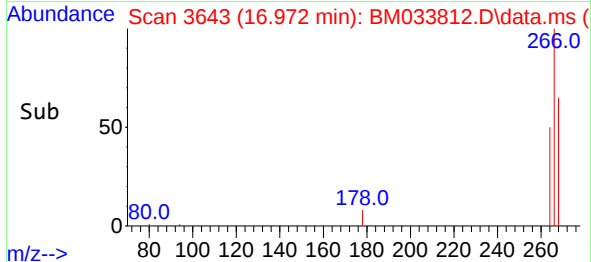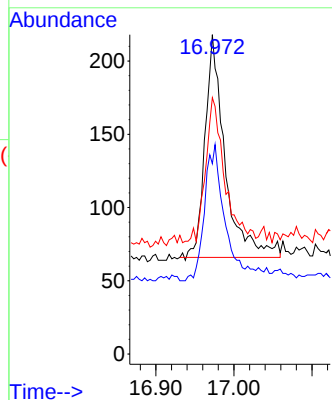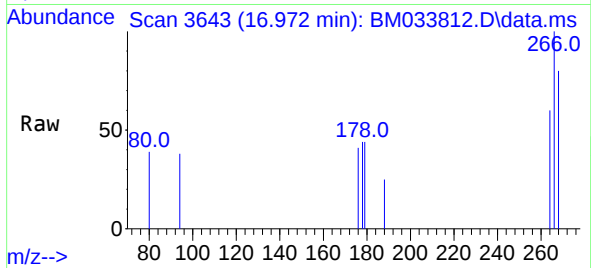

#24
Benzo(b)fluoranthene
Concen: 0.021 ng/ul
RT: 23.148 min Scan# 5701
Delta R.T. -0.005 min
Lab File: BM033812.D
Acq: 21 Jan 2022 05:39

Tgt Ion:252 Resp: 746
Ion Ratio Lower Upper
252 100
253 91.4 0.0 64.2#
125 126.2 0.0 28.8#

