

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012022\
 Data File : BM033827.D
 Acq On : 21 Jan 2022 17:42
 Operator : CG/JU
 Sample : N1199-10
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F39

Quant Time: Jan 22 00:08:13 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM010422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 21 01:34:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	3212	0.400	ng/u1	0.00
4) Naphthalene-d8	10.761	136	12525	0.400	ng/u1	# 0.00
9) Acenaphthene-d10	14.580	164	7894	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.316	188	15063	0.400	ng/u1	0.00
17) Chrysene-d12	21.482	240	8526	0.400	ng/u1	# 0.00
23) Perylene-d12	23.880	264	7547	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	12065	3.526	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.348	152	5933	0.348	ng/u1	0.00
18) Fluoranthene-d10	19.338	212	12741	0.482	ng/u1	0.00
Target Compounds						
14) Pentachlorophenol	16.973	266	188	0.032	ng/u1	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012022\
Data File : BM033827.D
Acq On : 21 Jan 2022 17:42
Operator : CG/JU
Sample : N1199-10
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F39


Quant Time: Jan 22 00:08:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM010422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 21 01:34:59 2022
Response via : Initial Calibration

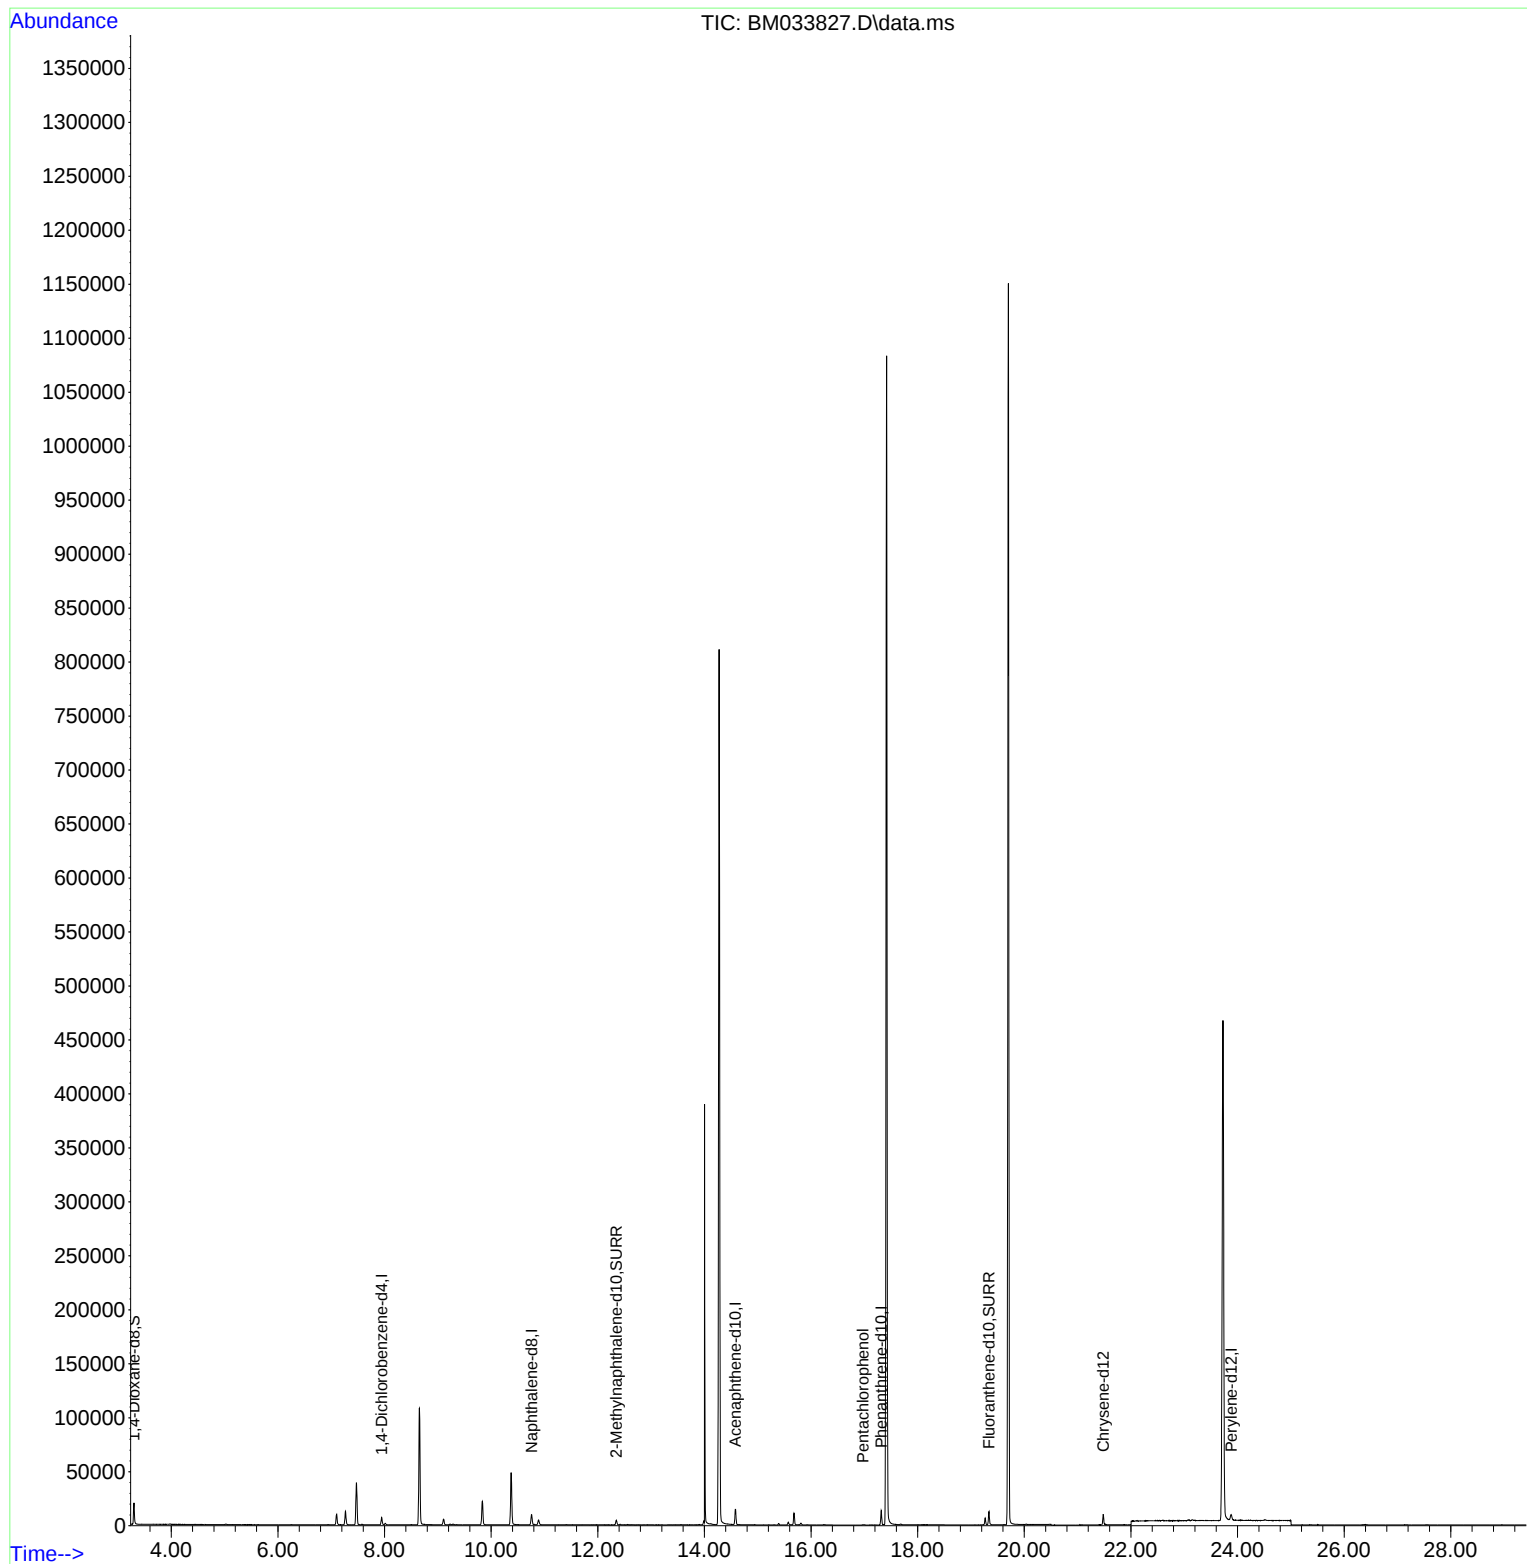

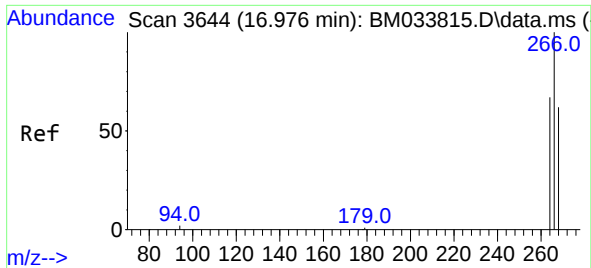

#14
 Pentachlorophenol
 Concen: 0.032 ng/ul
 RT: 16.973 min Scan# 30
 Delta R.T. -0.003 min
 Lab File: BM033827.D
 Acq: 21 Jan 2022 17:42

Instrument :
 BNA_M
 ClientSampleId :
 C0F39

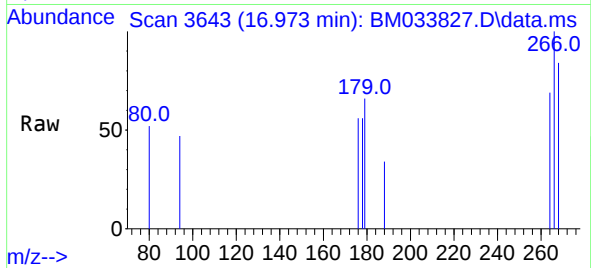

Tgt Ion:	266	Resp:	188
Ion	Ratio	Lower	Upper
266	100		
264	60.1	51.4	77.0
268	60.6	53.1	79.7

