
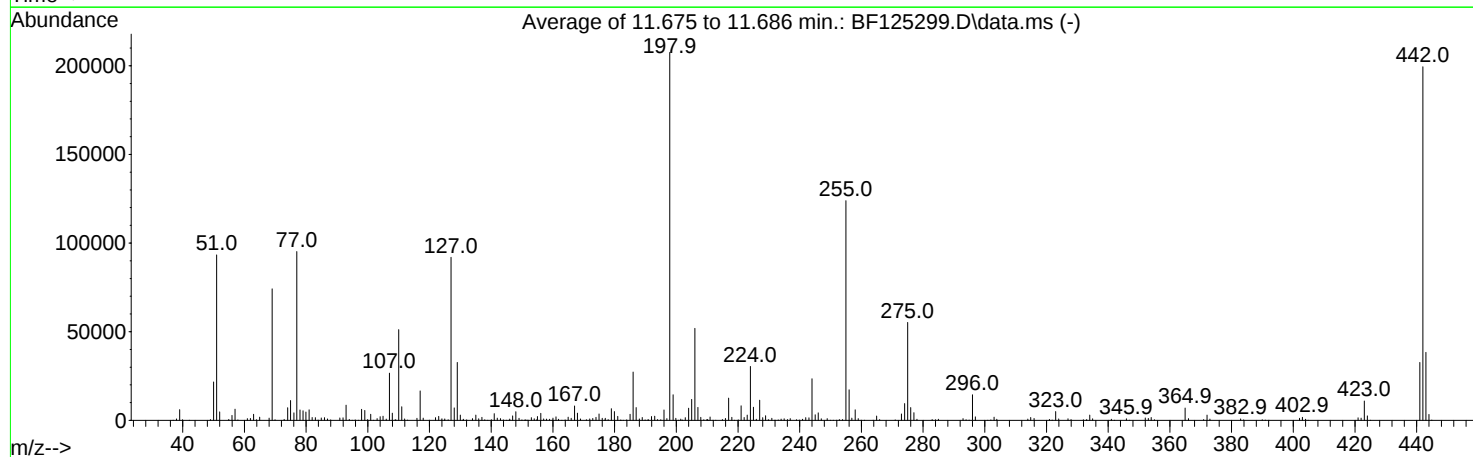


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF-2021\BF090121\
 Data File : BF125299.D
 Acq On : 1 Sep 2021 11:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 14 17:17:24 2021

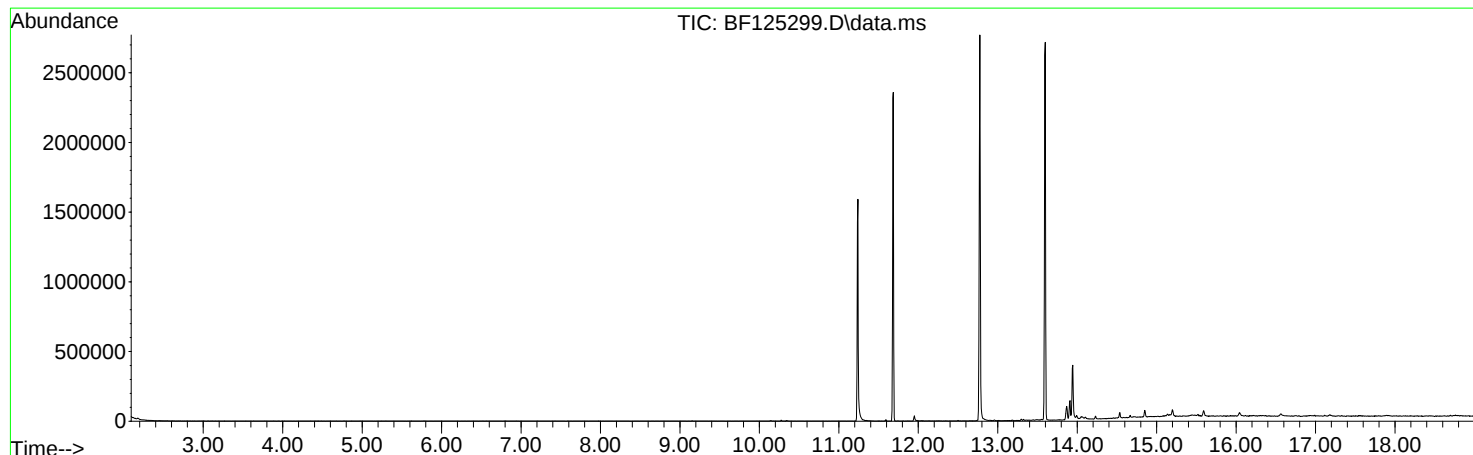

Spectrum Information: Average of 11.675 to 11.686 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	93355	PASS
68	69	0.00	2	1.7	1249	PASS
69	198	0.00	100	35.7	74176	PASS
70	69	0.00	2	0.5	400	PASS
127	198	10	80	44.3	91944	PASS
197	198	0.00	2	0.5	1045	PASS
198	198	100	100	100.0	207493	PASS
199	198	5	9	7.0	14481	PASS
275	198	10	60	26.6	55229	PASS
365	198	1	100	3.4	6988	PASS
441	198	0.01	100	15.7	32638	PASS
442	442	50	100	100.0	199445	PASS
443	442	15	24	19.2	38324	PASS