
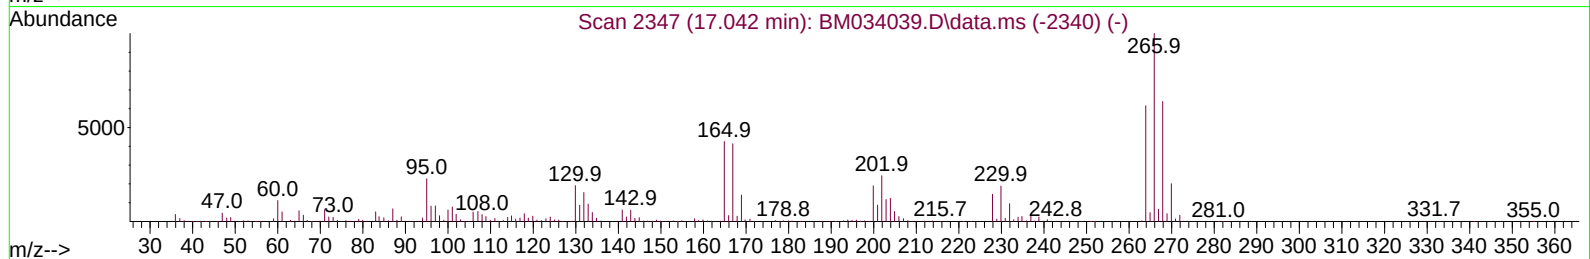
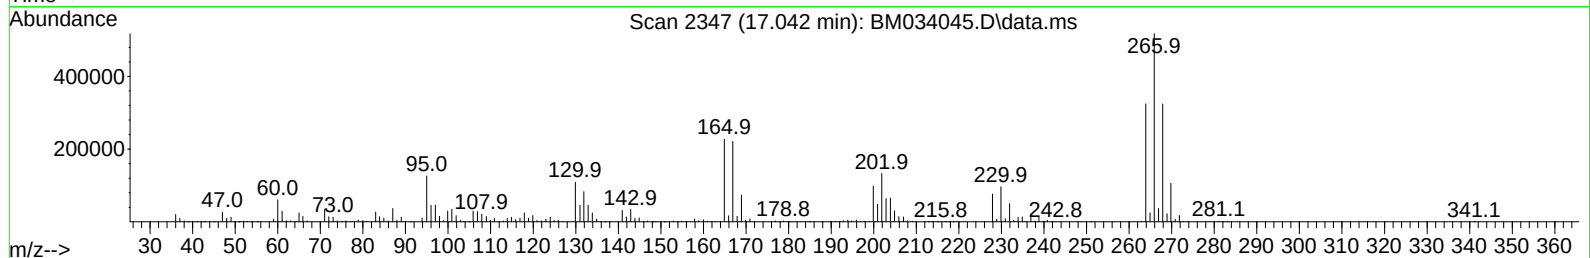


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022322\
Data File : BM034045.D
Acq On : 23 Feb 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 11:36:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 22 17:55:56 2022
Response via : Initial Calibration

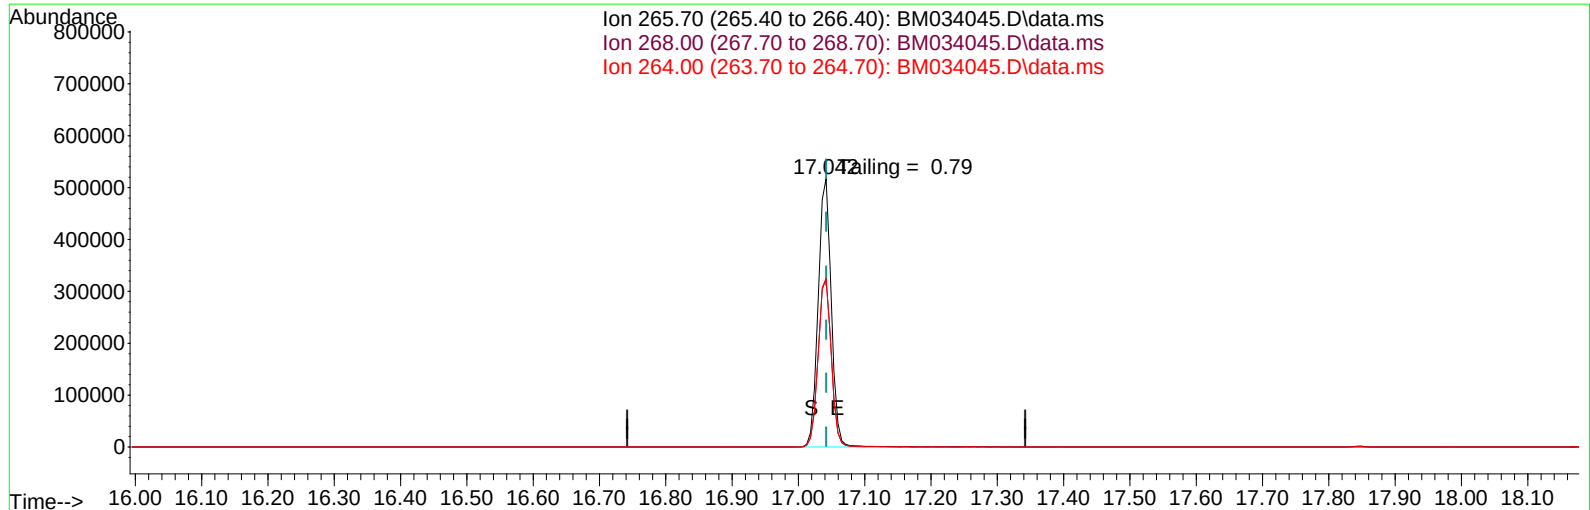

TIC: BM034045.D\data.ms

(70) Pentachlorophenol (C)




17.042min (-0.000) 131926.22 ng

response 712679

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.69
264.00	61.40	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022322\
Data File : BM034045.D
Acq On : 23 Feb 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 11:36:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 22 17:55:56 2022
Response via : Initial Calibration

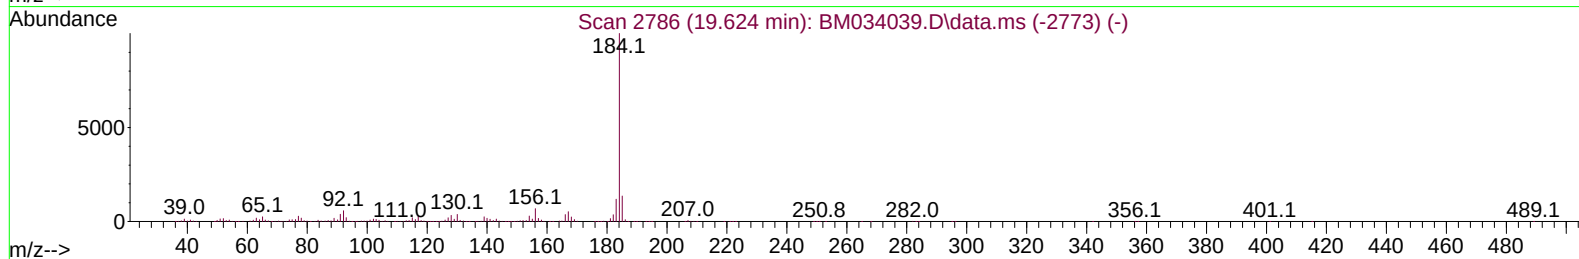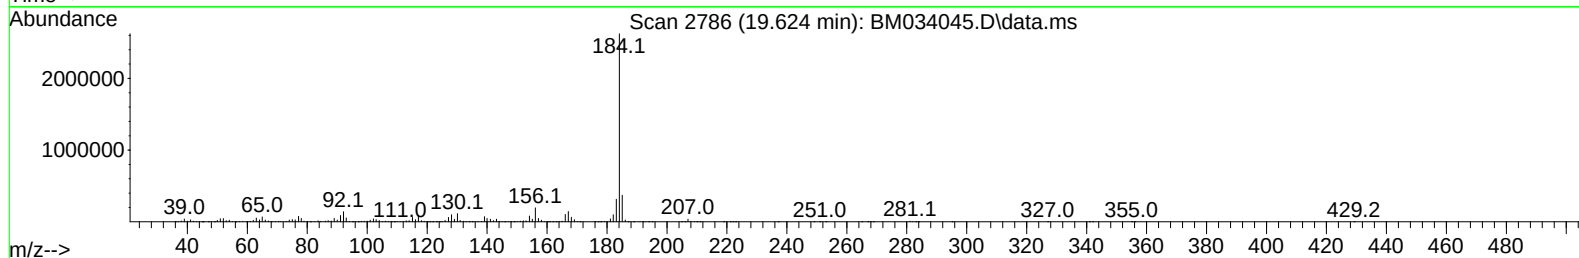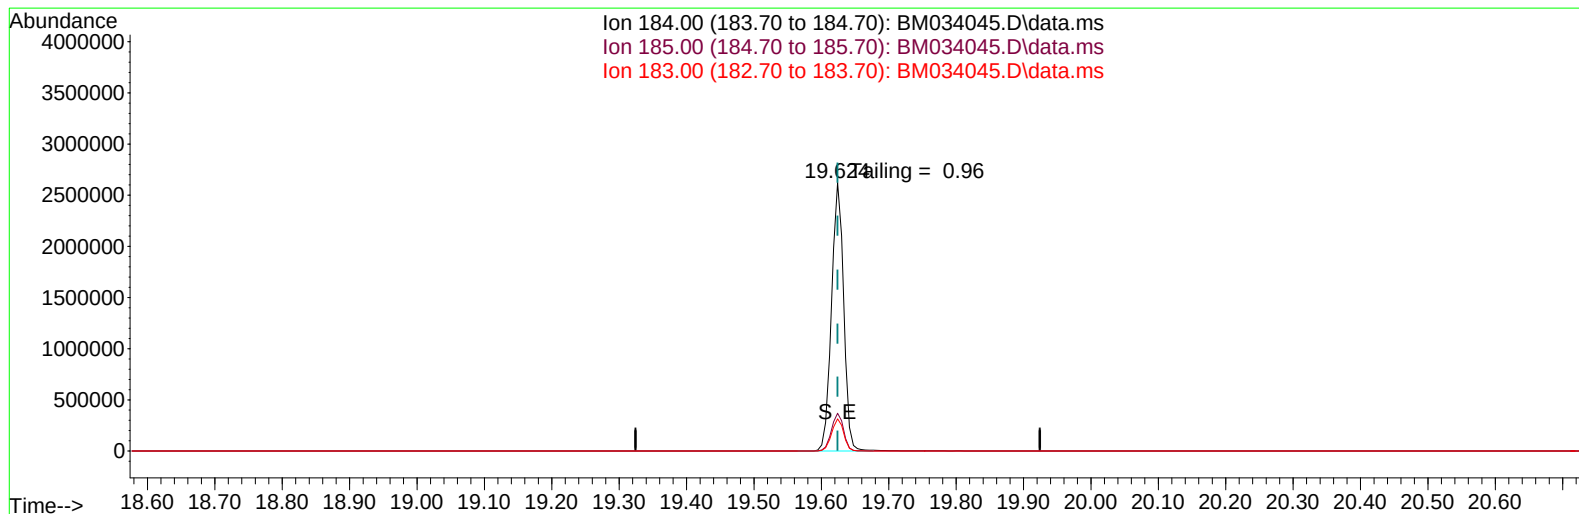

TIC: BM034045.D\data.ms

(77) Benzidine

19.624min (-0.000) 103168.46 ng

response 3279697

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.12
183.00	12.10	12.02
0.00	0.00	0.00