

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022322\
 Data File : BM034047.D
 Acq On : 23 Feb 2022 10:58
 Operator : CG/JU
 Sample : PB142857BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB142857BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.566	389	396	410	rBV	4504061	6446866	37.22%	9.508%
2	7.172	660	669	679	rBV	4298539	6735854	38.89%	9.934%
3	8.019	806	813	822	rBV	836074	1310664	7.57%	1.933%
4	9.178	1001	1010	1020	rBV	2568676	4260078	24.60%	6.283%
5	10.836	1284	1292	1299	rBV	1030196	1769836	10.22%	2.610%
6	13.283	1701	1708	1722	rBV	7792670	11075649	63.94%	16.334%
7	14.654	1934	1941	1947	rBV	1701197	2461045	14.21%	3.629%
8	16.130	2185	2192	2209	rBV	5607455	7894620	45.58%	11.643%
9	17.389	2399	2406	2415	rBV	2118594	3004250	17.34%	4.431%
10	20.012	2846	2852	2857	rBV	13931282	17320805	100.00%	25.544%
11	21.559	3111	3115	3124	rVB	2210352	2933857	16.94%	4.327%
12	24.024	3528	3534	3546	rVB2	1284922	2593243	14.97%	3.824%


Sum of corrected areas: 67806767

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022322\
Data File : BM034047.D
Acq On : 23 Feb 2022 10:58
Operator : CG/JU
Sample : PB142857BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142857BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

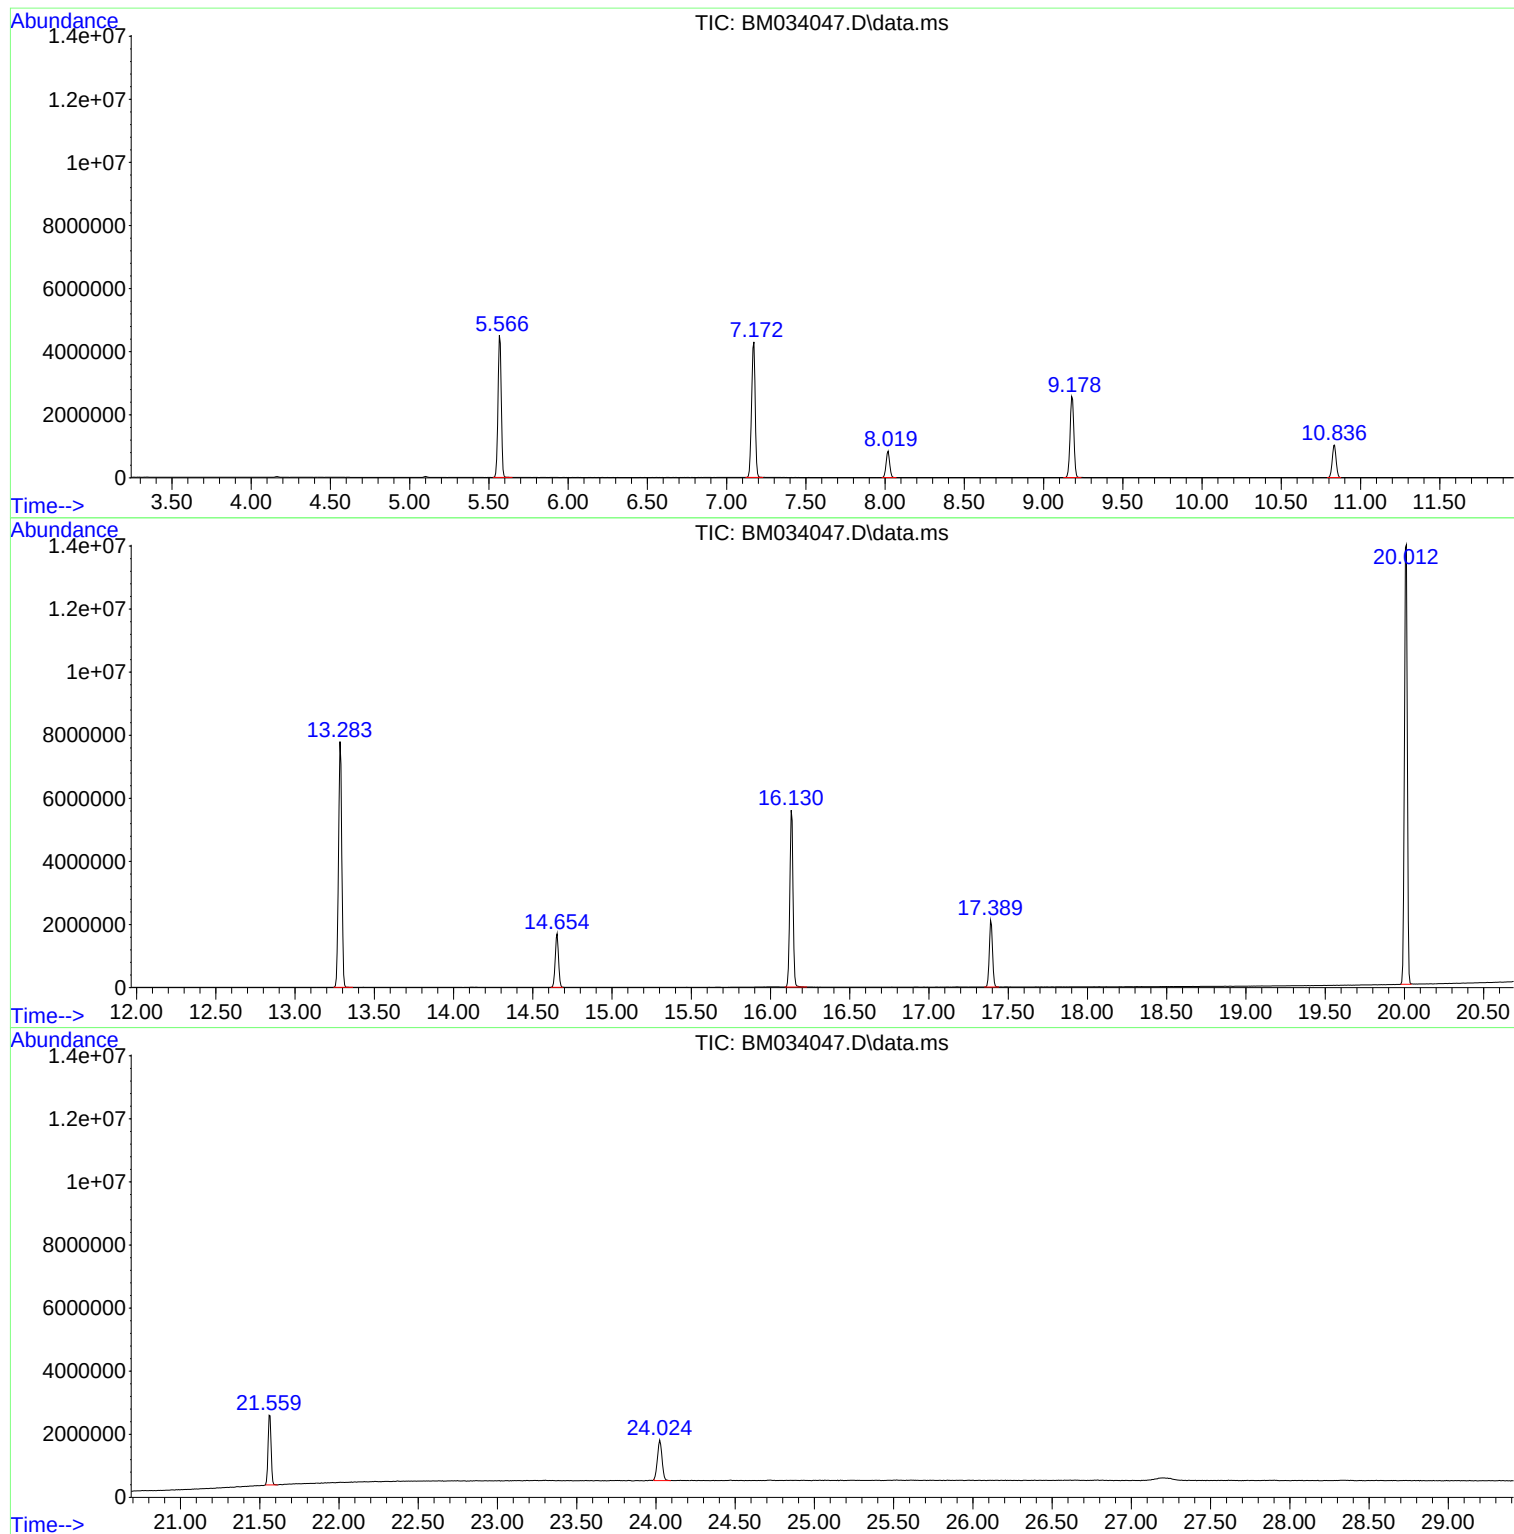

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022322\
Data File : BM034047.D
Acq On : 23 Feb 2022 10:58
Operator : CG/JU
Sample : PB142857BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142857BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022322\
Data File : BM034047.D
Acq On : 23 Feb 2022 10:58
Operator : CG/JU
Sample : PB142857BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142857BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------