
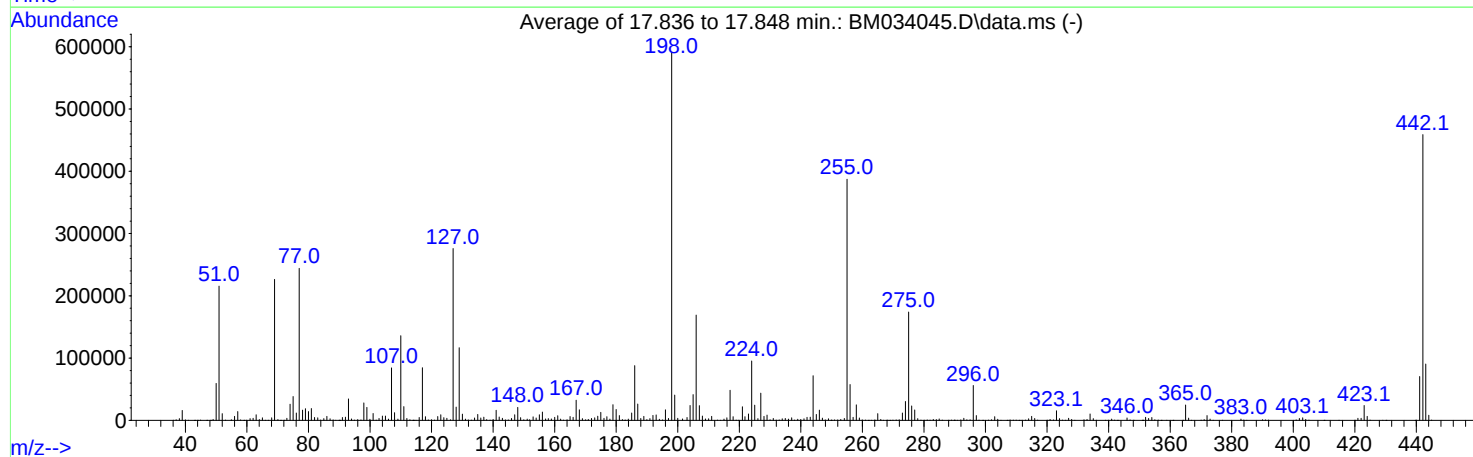


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022322\
 Data File : BM034045.D
 Acq On : 23 Feb 2022 09:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 22 17:55:56 2022

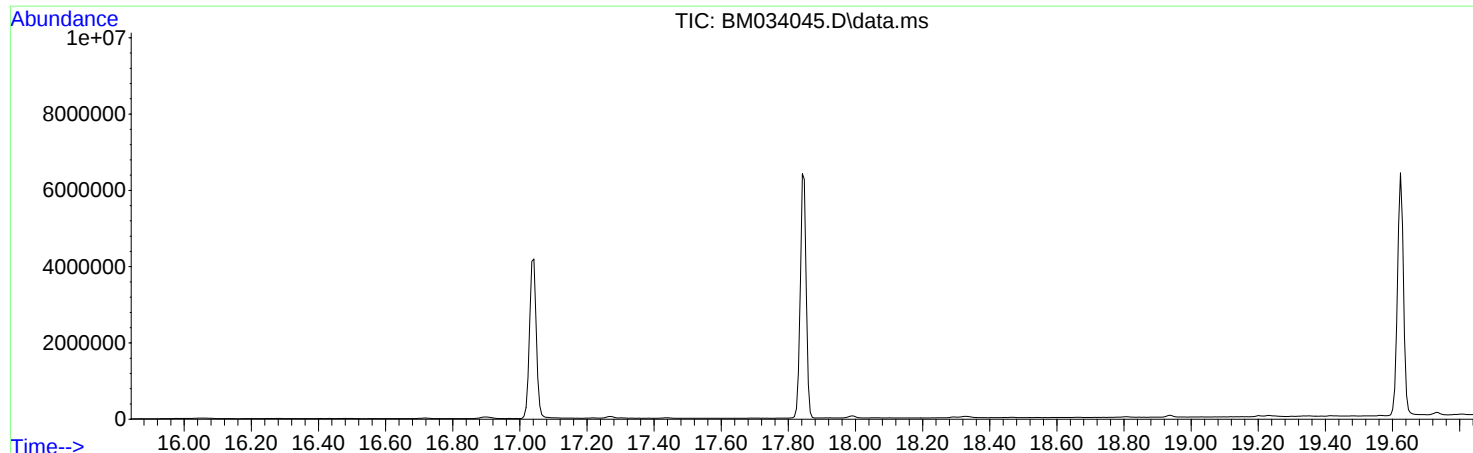




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	215637	PASS
68	69	0.00	2	1.9	4244	PASS
69	198	0.00	100	38.3	226432	PASS
70	69	0.00	2	0.5	1230	PASS
127	198	10	80	46.7	275968	PASS
197	198	0.00	2	0.5	3127	PASS
198	198	100	100	100.0	590720	PASS
199	198	5	9	6.9	40643	PASS
275	198	10	60	29.5	173968	PASS
365	198	1	100	4.2	24772	PASS
441	198	0.01	100	11.9	70381	PASS
442	442	50	100	100.0	458880	PASS
443	442	15	24	19.7	90459	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022322\
 Data File : BM034045.D
 Acq On : 23 Feb 2022 09:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Feb 23 11:36:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 22 17:55:56 2022
 Response via : Initial Calibration

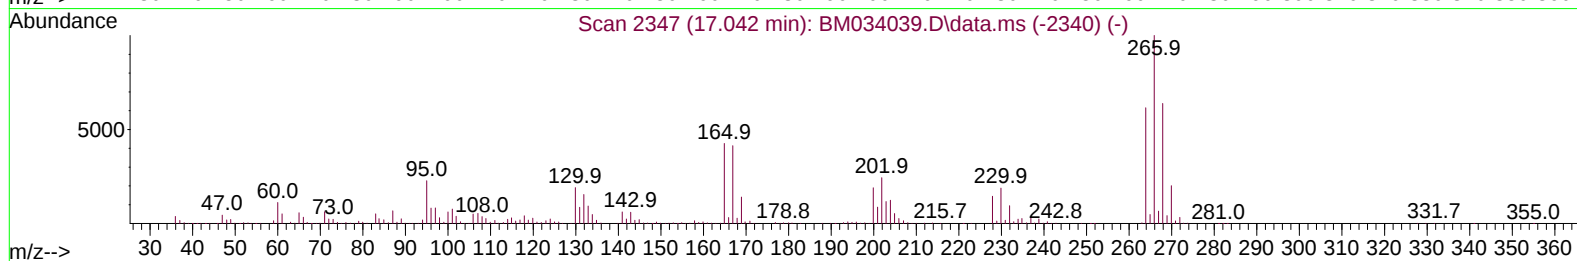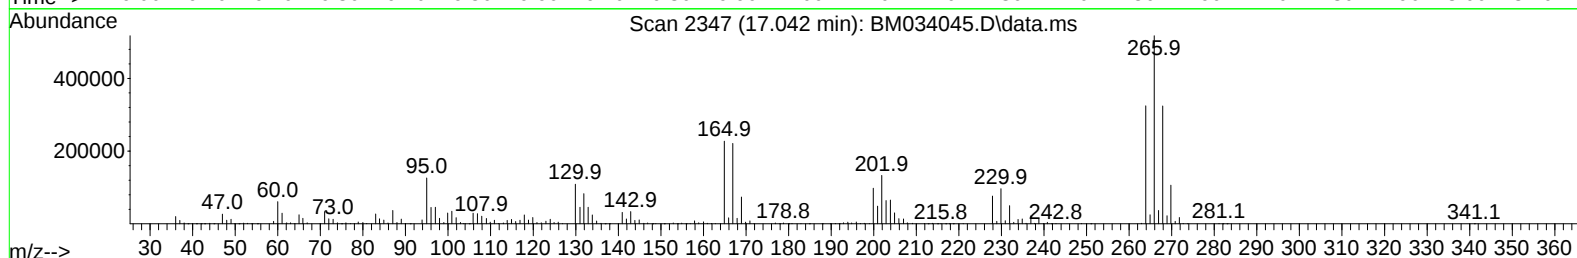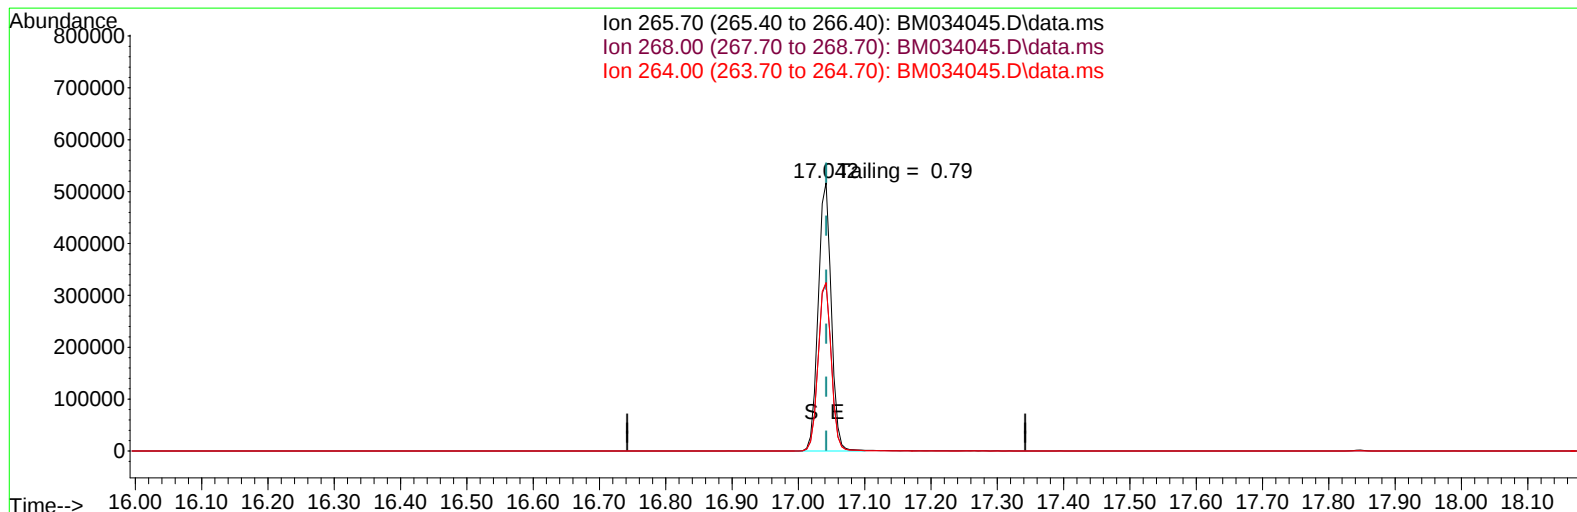

TIC: BM034045.D\data.ms

(70) Pentachlorophenol (C)

17.042min (-0.000) 131926.22 ng




response 712679

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.69
264.00	61.40	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022322\
Data File : BM034045.D
Acq On : 23 Feb 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 23 11:36:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 22 17:55:56 2022
Response via : Initial Calibration

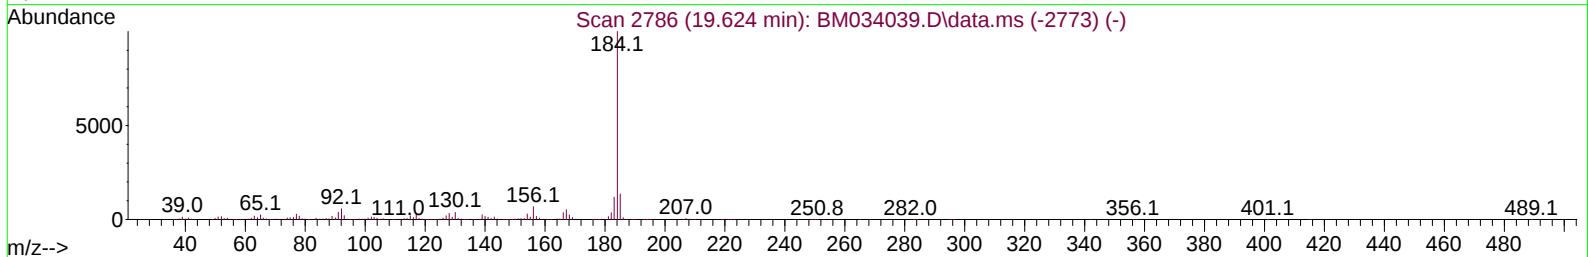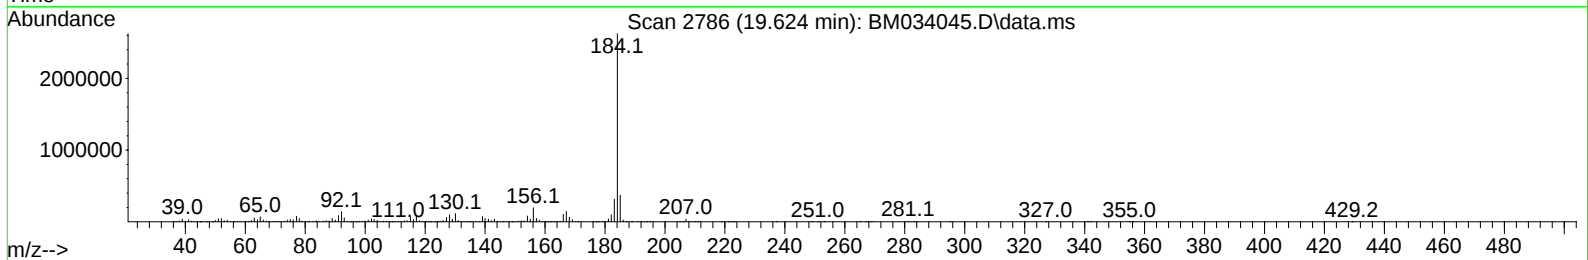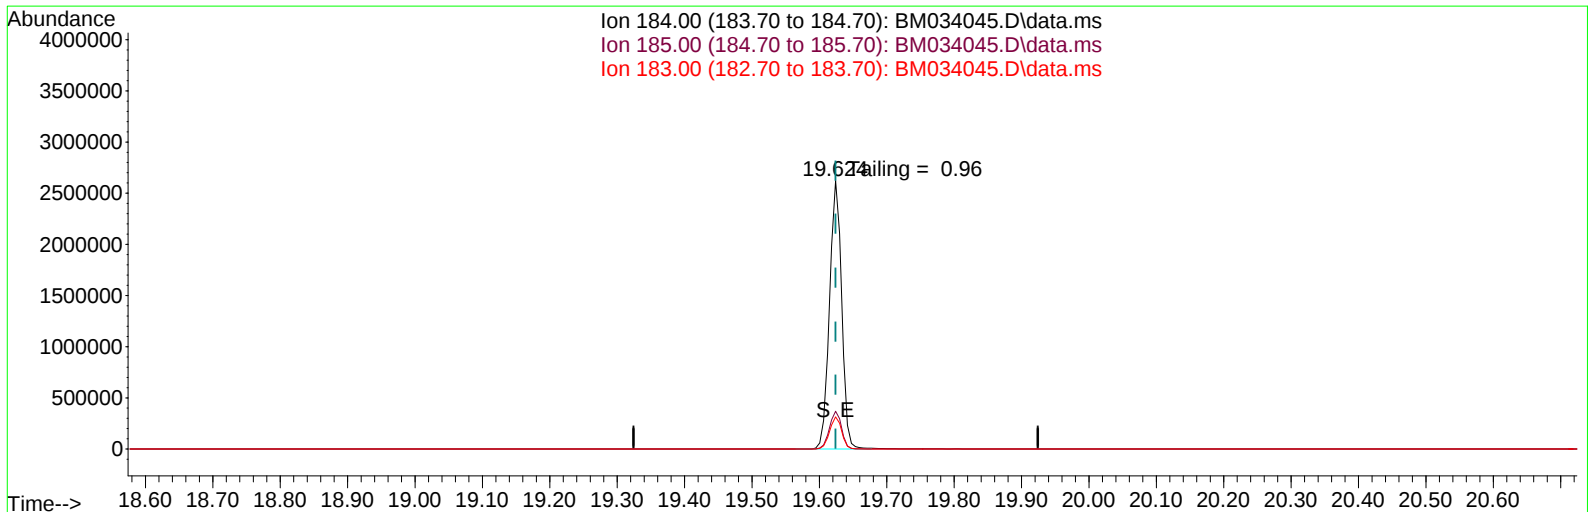

TIC: BM034045.D\data.ms

(77) Benzidine

19.624min (-0.000) 103168.46 ng

response 3279697

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.12
183.00	12.10	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/23/2022	BNA_M	<u>BM034045.D</u>
Compound Name	Response	Retention Time
DDT	2076860	20.86
DDD	10211	20.42
DDE	959	19.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11170	2088030	0.53

Instrument :
BNA_M
ClientSampleId :
DFTPP