


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050124\
Data File : BM045655.D
Acq On : 01 May 2024 10:14
Operator : MA/JU
Sample : DFTPP022
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP022

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 30 09:34:10 2024

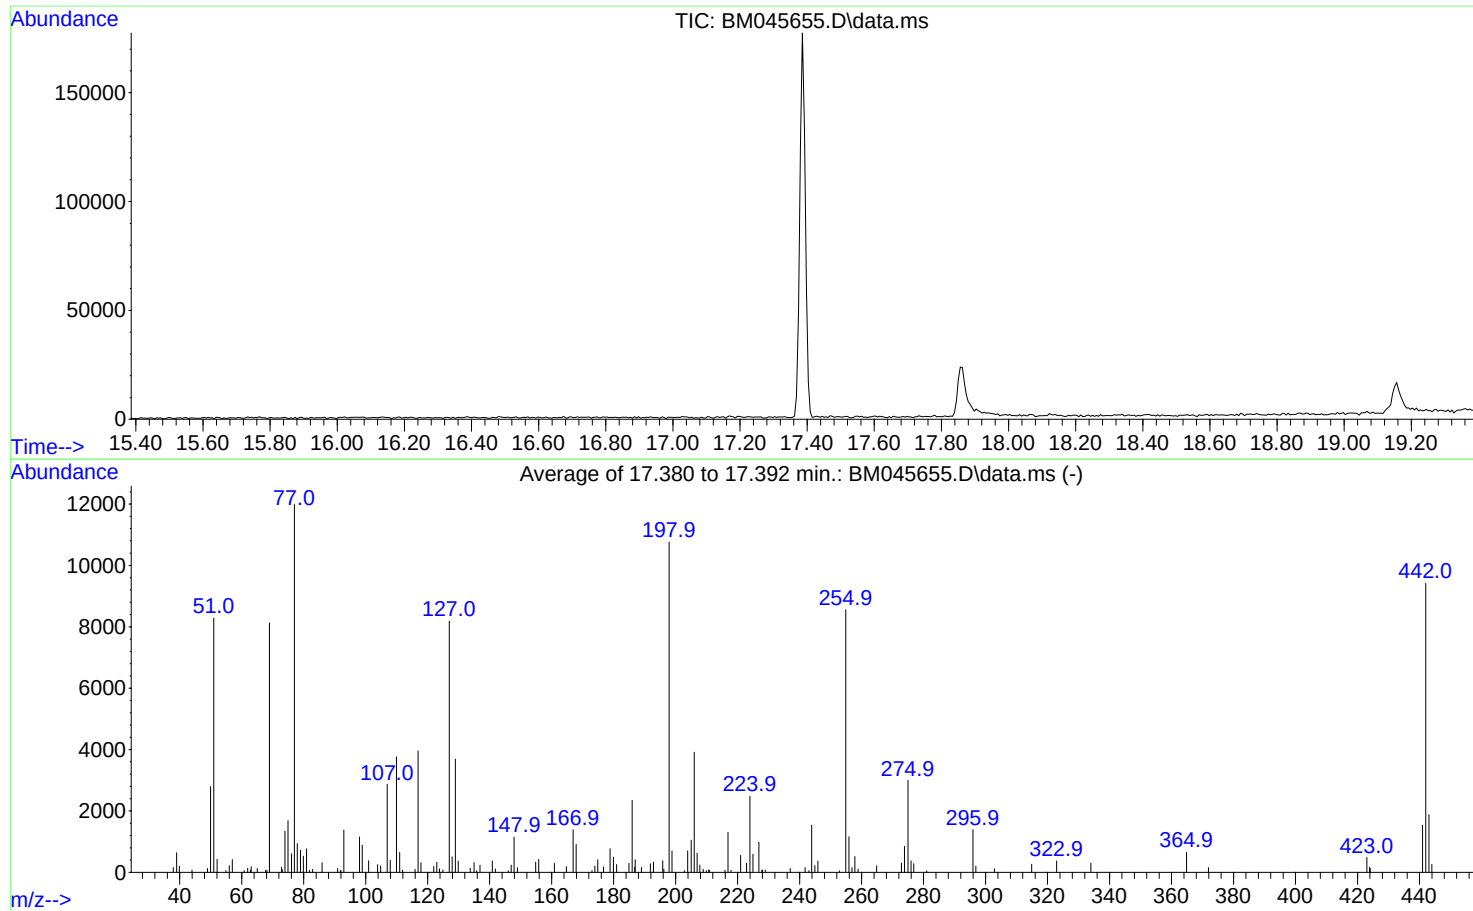

Scan 2425 (17.351 min): BM045655.D\data.ms
DFTPP022

m/z	Abundance
43.00	185.0
43.90	335.0
206.90	247.0

Instrument :

BNA_M

ClientSampleId :

DFTPP022

m/z	Abundance
37.90	166.0
39.00	688.0
39.90	340.0
44.00	461.0
50.00	2484.0
51.00	7830.0
52.10	316.0
56.00	214.0
57.00	392.0
60.80	166.0
62.00	164.0
63.10	292.0
69.00	7694.0
72.80	252.0
74.00	1329.0
75.00	1814.0
76.00	547.0
77.00	11903.0
78.00	853.0
78.90	544.0
80.00	531.0
80.90	875.0
86.00	277.0
90.90	198.0
91.80	177.0
92.90	1302.0
98.00	1114.0
98.90	966.0
100.90	462.0
103.90	231.0
104.80	167.0
106.90	2544.0
107.90	516.0
109.90	3179.0
111.00	671.0
111.90	224.0
116.90	3231.0
117.80	242.0
121.90	198.0
123.00	229.0
123.80	167.0
124.90	239.0
127.00	7434.0
127.90	370.0
128.90	3300.0
129.80	316.0
133.80	254.0
134.90	303.0
135.80	153.0
136.90	241.0
140.80	320.0
146.00	159.0
147.90	1102.0
149.00	197.0
154.90	300.0
155.90	309.0
160.90	255.0
164.80	230.0
166.90	1183.0
167.90	751.0
173.90	270.0
175.00	222.0
176.70	162.0
178.80	661.0
179.90	443.0
181.00	266.0
184.90	239.0
185.90	1718.0
186.80	511.0
188.90	152.0
191.90	269.0
192.80	227.0
195.90	303.0
196.20	308.0
197.90	8810.0
198.80	614.0
202.80	176.0
203.90	572.0
205.00	1009.0
206.00	3378.0
207.00	746.0
207.90	182.0
216.90	1139.0
220.90	551.0
222.90	284.0
223.90	1960.0
225.00	365.0
226.80	806.0
237.00	196.0
241.90	154.0
244.00	1161.0
245.80	277.0

Instrument :
BNA_M
ClientSampleId :
DFTPP022

254.90	7854.0
255.90	1047.0
256.90	282.0
257.80	530.0
258.90	171.0
265.00	182.0
272.80	243.0
273.90	500.0
274.90	2656.0
275.90	334.0
276.90	267.0
295.90	1155.0
314.80	178.0
322.90	364.0
334.00	232.0
364.80	401.0
423.00	332.0
423.90	164.0
441.00	986.0
442.00	5781.0
443.00	1249.0
444.00	232.0

Instrument :
BNA_M
ClientSampleId :
DFTPP022

m/z	Abundance
37.90	310.0
39.00	728.0
39.90	261.0
44.00	523.0
49.00	197.0
50.00	3599.0
51.00	9740.0
52.10	492.0
55.90	197.0
57.00	535.0
61.90	239.0
63.00	278.0
65.00	200.0
68.10	221.0
68.90	9603.0
73.10	268.0
73.90	1697.0
75.00	1952.0
76.00	804.0
77.00	13894.0
78.00	1230.0
79.00	731.0
79.80	689.0
80.90	783.0
81.90	205.0
82.90	292.0
85.90	293.0
91.00	171.0
92.00	166.0
93.00	1537.0
98.00	1478.0
98.90	1074.0
101.00	425.0
103.90	290.0
104.80	256.0
107.00	3742.0
107.90	372.0
109.90	4766.0
111.00	750.0
115.90	303.0
116.90	4857.0
117.90	381.0
122.00	382.0
123.00	469.0
123.80	180.0
126.90	9953.0
127.90	588.0
128.90	4545.0
129.90	394.0
133.70	153.0
135.00	362.0
136.90	195.0
140.80	491.0
141.90	168.0
146.90	446.0
147.90	1305.0
148.90	257.0
154.80	500.0
155.90	562.0
160.90	457.0
164.70	155.0
166.90	1683.0
167.90	1288.0
173.00	163.0
174.00	174.0
174.80	476.0
176.80	190.0
178.80	902.0
179.90	652.0
180.90	267.0
185.00	298.0
186.00	3030.0
187.00	799.0
189.00	151.0
191.80	315.0
192.90	499.0
195.80	391.0
197.90	13458.0
198.90	909.0
203.90	1004.0
204.90	1233.0
206.00	4487.0
207.00	1041.0
207.80	346.0
208.90	296.0
209.90	151.0
210.70	252.0
215.90	218.0
216.90	1431.0
217.90	200.0
221.00	636.0
222.90	315.0

Instrument :
BNA_M
ClientSampleId :
DFTPP022

224.00	3167.0
224.90	845.0
226.90	1193.0
227.80	187.0
228.90	223.0
237.00	180.0
241.70	159.0
243.80	1800.0
244.90	327.0
245.90	481.0
252.80	161.0
254.90	9732.0
255.90	1409.0
256.90	168.0
257.80	584.0
258.80	150.0
264.80	230.0
272.90	393.0
273.80	960.0
274.90	3633.0
275.90	478.0
276.80	264.0
295.90	1777.0
296.80	355.0
302.80	181.0
314.90	276.0
322.90	491.0
333.90	230.0
364.80	828.0
371.90	177.0
423.00	619.0
424.10	374.0
441.00	1690.0
442.00	11429.0
443.00	2635.0
443.90	233.0

Instrument :
BNA_M
ClientSampleId :
DFTPP022

m/z	Abundance
39.00	516.0
43.90	251.0
48.90	171.0
49.90	2299.0
51.00	7264.0
51.90	460.0
54.90	180.0
56.10	242.0
56.90	317.0
62.80	218.0
65.10	179.0
67.70	164.0
69.00	7088.0
72.90	229.0
74.00	1012.0
74.90	1284.0
76.10	457.0
77.00	10161.0
77.90	728.0
79.00	899.0
79.90	357.0
80.90	633.0
85.90	364.0
92.90	1283.0
98.00	867.0
98.90	611.0
100.90	258.0
103.70	224.0
104.80	202.0
107.00	2311.0
108.00	284.0
110.00	3350.0
110.90	519.0
116.90	3786.0
117.80	313.0
122.90	287.0
127.00	7161.0
127.90	563.0
129.00	3222.0
129.80	391.0
134.90	283.0
136.90	270.0
140.90	295.0
141.80	162.0
147.00	258.0
147.90	1031.0
154.80	197.0
155.80	390.0
160.80	162.0
164.80	177.0
166.90	1317.0
168.00	677.0
173.90	186.0
175.00	536.0
176.80	163.0
178.90	746.0
180.00	383.0
180.90	230.0
185.00	354.0
186.00	2286.0
186.90	430.0
188.90	181.0
191.90	239.0
192.90	278.0
195.80	452.0
197.90	10014.0
198.90	567.0
203.90	526.0
205.10	907.0
206.00	3873.0
207.00	825.0
207.70	174.0
210.90	196.0
216.90	1343.0
220.90	494.0
222.90	293.0
223.90	2321.0
224.90	553.0
226.80	965.0
228.00	229.0
241.80	150.0
243.00	174.0
243.90	1660.0
244.90	324.0
246.00	344.0
254.90	8087.0
255.90	1028.0
257.90	434.0
264.80	210.0
272.90	270.0
273.90	1071.0
275.00	2698.0

Instrument :
BNA_M
ClientSampleId :
DFTPP022

276.00	322.0
276.90	313.0
281.00	154.0
295.90	1250.0
296.90	247.0
302.90	177.0
314.90	347.0
322.80	258.0
334.00	438.0
364.90	730.0
371.90	273.0
423.00	511.0
423.90	321.0
441.00	1944.0
442.00	11042.0
443.10	1759.0
443.90	315.0

Instrument :
BNA_M
ClientSampleId :
DFTPP022