

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050619\
 Data File : BM020155.D
 Acq On : 07 May 2019 05:50
 Operator : JU/SJ
 Sample : K2672-02 5X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB-01-COMP

Quant Time: May 07 06:40:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 03:58:37 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	165695	20.00	ng	0.00
21) Naphthalene-d8	10.59	136	617011	20.00	ng	0.00
39) Acenaphthene-d10	14.44	164	354313	20.00	ng	0.00
64) Phenanthrene-d10	17.19	188	821993	20.00	ng	0.00
76) Chrysene-d12	21.37	240	814202	20.00	ng	0.00
87) Perylene-d12	23.67	264	952401	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	198028	19.54	ng	0.00
7) Phenol-d6	6.96	99	274870	19.85	ng	0.00
23) Nitrobenzene-d5	8.96	82	179468	11.48	ng	0.00
42) 2,4,6-Tribromophenol	15.93	330	103422	18.81	ng	0.00
45) 2-Fluorobiphenyl	13.05	172	358794	12.46	ng	0.00
79) Terphenyl-d14	19.80	244	533797	11.44	ng	0.00
Target Compounds						
32) Benzoic acid	9.84	122	384	6.668	ng	Qvalue # 56
71) Phenanthrene	17.23	178	124124	2.736	ng	96
75) Fluoranthene	19.24	202	304816	5.309	ng	98
78) Pyrene	19.61	202	264524	4.839	ng	99
81) Benzo(a)anthracene	21.35	228	172458	3.020	ng	92
83) Chrysene	21.35	228	168373	3.040	ng	95
88) Benzo(b)fluoranthene	22.97	252	239606	3.810	ng	# 87
89) Benzo(k)fluoranthene	22.97	252	228476	3.983	ng	# 87
90) Benzo(a)pyrene	23.56	252	175478	3.072	ng	# 85
92) Benzo(g,h,i)perylene	26.73	276	137043	2.430	ng	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050619\
Data File : BM020155.D
Acq On : 07 May 2019 05:50
Operator : JU/SJ
Sample : K2672-02 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-01-COMP

Quant Time: May 07 06:40:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:58:37 2019
Response via : Initial Calibration

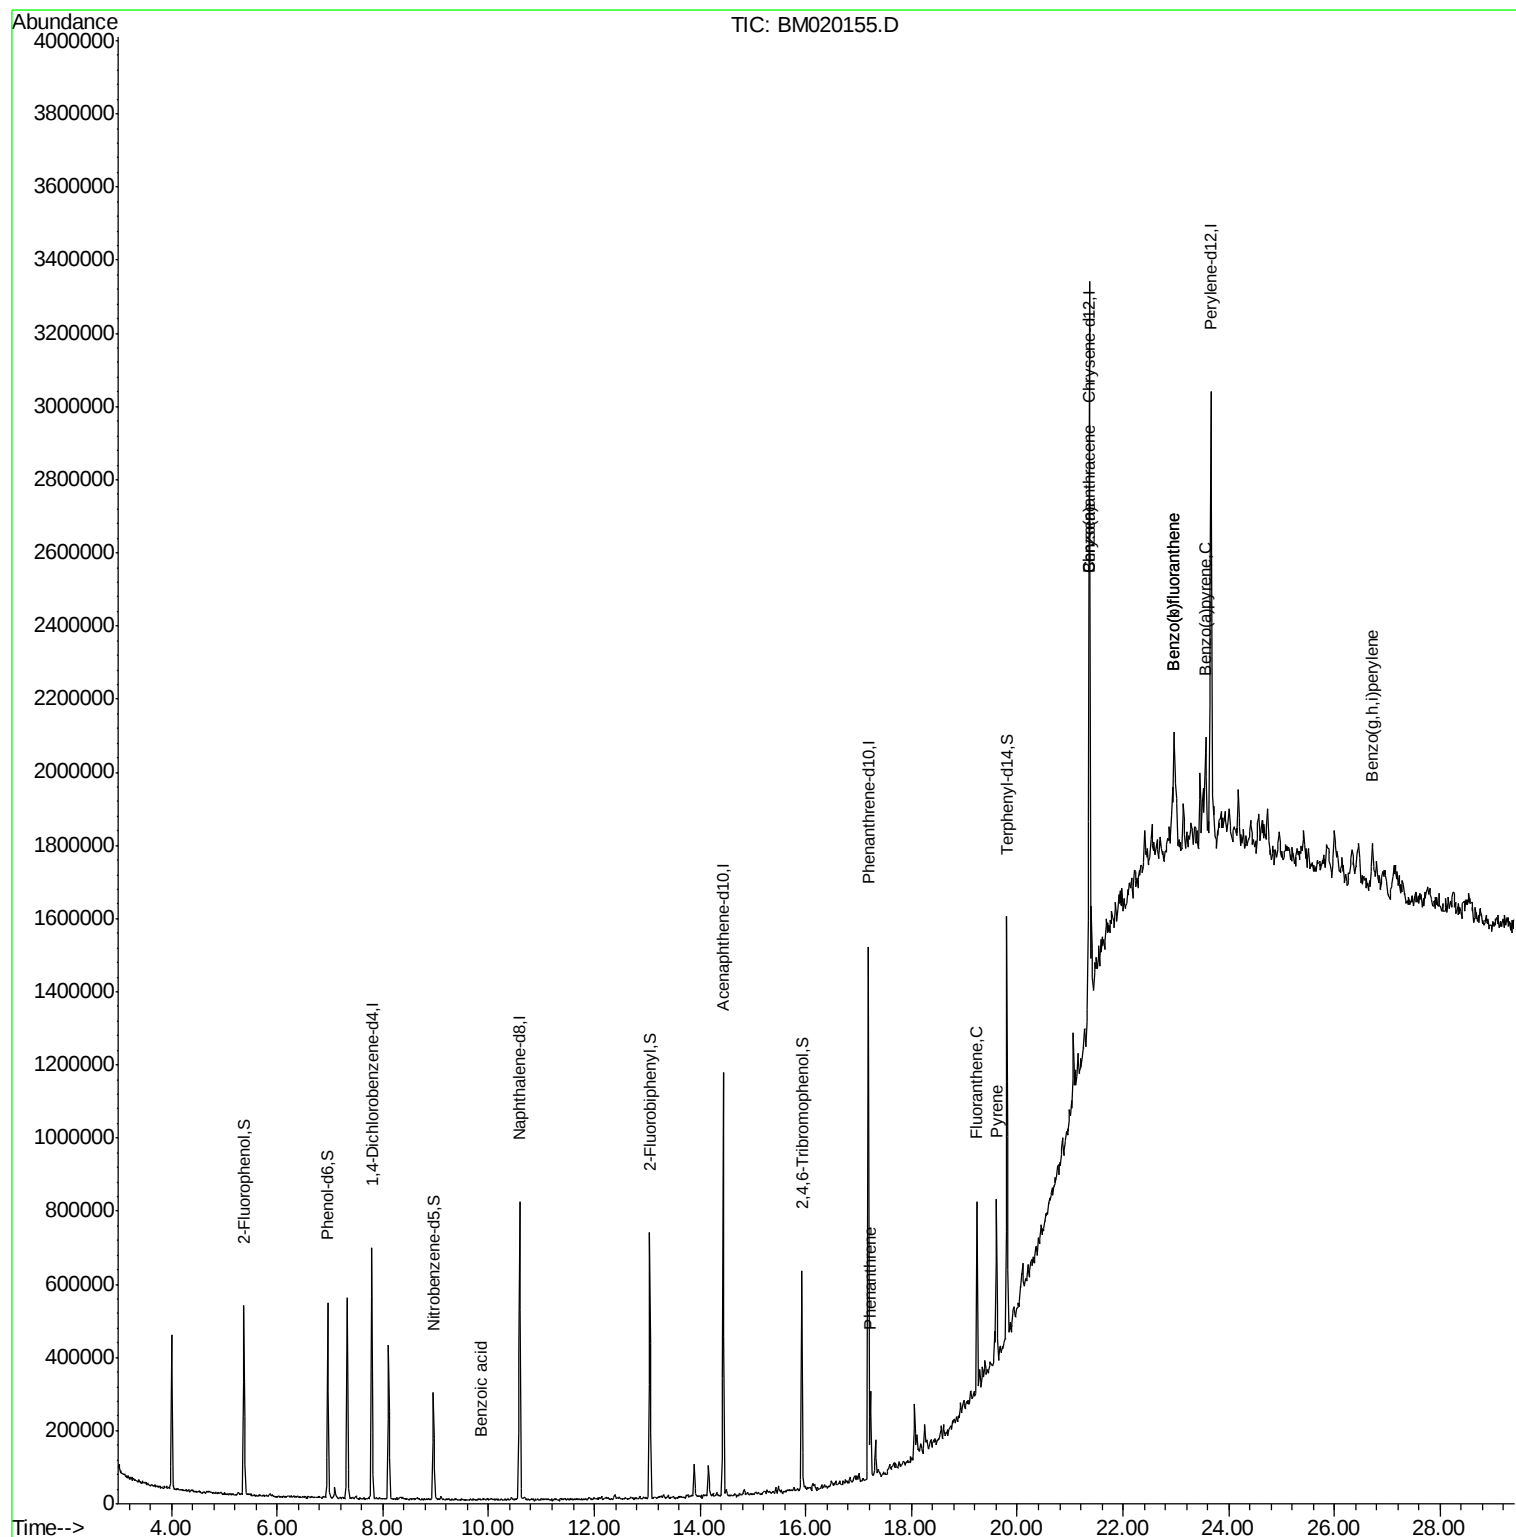

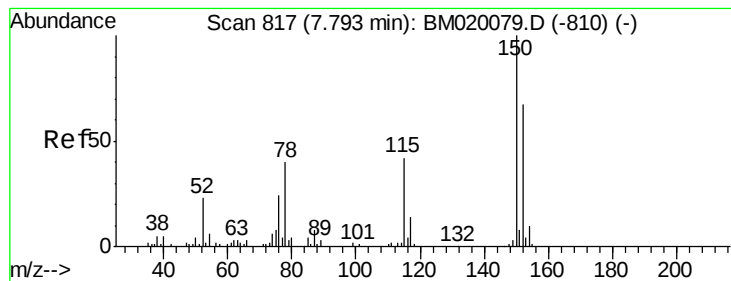


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.79 min Scan# 817
Delta R.T. -0.00 min
Lab File: BM020155.D
Acq: 07 May 2019 05:50

Instrument :
BNA_M
ClientSampleId :
SB-01-COMP

Tgt Ion:152 Resp: 165695
Ion Ratio Lower Upper
152 100
150 154.5 119.8 179.8
115 61.0 50.8 76.2

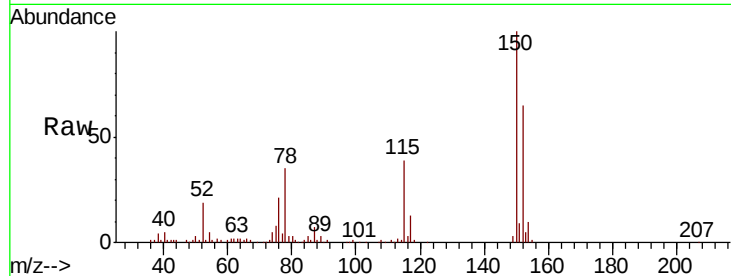


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

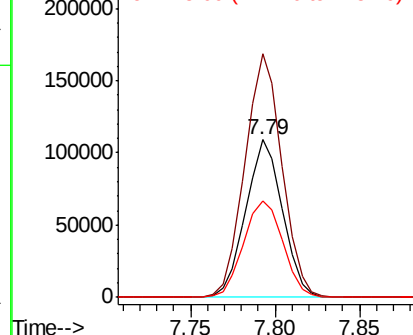



#5


2-Fluorophenol
Concen: 19.536 ng
RT: 5.37 min Scan# 406
Delta R.T. 0.01 min
Lab File: BM020155.D
Acq: 07 May 2019 05:50

Tgt Ion:112 Resp: 198028
Ion Ratio Lower Upper
112 100
64 68.1 53.8 80.6
63 37.6 32.3 48.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

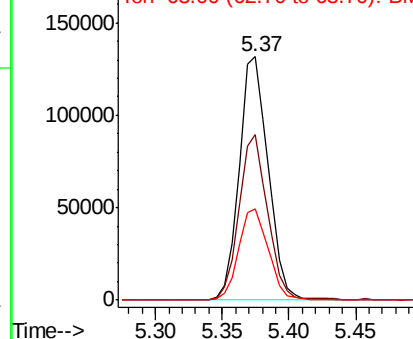



#7

Phenol-d6

Concen: 19.849 ng

RT: 6.96 min Scan# 675

Delta R.T. 0.01 min

Lab File: BM020155.D

Acq: 07 May 2019 05:50

Instrument :

BNA_M

ClientSampleId :

SB-01-COMP





Tgt Ion: 99 Resp: 274870

Ion Ratio Lower Upper

99 100

42 15.2 14.2 21.2

71 46.7 40.3 60.5

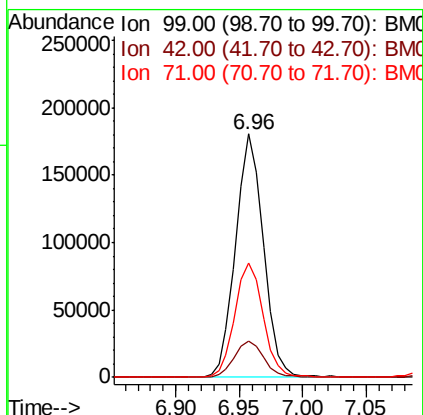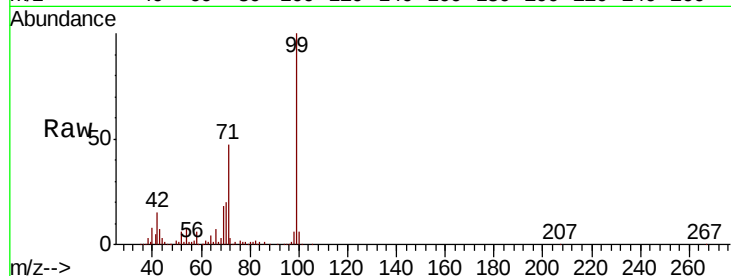

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.59 min Scan# 1292

Delta R.T. -0.00 min

Lab File: BM020155.D

Acq: 07 May 2019 05:50

Tgt Ion: 136 Resp: 617011




Ion Ratio Lower Upper


136 100

137 10.5 9.6 14.4

54 6.5 5.5 8.3

68 6.5 4.6 6.8


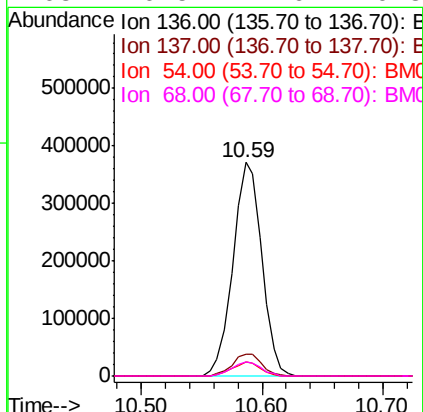






#23
 Nitrobenzene-d5
 Concen: 11.483 ng
 RT: 8.96 min Scan# 1015
 Delta R.T. -0.00 min
 Lab File: BM020155.D
 Acq: 07 May 2019 05:50




Instrument :
 BNA_M
 ClientSampleId :
 SB-01-COMP


Tgt Ion	Ratio	Lower	Upper
82	100		
128	33.0	25.2	37.8
54	38.3	31.9	47.9

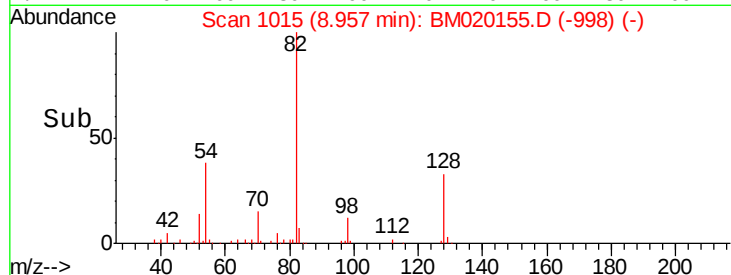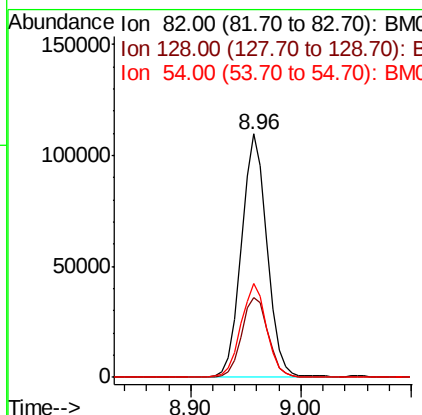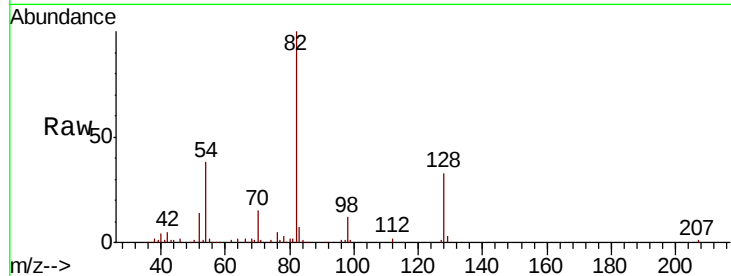

#32
 Benzoic acid
 Concen: 6.668 ng
 RT: 9.84 min Scan# 1165
 Delta R.T. -0.02 min
 Lab File: BM020155.D
 Acq: 07 May 2019 05:50

Tgt Ion	Ratio	Lower	Upper
122	100		
105	69.2	122.5	162.5#
77	108.8	123.3	163.3#

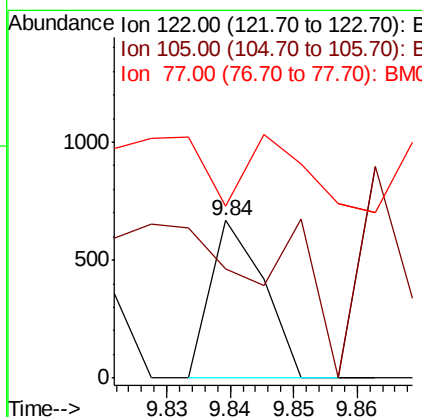

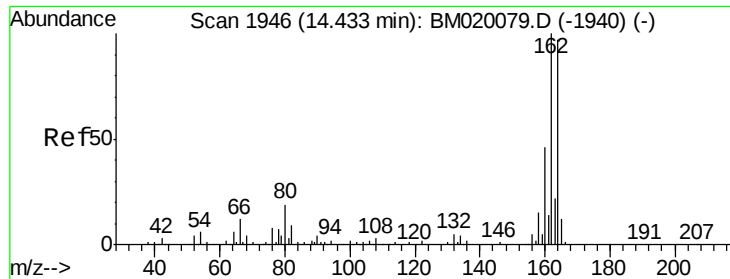

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.44 min Scan# 1947

Delta R.T. 0.01 min

Lab File: BM020155.D

Acq: 07 May 2019 05:50

Instrument :

BNA_M

ClientSampleId :

SB-01-COMP


Tgt Ion:164 Resp: 354313

Ion Ratio Lower Upper

164 100

162 103.7 82.2 123.2




160 45.9 37.6 56.4

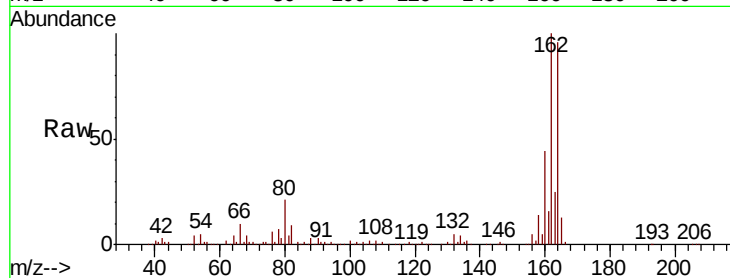

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

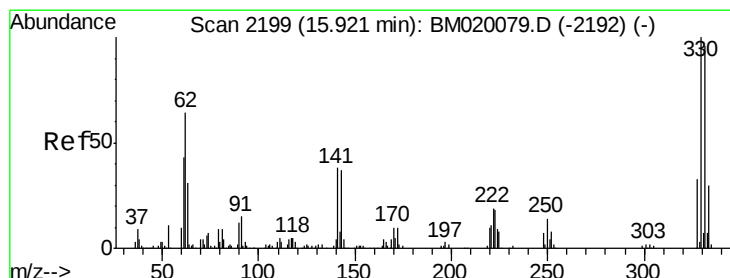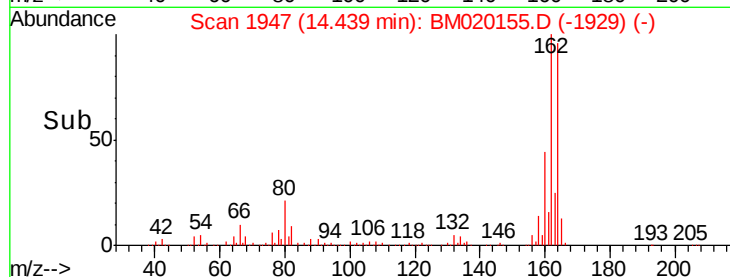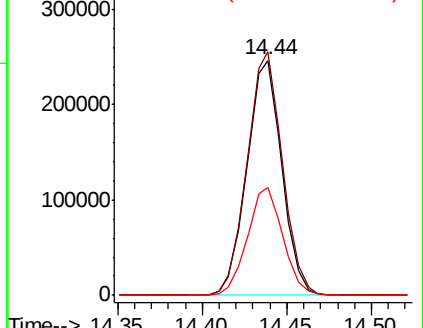

#42

2,4,6-Tribromophenol

Concen: 18.805 ng

RT: 15.93 min Scan# 2200

Delta R.T. 0.01 min

Lab File: BM020155.D

Acq: 07 May 2019 05:50


Tgt Ion:330 Resp: 103422

Ion Ratio Lower Upper

330 100

332 97.3 76.8 115.2



141 35.5 29.2 43.8

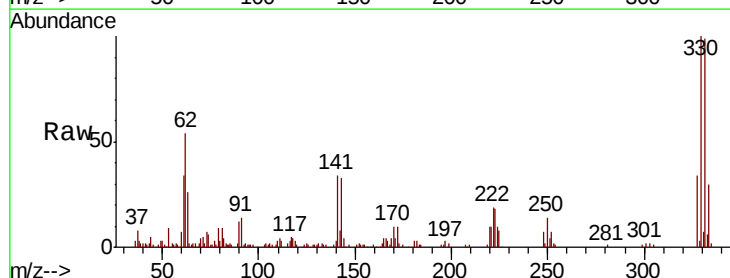


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



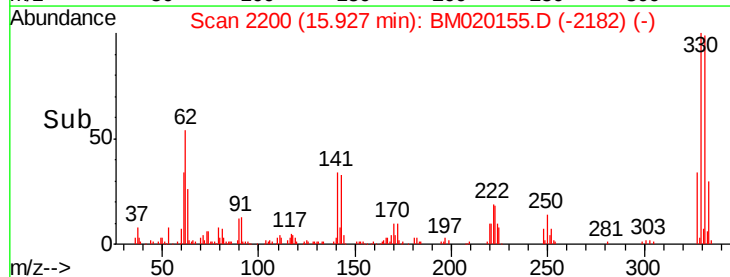
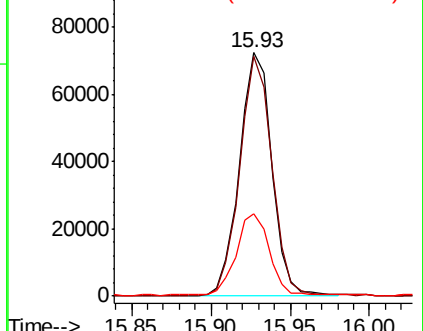




#45
 2-Fluorobiphenyl
 Concen: 12.459 ng
 RT: 13.05 min Scan# 1711
 Delta R.T. -0.01 min
 Lab File: BM020155.D
 Acq: 07 May 2019 05:50




Instrument :
 BNA_M
 ClientSampleId :
 SB-01-COMP


Tgt Ion:172 Resp: 358794
 Ion Ratio Lower Upper
 172 100
 171 33.5 27.3 40.9
 170 21.8 17.9 26.9

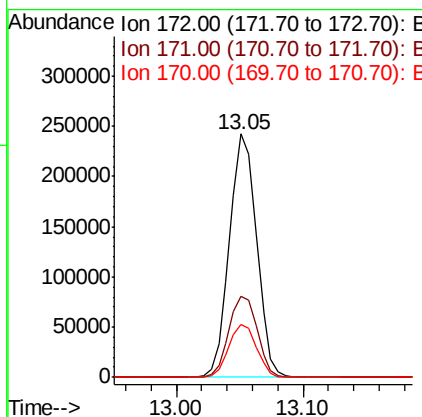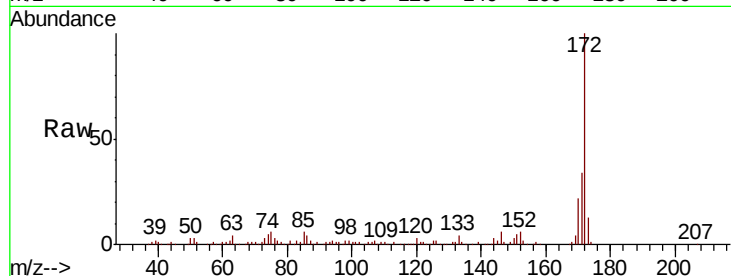

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.19 min Scan# 2414
 Delta R.T. 0.01 min
 Lab File: BM020155.D
 Acq: 07 May 2019 05:50

Tgt Ion:188 Resp: 821993
 Ion Ratio Lower Upper
 188 100
 94 8.0 5.8 8.6
 80 8.2 7.4 11.2

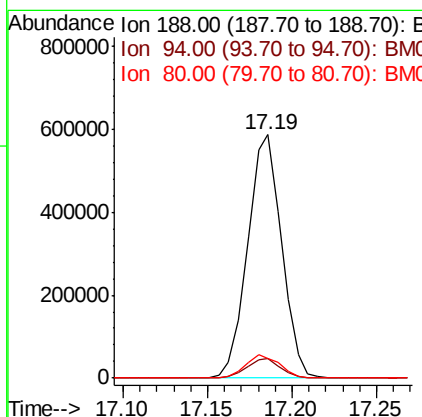


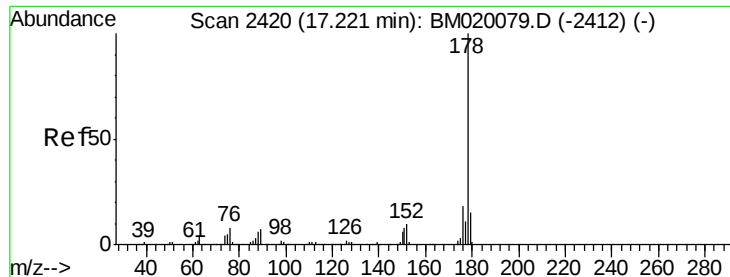




#71
Phenanthrene
Concen: 2.736 ng
RT: 17.23 min Scan# 2421
Delta R.T. 0.01 min
Lab File: BM020155.D
Acq: 07 May 2019 05:50

Instrument :
BNA_M
ClientSampleId :
SB-01-COMP

Tgt Ion:178 Resp: 124124
Ion Ratio Lower Upper
178 100
176 19.6 14.6 21.8
179 17.2 12.4 18.6

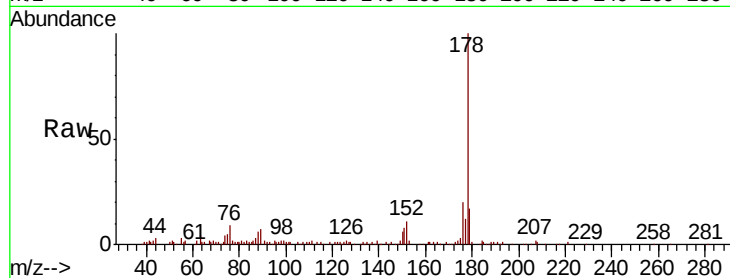


Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

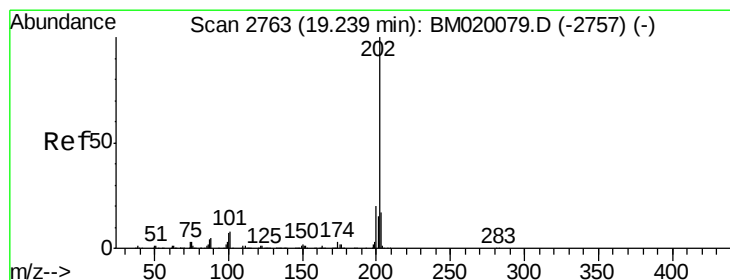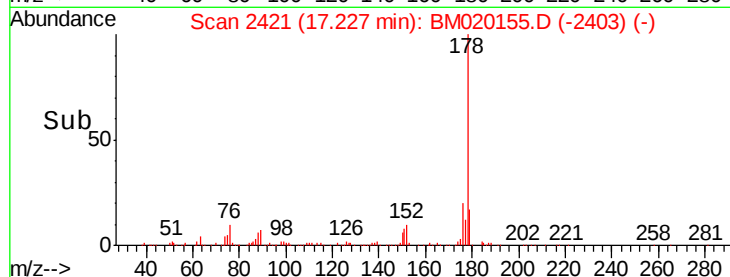
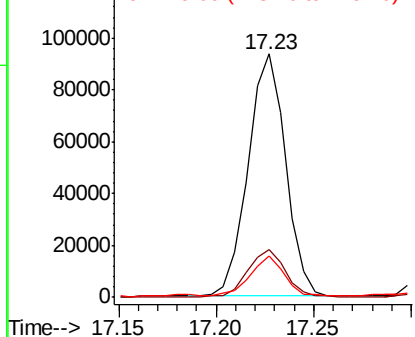



#75
Fluoranthene
Concen: 5.309 ng
RT: 19.24 min Scan# 2763
Delta R.T. -0.00 min
Lab File: BM020155.D
Acq: 07 May 2019 05:50

Tgt Ion:202 Resp: 304816
Ion Ratio Lower Upper
202 100
101 8.9 0.0 28.4
203 18.3 0.0 37.4

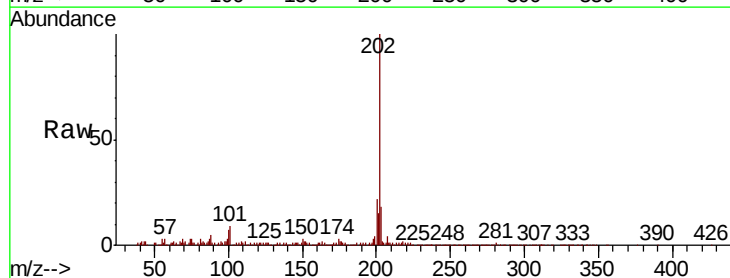

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E



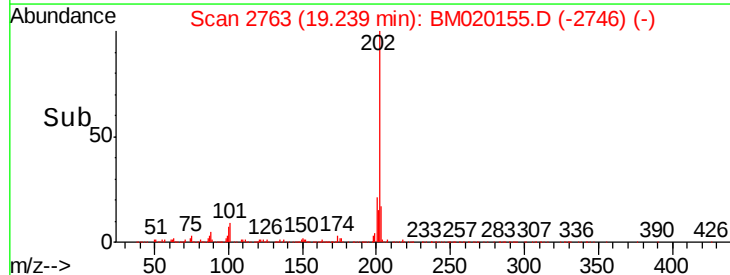
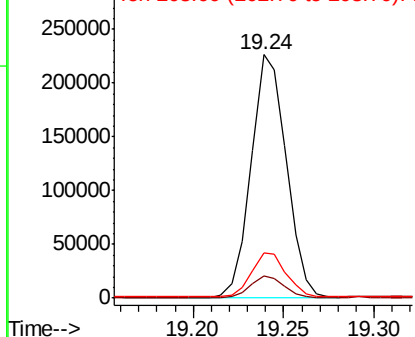


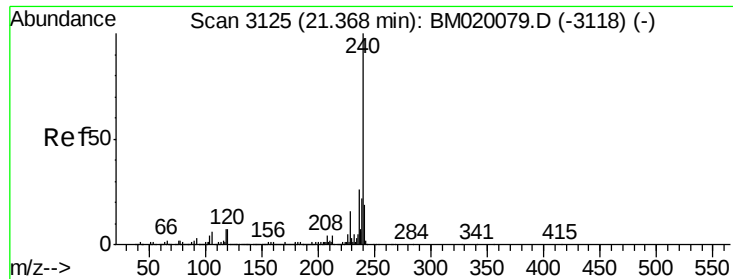

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.37 min Scan# 3125
Delta R.T. -0.00 min
Lab File: BM020155.D
Acq: 07 May 2019 05:50




Instrument :
BNA_M
ClientSampleId :
SB-01-COMP


Tgt Ion:240 Resp: 814202
Ion Ratio Lower Upper
240 100
120 7.2 5.6 8.4
236 25.7 20.9 31.3

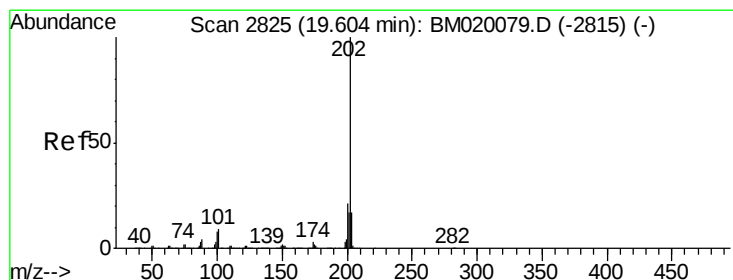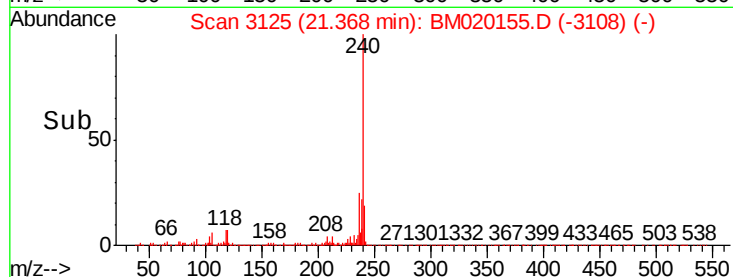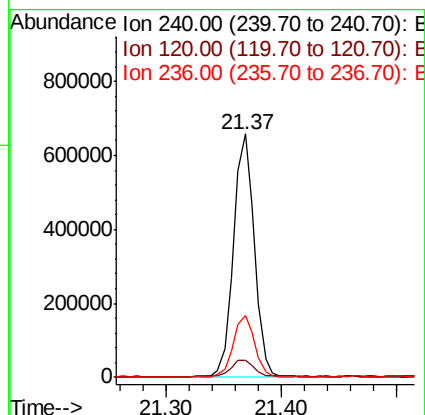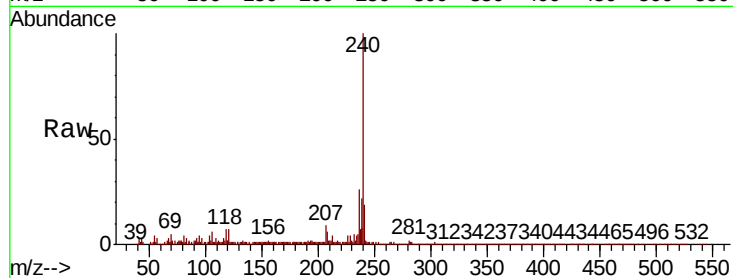

#78
Pyrene
Concen: 4.839 ng
RT: 19.61 min Scan# 2826
Delta R.T. 0.01 min
Lab File: BM020155.D
Acq: 07 May 2019 05:50

Tgt Ion:202 Resp: 264524
Ion Ratio Lower Upper
202 100
200 21.5 16.5 24.7
203 17.4 13.9 20.9

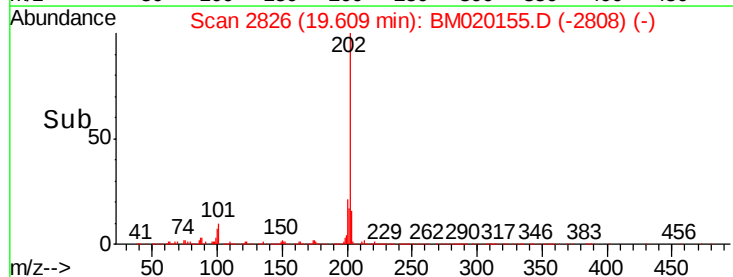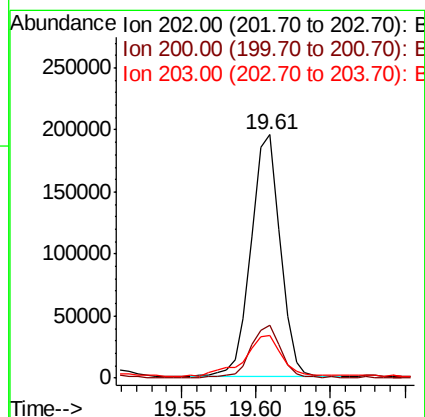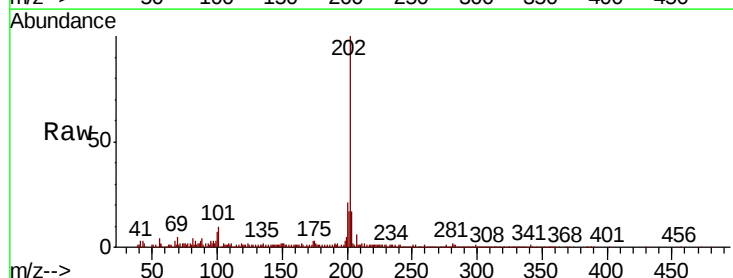

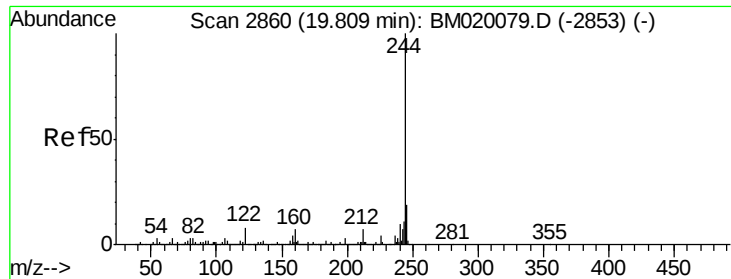

#79

Terphenyl-d14

Concen: 11.435 ng

RT: 19.80 min Scan# 2859

Delta R.T. -0.01 min

Lab File: BM020155.D

Acq: 07 May 2019 05:50

Instrument :

BNA_M

ClientSampleId :

SB-01-COMP


Tgt Ion:244 Resp: 533797

Ion Ratio Lower Upper

244 100

212 7.0 5.7 8.5




122 8.0 6.2 9.2

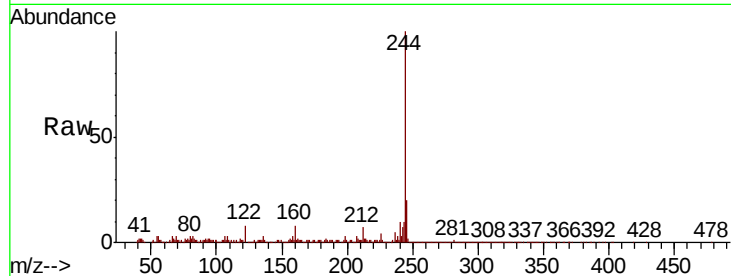

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

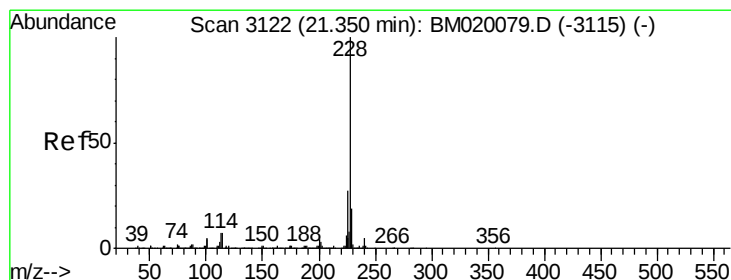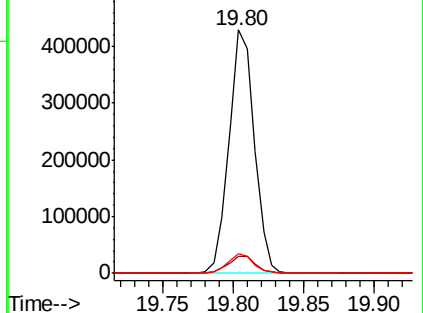

#81

Benzo(a)anthracene

Concen: 3.020 ng

RT: 21.35 min Scan# 3122

Delta R.T. -0.00 min

Lab File: BM020155.D

Acq: 07 May 2019 05:50


Tgt Ion:228 Resp: 172458

Ion Ratio Lower Upper

228 100

226 31.2 21.3 31.9



229 22.4 15.5 23.3




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E




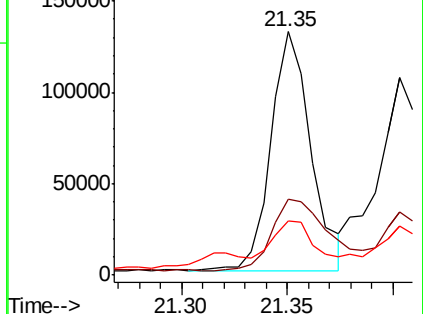


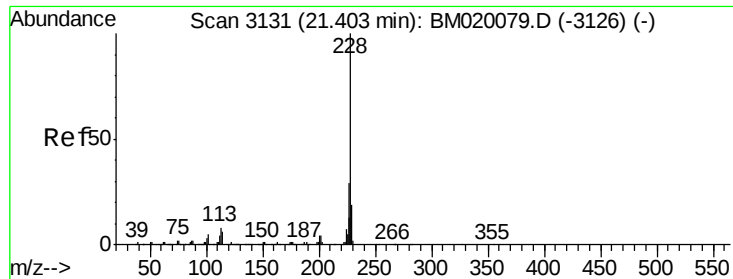

#83
Chrysene
Concen: 3.040 ng
RT: 21.35 min Scan# 3122
Delta R.T. -0.05 min
Lab File: BM020155.D
Acq: 07 May 2019 05:50




Instrument :
BNA_M
ClientSampleId :
SB-01-COMP


Tgt Ion:228 Resp: 168373
Ion Ratio Lower Upper
228 100
226 31.2 23.0 34.6
229 22.4 15.5 23.3

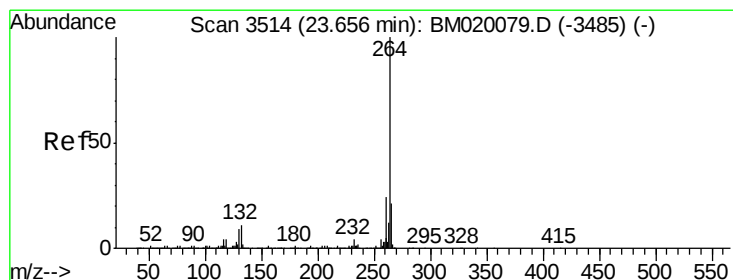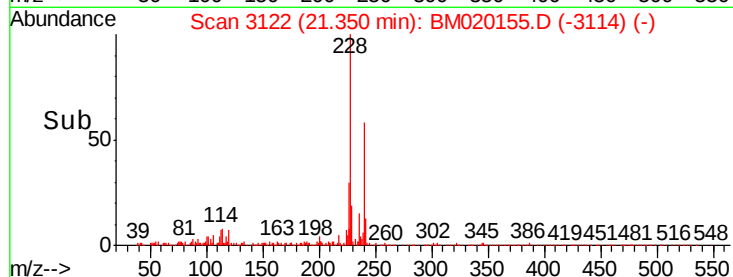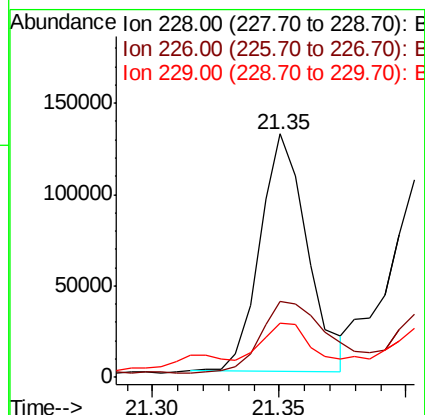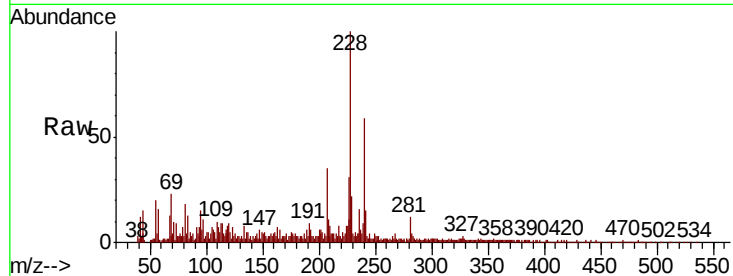

#87
Perylene-d12
Concen: 20.000 ng
RT: 23.67 min Scan# 3516
Delta R.T. 0.01 min
Lab File: BM020155.D
Acq: 07 May 2019 05:50

Tgt Ion:264 Resp: 952401
Ion Ratio Lower Upper
264 100
260 23.0 19.2 28.8
265 22.8 16.9 25.3

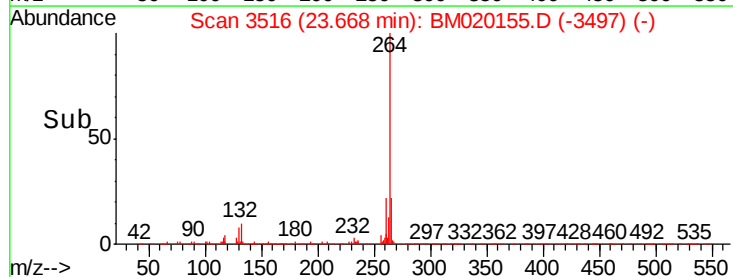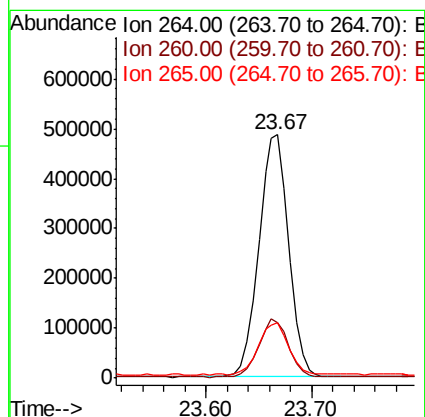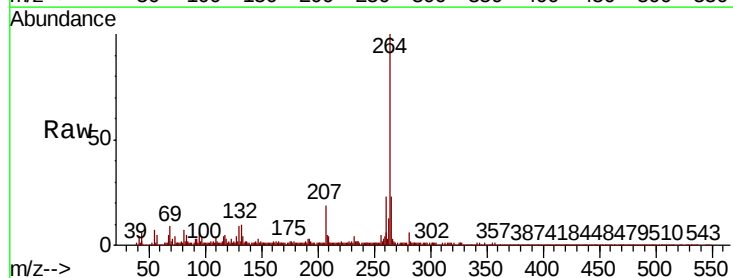

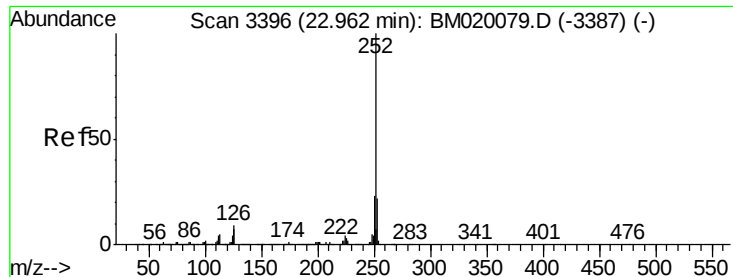

#88

Benzo(b)fluoranthene

Concen: 3.810 ng

RT: 22.97 min Scan# 3397

Delta R.T. 0.01 min

Lab File: BM020155.D

Acq: 07 May 2019 05:50

Instrument :

BNA_M

ClientSampleId :

SB-01-COMP


Tgt Ion:252 Resp: 239606

Ion Ratio Lower Upper

252 100

253 27.0 17.5 26.3#




125 14.4 5.4 8.2#

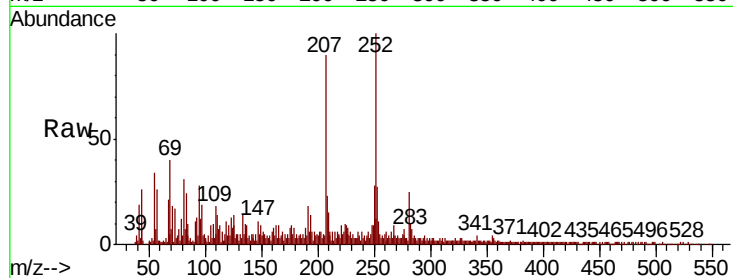

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

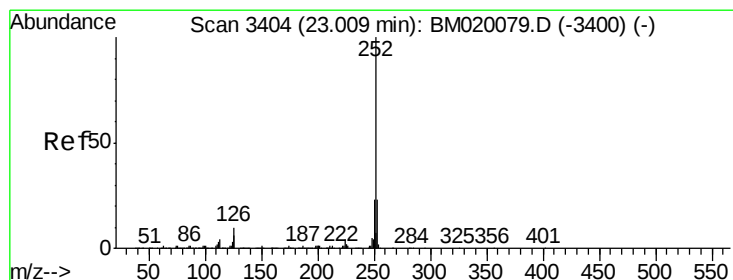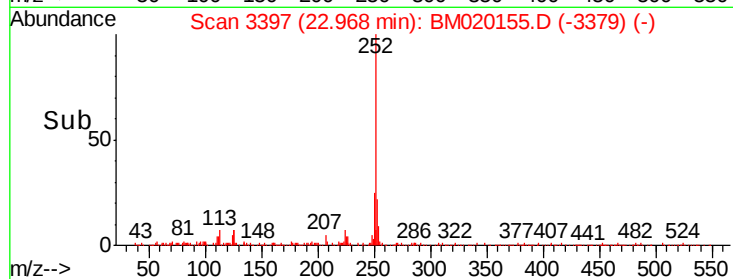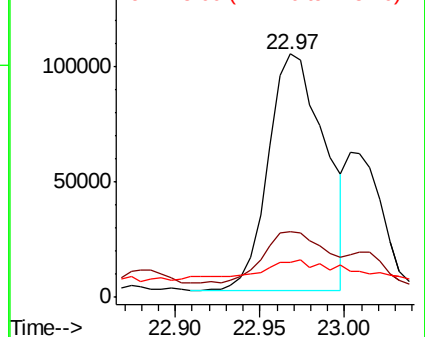

#89

Benzo(k)fluoranthene

Concen: 3.983 ng

RT: 22.97 min Scan# 3397

Delta R.T. -0.04 min

Lab File: BM020155.D

Acq: 07 May 2019 05:50


Tgt Ion:252 Resp: 228476

Ion Ratio Lower Upper

252 100

253 27.0 17.8 26.8#



125 14.4 5.4 8.0#

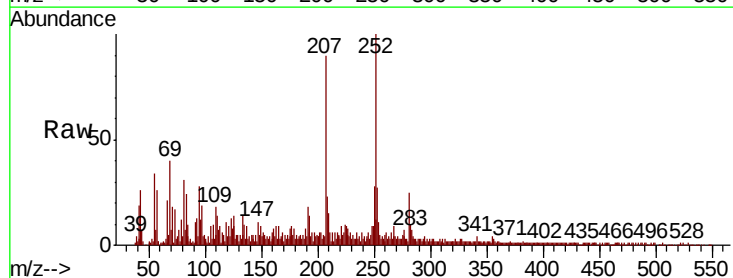


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

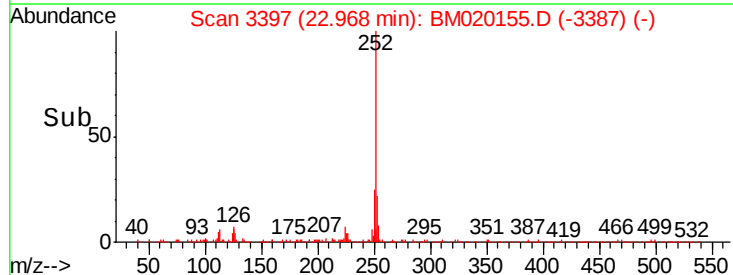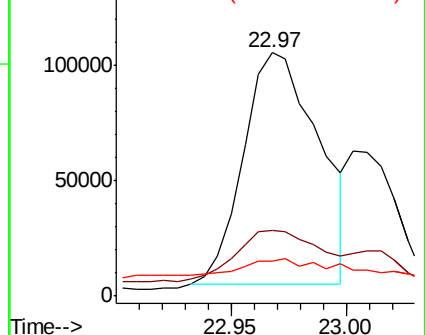



#90

Benzo(a)pyrene

Concen: 3.072 ng

RT: 23.56 min Scan# 3498

Delta R.T. 0.01 min

Lab File: BM020155.D

Acq: 07 May 2019 05:50

Instrument :

BNA_M

ClientSampleId :

SB-01-COMP


Tgt Ion:252 Resp: 175478

Ion Ratio Lower Upper

252 100

253 27.5 17.0 25.6#




125 13.9 5.5 8.3#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

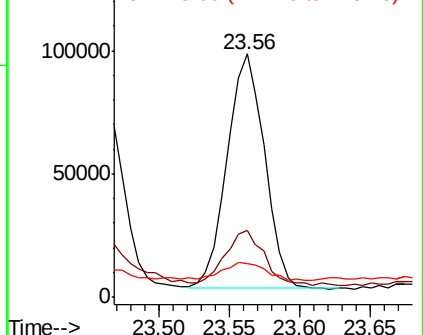

#92

Benzo(g,h,i)perylene

Concen: 2.430 ng

RT: 26.73 min Scan# 4036

Delta R.T. 0.02 min

Lab File: BM020155.D

Acq: 07 May 2019 05:50


Tgt Ion:276 Resp: 137043

Ion Ratio Lower Upper

276 100

277 29.0 18.4 27.6#

138 18.2 11.1 16.7#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

