

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050619\
 Data File : BM020133.D
 Acq On : 06 May 2019 13:36
 Operator : JU/SJ
 Sample : PB119435BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB119435BL

Quant Time: May 07 03:29:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 03:58:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	97725	20.00	ng	0.00
21) Naphthalene-d8	10.57	136	339876	20.00	ng	-0.01
39) Acenaphthene-d10	14.43	164	204640	20.00	ng	0.00
64) Phenanthrene-d10	17.17	188	496450	20.00	ng	0.00
76) Chrysene-d12	21.36	240	517542	20.00	ng	-0.01
87) Perylene-d12	23.64	264	600277	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.36	112	927051	155.06	ng	0.00
7) Phenol-d6	6.95	99	1276339	156.27	ng	0.00
23) Nitrobenzene-d5	8.95	82	902611	104.85	ng	0.00
42) 2,4,6-Tribromophenol	15.92	330	532601	167.67	ng	0.00
45) 2-Fluorobiphenyl	13.05	172	1784448	107.29	ng	-0.01
79) Terphenyl-d14	19.80	244	3182051	107.24	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050619\
Data File : BM020133.D
Acq On : 06 May 2019 13:36
Operator : JU/SJ
Sample : PB119435BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119435BL

Quant Time: May 07 03:29:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:58:37 2019
Response via : Initial Calibration

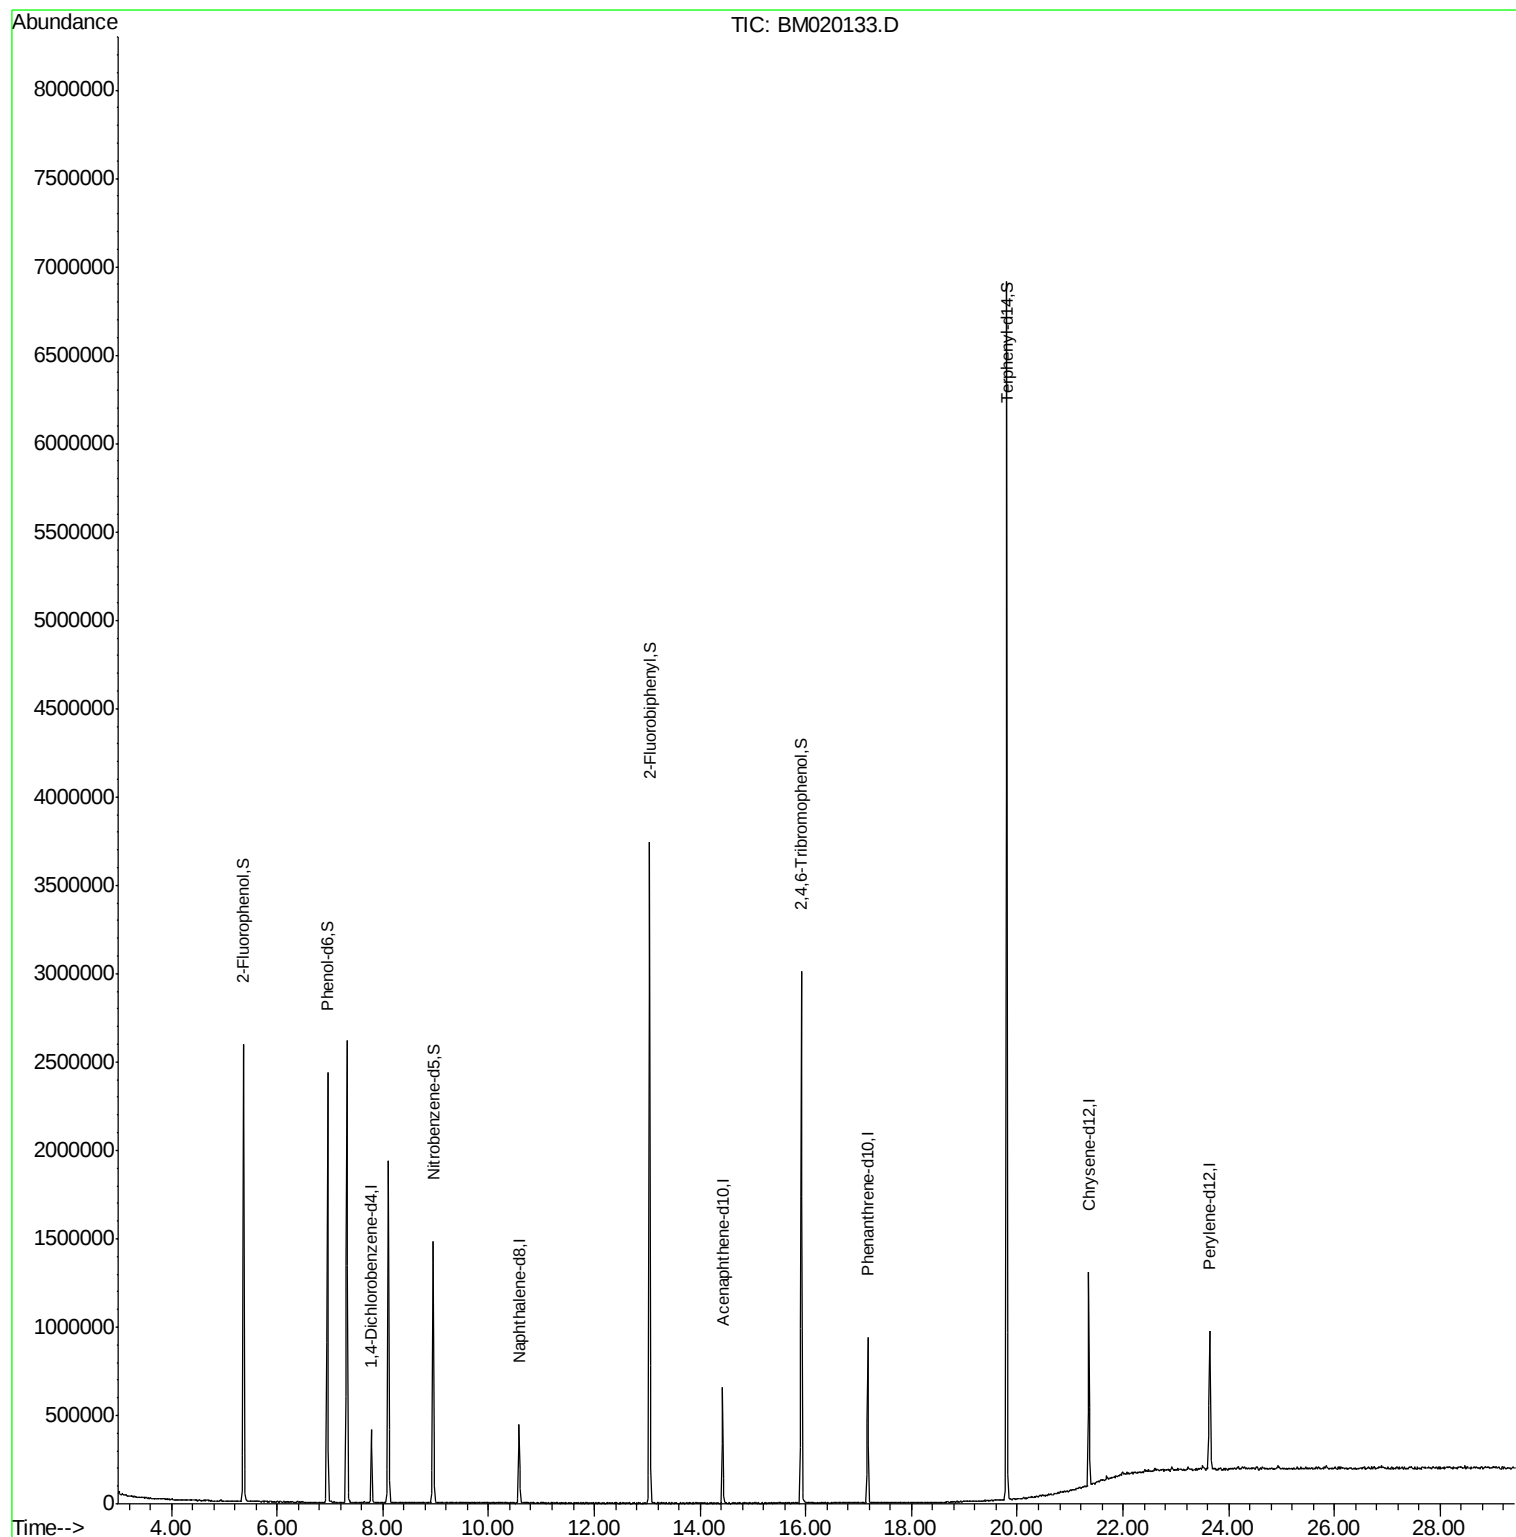

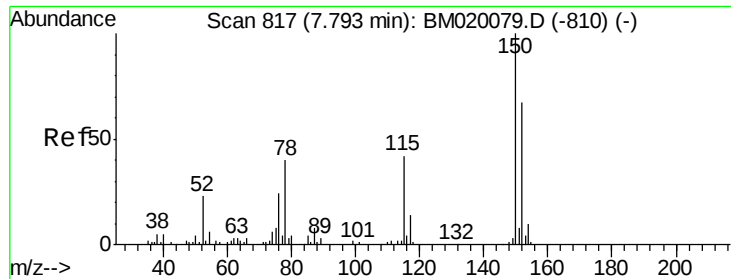


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.79 min Scan# 816
Delta R.T. -0.01 min
Lab File: BM020133.D
Acq: 06 May 2019 13:36

Instrument :
BNA_M
ClientSampleId :
PB119435BL

Tot Ion:152 Resp: 97725
Ion Ratio Lower Upper
152 100
150 159.9 119.8 179.8
115 64.3 50.8 76.2

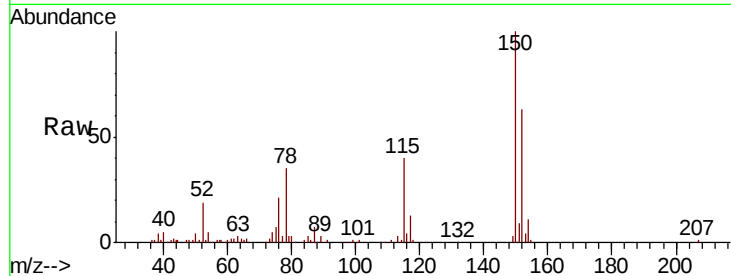


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

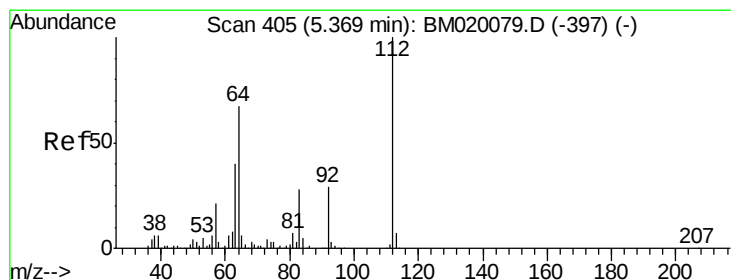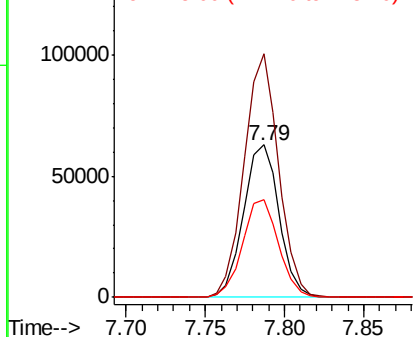



#5


2-Fluorophenol
Concen: 155.063 ng
RT: 5.36 min Scan# 404
Delta R.T. -0.01 min
Lab File: BM020133.D
Acq: 06 May 2019 13:36

Tgt Ion:112 Resp: 927051
Ion Ratio Lower Upper
112 100
64 67.9 53.8 80.6
63 38.8 32.3 48.5

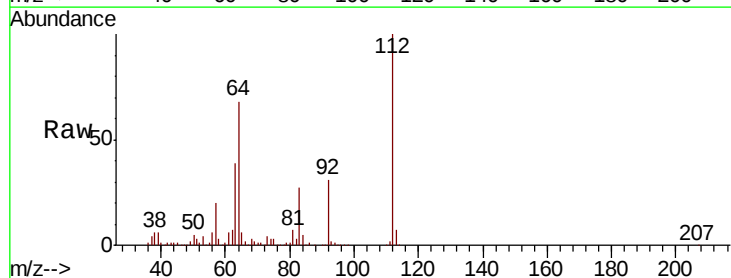

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

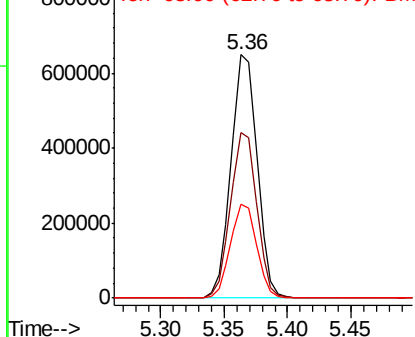

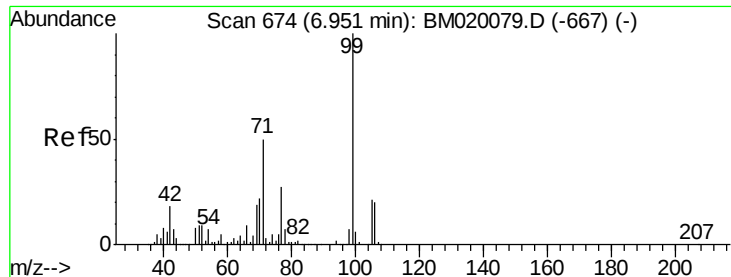

#7

Phenol-d6

Concen: 156.270 ng

RT: 6.95 min Scan# 674

Delta R.T. 0.00 min

Lab File: BM020133.D

Acq: 06 May 2019 13:36

Instrument :

BNA_M

ClientSampleId :

PB119435BL


Tot Ion: 99 Resp: 1276339

Ion Ratio Lower Upper

99 100

42 15.4 14.2 21.2




71 47.9 40.3 60.5

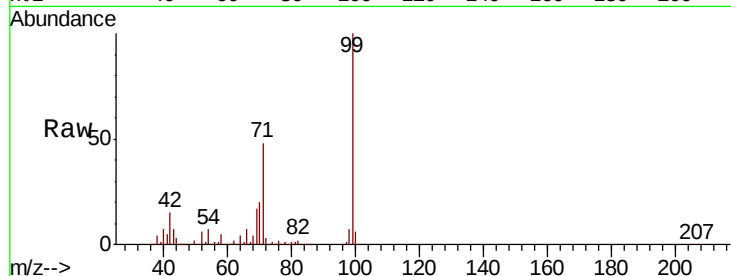

Abundance Ion 99.00 (98.70 to 99.70): BM020133.D (-657) (-)

Ion 42.00 (41.70 to 42.70): BM020133.D (-657) (-)

Ion 71.00 (70.70 to 71.70): BM020133.D (-657) (-)

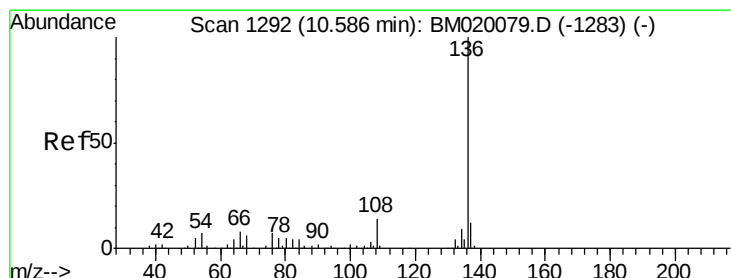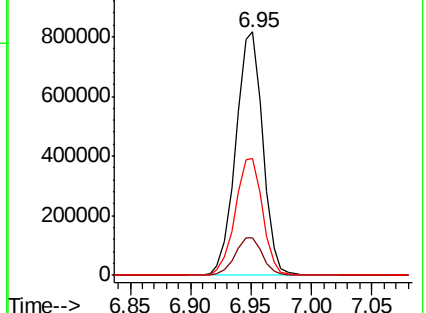

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.57 min Scan# 1290

Delta R.T. -0.01 min

Lab File: BM020133.D

Acq: 06 May 2019 13:36

Tgt Ion: 136 Resp: 339876


Ion Ratio Lower Upper

136 100

137 10.0 9.6 14.4

54 6.4 5.5 8.3

68 6.3 4.6 6.8


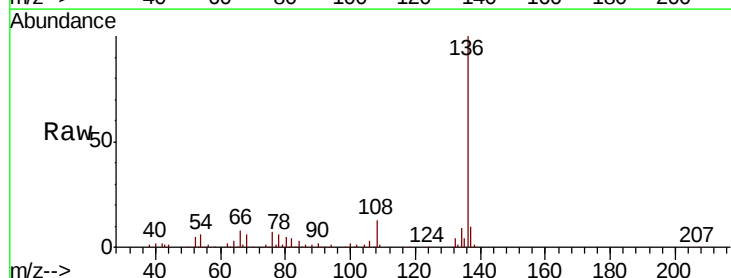


Abundance Ion 136.00 (135.70 to 136.70): BM020133.D (-1275) (-)

Ion 137.00 (136.70 to 137.70): BM020133.D (-1275) (-)

Ion 54.00 (53.70 to 54.70): BM020133.D (-1275) (-)

Ion 68.00 (67.70 to 68.70): BM020133.D (-1275) (-)



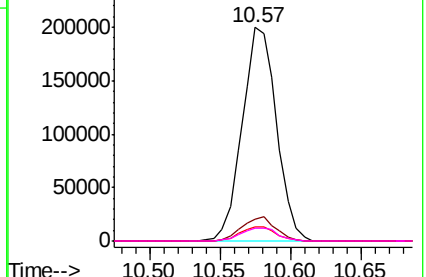





#23
Nitrobenzene-d5
Concen: 104.848 ng
RT: 8.95 min Scan# 1014
Delta R.T. -0.01 min
Lab File: BM020133.D
Acq: 06 May 2019 13:36




Instrument :
BNA_M
ClientSampleId :
PB119435BL


Tot Ion	82	Resp	902611
Ion Ratio	100	Lower	Upper
128	31.9	25.2	37.8
54	38.3	31.9	47.9

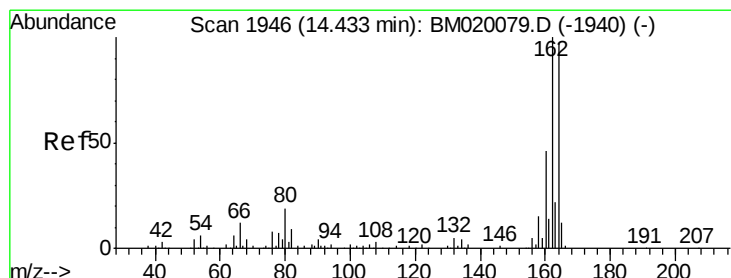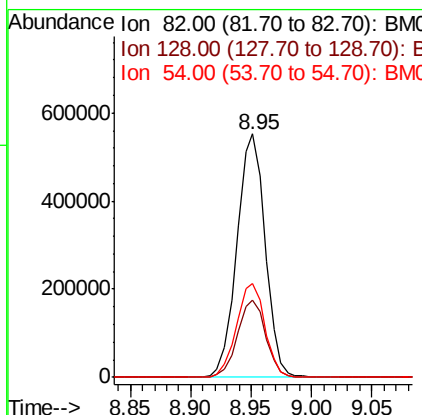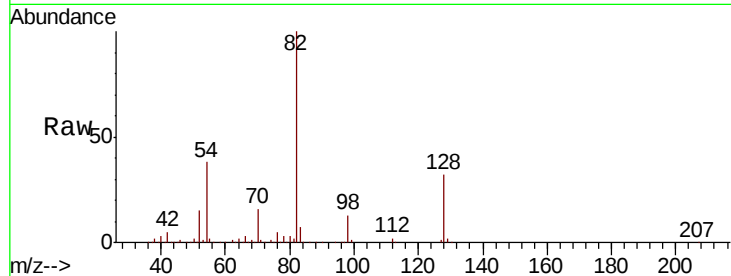

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.43 min Scan# 1945
Delta R.T. -0.01 min
Lab File: BM020133.D
Acq: 06 May 2019 13:36

Tgt Ion	164	Resp	204640
Ion Ratio	100	Lower	Upper
162	101.2	82.2	123.2
160	45.0	37.6	56.4

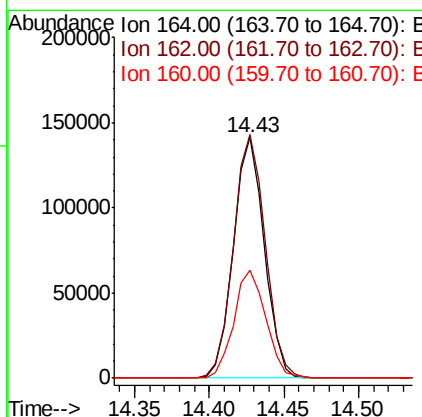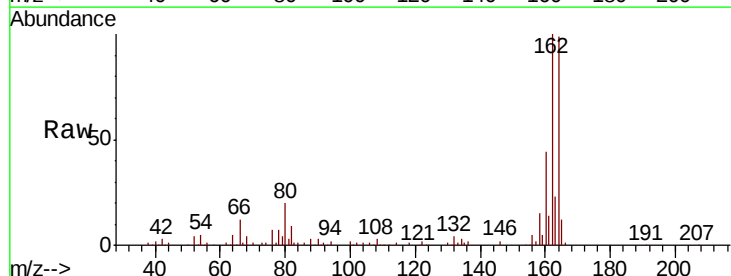


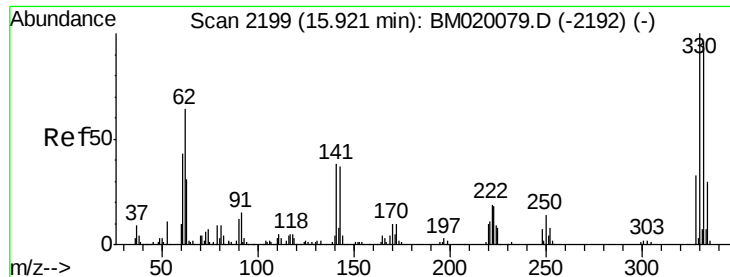

#42
 2,4,6-Tribromophenol
 Concen: 167.674 ng
 RT: 15.92 min Scan# 2199
 Delta R.T. 0.00 min
 Lab File: BM020133.D
 Acq: 06 May 2019 13:36

Instrument :
 BNA_M
 ClientSampleId :
 PB119435BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.7	76.8	115.2
141	33.7	29.2	43.8


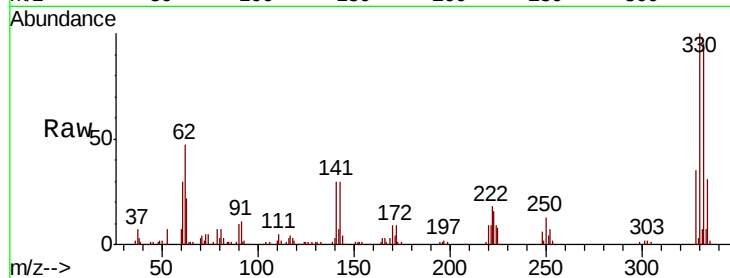


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

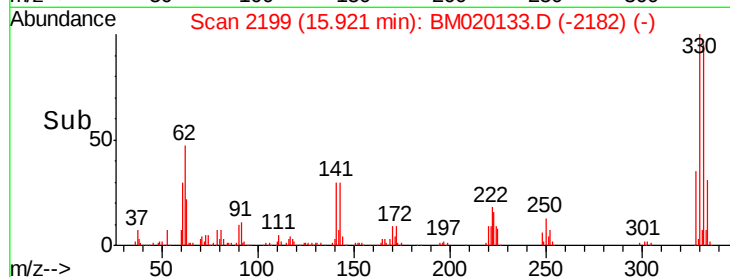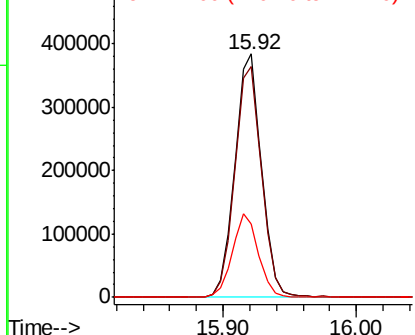

#45
 2-Fluorobiphenyl
 Concen: 107.287 ng
 RT: 13.05 min Scan# 1710
 Delta R.T. -0.01 min
 Lab File: BM020133.D
 Acq: 06 May 2019 13:36

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.7	27.3	40.9
170	23.1	17.9	26.9


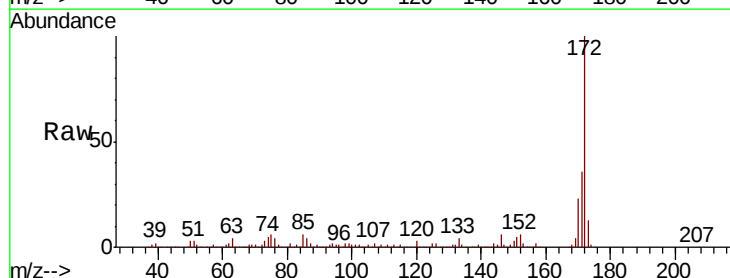



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

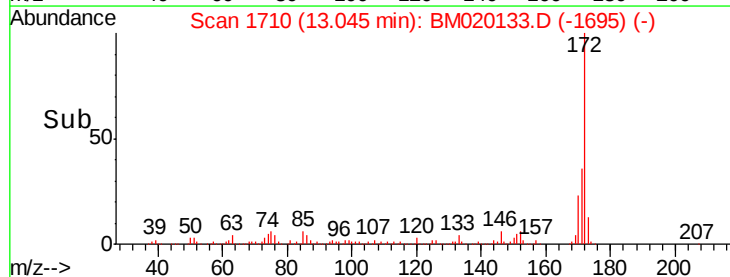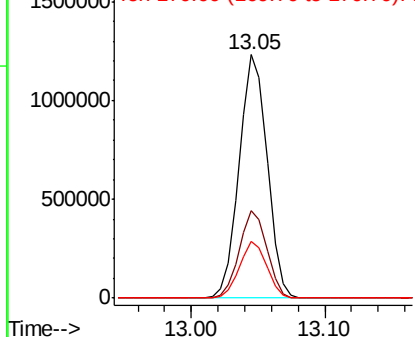


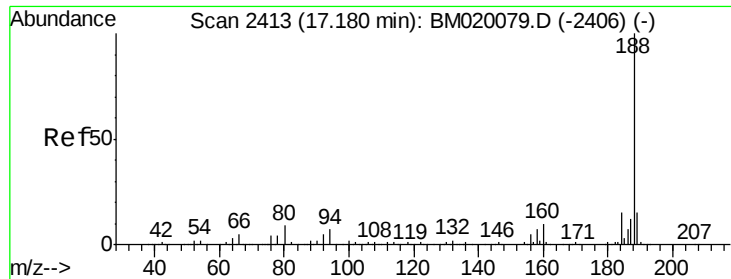




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.17 min Scan# 2412
Delta R.T. -0.01 min
Lab File: BM020133.D
Acq: 06 May 2019 13:36

Instrument :
BNA_M
ClientSampleId :
PB119435BL

Tot Ion:188 Resp: 496450
Ion Ratio Lower Upper
188 100
94 6.9 5.8 8.6
80 8.8 7.4 11.2

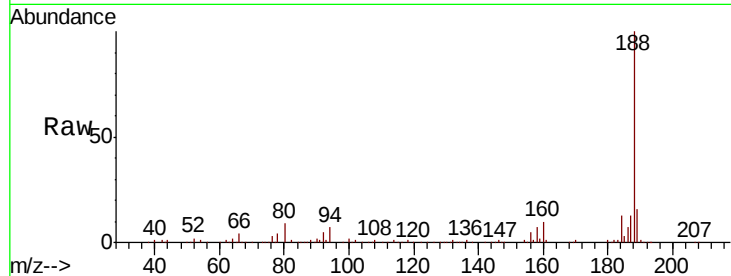


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM

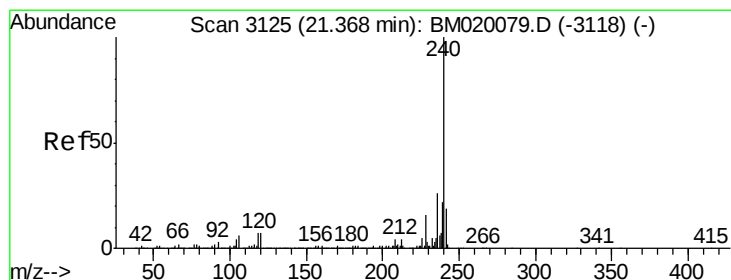
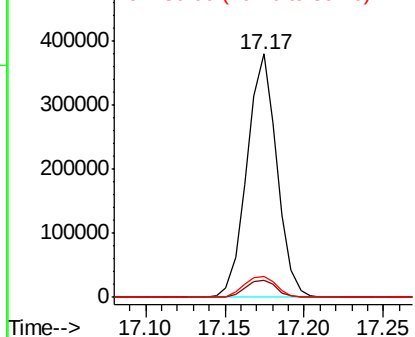



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.36 min Scan# 3123
Delta R.T. -0.01 min
Lab File: BM020133.D
Acq: 06 May 2019 13:36

Tgt Ion:240 Resp: 517542
Ion Ratio Lower Upper
240 100
120 7.1 5.6 8.4
236 26.7 20.9 31.3

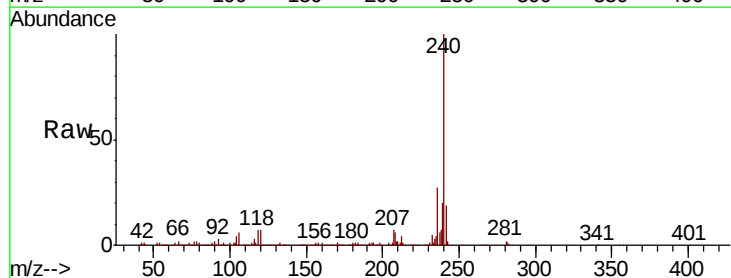

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

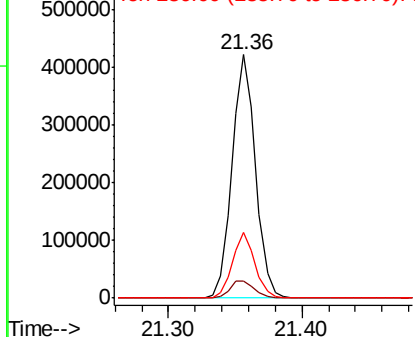

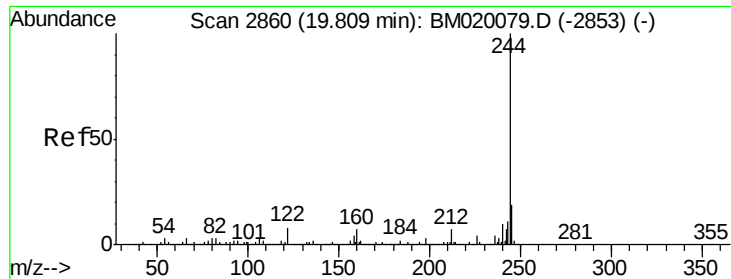

#79

Terphenyl-d14

Concen: 107.241 ng

RT: 19.80 min Scan# 2858

Delta R.T. -0.01 min

Lab File: BM020133.D

Acq: 06 May 2019 13:36

Instrument :

BNA_M

ClientSampleId :

PB119435BL


Tot Ion:244 Resp: 3182051

Ion Ratio Lower Upper




244 100

212 6.9 5.7 8.5

122 7.9 6.2 9.2

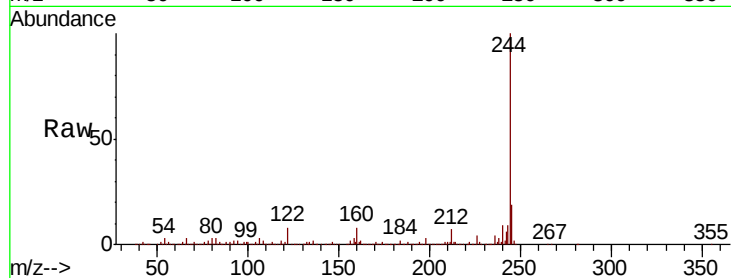

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

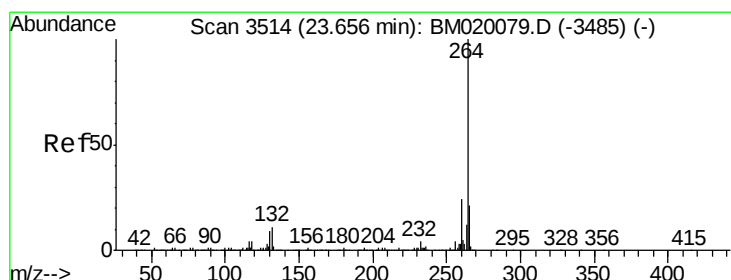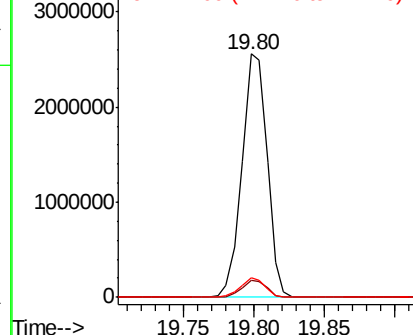

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.64 min Scan# 3512

Delta R.T. -0.01 min

Lab File: BM020133.D

Acq: 06 May 2019 13:36


Tgt Ion:264 Resp: 600277

Ion Ratio Lower Upper

264 100

260 24.4 19.2 28.8

265 22.4 16.9 25.3

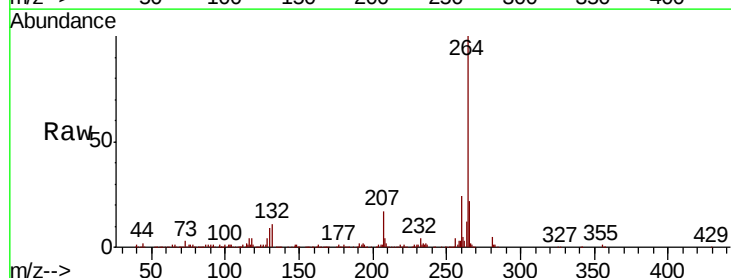

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

