

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050619\
 Data File : BM020139.D
 Acq On : 06 May 2019 17:13
 Operator : JU/SJ
 Sample : K2639-03 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 NB-08-050319-B

Quant Time: May 07 05:09:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 03:58:37 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	132796	20.00	ng	0.00
21) Naphthalene-d8	10.59	136	507580	20.00	ng	0.00
39) Acenaphthene-d10	14.43	164	309006	20.00	ng	0.00
64) Phenanthrene-d10	17.18	188	741429	20.00	ng	0.00
76) Chrysene-d12	21.37	240	735417	20.00	ng	0.00
87) Perylene-d12	23.66	264	870794	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	324413	39.93	ng	0.00
7) Phenol-d6	6.96	99	472816	42.60	ng	0.00
23) Nitrobenzene-d5	8.96	82	317112	24.67	ng	0.00
42) 2,4,6-Tribromophenol	15.93	330	199399	41.57	ng	0.00
45) 2-Fluorobiphenyl	13.05	172	610731	24.32	ng	0.00
79) Terphenyl-d14	19.81	244	1006586	23.87	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.89	163	56075	2.135	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050619\
Data File : BM020139.D
Acq On : 06 May 2019 17:13
Operator : JU/SJ
Sample : K2639-03 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
NB-08-050319-B

Quant Time: May 07 05:09:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:58:37 2019
Response via : Initial Calibration

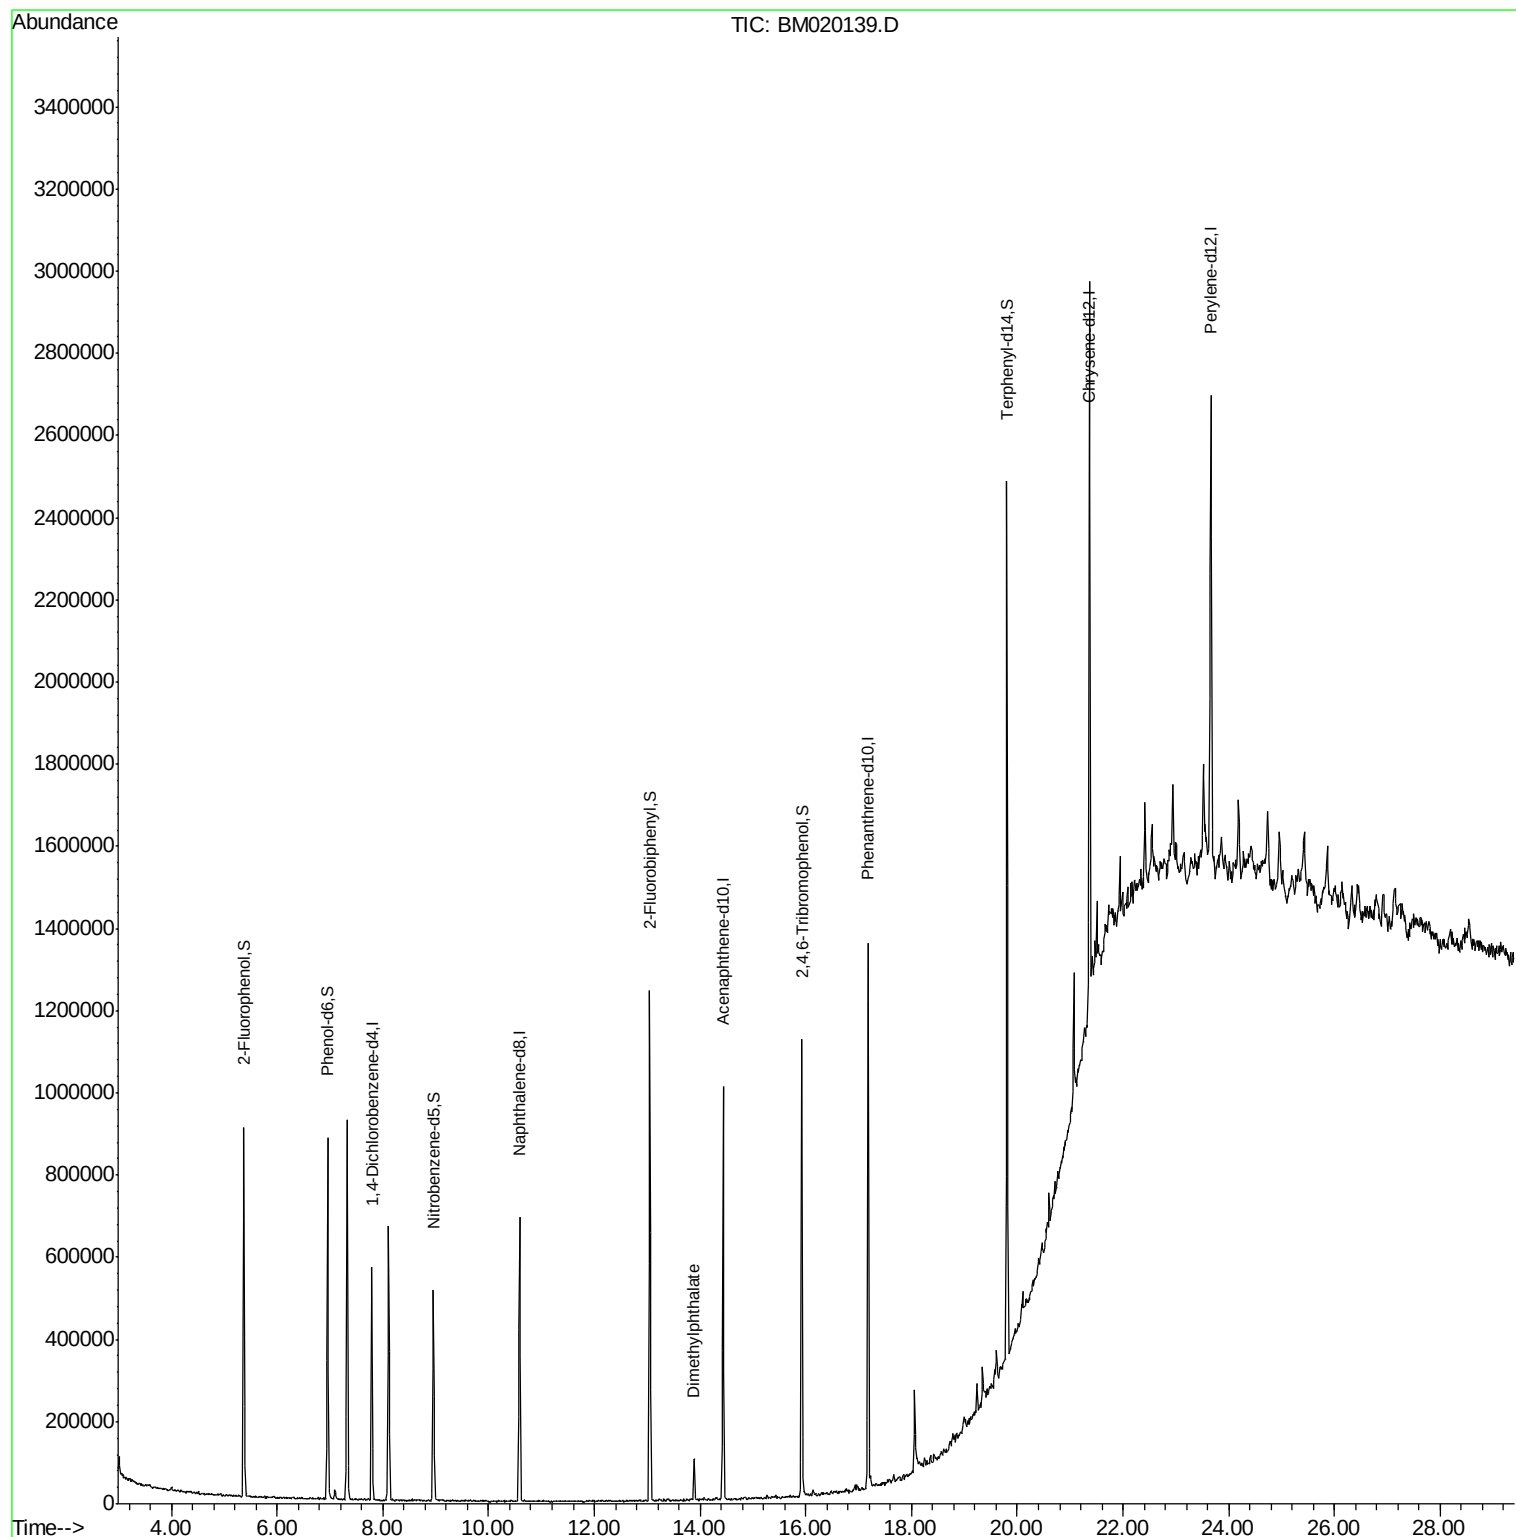

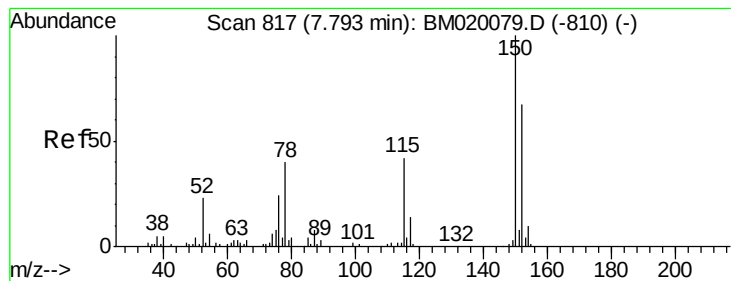


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.79 min Scan# 817
Delta R.T. -0.00 min
Lab File: BM020139.D
Acq: 06 May 2019 17:13

Instrument :
BNA_M
ClientSampled :
NB-08-050319-B

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.4	119.8	179.8
115	61.6	50.8	76.2



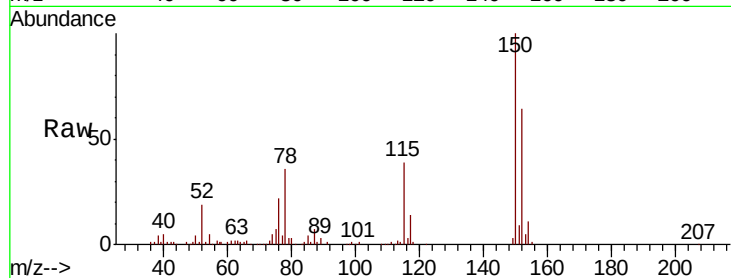


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

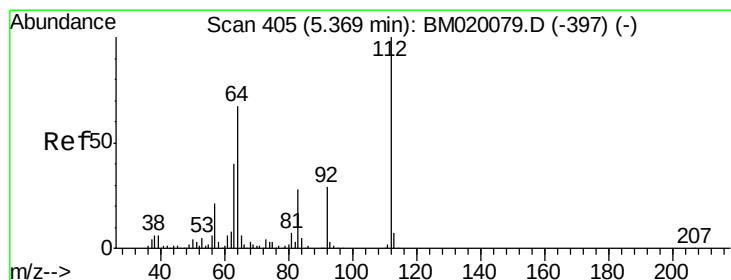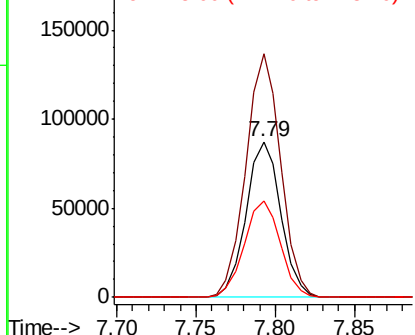

#5

2-Fluorophenol
Concen: 39.932 ng
RT: 5.37 min Scan# 405
Delta R.T. -0.00 min
Lab File: BM020139.D
Acq: 06 May 2019 17:13

Tgt Ion	Ratio	Lower	Upper
112	100		
64	69.3	53.8	80.6
63	41.0	32.3	48.5


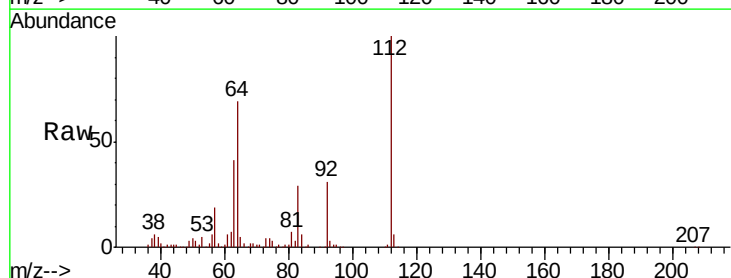



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

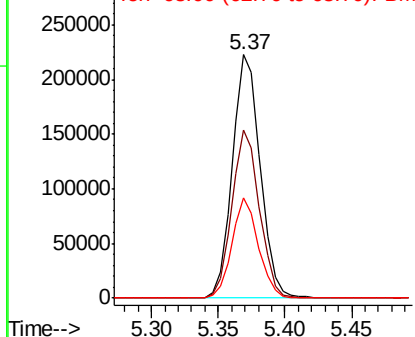



#7

Phenol-d6

Concen: 42.601 ng

RT: 6.96 min Scan# 675

Delta R.T. 0.01 min

Lab File: BM020139.D

Acq: 06 May 2019 17:13

Instrument :

BNA_M

ClientSampleId :

NB-08-050319-B


Tot Ion: 99 Resp: 472816

Ion Ratio Lower Upper

99 100

42 13.9 14.2 21.2#




71 46.7 40.3 60.5

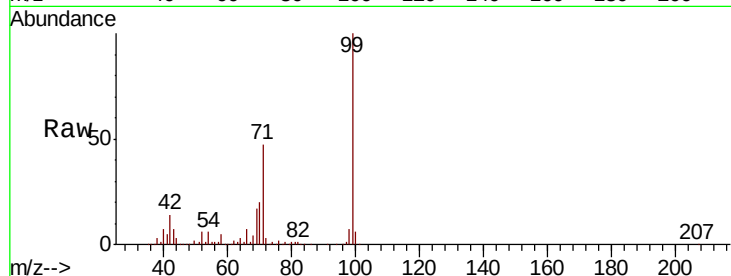

Abundance Ion 99.00 (98.70 to 99.70): BM020139.D (-667) (-)

Ion 42.00 (41.70 to 42.70): BM020139.D (-667) (-)

Ion 71.00 (70.70 to 71.70): BM020139.D (-667) (-)

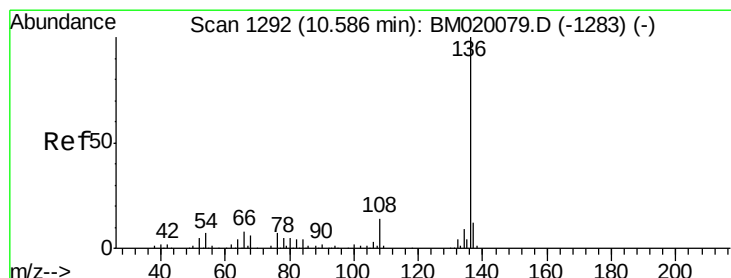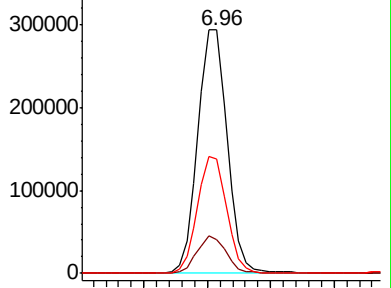

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.59 min Scan# 1292

Delta R.T. -0.00 min

Lab File: BM020139.D

Acq: 06 May 2019 17:13

Tgt Ion: 136 Resp: 507580


Ion Ratio Lower Upper

136 100

137 10.2 9.6 14.4

54 6.5 5.5 8.3

68 6.4 4.6 6.8


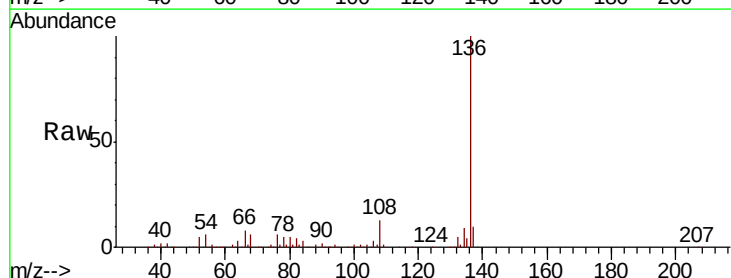



Abundance Ion 136.00 (135.70 to 136.70): BM020139.D (-1283) (-)

Ion 137.00 (136.70 to 137.70): BM020139.D (-1283) (-)

Ion 54.00 (53.70 to 54.70): BM020139.D (-1283) (-)

Ion 68.00 (67.70 to 68.70): BM020139.D (-1283) (-)




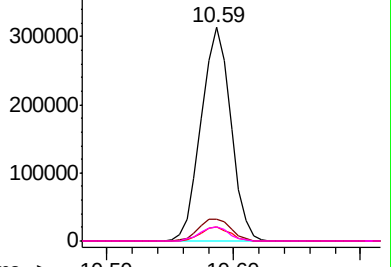




#23
 Nitrobenzene-d5
 Concen: 24.665 ng
 RT: 8.96 min Scan# 1015
 Delta R.T. -0.00 min
 Lab File: BM020139.D
 Acq: 06 May 2019 17:13




Instrument :
 BNA_M
 ClientSampleId :
 NB-08-050319-B


Tot Ion	Ratio	Lower	Upper
82	100		
128	33.9	25.2	37.8
54	39.6	31.9	47.9

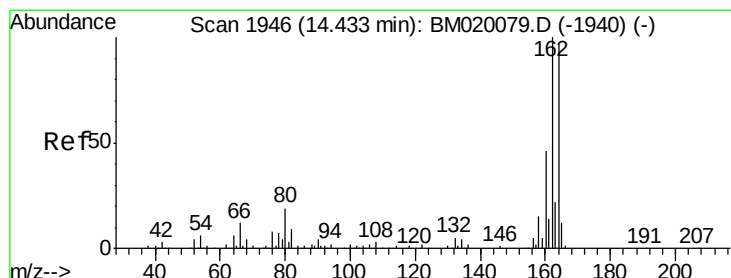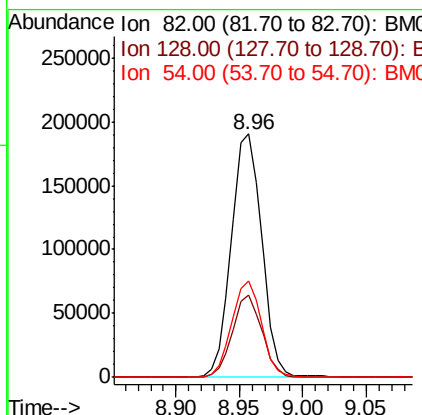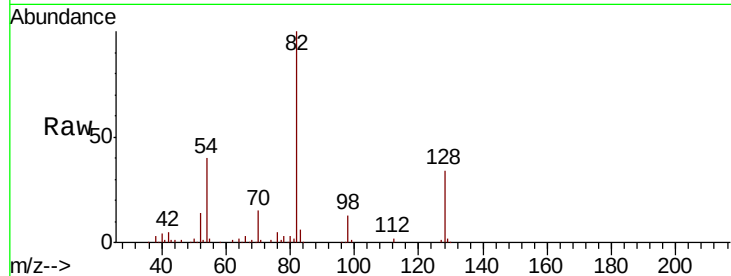

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.43 min Scan# 1946
 Delta R.T. -0.00 min
 Lab File: BM020139.D
 Acq: 06 May 2019 17:13

Tgt Ion	Ratio	Lower	Upper
164	100		
162	106.7	82.2	123.2
160	47.9	37.6	56.4

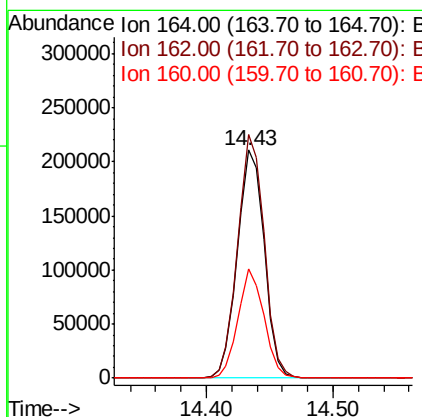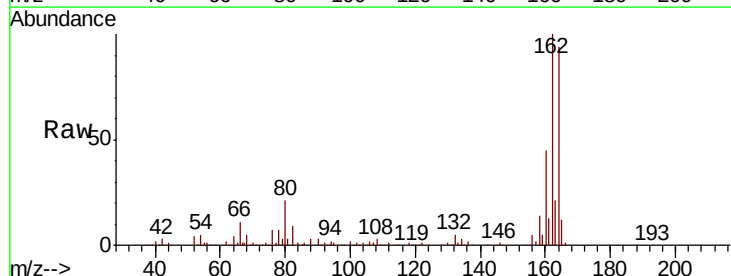


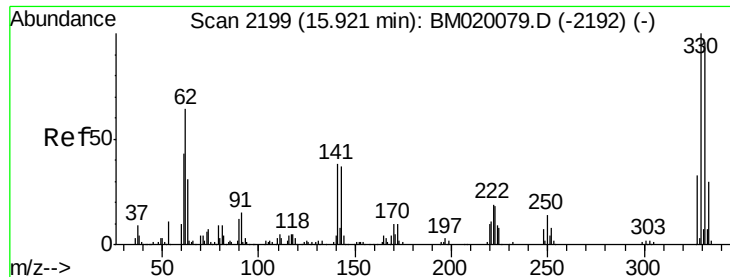

#42
 2,4,6-Tribromophenol
 Concen: 41.573 ng
 RT: 15.93 min Scan# 2200
 Delta R.T. 0.01 min
 Lab File: BM020139.D
 Acq: 06 May 2019 17:13

Instrument :
 BNA_M
 ClientSampleId :
 NB-08-050319-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.6	76.8	115.2
141	34.3	29.2	43.8



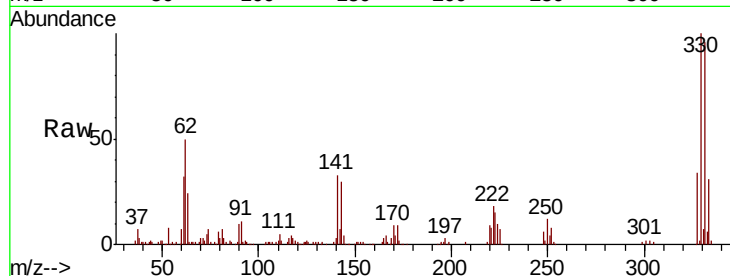


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

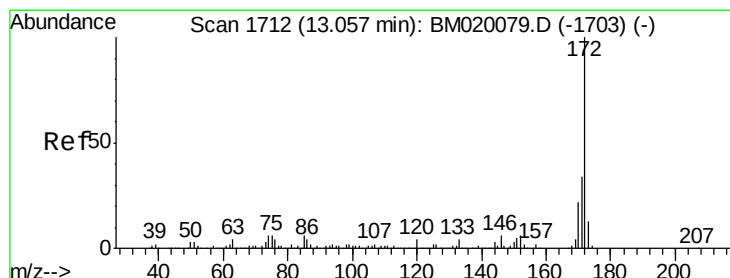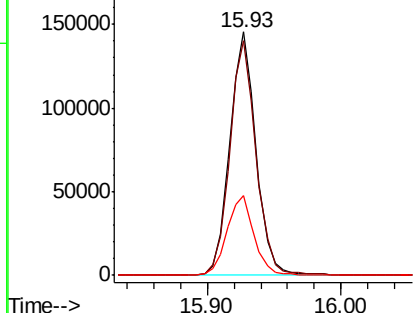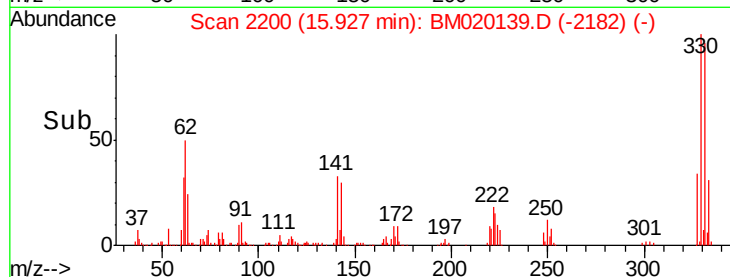

#45
 2-Fluorobiphenyl
 Concen: 24.317 ng
 RT: 13.05 min Scan# 1711
 Delta R.T. -0.01 min
 Lab File: BM020139.D
 Acq: 06 May 2019 17:13

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.3	27.3	40.9
170	23.4	17.9	26.9


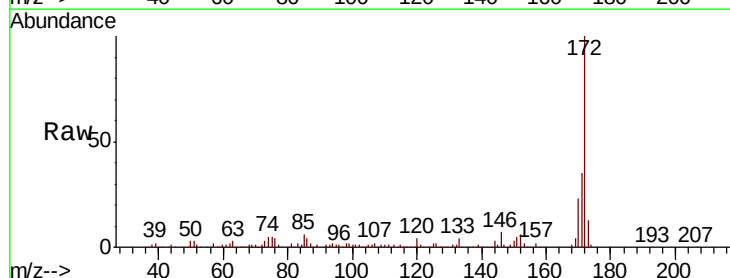



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

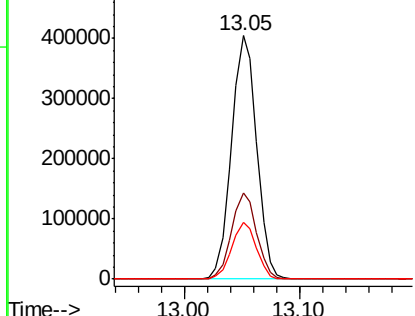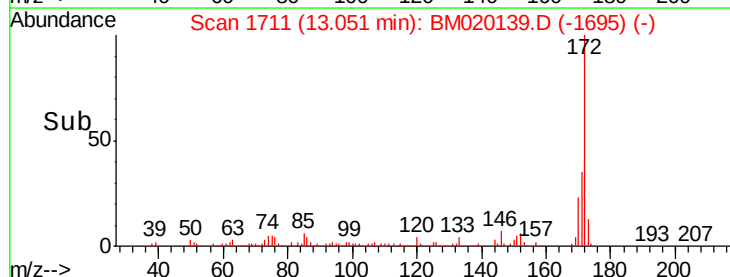



#50

Dimethylphthalate

Concen: 2.135 ng

RT: 13.89 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BM020139.D

Acq: 06 May 2019 17:13

Instrument :

BNA_M

ClientSampleId :

NB-08-050319-B


Tot Ion:163 Resp: 56075

Ion Ratio Lower Upper

163 100

194 4.7 3.6 5.4




164 11.5 8.4 12.6

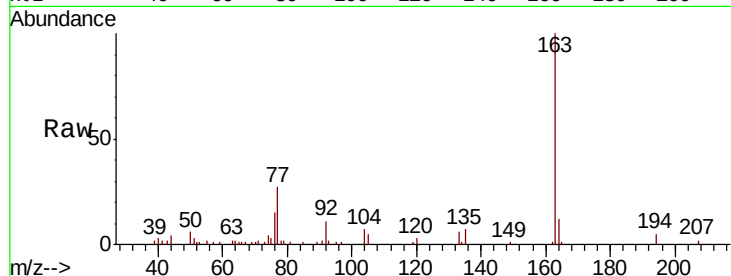

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

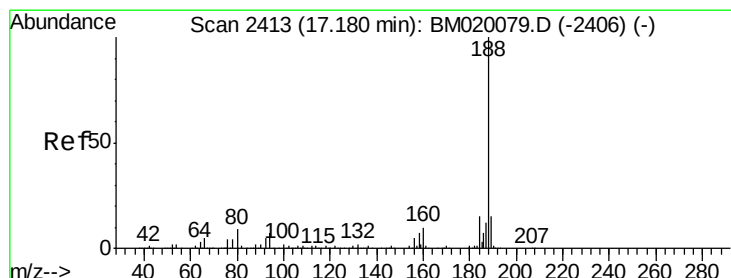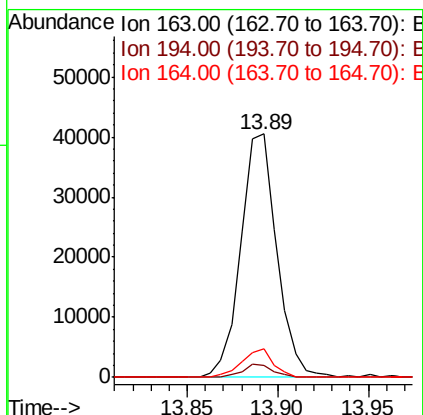

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.18 min Scan# 2413

Delta R.T. -0.00 min

Lab File: BM020139.D

Acq: 06 May 2019 17:13


Tgt Ion:188 Resp: 741429

Ion Ratio Lower Upper

188 100

94 7.5 5.8 8.6



80 9.9 7.4 11.2

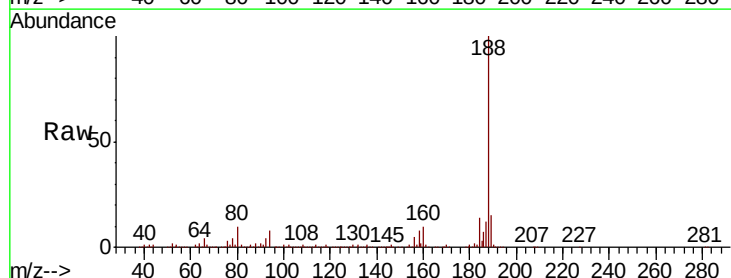


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

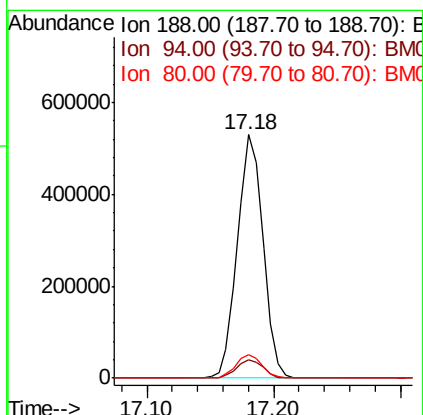

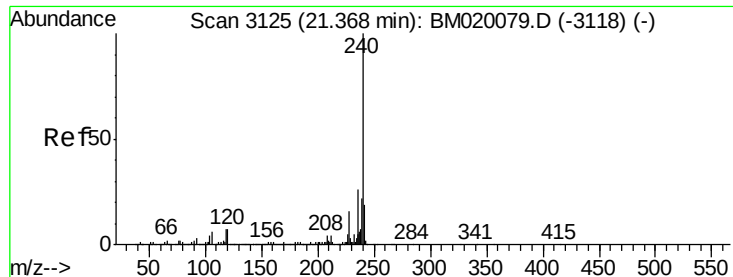

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.37 min Scan# 3125

Delta R.T. -0.00 min

Lab File: BM020139.D

Acq: 06 May 2019 17:13

Instrument :

BNA_M

ClientSampleId :

NB-08-050319-B


Tot Ion:240 Resp: 735417

Ion Ratio Lower Upper

240 100

120 7.3 5.6 8.4

236 26.2 20.9 31.3



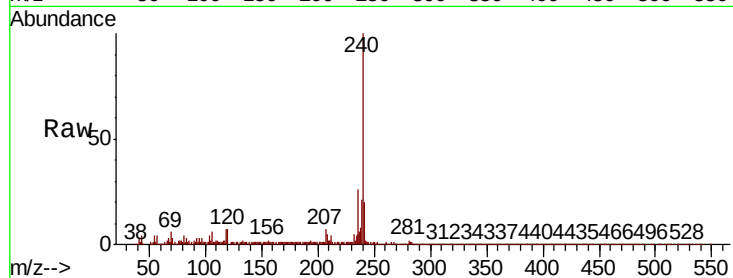


Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

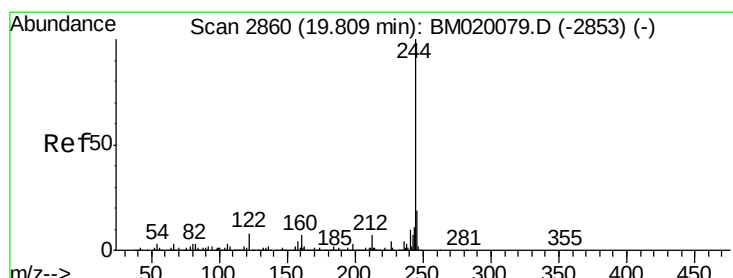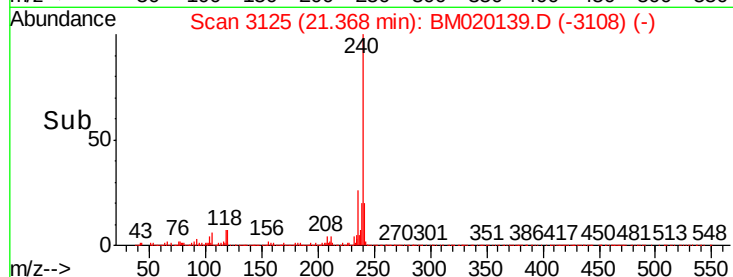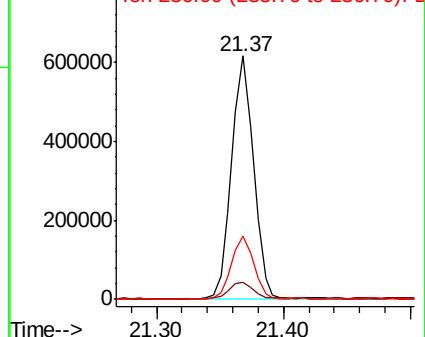

#79

Terphenyl-d14

Concen: 23.874 ng

RT: 19.81 min Scan# 2860

Delta R.T. -0.00 min

Lab File: BM020139.D

Acq: 06 May 2019 17:13


Tgt Ion:244 Resp: 1006586

Ion Ratio Lower Upper

244 100

212 6.9 5.7 8.5

122 6.8 6.2 9.2


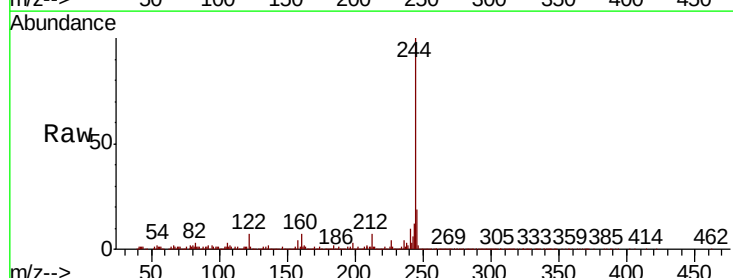



Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

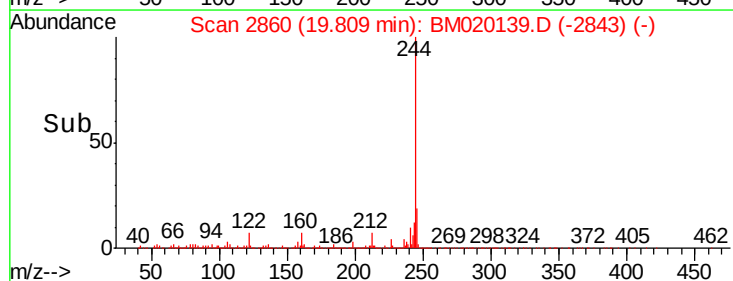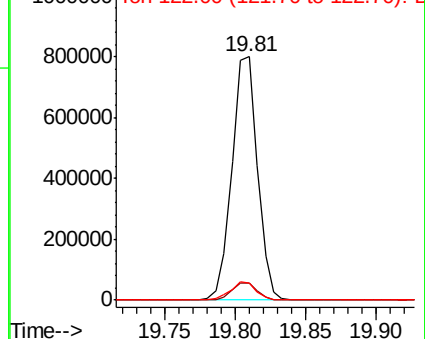



#87
Pervlene-d12
Concen: 20.000 ng
RT: 23.66 min Scan# 3515
Delta R.T. 0.01 min
Lab File: BM020139.D
Acq: 06 May 2019 17:13

Instrument :
BNA_M
ClientSampleId :
NB-08-050319-B

Tot Ion: 264 Resp: 870794

Ion	Ratio	Lower	Upper
264	100		
260	23.3	19.2	28.8
265	22.6	16.9	25.3

