


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050619\
 Data File : BM020149.D
 Acq On : 07 May 2019 02:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 01 03:58:37 2019

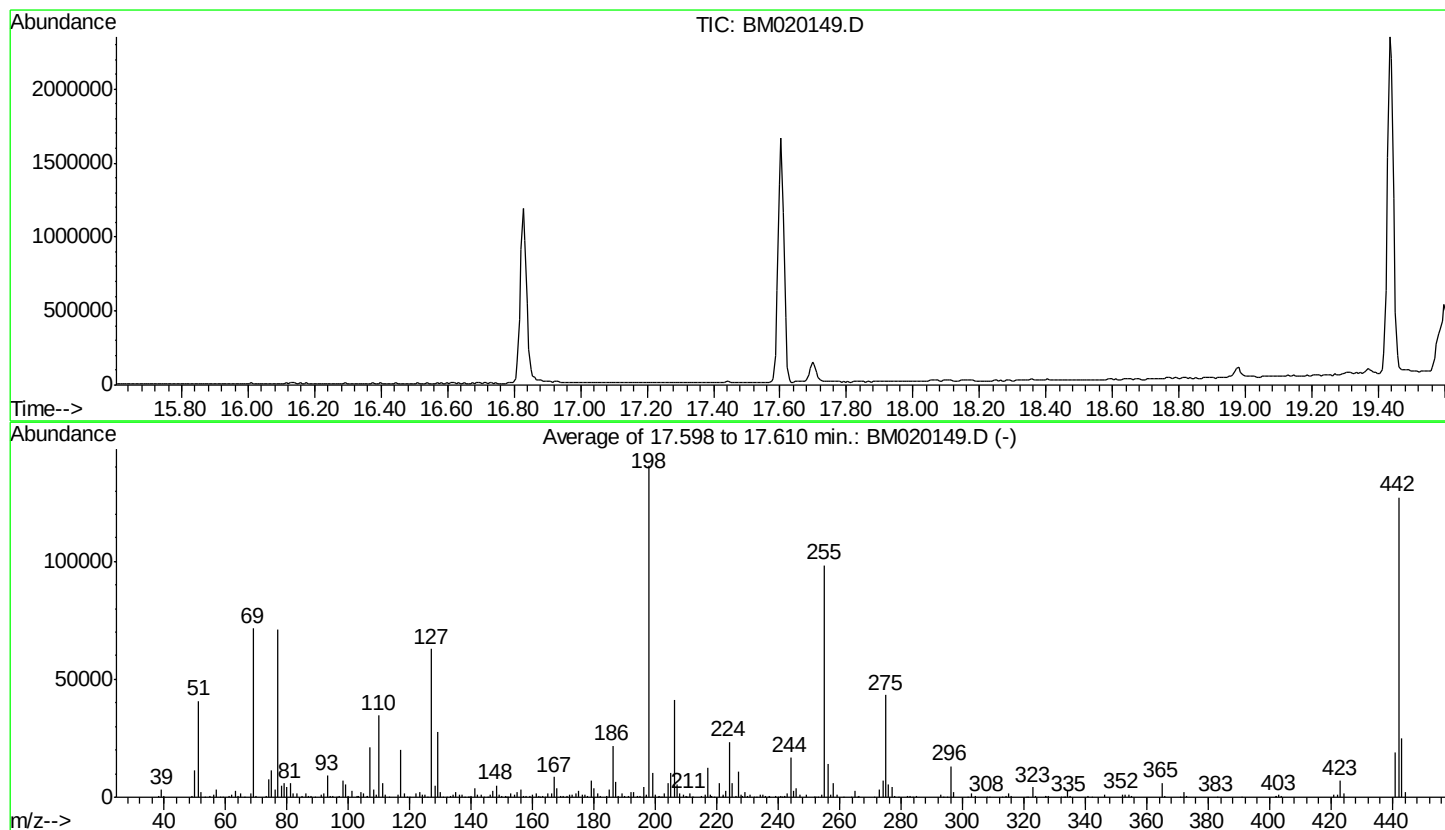

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	40792	PASS
68	69	0.00	2	2.0	1445	PASS
69	198	0.00	100	50.9	71595	PASS
70	69	0.00	2	0.5	357	PASS
127	198	10	80	44.7	62898	PASS
197	198	0.00	2	0.9	1265	PASS
198	198	100	100	100.0	140618	PASS
199	198	5	9	7.2	10183	PASS
275	198	10	60	30.8	43261	PASS
365	198	1	100	4.4	6143	PASS
441	198	0.01	100	13.4	18808	PASS
442	198	50	100	90.4	127088	PASS
443	442	15	24	19.6	24858	PASS